
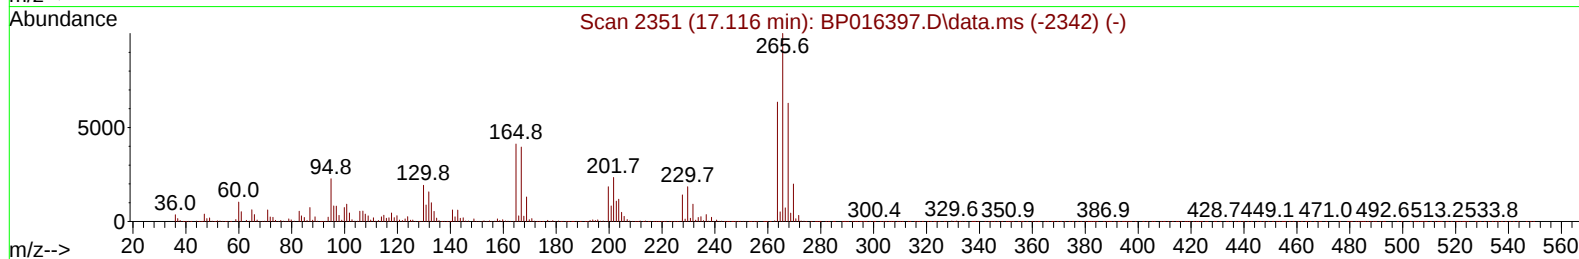
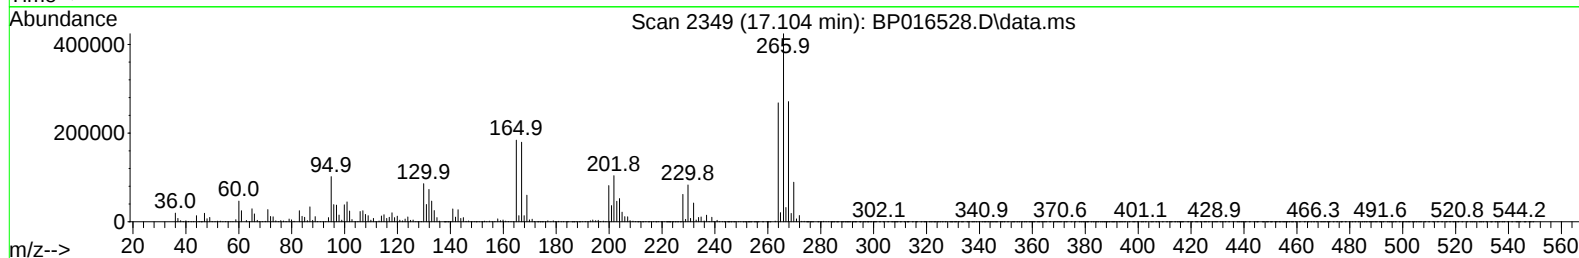


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080823\
Data File : BP016528.D
Acq On : 08 Aug 2023 08:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 09:03:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 18:07:40 2023
Response via : Initial Calibration

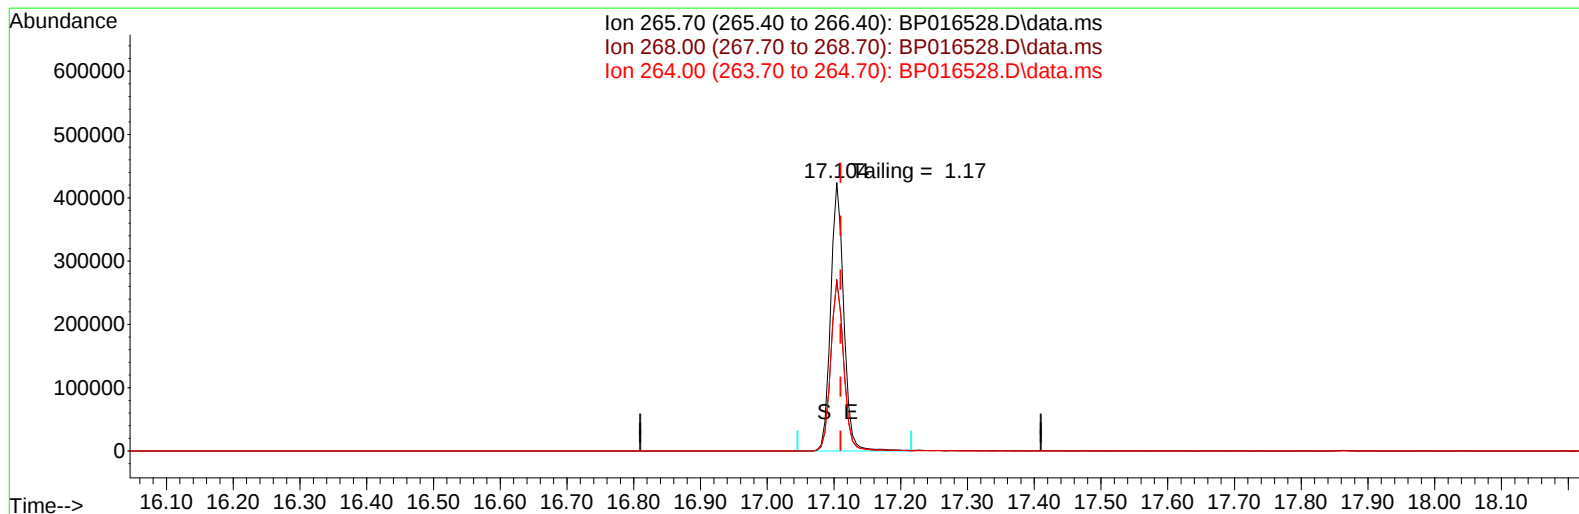

TIC: BP016528.D\data.ms

(70) Pentachlorophenol (C)




17.104min (-0.006) 251401.21 ng

response 579327

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	63.89
264.00	68.60	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080823\
Data File : BP016528.D
Acq On : 08 Aug 2023 08:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 09:03:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 03 18:07:40 2023
Response via : Initial Calibration

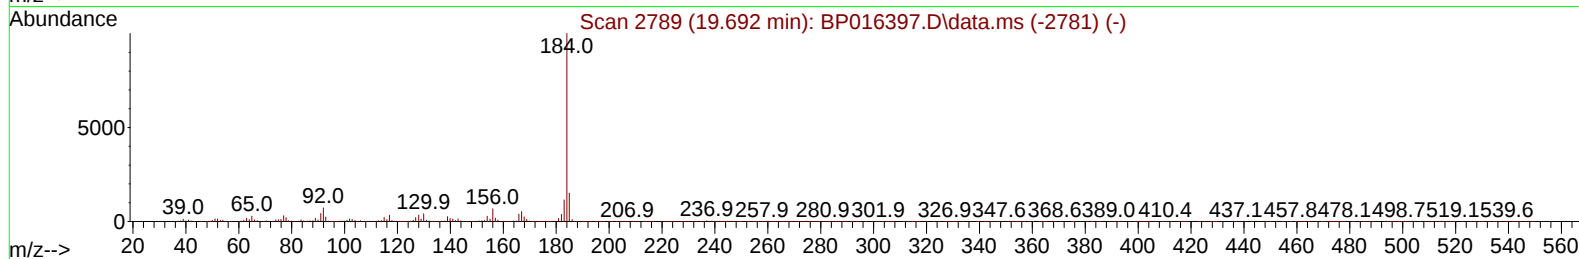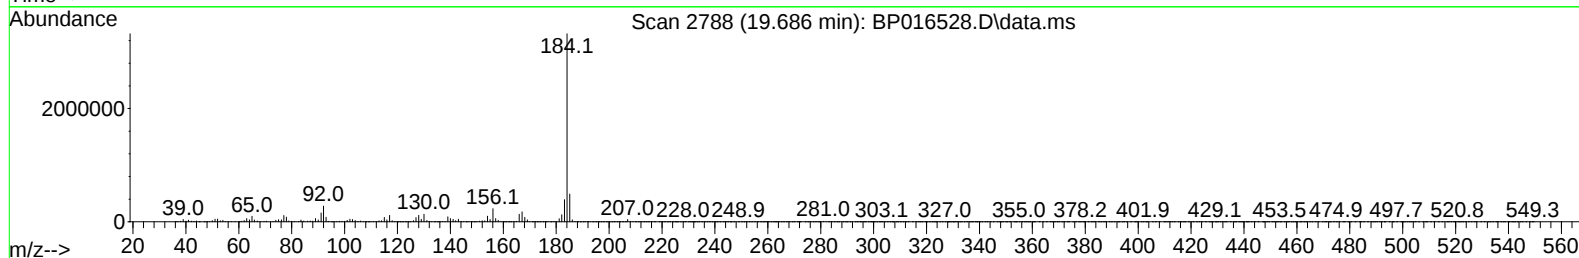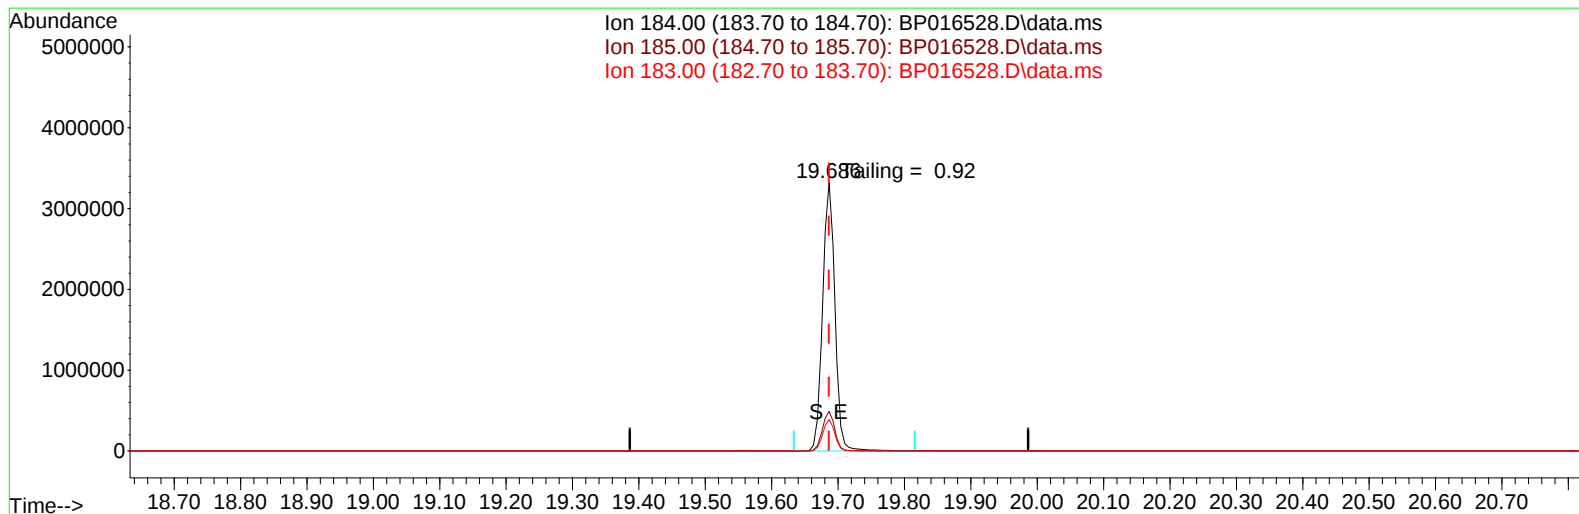

TIC: BP016528.D\data.ms

(77) Benzidine**19.686min (+ 0.000) 201750.90 ng****response 4295420**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.77
183.00	11.50	11.75
0.00	0.00	0.00