


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080823\
Data File : BP016528.D
Acq On : 08 Aug 2023 08:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 08 16:03:02 2023

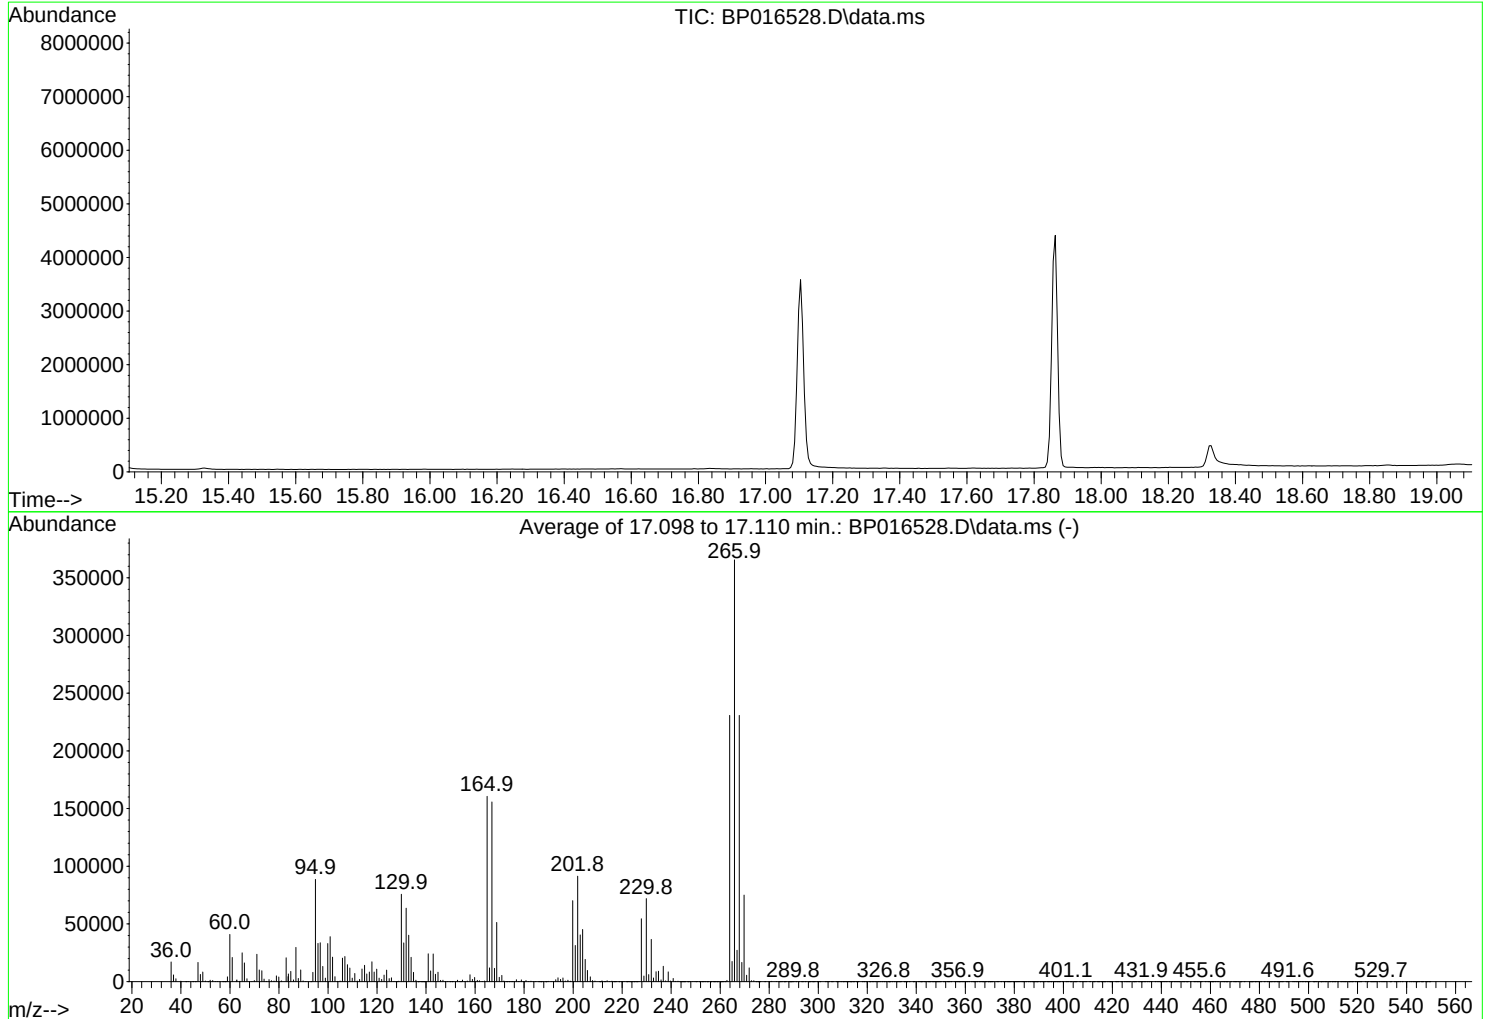

AutoFind: Scans 2348, 2349, 2350; Background Corrected with Scan 2340

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	0.6	515	FAIL*
75	95	30	60	0.3	306	FAIL*
95	95	100	100	100.0	88684	PASS
96	95	5	9	37.3	33120	FAIL*
173	174	0.00	2	358.3	86	FAIL*
174	95	50	100	0.0	24	FAIL*
175	174	5	9	116.7	28	FAIL*
176	174	95	101	654.2	157	FAIL*
177	176	5	9	1021.7	1604	FAIL*

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/8/2023	BNA_P	<u>BP016528.D</u>
Compound Name	Response	Retention Time
DDT	1695464	20.857
DDD	84236	20.428
DDE	2447	19.928
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
86683	1782147	4.86

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080823\
 Data File : BP016528.D
 Acq On : 08 Aug 2023 08:21
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 08 09:03:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 03 18:07:40 2023
 Response via : Initial Calibration

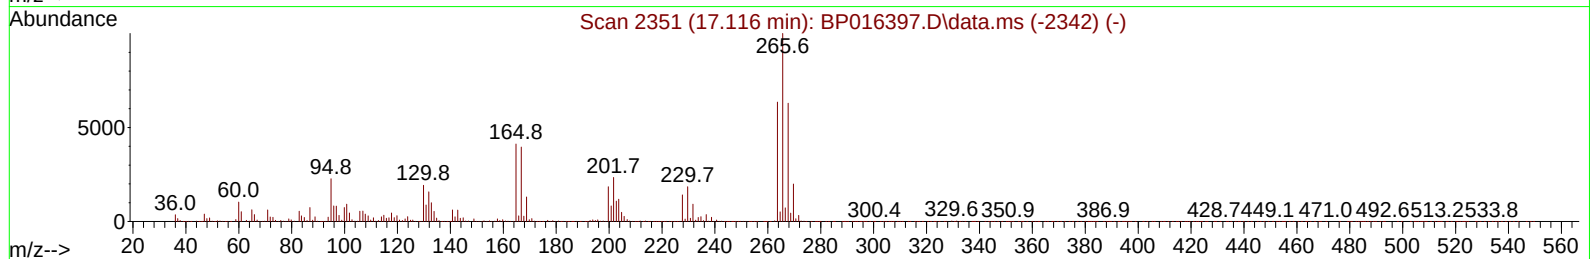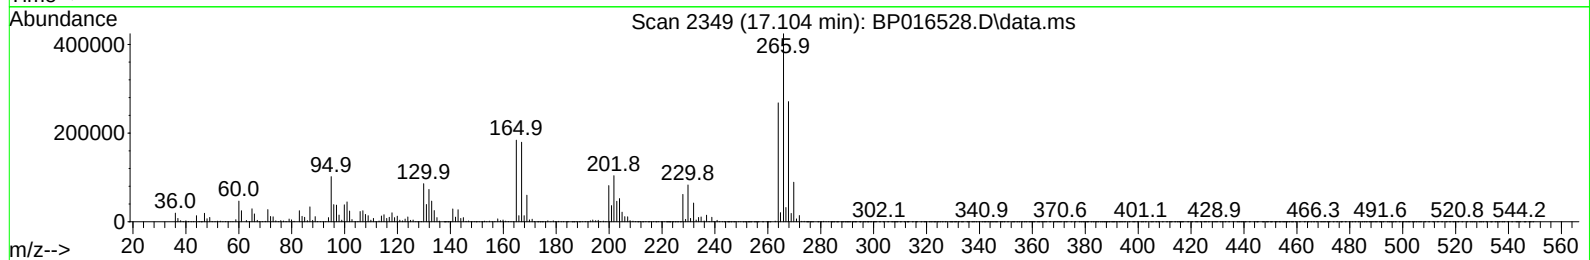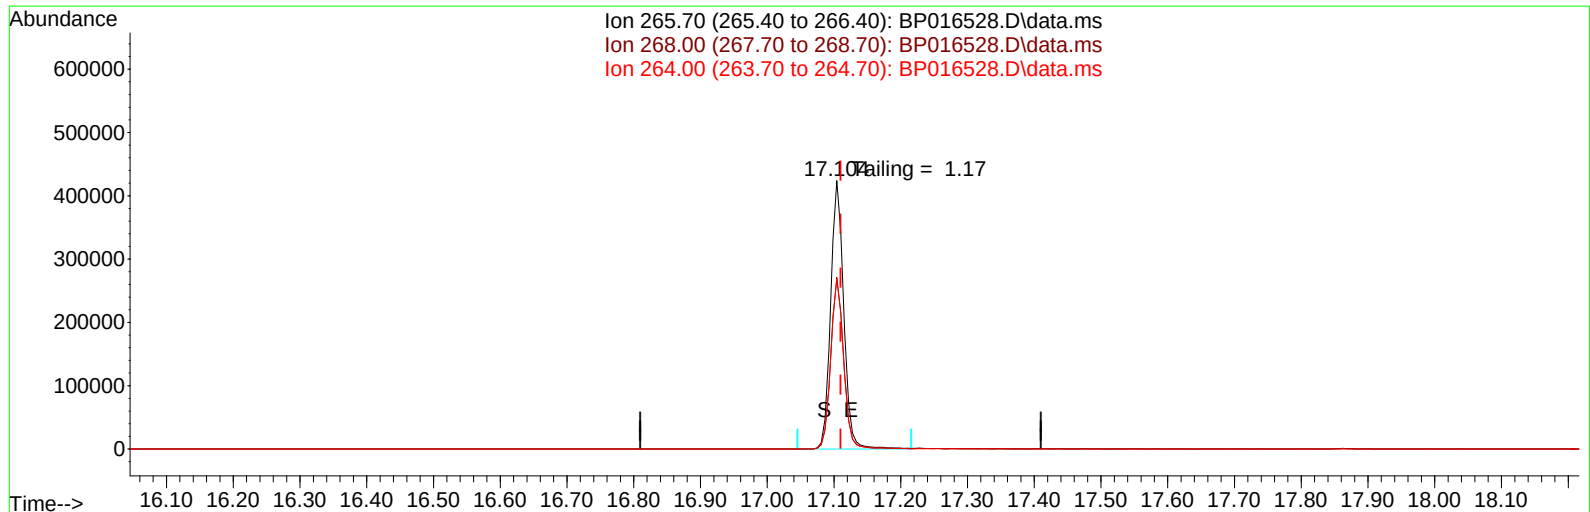

TIC: BP016528.D\data.ms

(70) Pentachlorophenol (C)

17.104min (-0.006) 251401.21 ng




response 579327

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	63.89
264.00	68.60	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080823\
 Data File : BP016528.D
 Acq On : 08 Aug 2023 08:21
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 08 09:03:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 03 18:07:40 2023
 Response via : Initial Calibration

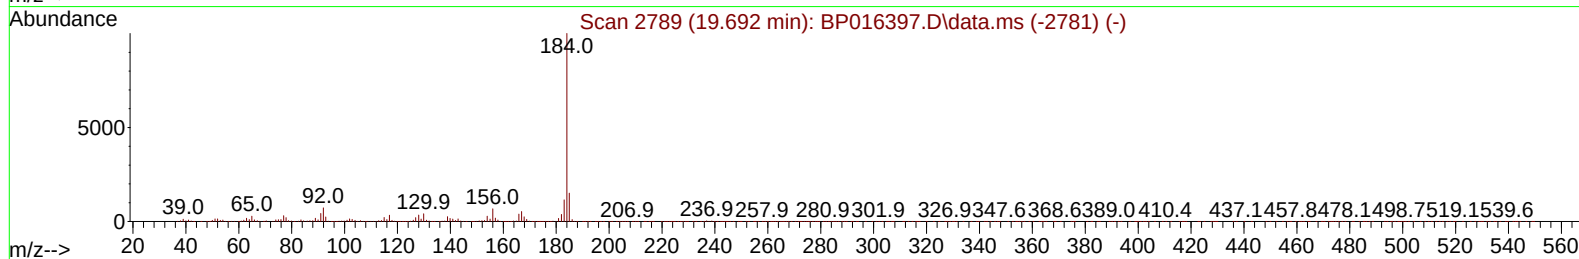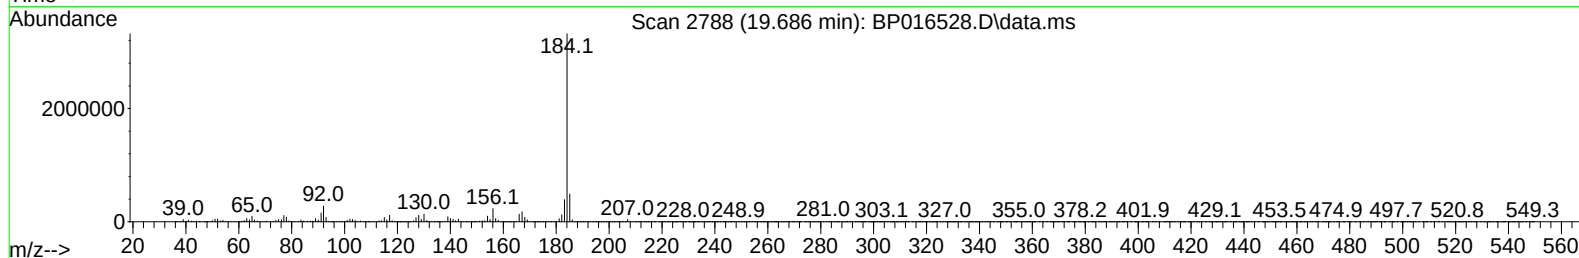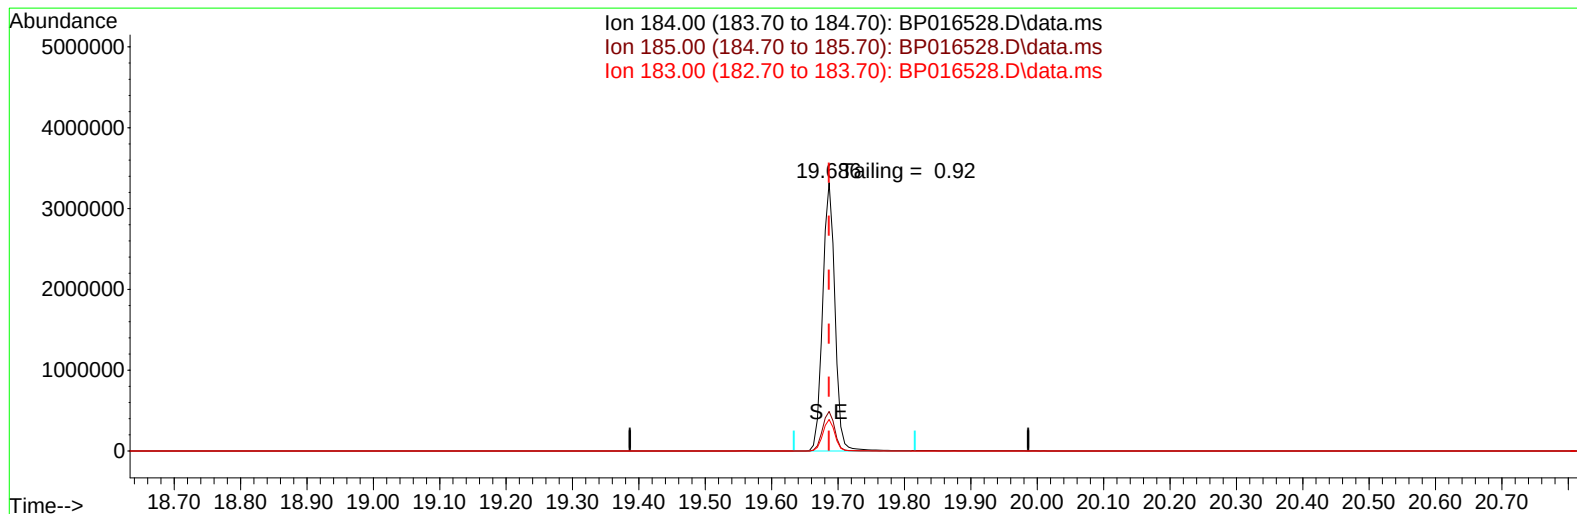

TIC: BP016528.D\data.ms

(77) Benzidine

19.686min (+ 0.000) 201750.90 ng

response 4295420

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.77
183.00	11.50	11.75
0.00	0.00	0.00