

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006625.D
 Acq On : 10 Aug 2021 16:08
 Operator : CG/JU
 Sample : PB138137BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006625.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	21	23	31	rVB	51717	76245	2.04%	0.184%
2	3.634	89	93	105	rBV	565694	860856	23.00%	2.075%
3	6.899	642	648	656	rVB	739450	1118532	29.89%	2.697%
4	7.064	671	676	685	rVB	581142	883691	23.61%	2.130%
5	7.252	702	708	718	rVB	753572	1163571	31.09%	2.805%
6	7.717	782	787	796	rVB	551327	866098	23.14%	2.088%
7	8.434	902	909	918	rVB	869457	1394291	37.26%	3.361%
8	8.875	977	984	991	rVB	725159	1159553	30.98%	2.796%
9	9.593	1100	1106	1117	rVB	601943	976102	26.08%	2.353%
10	10.128	1190	1197	1205	rBV	825514	1355953	36.23%	3.269%
11	10.505	1254	1261	1268	rVB	778118	1270641	33.95%	3.063%
12	10.646	1278	1285	1298	rVB	856220	1495645	39.96%	3.606%
13	12.099	1527	1532	1538	rBV4	15393	26537	0.71%	0.064%
14	12.310	1564	1568	1573	rBV8	2750	5409	0.14%	0.013%
15	13.081	1695	1699	1703	rBV5	3300	4838	0.13%	0.012%
16	13.322	1738	1740	1746	rVB4	4314	6186	0.17%	0.015%
17	13.781	1811	1818	1828	rBV	1667611	2205952	58.94%	5.318%
18	14.051	1857	1864	1877	rBV	1694746	2466510	65.91%	5.946%
19	14.357	1909	1916	1924	rBV	1165054	1676892	44.81%	4.043%
20	14.481	1935	1937	1943	rVB7	2839	4611	0.12%	0.011%
21	14.569	1946	1952	1966	rBV	833462	1225925	32.76%	2.956%
22	14.728	1974	1979	1983	rBV8	2277	4161	0.11%	0.010%
23	15.357	2079	2086	2099	rBV	2147866	2998456	80.12%	7.229%
24	15.481	2101	2107	2116	rBV	802810	1080476	28.87%	2.605%
25	15.598	2122	2127	2132	rVB	25900	37545	1.00%	0.091%
26	16.040	2197	2202	2209	rVB10	3693	8171	0.22%	0.020%
27	16.140	2216	2219	2223	rBV5	5151	8147	0.22%	0.020%
28	16.904	2343	2349	2353	rBV5	6538	11471	0.31%	0.028%
29	17.116	2378	2385	2395	rBV	1404344	1941945	51.89%	4.682%
30	17.216	2395	2402	2413	rVB2	2393180	3275434	87.52%	7.897%
31	17.498	2445	2450	2452	rBV5	2845	4120	0.11%	0.010%
32	17.534	2452	2456	2461	rVB6	3400	6101	0.16%	0.015%
33	17.751	2488	2493	2496	rBV7	4819	6485	0.17%	0.016%
34	18.022	2535	2539	2543	rBV6	7787	12125	0.32%	0.029%
35	18.087	2543	2550	2557	rBV7	9693	19990	0.53%	0.048%
36	18.539	2623	2627	2632	rBV8	8383	12589	0.34%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006625.D
 Acq On : 10 Aug 2021 16:08
 Operator : CG/JU
 Sample : PB138137BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK137

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

37	19.039	2708	2712	2718	rBV6	18791	29474	0.79%	0.071%
38	19.104	2719	2723	2727	rBV	27135	39788	1.06%	0.096%
39	19.351	2762	2765	2770	rBV3	11640	15155	0.40%	0.037%
40	19.463	2778	2784	2792	rBV	2916906	3659822	97.79%	8.823%
41	21.222	3078	3083	3088	rBV	1665947	2116406	56.55%	5.102%
42	23.386	3445	3451	3459	rVB2	2019664	3742409	100.00%	9.022%
43	23.533	3470	3476	3485	rVB2	1102587	2204811	58.91%	5.315%


Sum of corrected areas: 41479119

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006625.D
Acq On : 10 Aug 2021 16:08
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

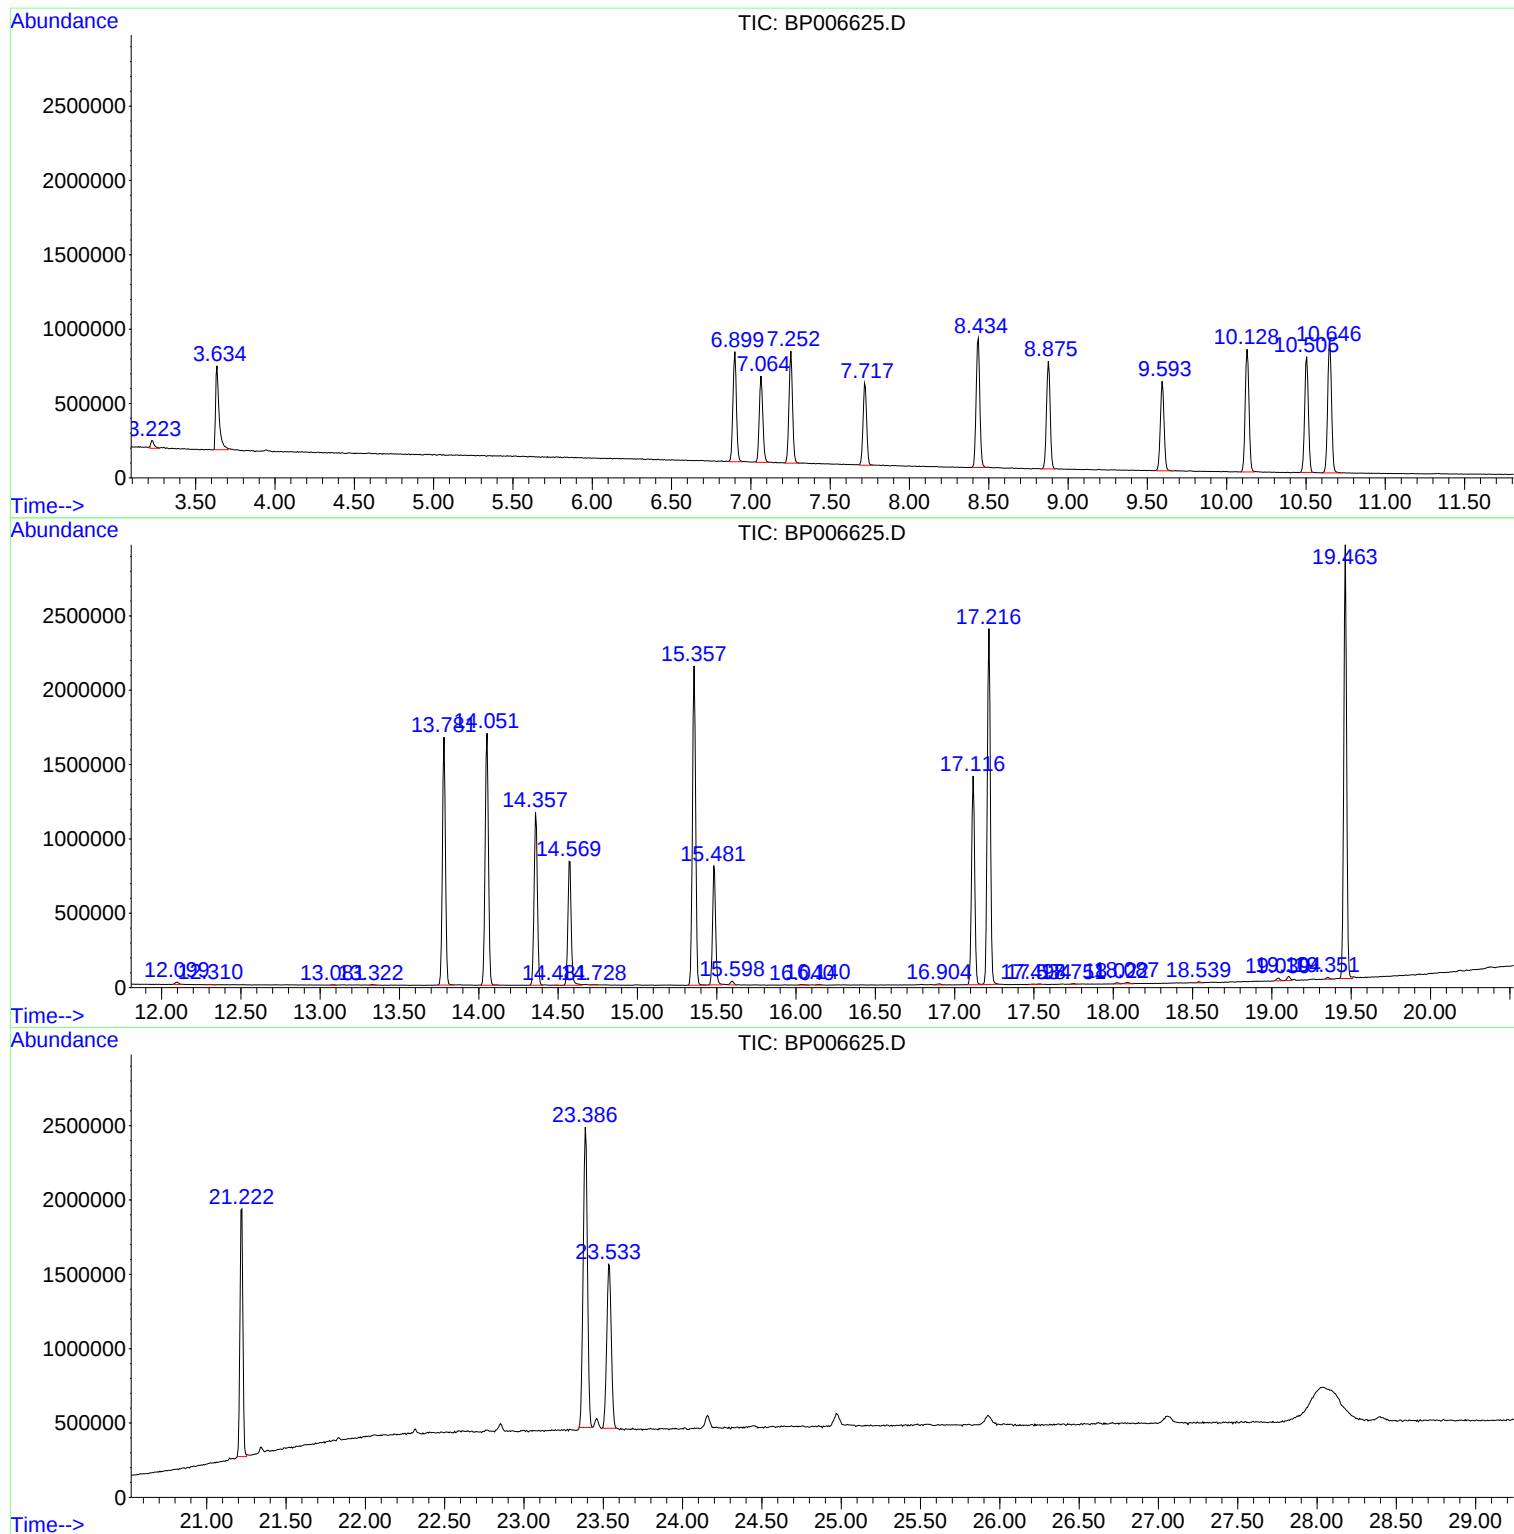

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006625.D
Acq On : 10 Aug 2021 16:08
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006625.D
Acq On : 10 Aug 2021 16:08
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
