

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006626.D
 Acq On : 10 Aug 2021 16:43
 Operator : CG/JU
 Sample : PB138137BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006626.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.634	89	93	108	rBV	575717	875405	22.89%	2.143%
2	6.899	642	648	660	rVB	734736	1117709	29.23%	2.736%
3	7.064	671	676	687	rVB	568595	895181	23.41%	2.191%
4	7.252	702	708	716	rVB	747066	1150391	30.08%	2.816%
5	7.722	782	788	797	rVB	520233	828437	21.66%	2.028%
6	8.434	903	909	918	rVB	890307	1379943	36.08%	3.378%
7	8.875	978	984	992	rVB	717039	1148182	30.02%	2.811%
8	9.593	1100	1106	1121	rVB	592574	975674	25.51%	2.389%
9	10.128	1191	1197	1205	rBV	803242	1324528	34.63%	3.243%
10	10.505	1254	1261	1270	rVB	737226	1202400	31.44%	2.944%
11	10.652	1278	1286	1298	rBV	895419	1484457	38.82%	3.634%
12	12.099	1525	1532	1540	rVB3	16560	30283	0.79%	0.074%
13	12.310	1566	1568	1576	rVB7	3050	5433	0.14%	0.013%
14	13.334	1737	1742	1746	rVB6	3665	5841	0.15%	0.014%
15	13.781	1811	1818	1829	rVV	1599825	2190566	57.28%	5.363%
16	14.051	1855	1864	1877	rBV	1719179	2476962	64.77%	6.064%
17	14.357	1910	1916	1924	rBV	1093573	1574607	41.17%	3.855%
18	14.569	1945	1952	1965	rBV	839961	1226682	32.07%	3.003%
19	15.357	2079	2086	2094	rBV	2114919	2968341	77.62%	7.267%
20	15.481	2101	2107	2117	rBV	770422	1079235	28.22%	2.642%
21	15.598	2122	2127	2132	rVB3	23832	34271	0.90%	0.084%
22	15.928	2175	2183	2190	rBV3	2857	5996	0.16%	0.015%
23	16.045	2197	2203	2211	rVB3	4928	9620	0.25%	0.024%
24	16.145	2216	2220	2224	rVV6	4803	6833	0.18%	0.017%
25	16.798	2327	2331	2336	rVB7	3816	6045	0.16%	0.015%
26	16.904	2344	2349	2356	rVB3	6633	13074	0.34%	0.032%
27	17.116	2378	2385	2392	rBV	1362272	1829551	47.84%	4.479%
28	17.216	2395	2402	2413	rBV	2358482	3258081	85.19%	7.976%
29	17.745	2490	2492	2497	rVB6	3438	5257	0.14%	0.013%
30	18.022	2535	2539	2543	rBV7	6713	10629	0.28%	0.026%
31	18.087	2545	2550	2555	rVV6	6533	11894	0.31%	0.029%
32	18.539	2623	2627	2630	rBV5	6171	10026	0.26%	0.025%
33	19.039	2708	2712	2716	rBV4	18201	24504	0.64%	0.060%
34	19.104	2719	2723	2732	rBV2	28000	49415	1.29%	0.121%
35	19.463	2777	2784	2792	rBV	2709941	3643919	95.28%	8.921%
36	21.216	3077	3082	3087	rBV	1676668	2024060	52.92%	4.955%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006626.D
Acq On : 10 Aug 2021 16:43
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Title : SVOA CALIBRATION

37	23.386	3444	3451	3458	rBV2	2066254	3824440	100.00%	9.363%
38	23.533	3470	3476	3487	rVB	1063573	2140472	55.97%	5.240%




Sum of corrected areas: 40848344

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006626.D
Acq On : 10 Aug 2021 16:43
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

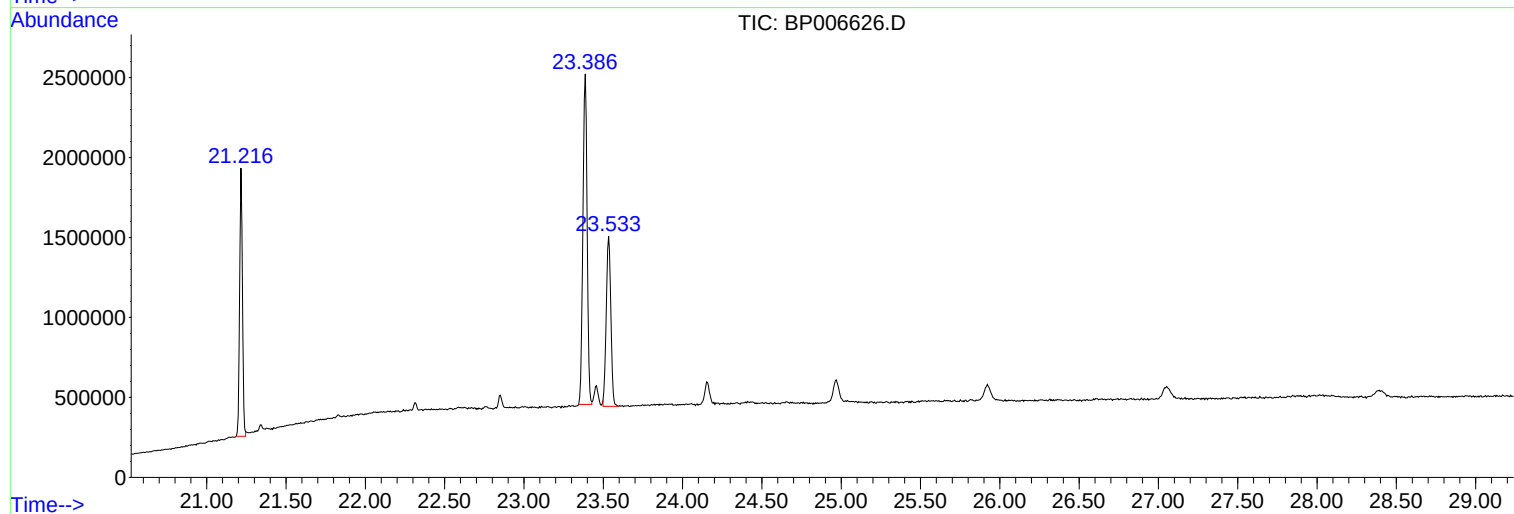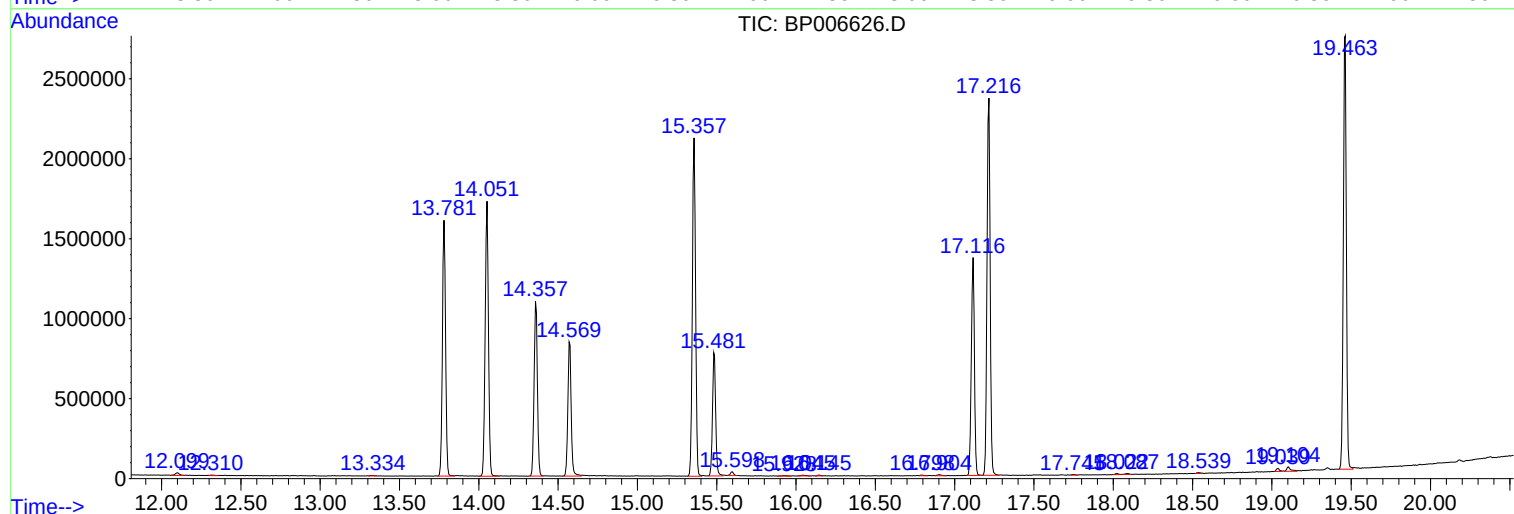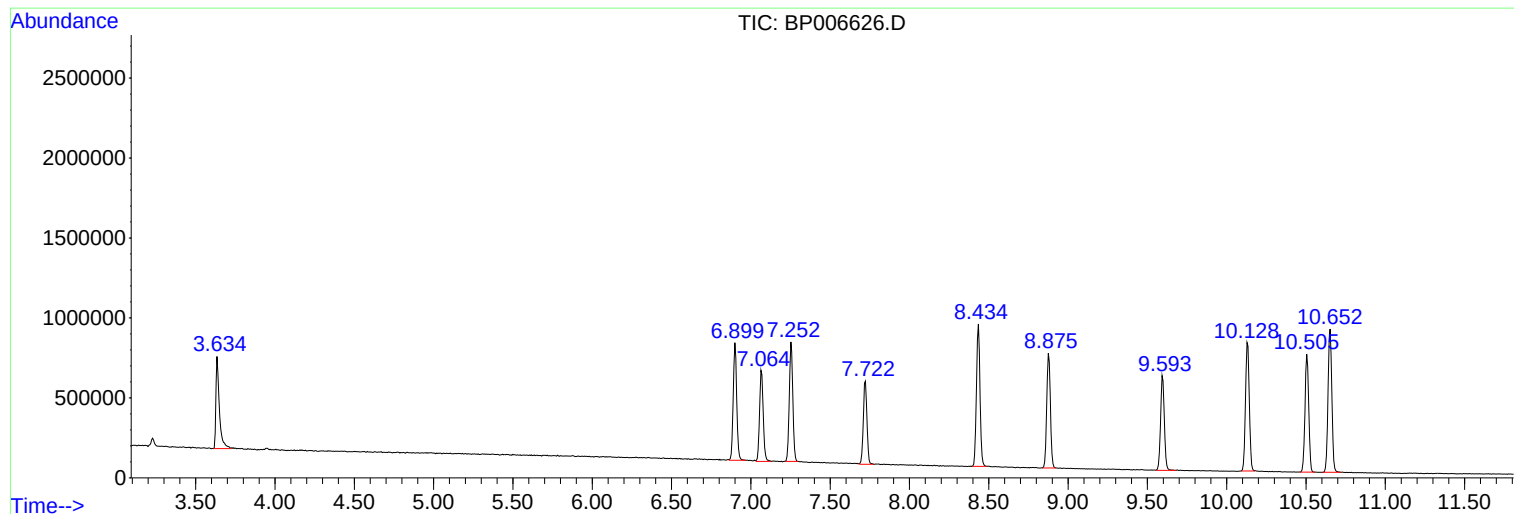

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006626.D
Acq On : 10 Aug 2021 16:43
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006626.D
Acq On : 10 Aug 2021 16:43
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
