

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006627.D
 Acq On : 10 Aug 2021 17:17
 Operator : CG/JU
 Sample : M3208-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00F1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006627.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.646	92	95	105	rVB	95711	157259	7.46%	0.610%
2	6.899	643	648	655	rVB	351813	540011	25.62%	2.095%
3	7.064	671	676	683	rVB	275737	432609	20.53%	1.678%
4	7.252	703	708	716	rVB	369189	571975	27.14%	2.219%
5	7.722	782	788	797	rVB	511787	810964	38.48%	3.146%
6	8.434	903	909	916	rBV	316504	504834	23.95%	1.958%
7	8.875	978	984	993	rVB	370396	594094	28.19%	2.305%
8	9.593	1100	1106	1113	rBV	304623	487721	23.14%	1.892%
9	9.899	1156	1158	1160	rBV2	4233	3333	0.16%	0.013%
10	10.128	1191	1197	1207	rVB	414846	679817	32.26%	2.637%
11	10.305	1222	1227	1238	rVB2	34943	74074	3.51%	0.287%
12	10.505	1254	1261	1268	rBV	726405	1197300	56.81%	4.645%
13	10.652	1279	1286	1293	rBV	316717	540768	25.66%	2.098%
14	10.916	1329	1331	1334	rVB3	3549	3501	0.17%	0.014%
15	11.316	1395	1399	1404	rVB8	4789	6672	0.32%	0.026%
16	11.546	1433	1438	1441	rBV6	7210	10928	0.52%	0.042%
17	11.946	1501	1506	1511	rVB3	8917	16318	0.77%	0.063%
18	12.028	1515	1520	1525	rVV8	3885	8094	0.38%	0.031%
19	12.093	1525	1531	1537	rVB4	9570	21290	1.01%	0.083%
20	12.175	1539	1545	1551	rVB3	10325	17982	0.85%	0.070%
21	12.310	1564	1568	1572	rBV5	2448	3390	0.16%	0.013%
22	12.393	1576	1582	1587	rVB4	6898	12038	0.57%	0.047%
23	12.640	1617	1624	1630	rBV4	4325	11210	0.53%	0.043%
24	12.704	1630	1635	1636	rBV4	4430	4785	0.23%	0.019%
25	12.763	1642	1645	1648	rBV5	2073	3185	0.15%	0.012%
26	12.904	1665	1669	1675	rVB7	4419	7168	0.34%	0.028%
27	12.975	1675	1681	1684	rBV7	5403	9247	0.44%	0.036%
28	13.193	1711	1718	1723	rBV4	13018	21159	1.00%	0.082%
29	13.269	1725	1731	1734	rBV7	5368	10402	0.49%	0.040%
30	13.328	1738	1741	1749	rVB10	2749	5426	0.26%	0.021%
31	13.534	1767	1776	1780	rBV10	5723	17063	0.81%	0.066%
32	13.681	1796	1801	1806	rVV7	7123	14506	0.69%	0.056%
33	13.734	1806	1810	1812	rVV5	5801	9463	0.45%	0.037%
34	13.781	1812	1818	1827	rVV	810827	1111841	52.76%	4.313%
35	13.857	1827	1831	1833	rVV5	6323	8850	0.42%	0.034%
36	13.898	1833	1838	1839	rVV5	4176	6366	0.30%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006627.D
 Acq On : 10 Aug 2021 17:17
 Operator : CG/JU
 Sample : M3208-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00F1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

37	13.916	1839	1841	1844	rVB4	4495	3719	0.18%	0.014%
38	14.051	1856	1864	1874	rBV	880359	1287182	61.08%	4.993%
39	14.181	1883	1886	1888	rBV4	2733	3431	0.16%	0.013%
40	14.275	1897	1902	1907	rVB2	12992	17759	0.84%	0.069%
41	14.357	1907	1916	1924	rBV	1091086	1567787	74.39%	6.082%
42	14.569	1946	1952	1962	rBV	355916	535816	25.42%	2.079%
43	14.722	1972	1978	1982	rBV7	8836	16029	0.76%	0.062%
44	14.763	1984	1985	1987	rVV2	6435	4760	0.23%	0.018%
45	14.793	1987	1990	1995	rVV7	6591	8572	0.41%	0.033%
46	14.840	1995	1998	2002	rVB6	5752	8187	0.39%	0.032%
47	14.893	2002	2007	2011	rVB8	4160	5849	0.28%	0.023%
48	14.975	2015	2021	2022	rBV6	4445	7101	0.34%	0.028%
49	14.993	2022	2024	2027	rVB4	4804	4397	0.21%	0.017%
50	15.034	2027	2031	2035	rVB6	6534	8734	0.41%	0.034%
51	15.116	2035	2045	2050	rBV	37840	60974	2.89%	0.237%
52	15.228	2061	2064	2069	rVB	15610	17205	0.82%	0.067%
53	15.357	2078	2086	2099	rVB	1105422	1555771	73.82%	6.035%
54	15.481	2099	2107	2116	rBV	335401	459253	21.79%	1.782%
55	15.593	2120	2126	2131	rVV3	12822	20019	0.95%	0.078%
56	15.628	2131	2132	2139	rVB7	5297	7410	0.35%	0.029%
57	15.710	2142	2146	2148	rBV5	3258	4478	0.21%	0.017%
58	15.934	2179	2184	2190	rBV9	4598	8951	0.42%	0.035%
59	16.092	2207	2211	2218	rBV2	18975	30746	1.46%	0.119%
60	16.269	2235	2241	2247	rVB2	4504	9108	0.43%	0.035%
61	16.387	2256	2261	2262	rBV5	3696	4805	0.23%	0.019%
62	16.434	2267	2269	2271	rVV3	3499	3395	0.16%	0.013%
63	16.469	2271	2275	2278	rVB6	3351	4788	0.23%	0.019%
64	16.551	2286	2289	2292	rVB5	2744	3548	0.17%	0.014%
65	16.663	2302	2308	2312	rBV6	18090	32103	1.52%	0.125%
66	16.722	2316	2318	2321	rVB4	4004	3125	0.15%	0.012%
67	16.769	2322	2326	2335	rVB9	9377	16368	0.78%	0.063%
68	16.851	2335	2340	2343	rBV6	5809	10781	0.51%	0.042%
69	16.892	2343	2347	2351	rVV2	28863	36586	1.74%	0.142%
70	16.940	2351	2355	2361	rVB8	5242	8892	0.42%	0.034%
71	16.992	2362	2364	2369	rVB5	2590	3131	0.15%	0.012%
72	17.116	2378	2385	2390	rBV	1274804	1791721	85.02%	6.951%
73	17.157	2390	2392	2395	rVV	30859	34205	1.62%	0.133%
74	17.216	2395	2402	2413	rVB2	1074738	1563272	74.18%	6.064%
75	17.322	2413	2420	2423	rBV9	6278	13306	0.63%	0.052%
76	17.434	2435	2439	2443	rVB6	8875	13078	0.62%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006627.D
 Acq On : 10 Aug 2021 17:17
 Operator : CG/JU
 Sample : M3208-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00F1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

77	17.498	2447	2450	2451	rBV3	3672	3820	0.18%	0.015%
78	17.634	2469	2473	2477	rBV3	17660	23925	1.14%	0.093%
79	17.698	2481	2484	2488	rVB5	5550	8568	0.41%	0.033%
80	17.804	2498	2502	2512	rVB5	14032	30672	1.46%	0.119%
81	17.910	2517	2520	2523	rVB5	4240	5246	0.25%	0.020%
82	17.986	2530	2533	2535	rBV3	12228	13548	0.64%	0.053%
83	18.022	2535	2539	2545	rVV2	114120	166605	7.91%	0.646%
84	18.092	2548	2551	2554	rVB3	8216	11314	0.54%	0.044%
85	18.169	2561	2564	2568	rVV3	16557	19635	0.93%	0.076%
86	18.216	2568	2572	2576	rVB4	11441	14193	0.67%	0.055%
87	18.310	2584	2588	2591	rBV2	17710	23351	1.11%	0.091%
88	18.481	2613	2617	2621	rBV3	16449	22652	1.07%	0.088%
89	18.763	2662	2665	2668	rBV4	8890	10838	0.51%	0.042%
90	18.881	2681	2685	2689	rBV4	21627	35277	1.67%	0.137%
91	18.922	2689	2692	2695	rVV2	21001	23891	1.13%	0.093%
92	19.104	2720	2723	2725	rBV	15847	19735	0.94%	0.077%
93	19.134	2725	2728	2734	rVB	57332	71863	3.41%	0.279%
94	19.263	2746	2750	2756	rBV4	45905	60294	2.86%	0.234%
95	19.457	2778	2783	2792	rBV	1425393	1946682	92.37%	7.552%
96	20.004	2874	2876	2880	rVB	25869	27529	1.31%	0.107%
97	20.945	3032	3036	3042	rBV	250774	360386	17.10%	1.398%
98	21.216	3077	3082	3087	rBV	1637932	1998651	94.83%	7.753%
99	23.380	3444	3450	3457	rVB2	894785	1639874	77.81%	6.362%
100	23.533	3469	3476	3484	rVB2	1052146	2107524	100.00%	8.176%



Sum of corrected areas: 25778058

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006627.D
Acq On : 10 Aug 2021 17:17
Operator : CG/JU
Sample : M3208-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00F1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

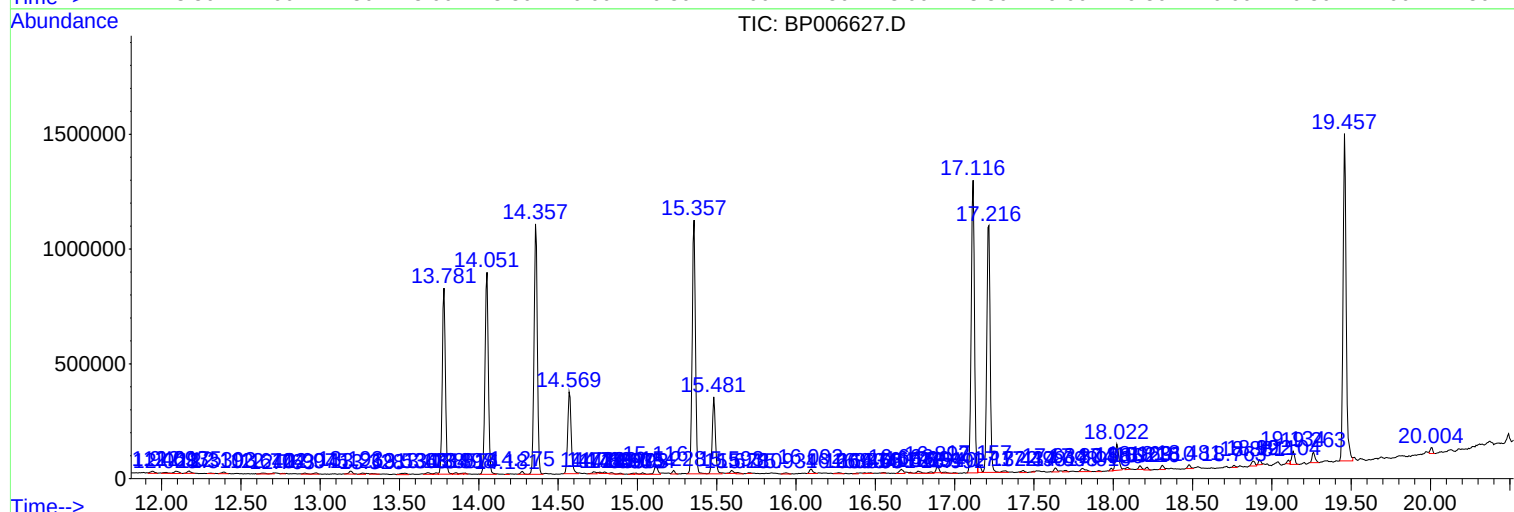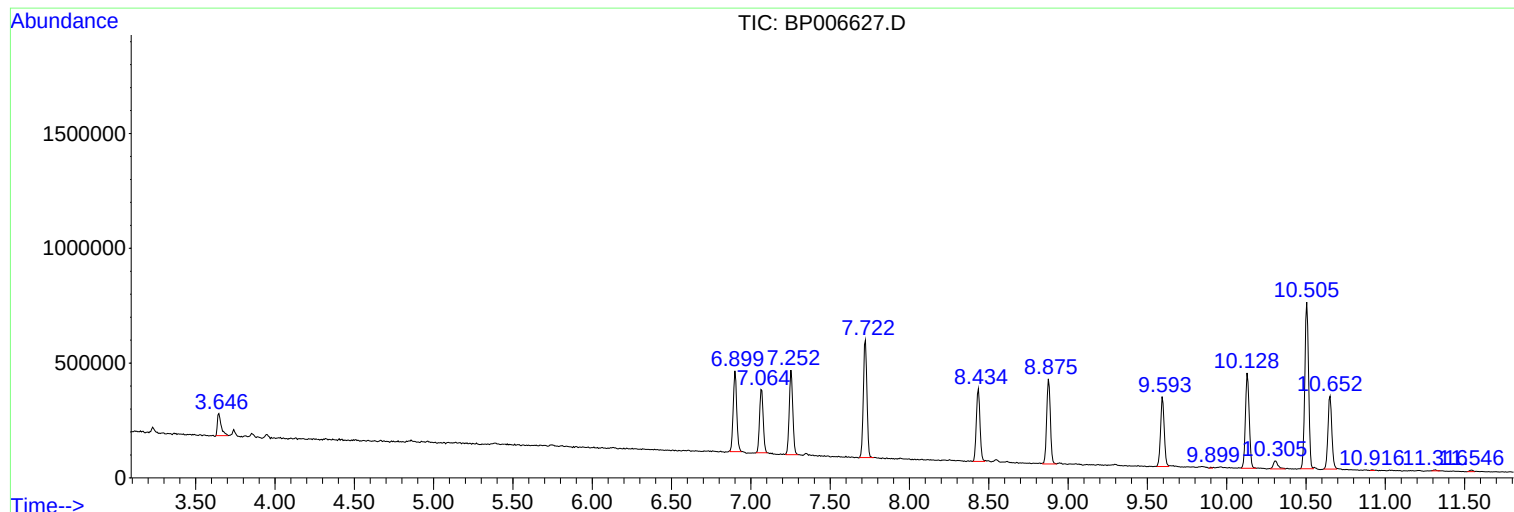

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006627.D
Acq On : 10 Aug 2021 17:17
Operator : CG/JU
Sample : M3208-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00F1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(tetradecyloxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.950	3.61 ng/ul	360386	Chrysene-d12	21.216

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	95
2			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	93
3			1-Triacontanol	438	C30H62O	000593-50-0	91
4			1-Heneicosanol	312	C21H44O	015594-90-8	91
5			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	90

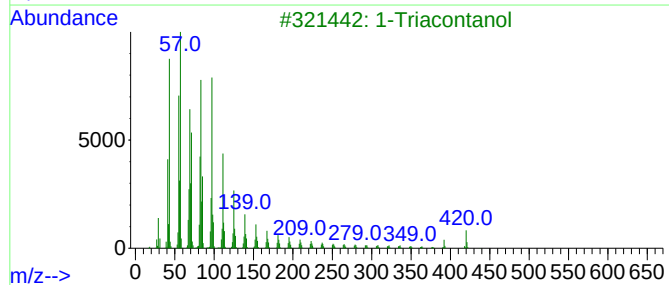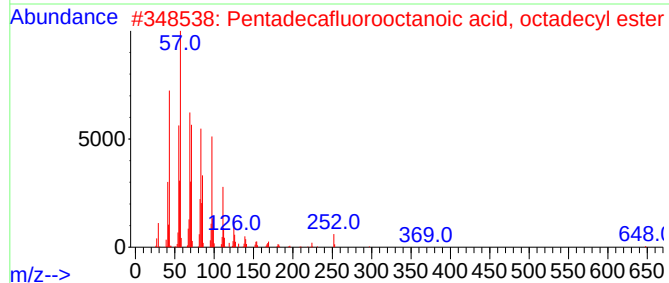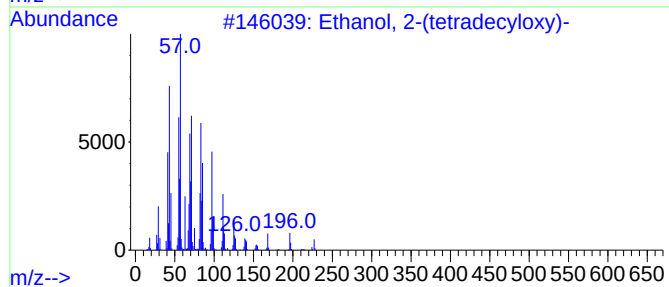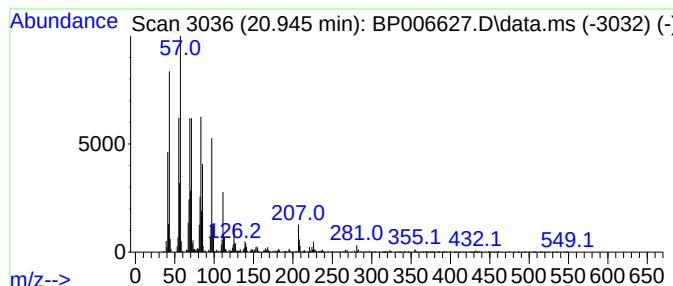

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006627.D
Acq On : 10 Aug 2021 17:17
Operator : CG/JU
Sample : M3208-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00F1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(tet...	20.950	3.6	ng/u1	360386	5	21.216	1998650	20.0