

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006634.D
 Acq On : 10 Aug 2021 21:51
 Operator : CG/JU
 Sample : PB138137BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006634.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	32	rVB	65179	82351	1.80%	0.160%
2	3.634	89	93	111	rVB	744683	1135416	24.84%	2.209%
3	6.899	642	648	659	rVB	957042	1471203	32.19%	2.863%
4	7.063	671	676	688	rVB	736235	1153796	25.24%	2.245%
5	7.252	702	708	718	rVB	989919	1502623	32.87%	2.924%
6	7.716	781	787	795	rVB	634990	1012849	22.16%	1.971%
7	8.434	902	909	917	rBV	1193595	1850805	40.49%	3.602%
8	8.875	978	984	996	rVB	968191	1537050	33.63%	2.991%
9	9.593	1099	1106	1115	rVB	800728	1292188	28.27%	2.515%
10	10.128	1190	1197	1211	rVB	1136006	1813496	39.67%	3.529%
11	10.504	1253	1261	1270	rVB	893982	1501507	32.85%	2.922%
12	10.651	1278	1286	1300	rVB	1162500	1969555	43.09%	3.833%
13	12.098	1526	1532	1540	rVB3	21118	37071	0.81%	0.072%
14	13.322	1734	1740	1743	rBV6	3954	6750	0.15%	0.013%
15	13.781	1810	1818	1827	rBV	2071973	2749470	60.15%	5.350%
16	13.869	1829	1833	1838	rVB8	2595	4965	0.11%	0.010%
17	14.051	1856	1864	1871	rBV	2157489	3221353	70.47%	6.269%
18	14.357	1908	1916	1926	rBV	1339517	1908263	41.75%	3.713%
19	14.569	1945	1952	1968	rBV	1131321	1589943	34.78%	3.094%
20	15.357	2076	2086	2095	rBV	2611044	3808763	83.32%	7.412%
21	15.481	2100	2107	2121	rVV	1013279	1327066	29.03%	2.582%
22	15.592	2121	2126	2131	rVB2	29950	47044	1.03%	0.092%
23	16.045	2197	2203	2206	rBV7	4601	8309	0.18%	0.016%
24	16.145	2216	2220	2223	rVB6	4781	5988	0.13%	0.012%
25	16.422	2263	2267	2275	rVB7	7045	9948	0.22%	0.019%
26	16.786	2327	2329	2335	rVB7	4109	4788	0.10%	0.009%
27	16.898	2340	2348	2355	rBV4	7790	17621	0.39%	0.034%
28	17.110	2377	2384	2393	rBV	1555357	2176797	47.62%	4.236%
29	17.210	2395	2401	2414	rVV	2951082	4147744	90.74%	8.071%
30	17.498	2445	2450	2452	rBV6	4179	6271	0.14%	0.012%
31	18.016	2535	2538	2544	rVB8	7068	9763	0.21%	0.019%
32	19.033	2707	2711	2717	rBV2	27235	37767	0.83%	0.073%
33	19.098	2718	2722	2727	rVV	33059	46453	1.02%	0.090%
34	19.457	2777	2783	2790	rBV	3576656	4571005	100.00%	8.895%
35	21.210	3076	3081	3088	rBV	1885783	2327216	50.91%	4.529%
36	23.380	3443	3450	3457	rVB2	2447171	4568982	99.96%	8.891%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006634.D
Acq On : 10 Aug 2021 21:51
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Title : SVOA CALIBRATION

37	23.527	3468	3475	3484	rVB2	1227254	2426602	53.09%	4.722%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 51388781

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006634.D
Acq On : 10 Aug 2021 21:51
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

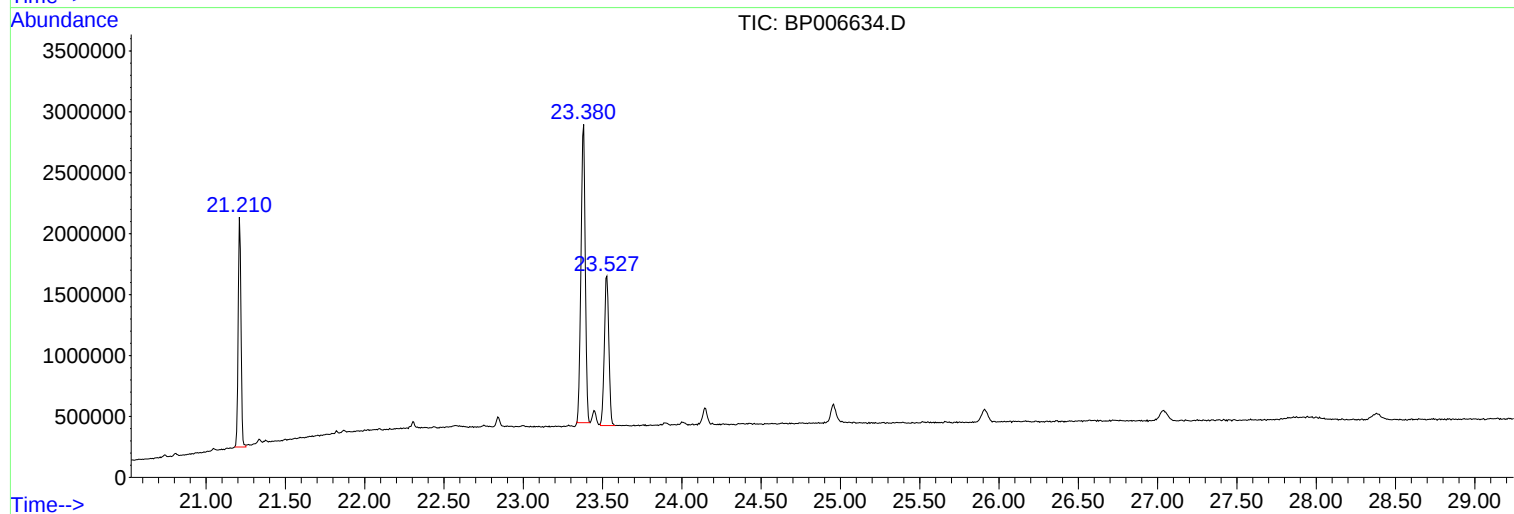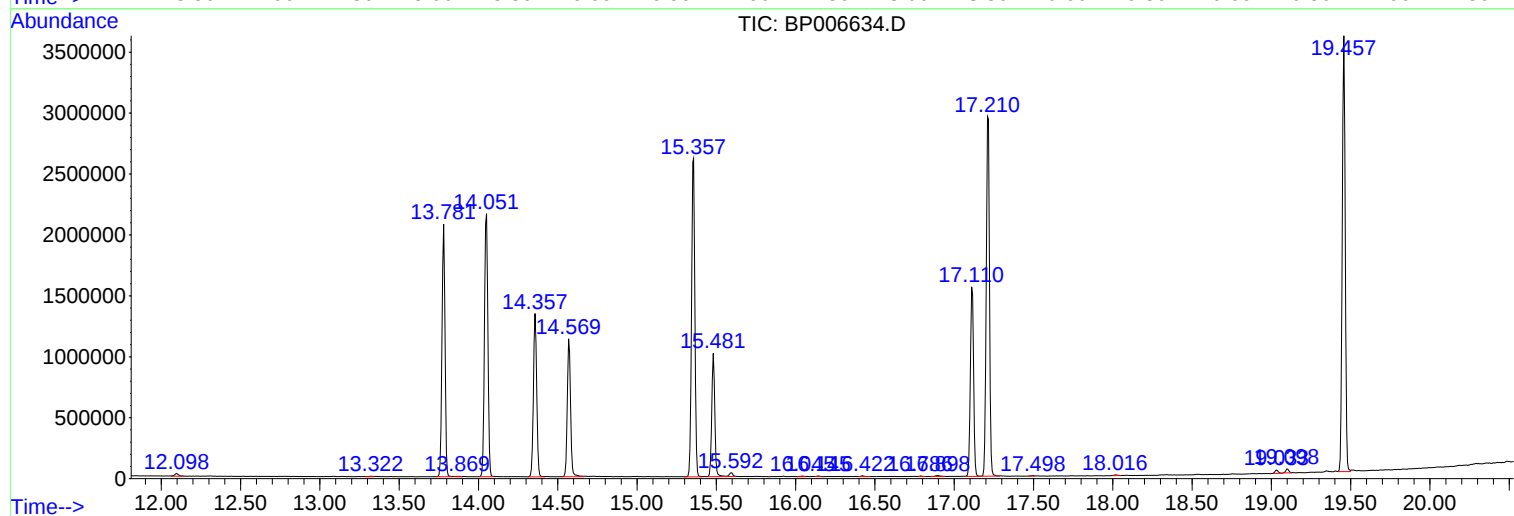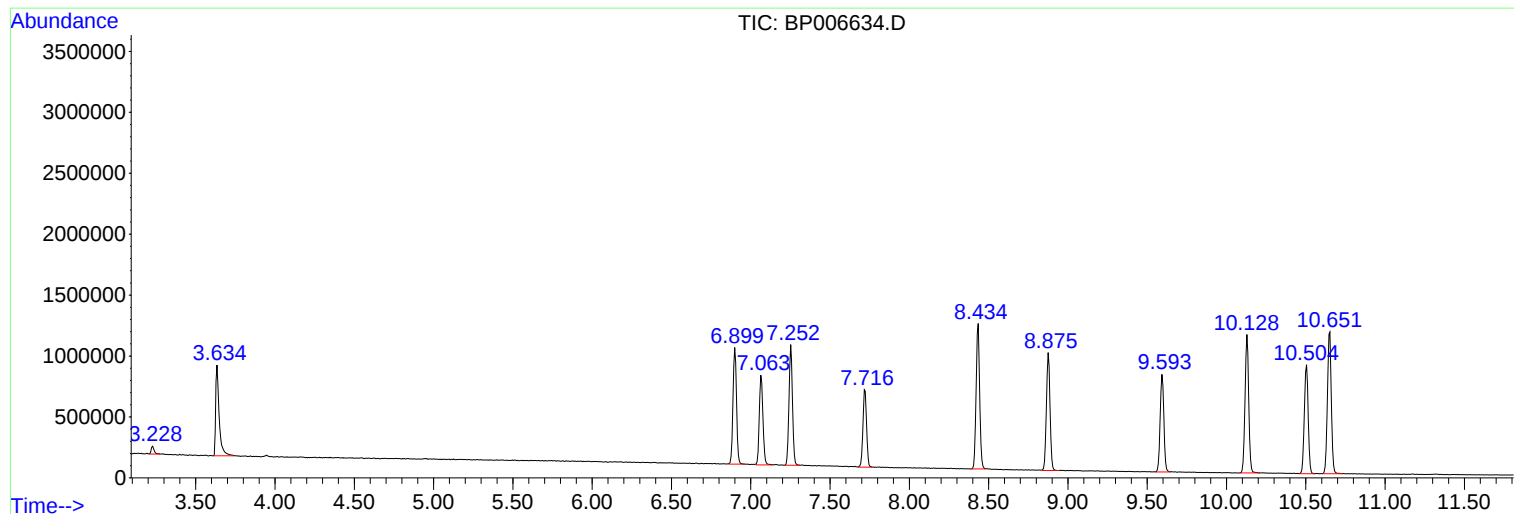

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006634.D
Acq On : 10 Aug 2021 21:51
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006634.D
Acq On : 10 Aug 2021 21:51
Operator : CG/JU
Sample : PB138137BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
