

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006649.D
 Acq On : 11 Aug 2021 10:21
 Operator : CG/JU
 Sample : PB138246BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006649.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	20	23	29	rVB	64246	80814	1.96%	0.174%
2	3.628	88	92	104	rBV	720687	1113730	27.04%	2.405%
3	6.893	641	647	655	rVB	918037	1407367	34.17%	3.039%
4	7.058	669	675	684	rVB	712645	1103693	26.79%	2.383%
5	7.246	701	707	718	rVB	912646	1448566	35.17%	3.128%
6	7.711	780	786	795	rVB	614938	943060	22.89%	2.036%
7	8.428	901	908	919	rVB	1105640	1768838	42.94%	3.819%
8	8.869	977	983	992	rVB	914693	1445142	35.08%	3.120%
9	9.587	1099	1105	1116	rVB	760260	1206273	29.28%	2.604%
10	10.122	1189	1196	1210	rBV	1037956	1690820	41.05%	3.651%
11	10.499	1253	1260	1270	rVB	828460	1367542	33.20%	2.953%
12	10.646	1277	1285	1298	rBV	1065453	1787381	43.39%	3.859%
13	12.093	1526	1531	1537	rVB3	18890	30483	0.74%	0.066%
14	13.781	1811	1818	1828	rBV	1735553	2352680	57.11%	5.080%
15	14.051	1855	1864	1876	rVB	1890362	2862924	69.50%	6.181%
16	14.357	1909	1916	1924	rBV	1168336	1670426	40.55%	3.607%
17	14.575	1946	1953	1970	rBV	947194	1382009	33.55%	2.984%
18	15.357	2079	2086	2094	rBV	2365760	3327416	80.78%	7.184%
19	15.487	2101	2108	2120	rBV	749457	1033778	25.10%	2.232%
20	15.593	2123	2126	2133	rVB	28288	41958	1.02%	0.091%
21	15.757	2150	2154	2160	rVB10	2919	5505	0.13%	0.012%
22	15.928	2179	2183	2187	rBV6	2787	4410	0.11%	0.010%
23	16.045	2197	2203	2206	rBV8	3174	5484	0.13%	0.012%
24	16.251	2233	2238	2243	rBV8	4288	7987	0.19%	0.017%
25	16.792	2326	2330	2335	rVB7	3408	5469	0.13%	0.012%
26	16.904	2342	2349	2355	rBV4	7730	14401	0.35%	0.031%
27	17.116	2377	2385	2395	rBV	1411629	1877387	45.58%	4.053%
28	17.216	2395	2402	2418	rVV	2726269	3685426	89.47%	7.957%
29	17.375	2425	2429	2435	rVB4	6663	10950	0.27%	0.024%
30	17.745	2488	2492	2495	rBV6	5553	7119	0.17%	0.015%
31	17.798	2498	2501	2506	rVB7	4104	6553	0.16%	0.014%
32	17.922	2516	2522	2523	rBV6	2531	4161	0.10%	0.009%
33	18.022	2534	2539	2544	rBV7	12844	20033	0.49%	0.043%
34	18.539	2624	2627	2631	rBV5	12934	17459	0.42%	0.038%
35	19.039	2708	2712	2717	rBV2	36395	47280	1.15%	0.102%
36	19.110	2720	2724	2727	rBV	28048	37203	0.90%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006649.D
Acq On : 11 Aug 2021 10:21
Operator : CG/JU
Sample : PB138246BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP




If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Title : SVOA CALIBRATION

37	19.463	2778	2784	2791	rBV	3140023	4028724	97.80%	8.698%
38	21.222	3078	3083	3088	rBV	1590826	2066815	50.17%	4.462%
39	21.345	3100	3104	3109	rBV	121031	170364	4.14%	0.368%
40	23.392	3445	3452	3460	rBV2	2306592	4119290	100.00%	8.894%
41	23.539	3471	3477	3487	rVB2	1081737	2108658	51.19%	4.553%

Sum of corrected areas: 46315578

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

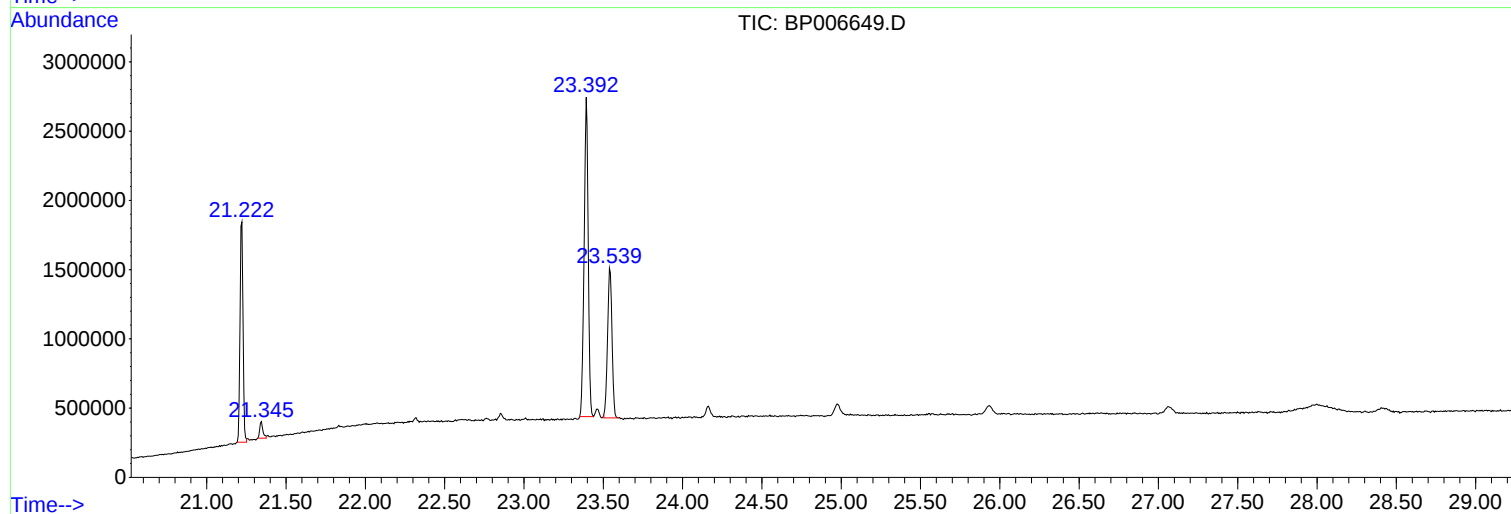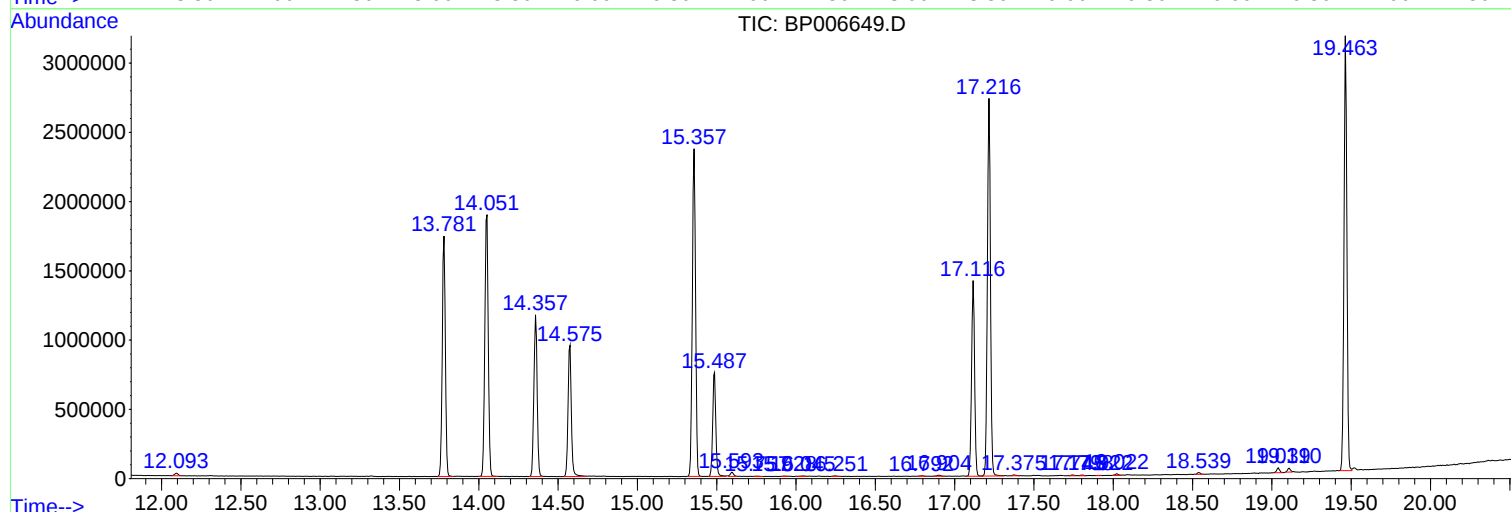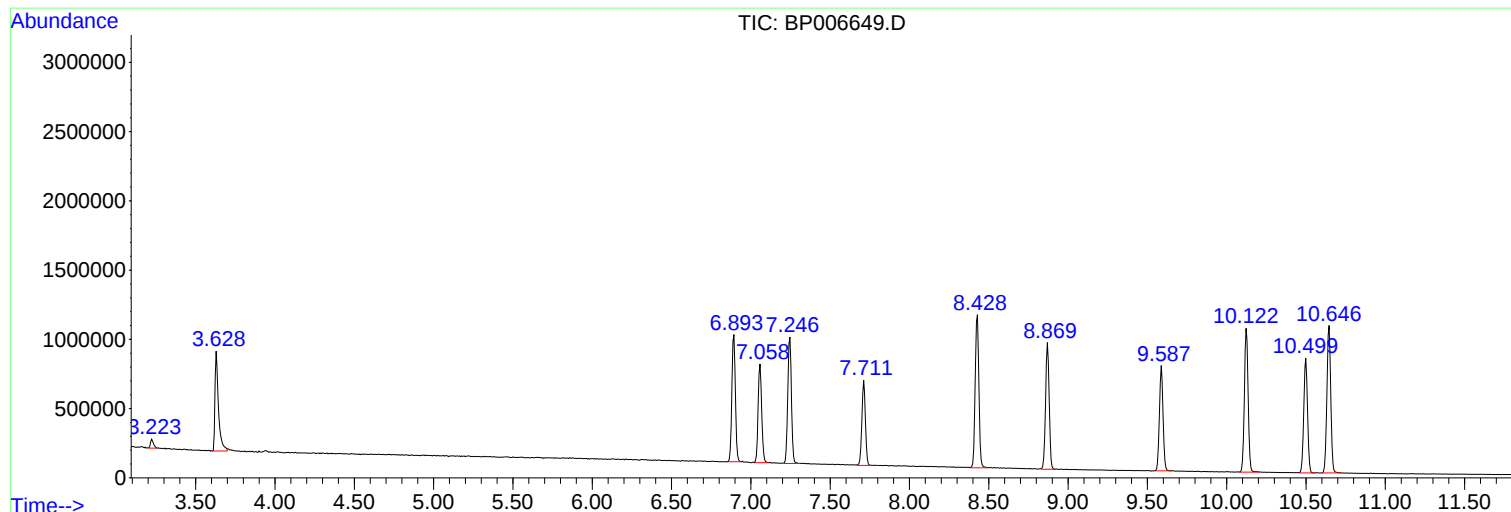

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006649.D
Acq On : 11 Aug 2021 10:21
Operator : CG/JU
Sample : PB138246BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006649.D
Acq On : 11 Aug 2021 10:21
Operator : CG/JU
Sample : PB138246BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------