

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006651.D
 Acq On : 11 Aug 2021 12:11
 Operator : CG/JU
 Sample : M3246-01 30X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006651.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.716	781	787	795	rVB	583623	912076	44.07%	8.516%
2	10.134	1193	1198	1204	rVB3	18389	33223	1.61%	0.310%
3	10.498	1253	1260	1267	rBV	814496	1337588	64.63%	12.489%
4	11.034	1349	1351	1353	rBV3	2524	2307	0.11%	0.022%
5	12.169	1540	1544	1551	rVB3	12229	19503	0.94%	0.182%
6	12.387	1576	1581	1586	rVB	9494	15159	0.73%	0.142%
7	12.687	1630	1632	1636	rBV4	1869	2249	0.11%	0.021%
8	12.898	1664	1668	1672	rVB7	2303	3034	0.15%	0.028%
9	13.081	1695	1699	1705	rVB7	2697	4076	0.20%	0.038%
10	13.187	1715	1717	1720	rVB4	2820	3233	0.16%	0.030%
11	13.381	1746	1750	1752	rBV5	2054	2625	0.13%	0.025%
12	13.416	1755	1756	1760	rVB4	2893	2409	0.12%	0.022%
13	13.522	1767	1774	1775	rBV7	2489	4197	0.20%	0.039%
14	13.675	1795	1800	1805	rBV5	4887	8796	0.43%	0.082%
15	13.734	1805	1810	1812	rVV4	4668	6371	0.31%	0.059%
16	13.775	1812	1817	1824	rVV	39037	57556	2.78%	0.537%
17	13.845	1827	1829	1833	rBV4	2271	3399	0.16%	0.032%
18	13.910	1836	1840	1845	rVV3	6102	10376	0.50%	0.097%
19	13.945	1845	1846	1849	rVB3	3346	2364	0.11%	0.022%
20	14.045	1855	1863	1873	rVB	40058	70791	3.42%	0.661%
21	14.234	1891	1895	1898	rBV6	2378	4050	0.20%	0.038%
22	14.269	1898	1901	1905	rVB5	2615	3416	0.17%	0.032%
23	14.357	1908	1916	1923	rVV	1147822	1691539	81.74%	15.794%
24	14.410	1923	1925	1928	rVB4	2653	2990	0.14%	0.028%
25	14.581	1946	1954	1959	rBV7	8729	19873	0.96%	0.186%
26	14.657	1965	1967	1971	rVB5	3110	3299	0.16%	0.031%
27	14.710	1971	1976	1978	rBV6	1396	2327	0.11%	0.022%
28	14.757	1978	1984	1987	rBV7	4846	8766	0.42%	0.082%
29	14.828	1993	1996	2003	rVB7	3201	6310	0.30%	0.059%
30	14.910	2003	2010	2013	rBV9	2600	5589	0.27%	0.052%
31	14.981	2017	2022	2027	rVB5	2761	5128	0.25%	0.048%
32	15.033	2027	2031	2035	rBV7	1961	2740	0.13%	0.026%
33	15.151	2044	2051	2054	rVB8	3594	6089	0.29%	0.057%
34	15.228	2061	2064	2066	rVB4	2838	3047	0.15%	0.028%
35	15.351	2079	2085	2090	rBV	55853	82594	3.99%	0.771%
36	15.398	2090	2093	2099	rVB6	6718	10049	0.49%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006651.D
 Acq On : 11 Aug 2021 12:11
 Operator : CG/JU
 Sample : M3246-01 30X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

37	15.481	2101	2107	2115	rBV6	8609	15309	0.74%	0.143%
38	15.557	2118	2120	2123	rBV4	1626	2462	0.12%	0.023%
39	15.633	2127	2133	2138	rVB10	2461	5112	0.25%	0.048%
40	15.704	2142	2145	2147	rBV3	2576	2110	0.10%	0.020%
41	15.851	2167	2170	2172	rBV3	2561	3116	0.15%	0.029%
42	15.922	2177	2182	2183	rBV4	2062	2919	0.14%	0.027%
43	16.098	2207	2212	2213	rVV5	7103	10945	0.53%	0.102%
44	16.116	2213	2215	2221	rVB3	9982	11281	0.55%	0.105%
45	16.304	2244	2247	2249	rBV4	2061	2279	0.11%	0.021%
46	16.651	2302	2306	2309	rBV6	2299	3713	0.18%	0.035%
47	16.686	2310	2312	2315	rVB4	3117	3536	0.17%	0.033%
48	16.775	2322	2327	2330	rBV6	2572	4254	0.21%	0.040%
49	16.892	2342	2347	2351	rBV4	8106	13730	0.66%	0.128%
50	16.945	2351	2356	2361	rVB9	2778	5876	0.28%	0.055%
51	17.016	2364	2368	2369	rBV4	2099	2412	0.12%	0.023%
52	17.110	2377	2384	2390	rBV	1327015	1898729	91.75%	17.728%
53	17.210	2396	2401	2407	rBV2	55691	84580	4.09%	0.790%
54	17.422	2435	2437	2441	rBV5	2979	3823	0.18%	0.036%
55	17.633	2470	2473	2476	rVB5	3771	4723	0.23%	0.044%
56	17.804	2499	2502	2504	rBV4	3052	3483	0.17%	0.033%
57	17.986	2529	2533	2535	rBV5	6294	8241	0.40%	0.077%
58	18.022	2535	2539	2546	rVB4	13683	27313	1.32%	0.255%
59	18.169	2562	2564	2567	rVB3	6412	5123	0.25%	0.048%
60	18.210	2568	2571	2575	rVB6	6538	8618	0.42%	0.080%
61	18.304	2585	2587	2591	rBV5	4584	4859	0.23%	0.045%
62	18.586	2633	2635	2638	rBV3	3622	3790	0.18%	0.035%
63	18.880	2681	2685	2689	rBV3	10795	19644	0.95%	0.183%
64	18.922	2690	2692	2696	rVB5	9550	11931	0.58%	0.111%
65	19.127	2725	2727	2731	rBV2	11027	13265	0.64%	0.124%
66	19.457	2779	2783	2786	rBV	75487	93082	4.50%	0.869%
67	21.216	3077	3082	3087	rBV	1639666	2001330	96.71%	18.686%
68	23.527	3469	3475	3486	rVB2	1027566	2069516	100.00%	19.323%




Sum of corrected areas: 10710242

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006651.D
Acq On : 11 Aug 2021 12:11
Operator : CG/JU
Sample : M3246-01 30X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

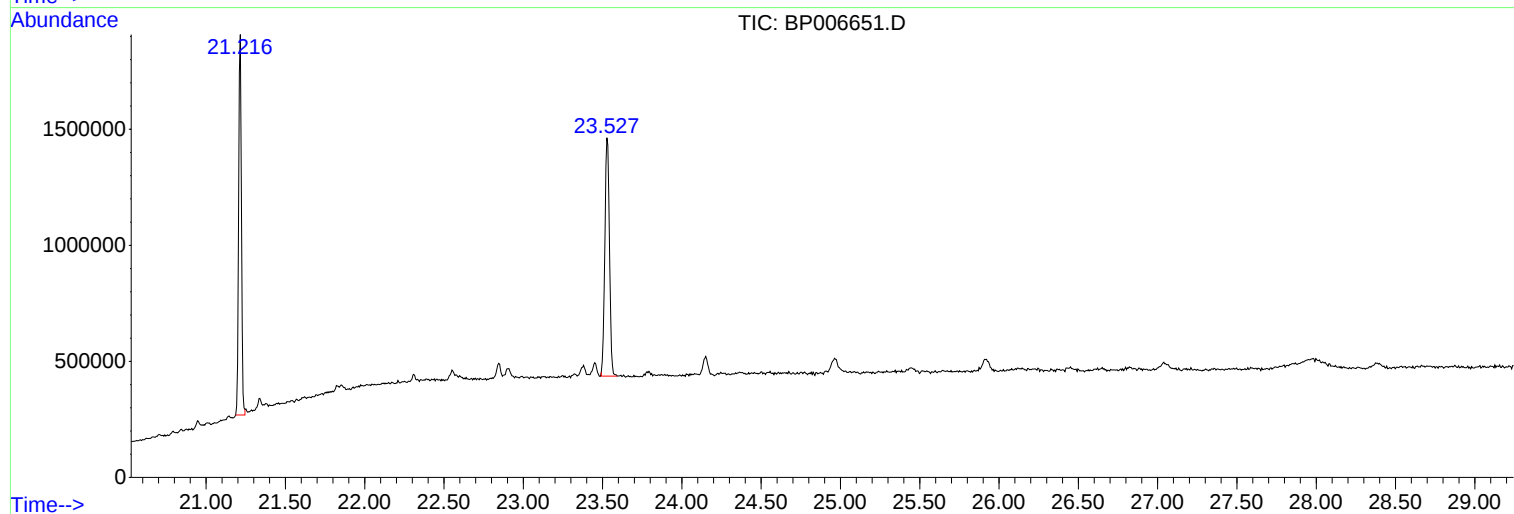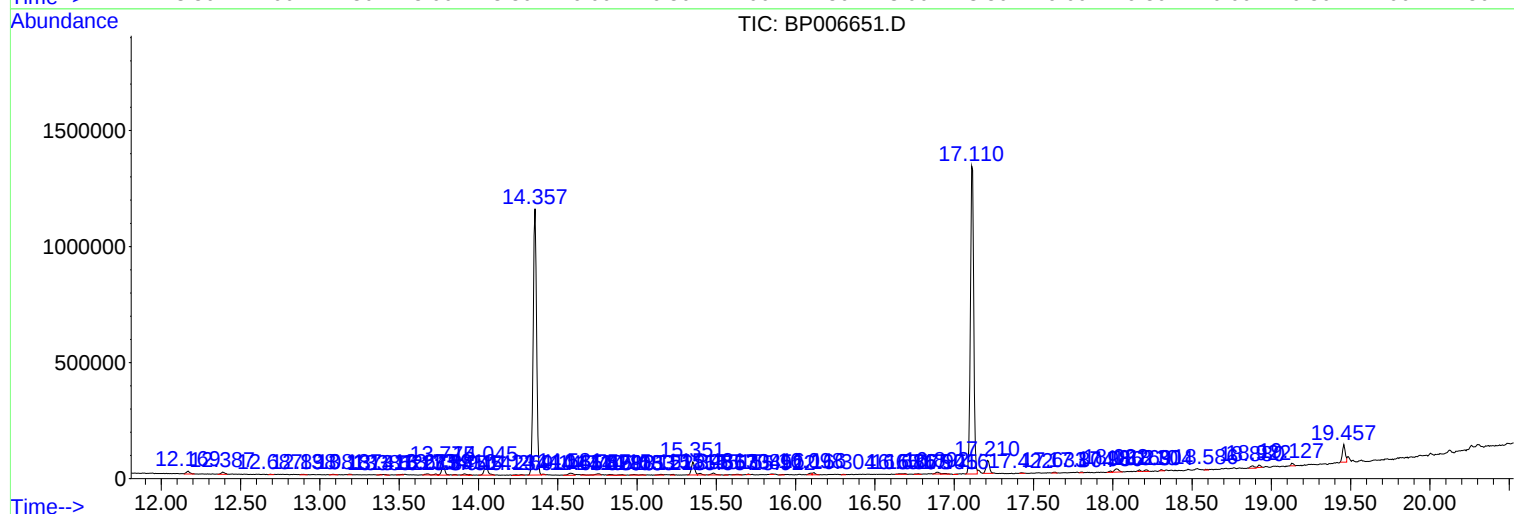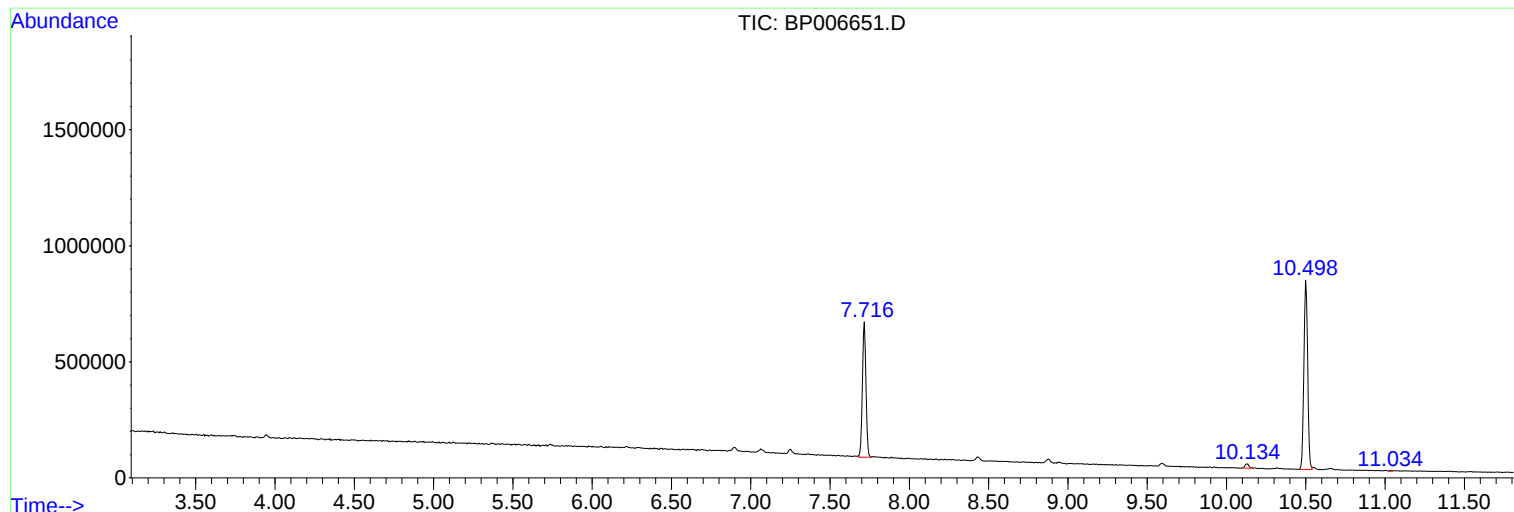

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006651.D
Acq On : 11 Aug 2021 12:11
Operator : CG/JU
Sample : M3246-01 30X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006651.D
Acq On : 11 Aug 2021 12:11
Operator : CG/JU
Sample : M3246-01 30X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
