

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006652.D
 Acq On : 11 Aug 2021 12:45
 Operator : CG/JU
 Sample : M3246-05 30X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006652.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.716	781	787	796	rVB	662719	1005580	38.20%	5.440%
2	10.134	1193	1198	1203	rVB4	16632	30088	1.14%	0.163%
3	10.222	1209	1213	1221	rVB3	18901	33319	1.27%	0.180%
4	10.498	1253	1260	1267	rBV	877542	1474691	56.03%	7.978%
5	10.704	1291	1295	1303	rVB5	10738	20775	0.79%	0.112%
6	12.175	1539	1545	1554	rVB7	5954	13242	0.50%	0.072%
7	12.298	1560	1566	1574	rBV8	3581	8697	0.33%	0.047%
8	12.387	1577	1581	1587	rVV4	5567	7480	0.28%	0.040%
9	13.075	1696	1698	1703	rVB5	2265	3285	0.12%	0.018%
10	13.187	1713	1717	1723	rBV5	5109	9503	0.36%	0.051%
11	13.339	1738	1743	1747	rVB7	6534	10857	0.41%	0.059%
12	13.657	1793	1797	1798	rBV4	2236	2755	0.10%	0.015%
13	13.681	1798	1801	1805	rVB6	2886	4459	0.17%	0.024%
14	13.728	1805	1809	1812	rVB6	2658	3817	0.15%	0.021%
15	13.775	1812	1817	1823	rBV	34224	50260	1.91%	0.272%
16	13.910	1834	1840	1847	rBV10	3558	6617	0.25%	0.036%
17	14.045	1857	1863	1868	rBV	38178	57027	2.17%	0.309%
18	14.357	1908	1916	1922	rBV	1310148	1843852	70.05%	9.976%
19	14.416	1922	1926	1932	rVV	26821	40402	1.53%	0.219%
20	14.481	1932	1937	1942	rVB	43562	63197	2.40%	0.342%
21	14.581	1949	1954	1961	rBV9	11038	22433	0.85%	0.121%
22	14.757	1978	1984	1988	rBV2	14101	20711	0.79%	0.112%
23	14.992	2020	2024	2027	rVB5	2096	2928	0.11%	0.016%
24	15.081	2034	2039	2045	rBV5	15634	27673	1.05%	0.150%
25	15.145	2045	2050	2055	rVV9	2546	4889	0.19%	0.026%
26	15.216	2057	2062	2068	rVB9	4317	10218	0.39%	0.055%
27	15.304	2071	2077	2080	rBV2	12572	19714	0.75%	0.107%
28	15.351	2080	2085	2090	rVV2	46542	65953	2.51%	0.357%
29	15.410	2090	2095	2099	rVB	28227	41377	1.57%	0.224%
30	15.481	2102	2107	2110	rBV6	6912	11149	0.42%	0.060%
31	15.575	2120	2123	2124	rBV3	3192	3108	0.12%	0.017%
32	15.616	2127	2130	2135	rVB2	16460	23575	0.90%	0.128%
33	15.710	2142	2146	2148	rBV3	6555	10420	0.40%	0.056%
34	15.733	2148	2150	2158	rVB4	8836	12181	0.46%	0.066%
35	15.851	2165	2170	2177	rBV4	7210	15133	0.57%	0.082%
36	15.904	2177	2179	2184	rVV5	3112	5695	0.22%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006652.D
 Acq On : 11 Aug 2021 12:45
 Operator : CG/JU
 Sample : M3246-05 30X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

37	15.945	2184	2186	2191	rVB6	2160	3308	0.13%	0.018%
38	16.069	2199	2207	2218	rBV10	12154	34017	1.29%	0.184%
39	16.228	2230	2234	2240	rVB7	8770	11989	0.46%	0.065%
40	16.310	2244	2248	2249	rBV4	2078	2660	0.10%	0.014%
41	16.345	2249	2254	2258	rVV3	25408	33593	1.28%	0.182%
42	16.422	2262	2267	2271	rVB7	5299	9449	0.36%	0.051%
43	16.463	2271	2274	2275	rBV3	2653	2707	0.10%	0.015%
44	16.528	2278	2285	2286	rBV6	1984	3232	0.12%	0.017%
45	16.622	2295	2301	2302	rBV6	2351	4028	0.15%	0.022%
46	16.645	2302	2305	2307	rBV4	3967	4242	0.16%	0.023%
47	16.763	2321	2325	2331	rVB3	10401	16402	0.62%	0.089%
48	16.839	2331	2338	2340	rBV7	6534	12491	0.47%	0.068%
49	16.886	2342	2346	2350	rVV4	20042	31822	1.21%	0.172%
50	16.928	2350	2353	2359	rVV	15157	21857	0.83%	0.118%
51	16.992	2362	2364	2369	rVB5	2926	4290	0.16%	0.023%
52	17.110	2376	2384	2389	rBV	1458902	2133880	81.07%	11.545%
53	17.151	2389	2391	2397	rVV	343061	427880	16.26%	2.315%
54	17.210	2397	2401	2404	rVV2	61049	92818	3.53%	0.502%
55	17.245	2404	2407	2412	rVV	74946	102008	3.88%	0.552%
56	17.304	2414	2417	2423	rVB	7550	13089	0.50%	0.071%
57	17.392	2428	2432	2434	rBV5	3361	4937	0.19%	0.027%
58	17.522	2445	2454	2461	rBV2	38870	69936	2.66%	0.378%
59	17.633	2470	2473	2478	rBV6	4383	6888	0.26%	0.037%
60	17.798	2499	2501	2504	rBV4	3447	4576	0.17%	0.025%
61	17.886	2514	2516	2517	rBV2	2853	2773	0.11%	0.015%
62	17.986	2525	2533	2536	rBV2	25138	41889	1.59%	0.227%
63	18.027	2536	2540	2546	rVB	45695	72462	2.75%	0.392%
64	18.110	2548	2554	2559	rVV3	14460	25099	0.95%	0.136%
65	18.175	2559	2565	2569	rVV3	58575	92763	3.52%	0.502%
66	18.210	2569	2571	2575	rVB3	17598	19470	0.74%	0.105%
67	18.280	2581	2583	2585	rBV3	3605	3249	0.12%	0.018%
68	18.410	2602	2605	2608	rBV5	5568	7550	0.29%	0.041%
69	18.475	2612	2616	2619	rVV	24080	33500	1.27%	0.181%
70	18.510	2619	2622	2633	rVB3	27068	49602	1.88%	0.268%
71	18.874	2681	2684	2690	rBV7	13552	23152	0.88%	0.125%
72	19.004	2702	2706	2710	rBV6	29003	42628	1.62%	0.231%
73	19.127	2722	2727	2732	rBV	495974	654677	24.87%	3.542%
74	19.204	2736	2740	2741	rBV4	11943	16622	0.63%	0.090%
75	19.274	2747	2752	2756	rVB6	38900	53272	2.02%	0.288%
76	19.457	2778	2783	2784	rBV2	155852	189482	7.20%	1.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006652.D
 Acq On : 11 Aug 2021 12:45
 Operator : CG/JU
 Sample : M3246-05 30X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

77	19.486	2784	2788	2797	rVB	375378	527261	20.03%	2.853%
78	19.663	2814	2818	2820	rBV	29773	40225	1.53%	0.218%
79	19.710	2824	2826	2833	rVB3	38889	54453	2.07%	0.295%
80	19.827	2844	2846	2849	rVB3	36766	35641	1.35%	0.193%
81	19.969	2866	2870	2875	rVB	150077	187639	7.13%	1.015%
82	20.069	2884	2887	2890	rBV	38809	46136	1.75%	0.250%
83	20.239	2912	2916	2921	rBV3	114838	154025	5.85%	0.833%
84	20.292	2922	2925	2934	rVV9	37050	75690	2.88%	0.410%
85	20.698	2990	2994	3000	rBV6	89851	138021	5.24%	0.747%
86	21.139	3065	3069	3075	rBV	2171441	2292233	87.09%	12.402%
87	21.210	3075	3081	3085	rVV2	1781578	2632101	100.00%	14.240%
88	21.245	3085	3087	3094	rVB	298015	373639	14.20%	2.021%
89	23.527	3469	3475	3490	rVB2	1217984	2558910	97.22%	13.844%



Sum of corrected areas: 18483323

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006652.D
Acq On : 11 Aug 2021 12:45
Operator : CG/JU
Sample : M3246-05 30X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

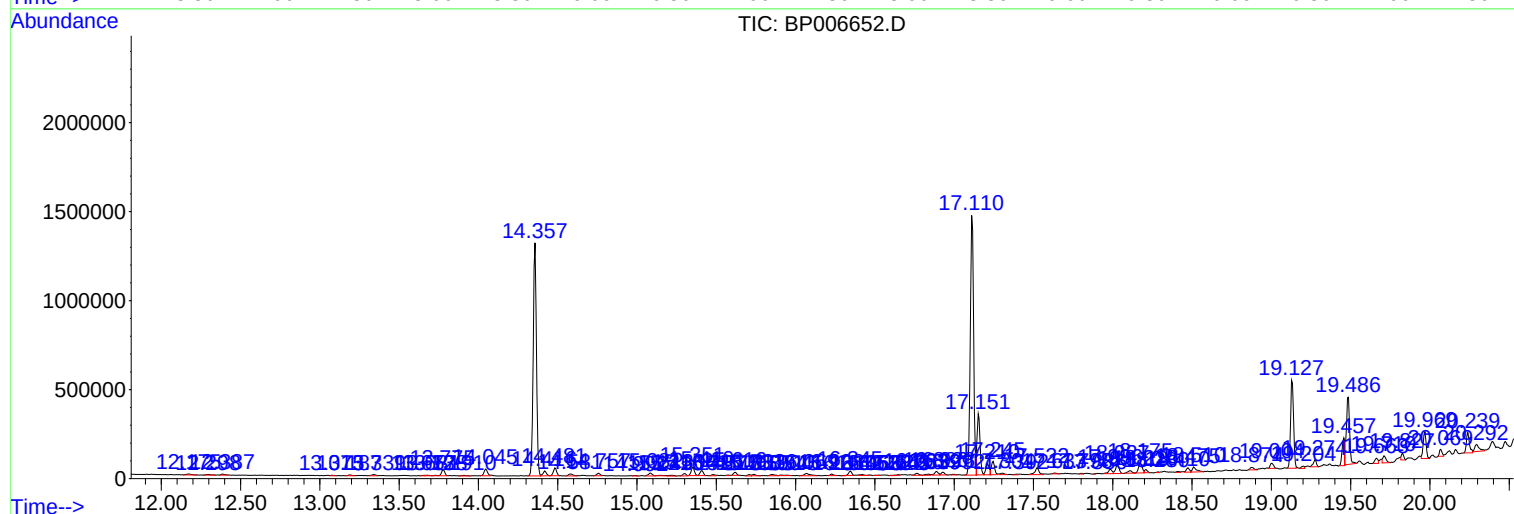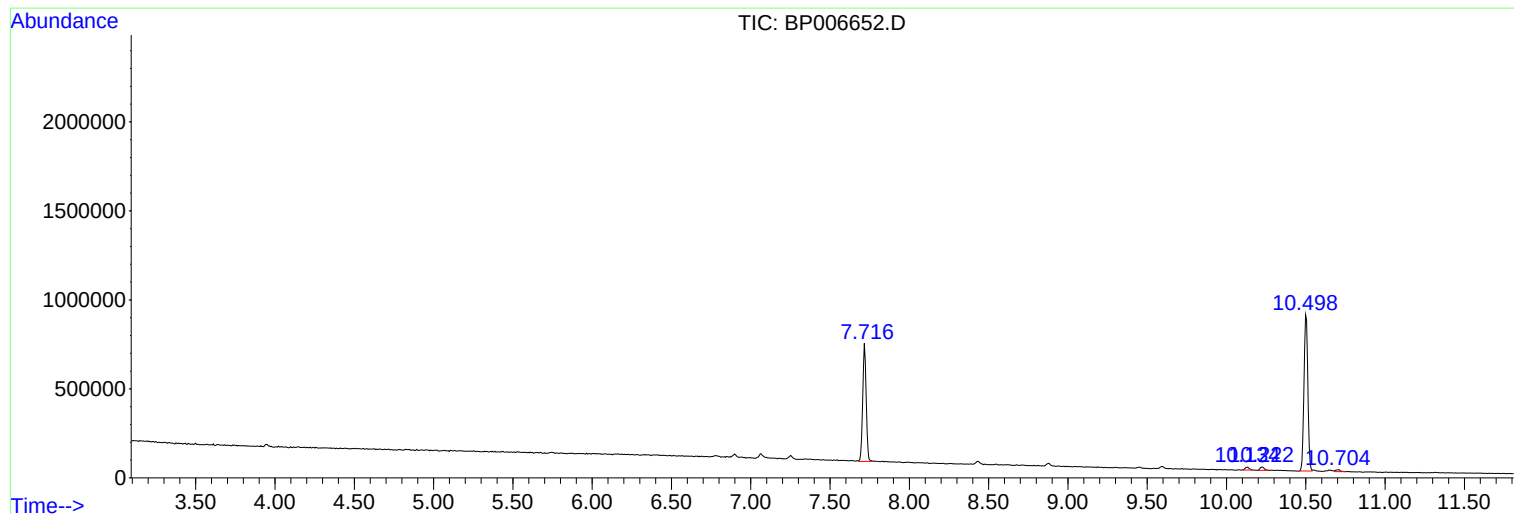

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006652.D
Acq On : 11 Aug 2021 12:45
Operator : CG/JU
Sample : M3246-05 30X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006652.D
Acq On : 11 Aug 2021 12:45
Operator : CG/JU
Sample : M3246-05 30X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
