

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
 Data File : BP006653.D
 Acq On : 11 Aug 2021 13:19
 Operator : CG/JU
 Sample : M3246-06 30X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006653.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.716	781	787	798	rVB	596349	930623	45.43%	8.783%
2	10.499	1253	1260	1268	rBV	809716	1355152	66.16%	12.790%
3	10.651	1283	1286	1292	rVB3	8054	12496	0.61%	0.118%
4	11.528	1433	1435	1437	rBV2	3067	2725	0.13%	0.026%
5	12.169	1539	1544	1548	rBV6	4088	5567	0.27%	0.053%
6	12.498	1595	1600	1605	rVB8	1854	2964	0.14%	0.028%
7	13.081	1693	1699	1704	rBV10	2638	4743	0.23%	0.045%
8	13.193	1716	1718	1722	rVB5	2675	2485	0.12%	0.023%
9	13.334	1738	1742	1750	rVB10	5609	9095	0.44%	0.086%
10	13.675	1792	1800	1801	rBV8	2116	3490	0.17%	0.033%
11	13.775	1811	1817	1822	rBV	26678	38974	1.90%	0.368%
12	14.045	1856	1863	1869	rBV	30293	48897	2.39%	0.461%
13	14.357	1905	1916	1923	rBV	1189951	1714433	83.70%	16.181%
14	14.416	1923	1926	1931	rVV7	3607	6480	0.32%	0.061%
15	14.481	1933	1937	1944	rVB5	7290	10996	0.54%	0.104%
16	14.587	1949	1955	1961	rBV10	3896	9358	0.46%	0.088%
17	14.740	1978	1981	1983	rBV3	2050	2476	0.12%	0.023%
18	15.351	2080	2085	2092	rBV2	39267	57152	2.79%	0.539%
19	15.481	2102	2107	2114	rVB10	3735	6043	0.30%	0.057%
20	15.622	2127	2131	2136	rBV8	2391	3750	0.18%	0.035%
21	15.716	2142	2147	2149	rBV5	2270	4067	0.20%	0.038%
22	15.910	2178	2180	2184	rBV5	1457	2652	0.13%	0.025%
23	16.057	2201	2205	2208	rBV6	2258	4606	0.22%	0.043%
24	16.234	2229	2235	2241	rBV10	2072	4594	0.22%	0.043%
25	16.345	2248	2254	2257	rBV8	4349	6621	0.32%	0.062%
26	16.763	2321	2325	2327	rBV5	3708	4714	0.23%	0.044%
27	16.892	2342	2347	2351	rBV2	6756	12264	0.60%	0.116%
28	17.110	2378	2384	2390	rBV	1335209	1913915	93.44%	18.063%
29	17.151	2390	2391	2397	rVB	25745	24357	1.19%	0.230%
30	17.210	2397	2401	2405	rBV2	41316	58324	2.85%	0.550%
31	17.410	2430	2435	2437	rBV6	1754	3367	0.16%	0.032%
32	17.528	2451	2455	2458	rVV3	4290	6787	0.33%	0.064%
33	17.798	2498	2501	2506	rBV6	2334	3747	0.18%	0.035%
34	18.016	2536	2538	2546	rBV9	8211	14624	0.71%	0.138%
35	19.133	2723	2728	2734	rBV	50232	71630	3.50%	0.676%
36	19.457	2779	2783	2785	rBV	52359	73605	3.59%	0.695%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006653.D
Acq On : 11 Aug 2021 13:19
Operator : CG/JU
Sample : M3246-06 30X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Title : SVOA CALIBRATION

37	21.139	3066	3069	3074	rBV	93796	101805	4.97%	0.961%
38	21.216	3077	3082	3087	rBV	1530389	2007570	98.01%	18.947%
39	23.527	3469	3475	3484	rVB2	1040007	2048371	100.00%	19.332%




Sum of corrected areas: 10595519

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006653.D
Acq On : 11 Aug 2021 13:19
Operator : CG/JU
Sample : M3246-06 30X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

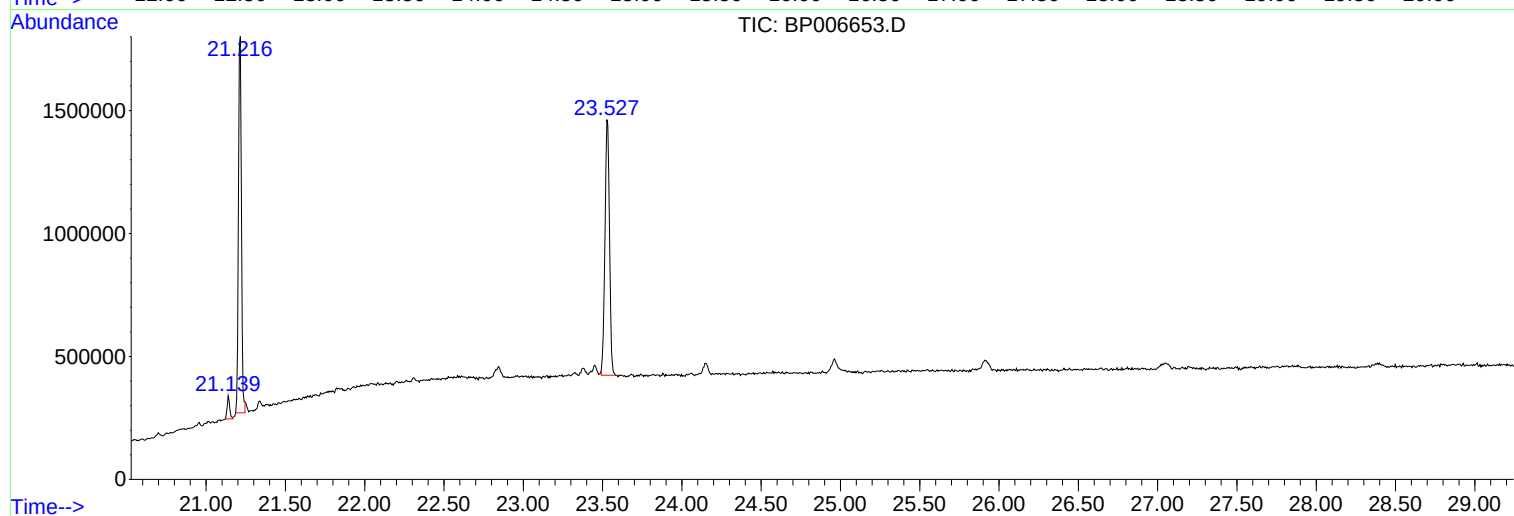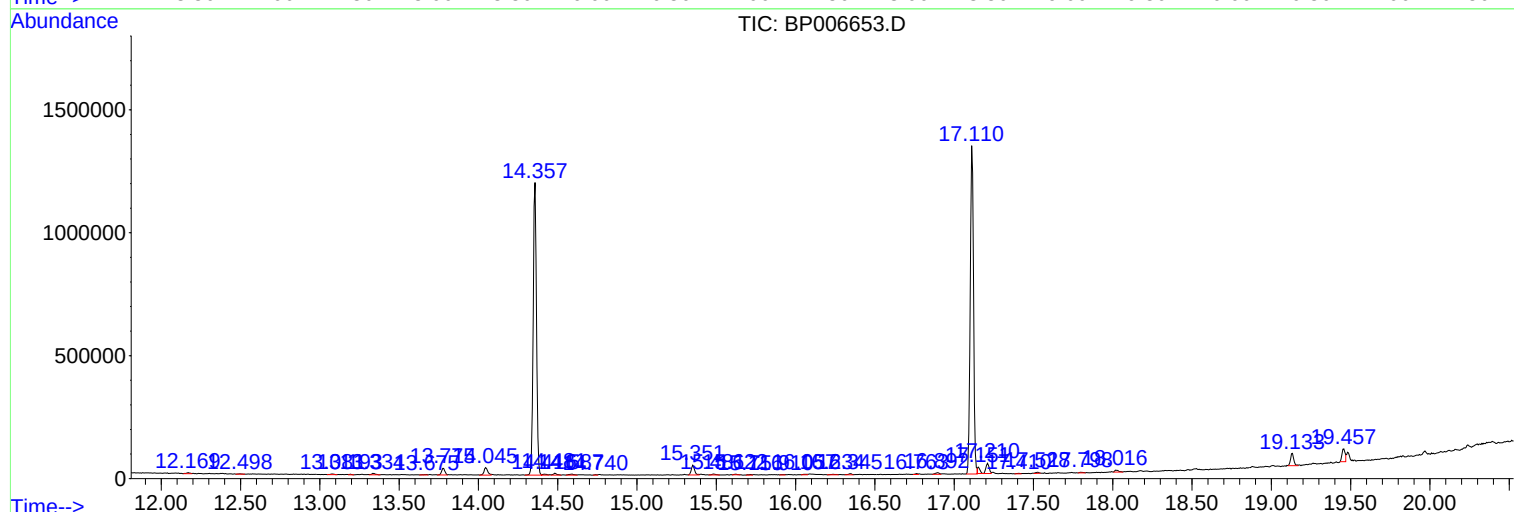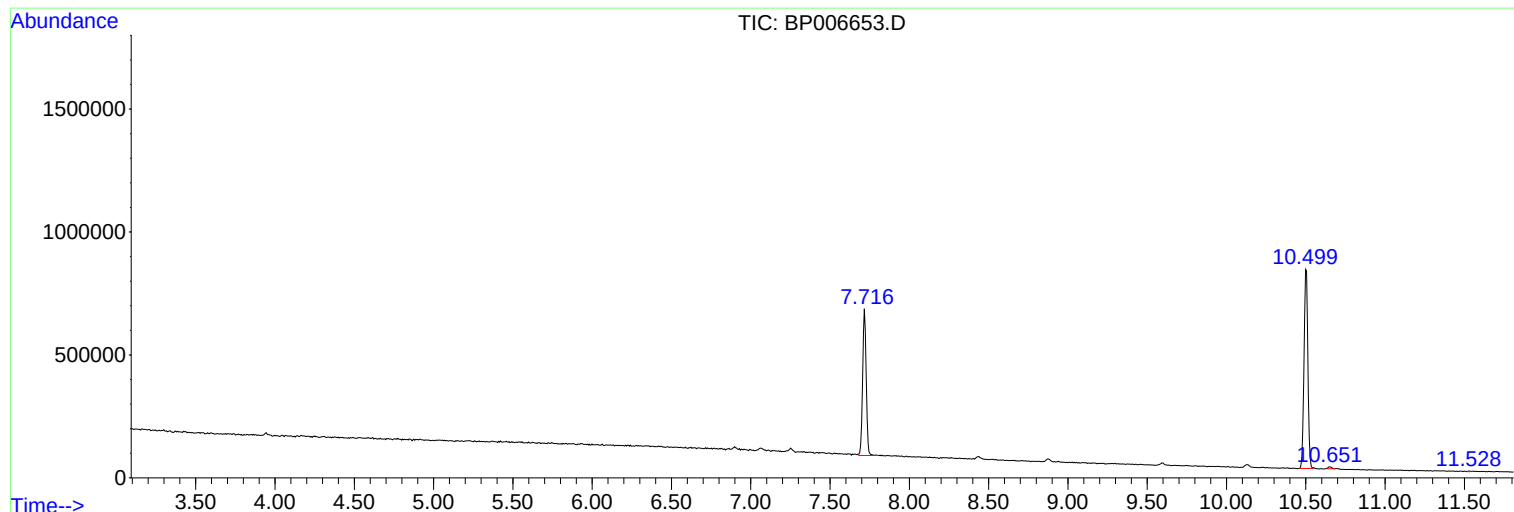

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006653.D
Acq On : 11 Aug 2021 13:19
Operator : CG/JU
Sample : M3246-06 30X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081021\
Data File : BP006653.D
Acq On : 11 Aug 2021 13:19
Operator : CG/JU
Sample : M3246-06 30X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
