

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016540.D
 Acq On : 10 Aug 2023 10:17
 Operator : MA/JU
 Sample : SSTD00518
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005618

Quant Time: Aug 10 16:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 10 14:05:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	508373	20.000	ng/ul	0.00
20) Naphthalene-d8	10.893	136	2219518	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	1427321	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.481	188	3194369	20.000	ng/ul	0.00
79) Chrysene-d12	21.575	240	2903866	20.000	ng/ul	0.00
88) Perylene-d12	24.169	264	3104819	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	25006	1.911	ng/uL	0.00
4) Pyridine-d5	3.834	84	166208	4.558	ng/ul	0.00
7) Phenol-d5	7.199	99	183664	4.346	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	129505	4.982	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	146532	4.466	ng/ul	0.00
15) 4-Methylphenol-d8	8.764	113	150001	4.430	ng/ul	0.00
21) Nitrobenzene-d5	9.258	128	67287	4.231	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	58601	3.798	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.499	165	136052	4.382	ng/ul	0.00
31) 4-Chloroaniline-d4	11.046	131	227786	4.780	ng/ul	0.00
46) Dimethylphthalate-d6	14.122	166	494491	4.830	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	536340	4.560	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	77042	3.839	ng/ul	0.00
60) Fluorene-d10	15.704	176	424037	4.855	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	48794	3.223	ng/ul	0.00
73) Anthracene-d10	17.581	188	662405	4.818	ng/ul	0.00
81) Pyrene-d10	19.810	212	768860	4.809	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.992	264	666809	4.476	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	25820	1.882	ng/uL	98
5) Pyridine	3.858	79	178458	4.768	ng/ul	98
6) Benzaldehyde	7.217	77	133872	6.107	ng/ul	98
8) Phenol	7.228	94	207592	4.677	ng/ul	99
10) Bis(2-Chloroethyl)ether	7.493	93	179625	4.954	ng/ul	97
12) 2-Chlorophenol	7.617	128	160861	4.719	ng/ul	98
13) 2-Methylphenol	8.493	108	145925	4.390	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.575	45	234040	5.233	ng/ul	99
16) Acetophenone	8.911	105	269477	5.139	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.875	70	131090	4.927	ng/ul	96
18) 4-Methylphenol	8.828	108	166866	4.634	ng/ul	99
19) Hexachloroethane	9.140	117	67699	4.817	ng/ul	99
22) Nitrobenzene	9.299	77	189669	4.688	ng/ul	97
23) Isophorone	9.816	82	356548	4.702	ng/ul	98
25) 2-Nitrophenol	10.010	139	72910	4.096	ng/ul	98
26) 2,4-Dimethylphenol	10.040	107	182751	4.766	ng/ul	98
27) Bis(2-Chloroethoxy)met...	10.305	93	251372	5.031	ng/ul	98
29) 2,4-Dichlorophenol	10.528	162	145874	4.604	ng/ul	98
30) Naphthalene	10.946	128	567329	4.967	ng/ul	100
32) 4-Chloroaniline	11.069	127	234197	4.998	ng/ul	97
33) Hexachlorobutadiene	11.181	225	96806	4.854	ng/ul	99
34) Caprolactam	11.869	113	41549	3.665	ng/ul	95
35) 4-Chloro-3-methylphenol	12.163	107	159648	4.630	ng/ul	97
36) 2-Methylnaphthalene	12.546	142	380975	4.999	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016540.D
 Acq On : 10 Aug 2023 10:17
 Operator : MA/JU
 Sample : SSTD00518
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005618

Quant Time: Aug 10 16:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 10 14:05:43 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.763	142	378163	4.941	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.893	216	195283	4.682	ng/ul	99
40) Hexachlorocyclopentadiene	12.846	237	97545	3.833	ng/ul	99
41) 2,4,6-Trichlorophenol	13.140	196	107937	4.204	ng/ul	99
42) 2,4,5-Trichlorophenol	13.204	196	115536	4.122	ng/ul	99
43) 1,1'-Biphenyl	13.546	154	519435	4.910	ng/ul	100
44) 2-Chloronaphthalene	13.593	162	396637	4.768	ng/ul	99
45) 2-Nitroaniline	13.816	65	92753	4.221	ng/ul	89
47) Dimethylphthalate	14.169	163	514972	4.969	ng/ul	100
48) 2,6-Dinitrotoluene	14.310	165	77147	4.051	ng/ul	98
50) Acenaphthylene	14.440	152	664193	4.885	ng/ul	99
51) 3-Nitroaniline	14.646	138	88394	4.403	ng/ul#	99
52) Acenaphthene	14.775	153	447196	4.977	ng/ul	99
53) 2,4-Dinitrophenol	14.840	184	27028	2.640	ng/ul	95
55) 4-Nitrophenol	14.922	109	64810	4.383	ng/ul	97
56) Dibenzofuran	15.110	168	625933	5.082	ng/ul	98
57) 2,4-Dinitrotoluene	15.087	165	118177	4.287	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.322	232	100878	4.354	ng/ul	96
61) Fluorene	15.763	166	519587	5.227	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.751	204	252957	5.186	ng/ul	99
63) 4-Nitroaniline	15.810	138	83078	4.574	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.834	198	56246	3.377	ng/ul#	91
67) N-Nitrosodiphenylamine	15.975	169	427528	4.922	ng/ul	99
68) 4-Bromophenyl-phenylether	16.657	248	145689	4.716	ng/ul	99
69) Hexachlorobenzene	16.740	284	176937	4.875	ng/ul	96
70) Atrazine	16.928	200	139796	4.552	ng/ul	98
71) Pentachlorophenol	17.098	266	80342	3.634	ng/ul	97
72) Phenanthrene	17.522	178	835120	5.064	ng/ul	99
74) Anthracene	17.610	178	825088	5.014	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.504	216	196671	4.401	ng/uL	99
76) Pentachlorobenzene	15.004	250	188704	4.696	ng/uL	98
77) Carbazole	17.892	167	736684	5.167	ng/ul	99
78) Di-n-butylphthalate	18.404	149	855082	4.896	ng/ul	99
80) Fluoranthene	19.481	202	936272	4.934	ng/ul	100
82) Pyrene	19.839	202	1010377	5.117	ng/ul	100
83) Butylbenzylphthalate	20.698	149	343108	4.451	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.492	252	276981	4.394	ng/ul	98
85) Benzo(a)anthracene	21.557	228	954893	4.912	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.439	149	495778	4.540	ng/ul	99
87) Chrysene	21.616	228	893500	4.964	ng/ul	100
89) Di-n-octyl phthalate	22.427	149	826843	4.801	ng/ul	100
90) Benzo(b)fluoranthene	23.357	252	871857	4.754	ng/ul	100
91) Benzo(k)fluoranthene	23.410	252	878984	4.767	ng/ul	99
93) Benzo(a)pyrene	24.045	252	800268	4.658	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.915	276	887640	4.452	ng/ul	97
95) Dibenzo(a,h)anthracene	26.945	278	741126	4.463	ng/ul	99
96) Benzo(g,h,i)perylene	27.780	276	693647	4.412	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016540.D
 Acq On : 10 Aug 2023 10:17
 Operator : MA/JU
 Sample : SSTD00518
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005618

Quant Time: Aug 10 16:47:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 10 14:05:43 2023
 Response via : Initial Calibration




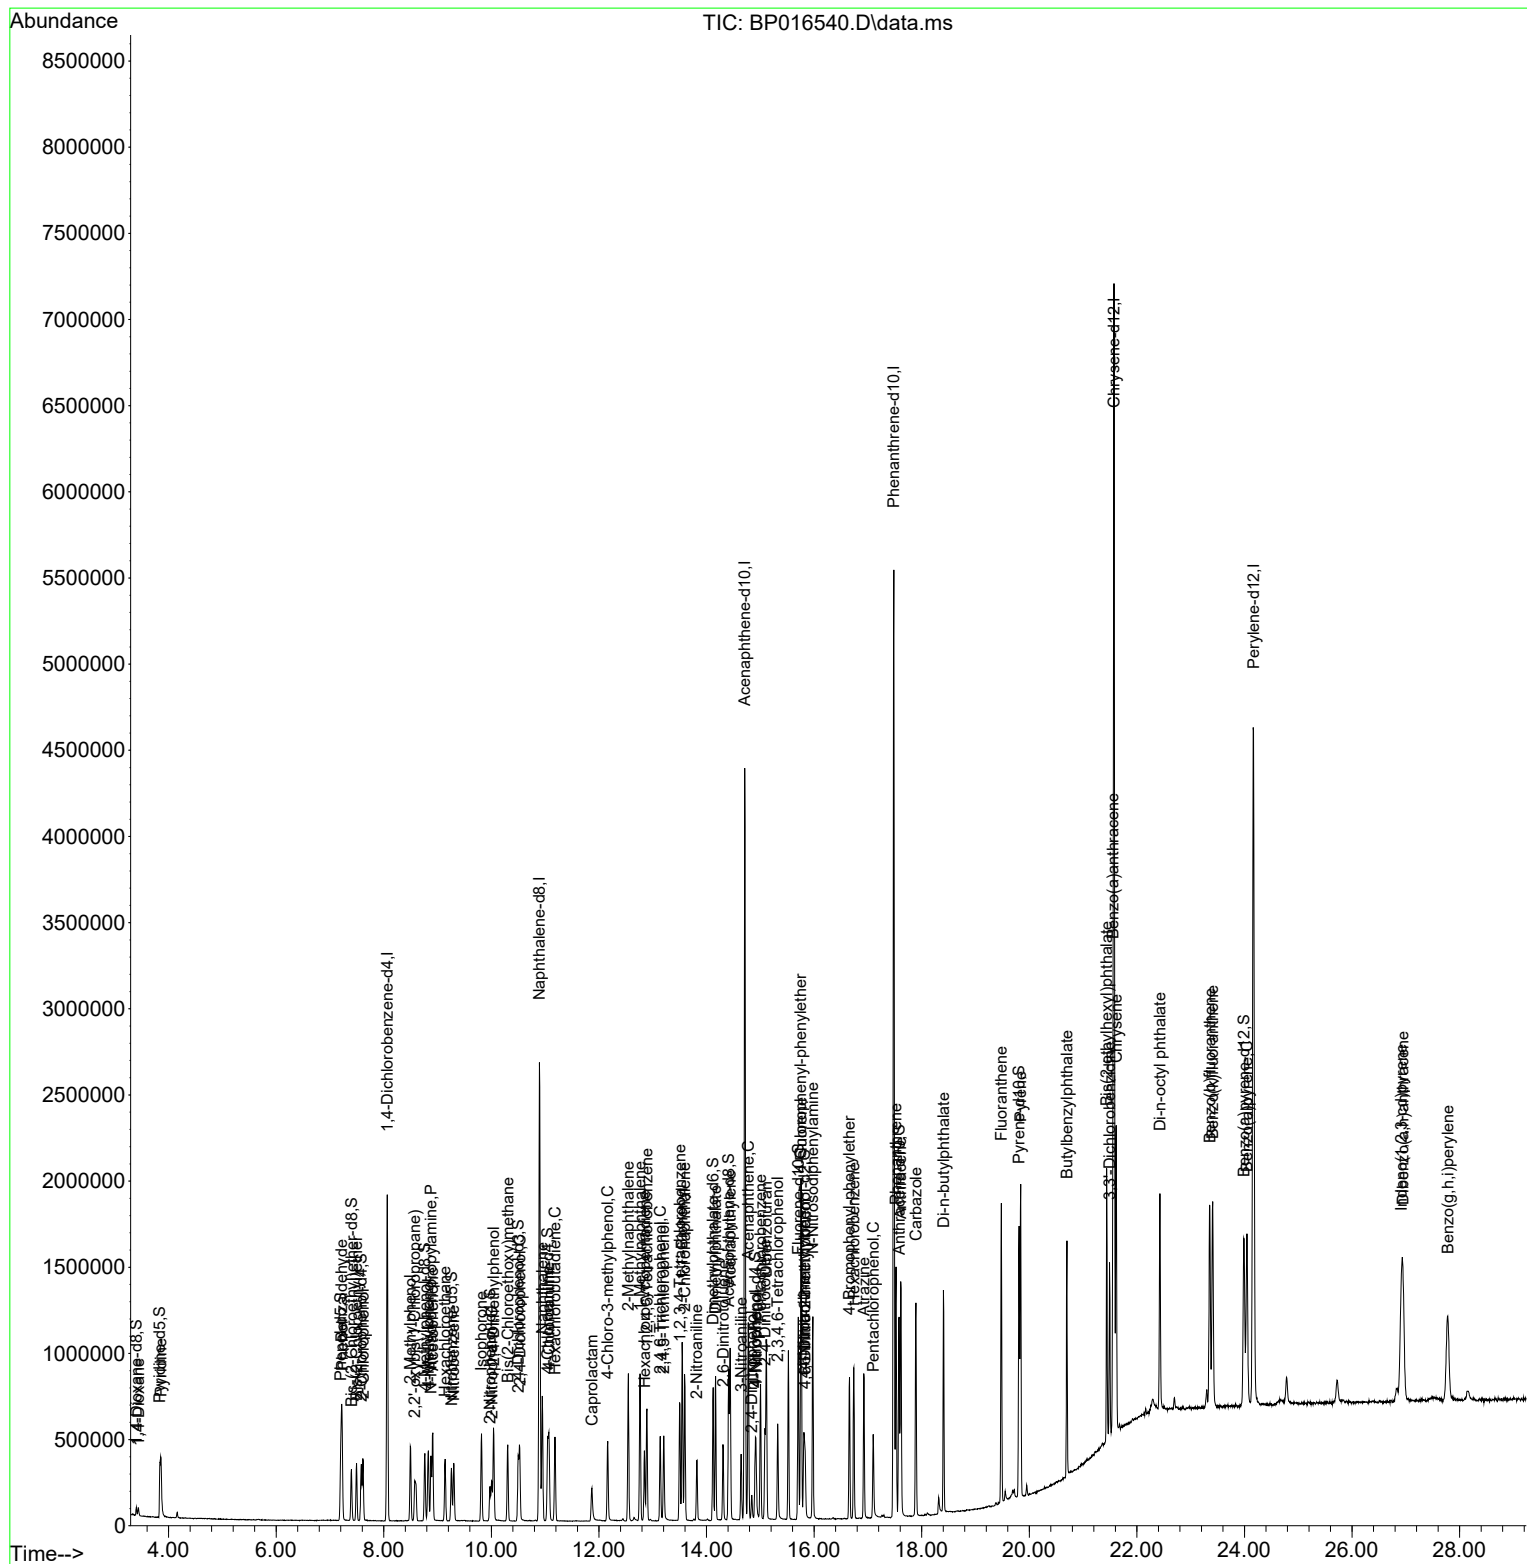


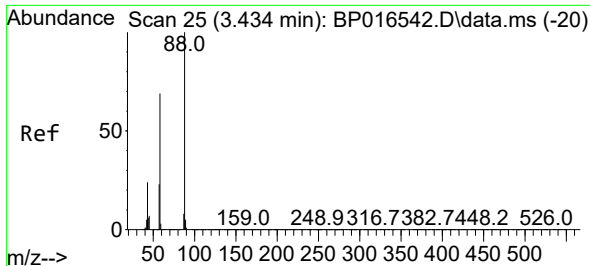

#2
1,4-Dioxane
Concen: 1.882 ng/uL
RT: 3.440 min Scan# 20
Delta R.T. 0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion: 88 Resp: 25820
Ion Ratio Lower Upper
88 100
43 23.9 20.1 30.1
58 70.1 55.1 82.7

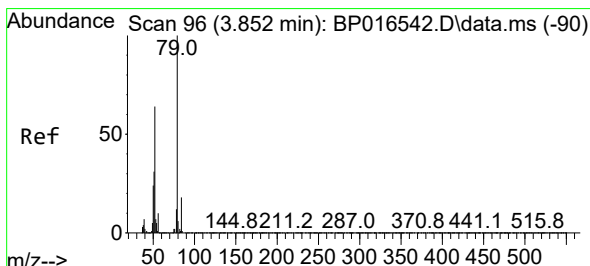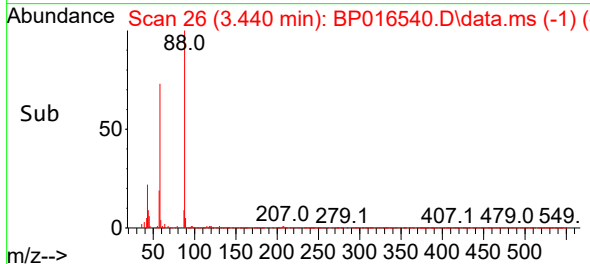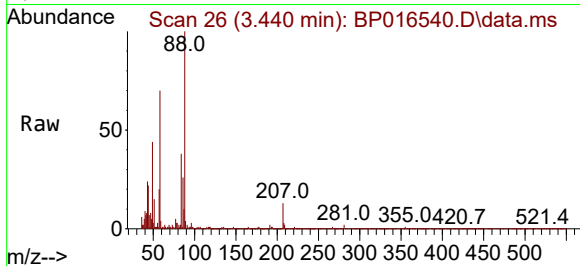

#5
Pyridine
Concen: 4.768 ng/uL
RT: 3.858 min Scan# 97
Delta R.T. 0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion: 79 Resp: 178458
Ion Ratio Lower Upper
79 100
52 64.5 52.9 79.3
51 32.7 24.6 37.0


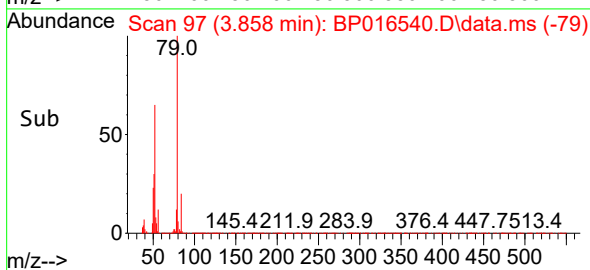

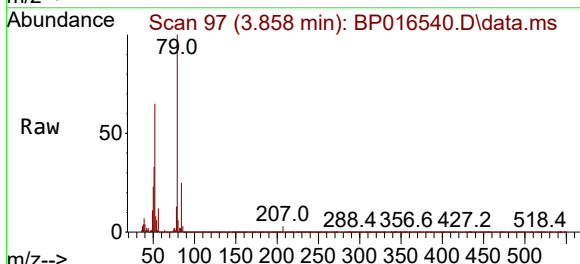




#6
Benzaldehyde
Concen: 6.107 ng/ul
RT: 7.217 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion: 77 Resp: 133872
Ion Ratio Lower Upper
77 100
105 97.2 79.6 119.4
106 94.5 76.5 114.7

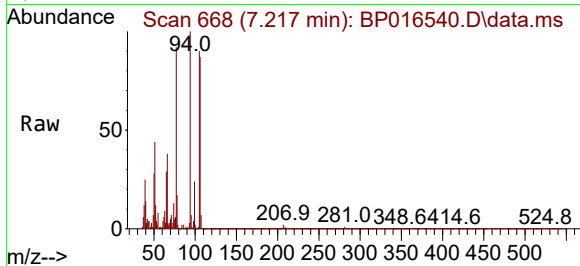

#8
Phenol
Concen: 4.677 ng/ul
RT: 7.228 min Scan# 670
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion: 94 Resp: 207592
Ion Ratio Lower Upper
94 100
65 25.6 20.7 31.1
66 33.8 26.7 40.1




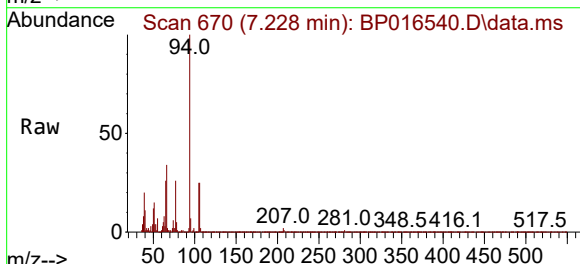




#10
Bis(2-Chloroethyl)ether
Concen: 4.954 ng/ul
RT: 7.493 min Scan# 715
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion: 93 Resp: 179625
Ion Ratio Lower Upper
93 100
63 74.4 57.0 85.6
95 33.5 26.0 39.0



#12
2-Chlorophenol
Concen: 4.719 ng/ul
RT: 7.617 min Scan# 736
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:128 Resp: 160861
Ion Ratio Lower Upper
128 100
64 44.7 34.7 52.1
130 31.4 25.9 38.9

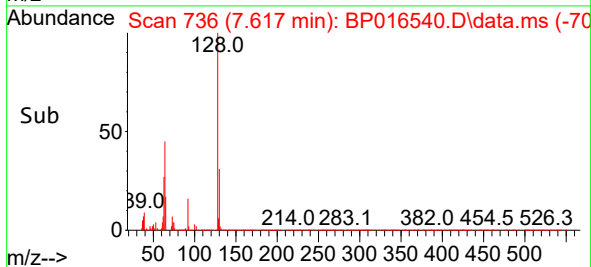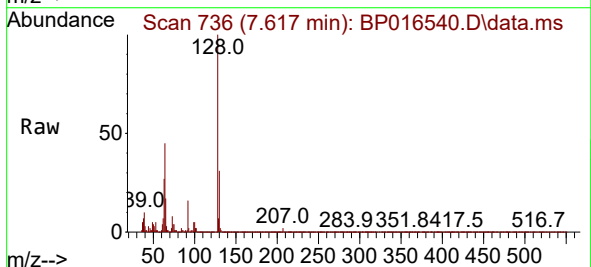



#13

2-Methylphenol

Concen: 4.390 ng/ul

RT: 8.493 min Scan# 886

Delta R.T. -0.006 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :





SSTD005618

Tgt Ion:108 Resp: 145925

Ion Ratio Lower Upper

108 100

107 87.3 71.9 107.9

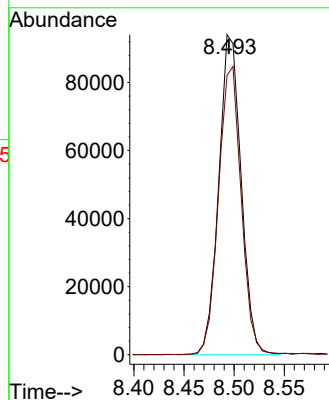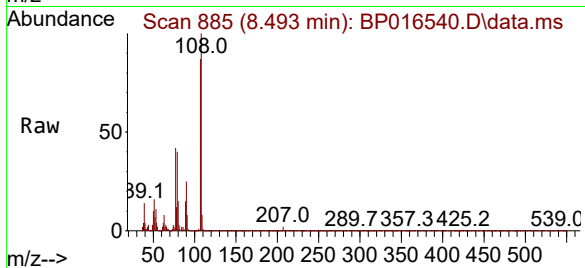

#14

2,2'-oxybis(1-Chloropropane)

Concen: 5.233 ng/ul

RT: 8.575 min Scan# 899

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion: 45 Resp: 234040


Ion Ratio Lower Upper

45 100

77 16.5 12.9 19.3

79 11.9 9.2 13.8


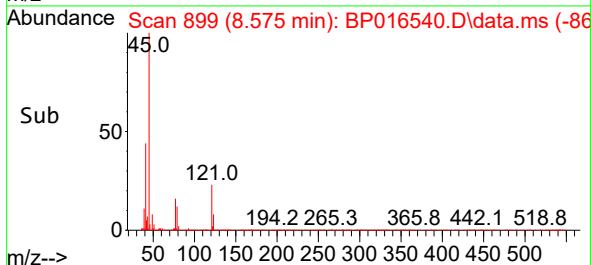
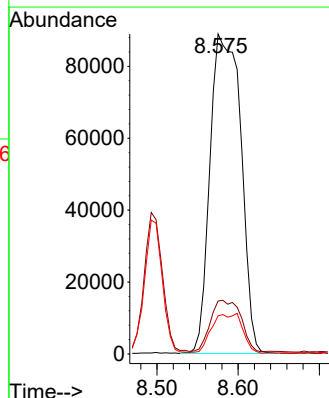
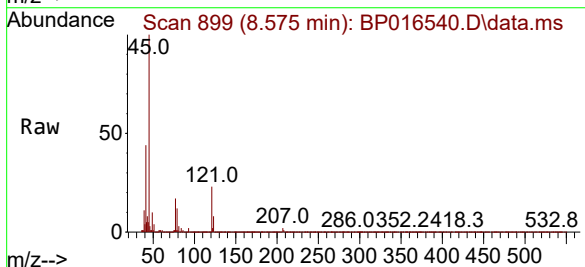




#16
Acetophenone
Concen: 5.139 ng/ul
RT: 8.911 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:105 Resp: 269477
Ion Ratio Lower Upper
105 100
77 74.2 61.0 91.4
51 23.6 18.7 28.1



#17
N-Nitroso-di-n-propylamine
Concen: 4.927 ng/ul
RT: 8.875 min Scan# 950
Delta R.T. -0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion: 70 Resp: 131090
Ion Ratio Lower Upper
70 100
42 53.5 39.9 59.9
101 9.3 7.9 11.9
130 19.0 16.6 25.0



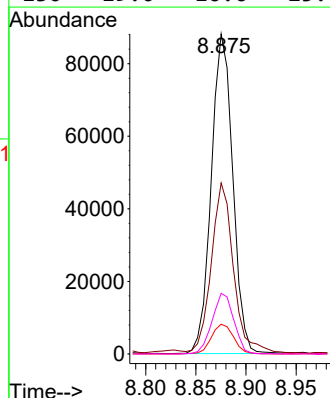





#18
4-Methylphenol
Concen: 4.634 ng/ul
RT: 8.828 min Scan# 942
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:108 Resp: 166866
Ion Ratio Lower Upper
108 100
107 110.6 89.5 134.3



#19
Hexachloroethane
Concen: 4.817 ng/ul
RT: 9.140 min Scan# 995
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:117 Resp: 67699
Ion Ratio Lower Upper
117 100
201 97.1 77.2 115.8
199 60.6 49.2 73.8









#22
Nitrobenzene
Concen: 4.688 ng/ul
RT: 9.299 min Scan# 1022
Delta R.T. -0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion: 77 Resp: 189669
Ion Ratio Lower Upper
77 100
123 43.0 36.4 54.6
65 12.4 10.3 15.5



#23
Isophorone
Concen: 4.702 ng/ul
RT: 9.816 min Scan# 1110
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion: 82 Resp: 356548
Ion Ratio Lower Upper
82 100
95 7.2 5.4 8.0
138 18.0 13.6 20.4









#25
2-Nitrophenol
Concen: 4.096 ng/ul
RT: 10.010 min Scan# 1143
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:139 Resp: 72910
Ion Ratio Lower Upper
139 100
65 49.9 38.9 58.3
109 30.2 23.1 34.7

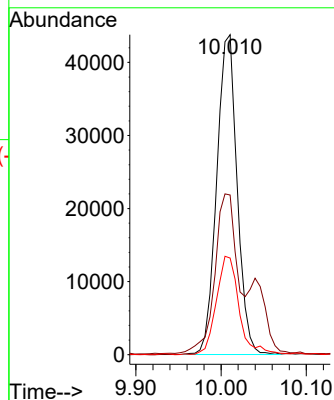

#26
2,4-Dimethylphenol
Concen: 4.766 ng/ul
RT: 10.040 min Scan# 1148
Delta R.T. -0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:107 Resp: 182751
Ion Ratio Lower Upper
107 100
121 48.8 40.2 60.4
122 84.5 69.2 103.8



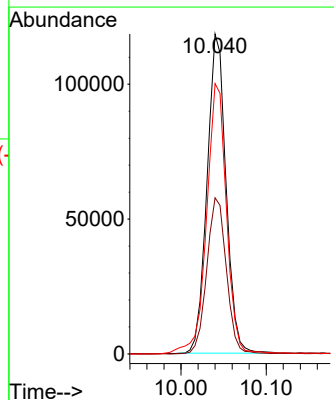



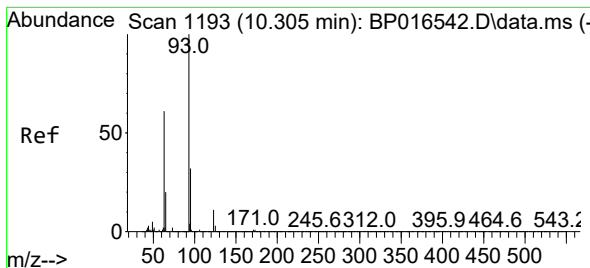

#27
 Bis(2-Chloroethoxy)methane
 Concen: 5.031 ng/ul
 RT: 10.305 min Scan# 1193
 Delta R.T. 0.000 min
 Lab File: BP016540.D
 Acq: 10 Aug 2023 10:17




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005618


Tgt Ion: 93 Resp: 251372
 Ion Ratio Lower Upper
 93 100
 95 31.5 26.0 39.0
 123 10.8 9.0 13.6

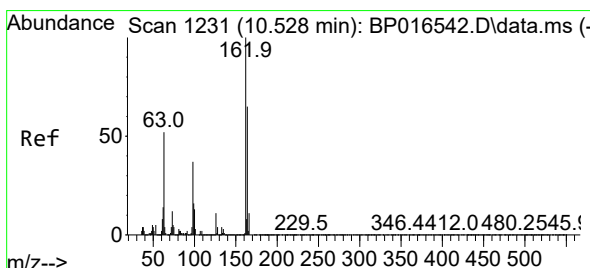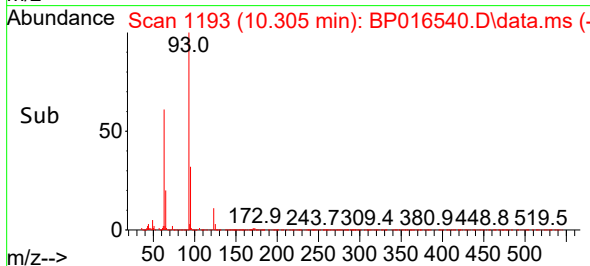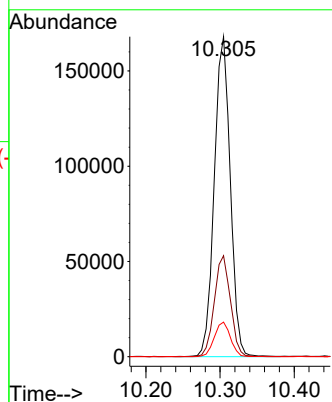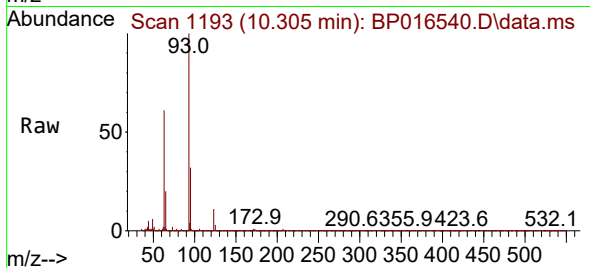

#29
 2,4-Dichlorophenol
 Concen: 4.604 ng/ul
 RT: 10.528 min Scan# 1231
 Delta R.T. 0.000 min
 Lab File: BP016540.D
 Acq: 10 Aug 2023 10:17

Tgt Ion: 162 Resp: 145874
 Ion Ratio Lower Upper
 162 100
 164 65.0 52.5 78.7
 98 39.8 29.4 44.2


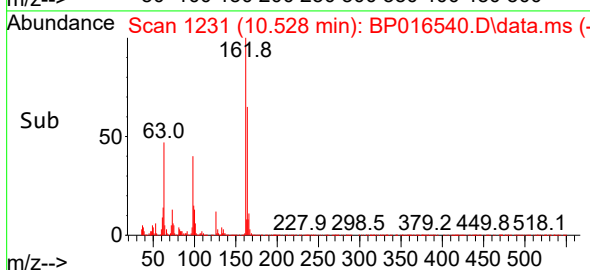
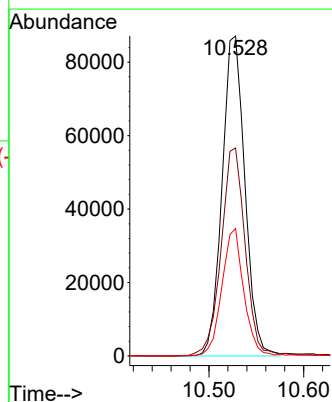
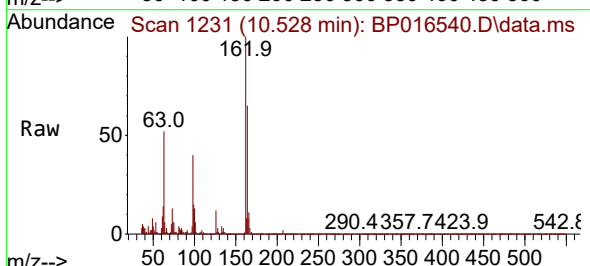




#30
Naphthalene
Concen: 4.967 ng/ul
RT: 10.946 min Scan# 1302
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:128 Resp: 567329
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 13.4 10.7 16.1



#32
4-Chloroaniline
Concen: 4.998 ng/ul
RT: 11.069 min Scan# 1323
Delta R.T. -0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:127 Resp: 234197
Ion Ratio Lower Upper
127 100
129 30.7 25.8 38.6









#33
Hexachlorobutadiene
Concen: 4.854 ng/ul
RT: 11.181 min Scan# 111
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:225 Resp: 96806
Ion Ratio Lower Upper
225 100
223 62.8 50.4 75.6
227 62.6 51.5 77.3



#34
Caprolactam
Concen: 3.665 ng/ul
RT: 11.869 min Scan# 1459
Delta R.T. -0.012 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:113 Resp: 41549
Ion Ratio Lower Upper
113 100
55 162.0 123.0 184.4
56 117.9 90.9 136.3









#35
4-Chloro-3-methylphenol
Concen: 4.630 ng/ul
RT: 12.163 min Scan# 1509
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:107 Resp: 159648
Ion Ratio Lower Upper
107 100
144 26.3 20.7 31.1
142 76.3 64.0 96.0

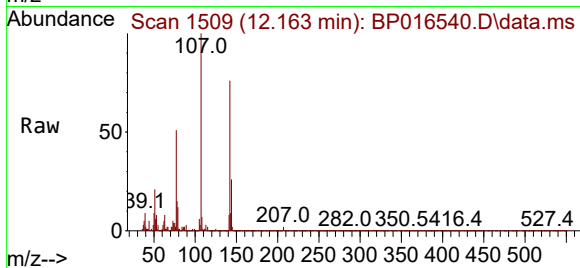

#36
2-Methylnaphthalene
Concen: 4.999 ng/ul
RT: 12.546 min Scan# 1574
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:142 Resp: 380975
Ion Ratio Lower Upper
142 100
141 89.0 71.7 107.5

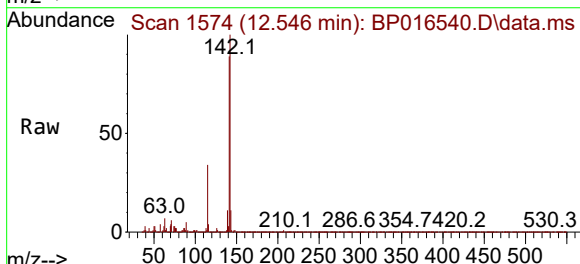



#37

1-Methylnaphthalene

Concen: 4.941 ng/ul

RT: 12.763 min Scan# 1611

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:142 Resp: 378163

Ion Ratio Lower Upper

142 100

141 90.5 73.2 109.8

116 3.5 3.0 4.4

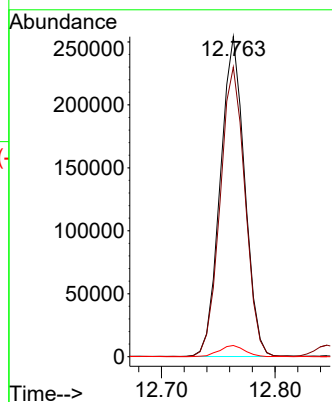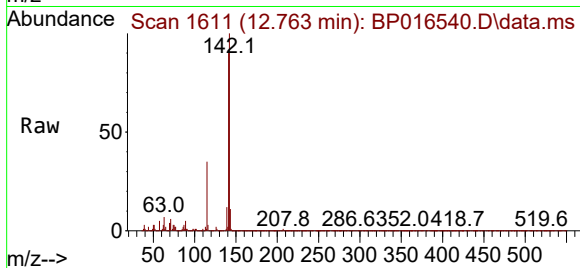

#39

1,2,4,5-Tetrachlorobenzene

Concen: 4.682 ng/ul

RT: 12.893 min Scan# 1633

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Tgt Ion:216 Resp: 195283




Ion Ratio Lower Upper


216 100

214 77.9 62.6 94.0

179 20.3 16.6 25.0

108 17.7 13.8 20.8

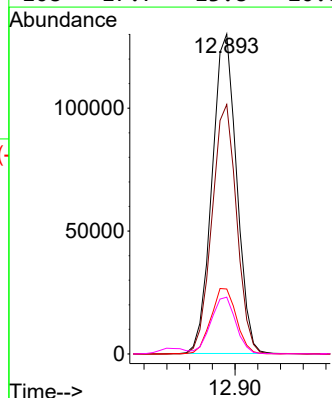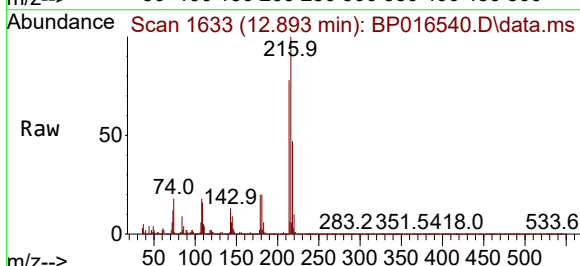



#40

Hexachlorocyclopentadiene

Concen: 3.833 ng/ul

RT: 12.846 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:237 Resp: 97545

Ion Ratio Lower Upper

237 100

235 61.6 49.3 73.9

272 11.9 10.7 16.1

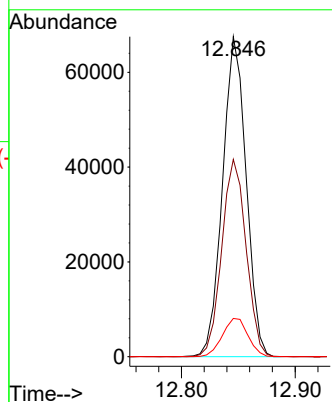

#41

2,4,6-Trichlorophenol

Concen: 4.204 ng/ul

RT: 13.140 min Scan# 1675

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:196 Resp: 107937


Ion Ratio Lower Upper

196 100

198 94.4 76.3 114.5

200 30.9 25.3 37.9



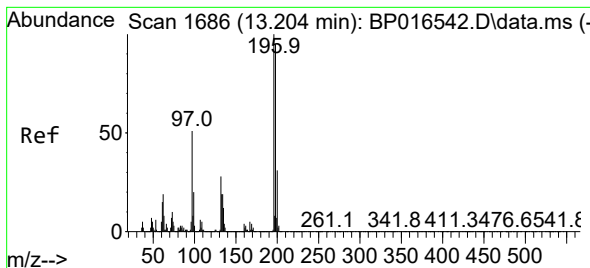

#42

2,4,5-Trichlorophenol

Concen: 4.122 ng/ul

RT: 13.204 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:196 Resp: 115536

Ion Ratio Lower Upper

196 100

198 96.3 75.7 113.5

200 30.8 24.6 37.0

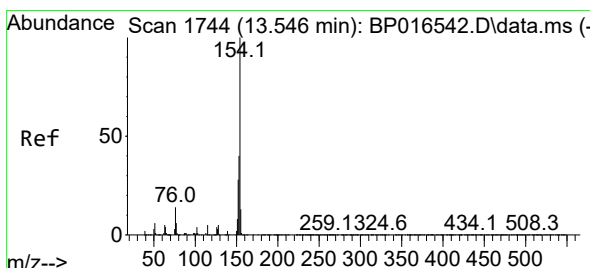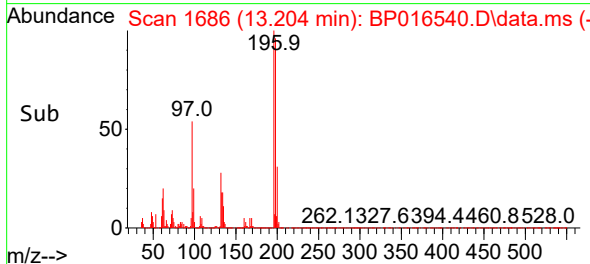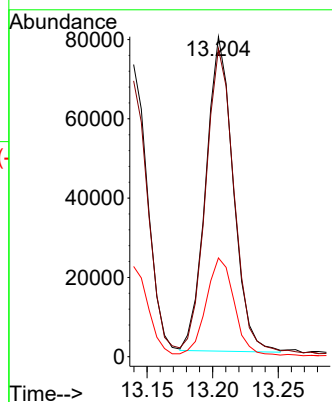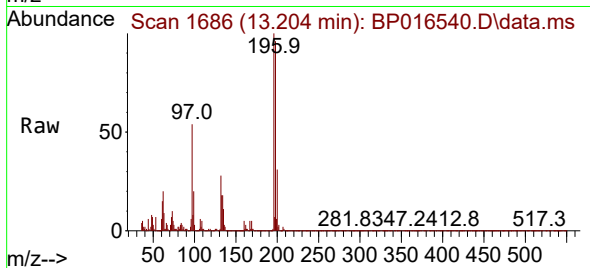

#43

1,1'-Biphenyl

Concen: 4.910 ng/ul

RT: 13.546 min Scan# 1744

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:154 Resp: 519435


Ion Ratio Lower Upper

154 100

153 39.6 31.7 47.5

76 14.3 11.3 16.9


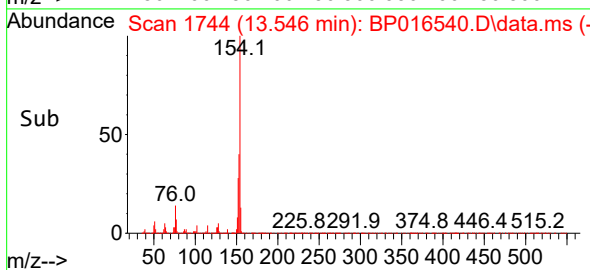

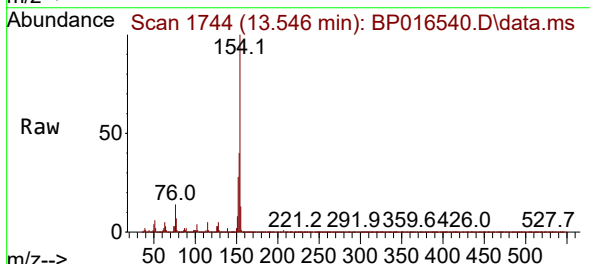


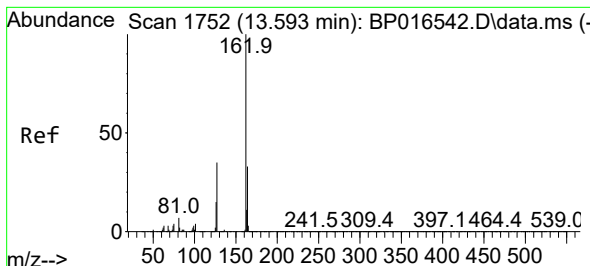

#44
2-Chloronaphthalene
Concen: 4.768 ng/ul
RT: 13.593 min Scan# 1752
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:162 Resp: 396637
Ion Ratio Lower Upper
162 100
164 32.9 26.6 40.0
127 40.2 31.2 46.8

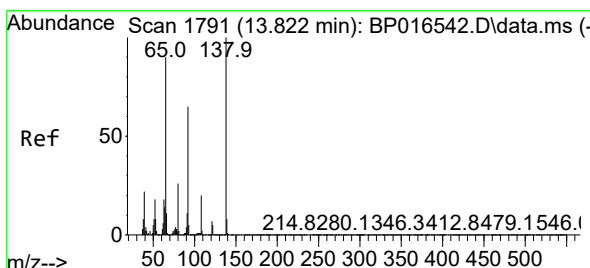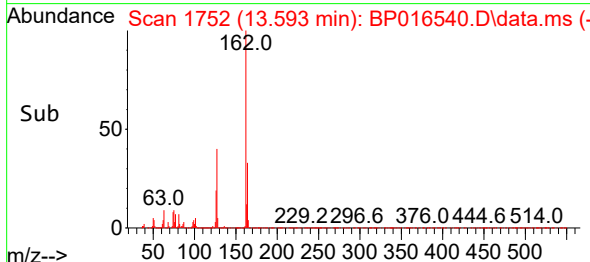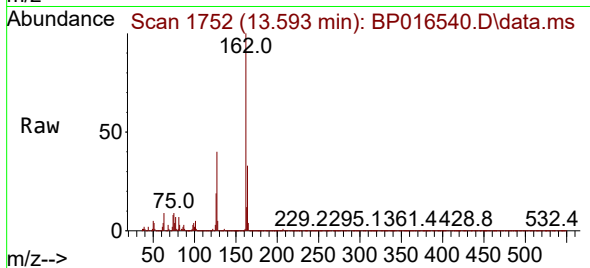

#45
2-Nitroaniline
Concen: 4.221 ng/ul
RT: 13.816 min Scan# 1790
Delta R.T. -0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion: 65 Resp: 92753
Ion Ratio Lower Upper
65 100
92 71.3 58.0 87.0
138 92.3 88.6 132.8


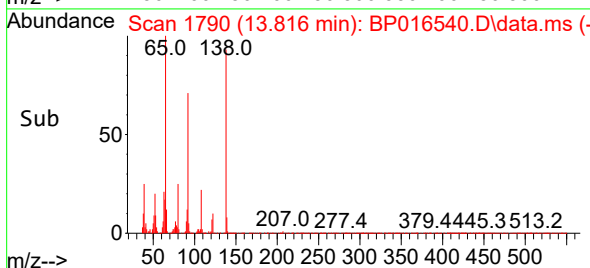

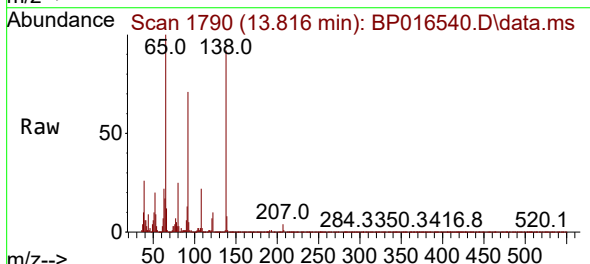




#47
Dimethylphthalate
Concen: 4.969 ng/ul
RT: 14.169 min Scan# 1850
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:163 Resp: 514972
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 10.1 8.1 12.1



#48
2,6-Dinitrotoluene
Concen: 4.051 ng/ul
RT: 14.310 min Scan# 1874
Delta R.T. -0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:165 Resp: 77147
Ion Ratio Lower Upper
165 100
89 58.0 46.4 69.6
121 24.6 16.8 25.2

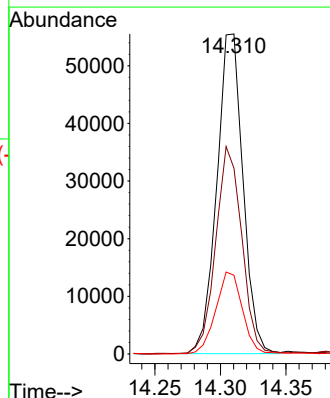



#50

Acenaphthylene

Concen: 4.885 ng/ul

RT: 14.440 min Scan# 1896

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:152 Resp: 664193

Ion Ratio Lower Upper

152 100

151 19.4 15.7 23.5

153 12.8 10.6 16.0



#51

3-Nitroaniline

Concen: 4.403 ng/ul

RT: 14.646 min Scan# 1931

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:138 Resp: 88394


Ion Ratio Lower Upper

138 100

108 14.2 9.4 14.2#

92 118.0 95.0 142.6





#52

Acenaphthene

Concen: 4.977 ng/ul

RT: 14.775 min Scan# 1953

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:153 Resp: 447196

Ion Ratio Lower Upper

153 100

152 47.9 38.6 58.0

154 88.1 71.0 106.6

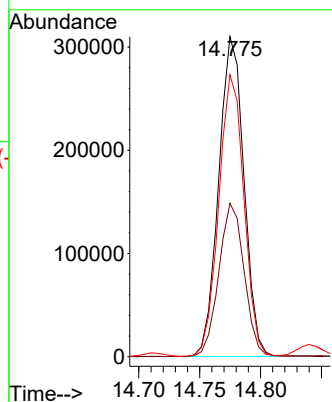

#53

2,4-Dinitrophenol

Concen: 2.640 ng/ul

RT: 14.840 min Scan# 1964

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:184 Resp: 27028


Ion Ratio Lower Upper

184 100

63 73.9 54.3 81.5

154 65.7 50.7 76.1









#55
4-Nitrophenol
Concen: 4.383 ng/ul
RT: 14.922 min Scan# 1978
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:109 Resp: 64810
Ion Ratio Lower Upper
109 100
139 133.5 109.4 164.0
65 126.7 105.4 158.2



#56
Dibenzofuran
Concen: 5.082 ng/ul
RT: 15.110 min Scan# 2010
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:168 Resp: 625933
Ion Ratio Lower Upper
168 100
139 37.9 29.4 44.0









#57
2,4-Dinitrotoluene
Concen: 4.287 ng/ul
RT: 15.087 min Scan# 2006
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:165 Resp: 118177
Ion Ratio Lower Upper
165 100
63 47.4 35.3 52.9
182 2.5 2.0 3.0

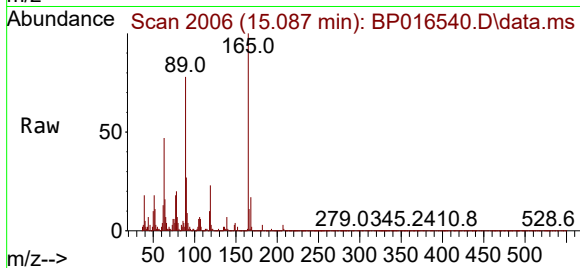

#58
2,3,4,6-Tetrachlorophenol
Concen: 4.354 ng/ul
RT: 15.322 min Scan# 2046
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:232 Resp: 100878
Ion Ratio Lower Upper
232 100
131 49.9 37.2 55.8
130 2.6 1.9 2.9
166 34.2 26.2 39.4

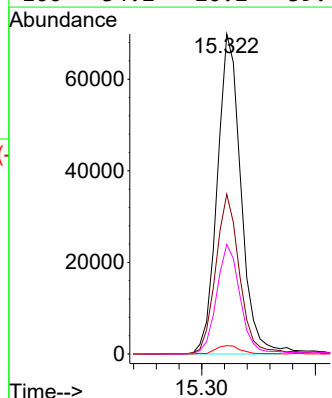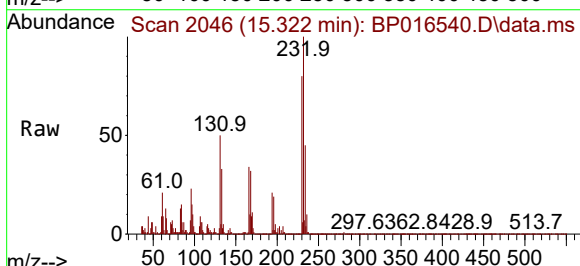



#61

Fluorene

Concen: 5.227 ng/ul

RT: 15.763 min Scan# 2121

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:166 Resp: 519587

Ion Ratio Lower Upper

166 100

165 96.1 77.3 115.9

167 13.6 10.7 16.1

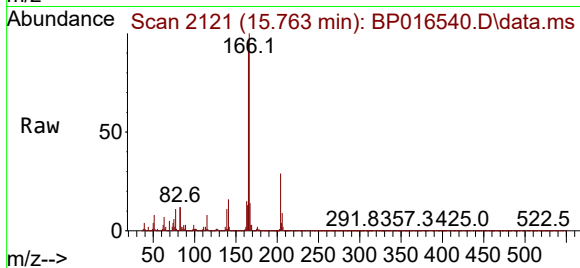

#62

4-Chlorophenyl-phenylether

Concen: 5.186 ng/ul

RT: 15.751 min Scan# 2119

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:204 Resp: 252957


Ion Ratio Lower Upper

204 100

206 32.1 26.4 39.6

141 60.3 48.6 73.0



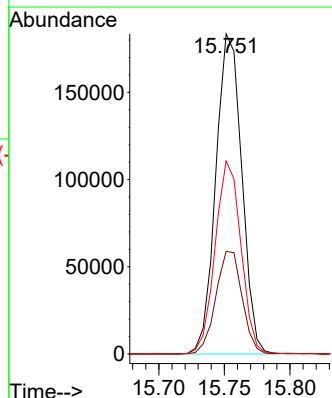
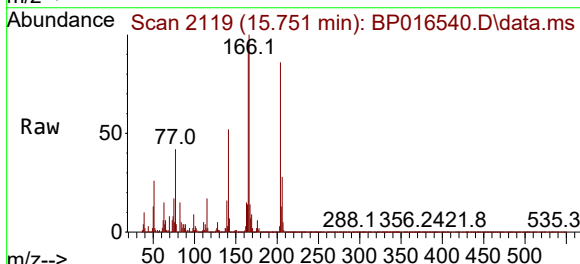




#63
4-Nitroaniline
Concen: 4.574 ng/ul
RT: 15.810 min Scan# 2129
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:138 Resp: 83078
Ion Ratio Lower Upper
138 100
92 53.7 42.2 63.4
108 85.0 64.0 96.0



#66
4,6-Dinitro-2-methylphenol
Concen: 3.377 ng/ul
RT: 15.834 min Scan# 2133
Delta R.T. -0.006 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:198 Resp: 56246
Ion Ratio Lower Upper
198 100
182 7.2 3.8 5.8#
77 30.6 20.5 30.7





#67

N-Nitrosodiphenylamine

Concen: 4.922 ng/ul

RT: 15.975 min Scan# 2157

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:169 Resp: 427528

Ion Ratio Lower Upper

169 100

168 66.9 53.0 79.6

167 36.0 29.0 43.6



#68

4-Bromophenyl-phenylether

Concen: 4.716 ng/ul

RT: 16.657 min Scan# 2273

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:248 Resp: 145689


Ion Ratio Lower Upper

248 100

250 98.0 78.2 117.4

141 75.7 58.4 87.6



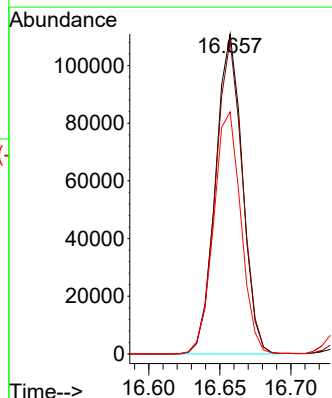





#69
Hexachlorobenzene
Concen: 4.875 ng/ul
RT: 16.740 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:284 Resp: 176937
Ion Ratio Lower Upper
284 100
142 32.7 28.6 42.8
249 29.4 24.6 37.0

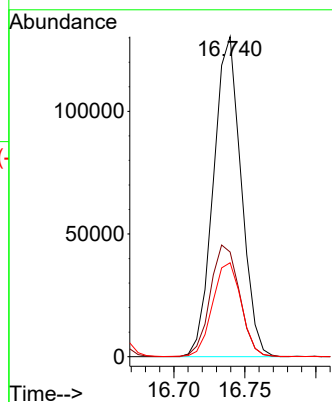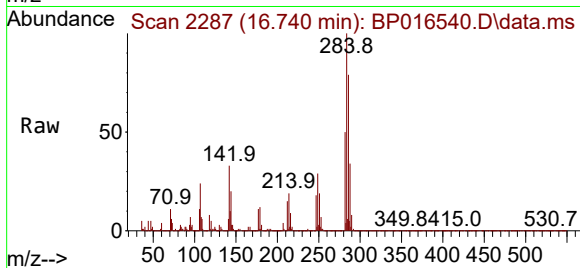

#70
Atrazine
Concen: 4.552 ng/ul
RT: 16.928 min Scan# 2319
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:200 Resp: 139796
Ion Ratio Lower Upper
200 100
173 26.8 21.4 32.2
215 49.7 38.0 57.0

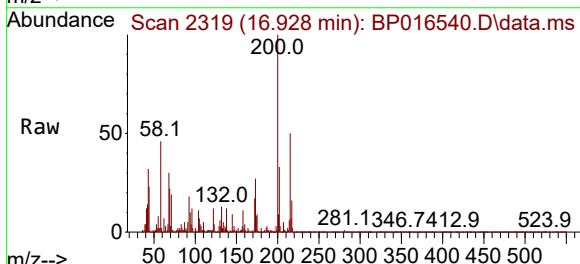



#71

Pentachlorophenol

Concen: 3.634 ng/ul

RT: 17.098 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:266 Resp: 80342

Ion Ratio Lower Upper

266 100

264 60.2 51.4 77.2

268 63.2 51.6 77.4



#72

Phenanthrene

Concen: 5.064 ng/ul

RT: 17.522 min Scan# 2420

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:178 Resp: 835120


Ion Ratio Lower Upper

178 100

179 15.3 12.6 18.8

176 18.8 15.5 23.3





#74

Anthracene

Concen: 5.014 ng/uI

RT: 17.610 min Scan# 2436

Delta R.T. -0.006 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:178 Resp: 825088

Ion Ratio Lower Upper

178 100

179 15.3 12.3 18.5

176 18.2 15.0 22.4

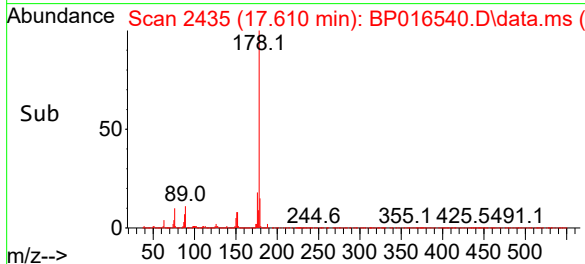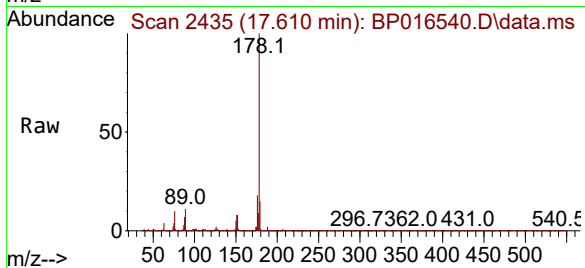

#75

1,2,3,4-Tetrachlorobenzene

Concen: 4.401 ng/uI

RT: 13.504 min Scan# 1737

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:216 Resp: 196671


Ion Ratio Lower Upper

216 100

214 78.2 61.8 92.8

218 48.7 38.9 58.3


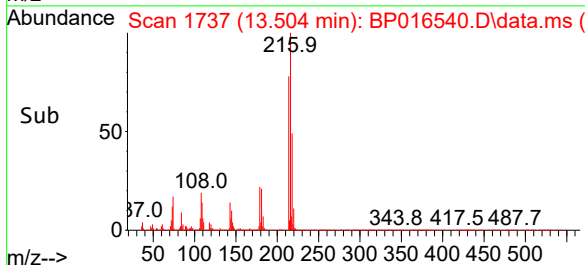
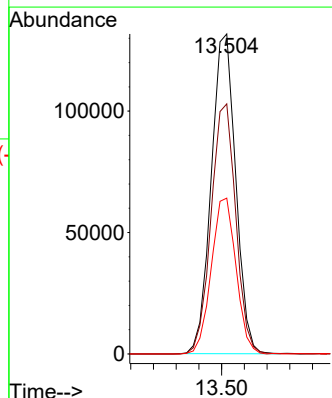
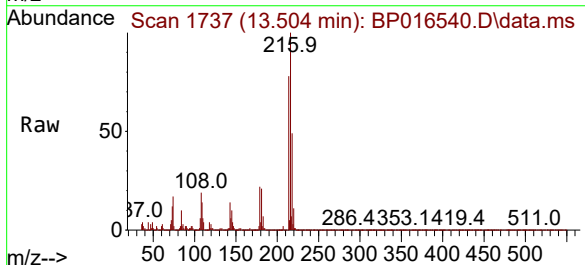




#76
Pentachlorobenzene
Concen: 4.696 ng/uL
RT: 15.004 min Scan# 1992
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:250 Resp: 188704
Ion Ratio Lower Upper
250 100
248 62.2 51.2 76.8
252 63.8 50.2 75.2

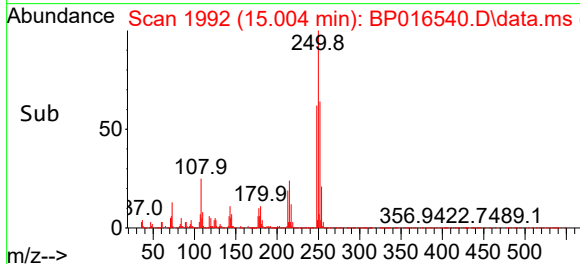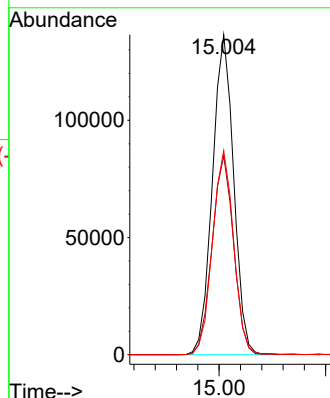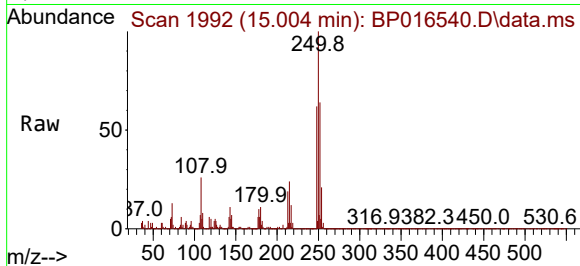

#77
Carbazole
Concen: 5.167 ng/uL
RT: 17.892 min Scan# 2483
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:167 Resp: 736684
Ion Ratio Lower Upper
167 100
166 21.5 17.0 25.6
139 12.9 10.1 15.1

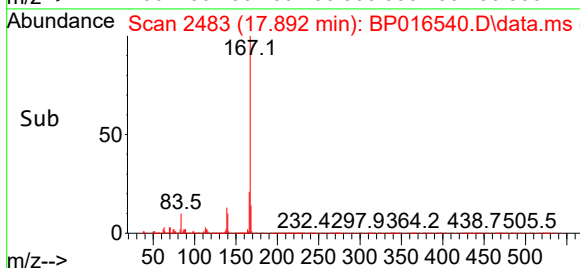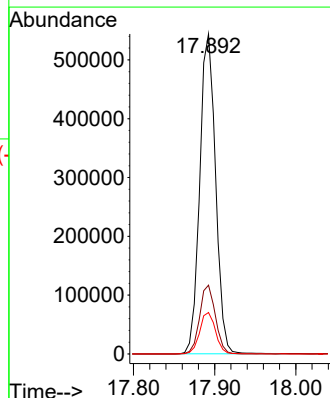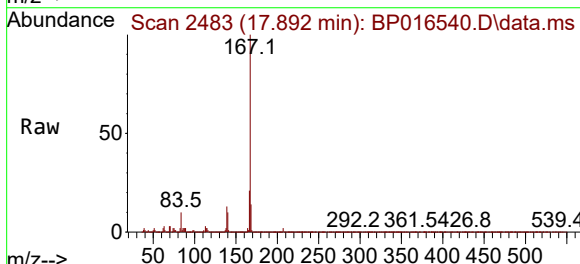



#78

Di-n-butylphthalate

Concen: 4.896 ng/ul

RT: 18.404 min Scan# 2570

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:149 Resp: 855082

Ion Ratio Lower Upper

149 100

150 9.0 7.6 11.4

104 5.3 4.3 6.5

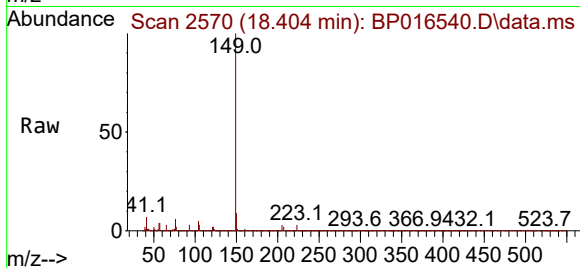

#80

Fluoranthene

Concen: 4.934 ng/ul

RT: 19.481 min Scan# 2753

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:202 Resp: 936272


Ion Ratio Lower Upper

202 100

101 12.5 9.9 14.9

100 9.7 7.5 11.3

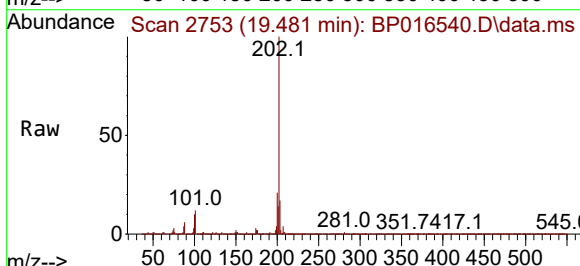



#82

Pyrene

Concen: 5.117 ng/ul

RT: 19.839 min Scan# 2814

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:202 Resp: 1010377

Ion Ratio Lower Upper

202 100

101 13.9 11.3 16.9

100 11.5 9.2 13.8



#83

Butylbenzylphthalate

Concen: 4.451 ng/ul

RT: 20.698 min Scan# 2960

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:149 Resp: 343108


Ion Ratio Lower Upper

149 100

91 74.7 58.5 87.7

206 20.0 16.5 24.7




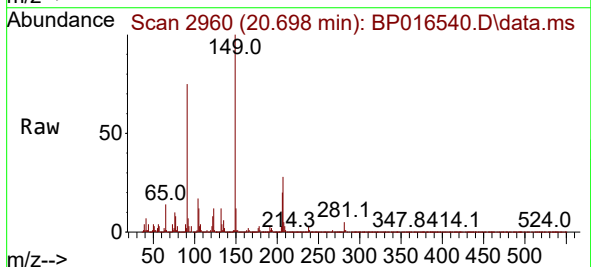




#84
3,3'-Dichlorobenzidine
Concen: 4.394 ng/ul
RT: 21.492 min Scan# 3095
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:252 Resp: 276981
Ion Ratio Lower Upper
252 100
254 63.1 51.8 77.8
126 12.1 9.7 14.5



#85
Benzo(a)anthracene
Concen: 4.912 ng/ul
RT: 21.557 min Scan# 3106
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:228 Resp: 954893
Ion Ratio Lower Upper
228 100
229 19.0 15.6 23.4
226 26.7 21.8 32.6









#86
Bis(2-ethylhexyl)phthalate
Concen: 4.540 ng/ul
RT: 21.439 min Scan# 3086
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17




Instrument :
BNA_P
ClientSampleId :
SSTD005618


Tgt Ion:149 Resp: 495778
Ion Ratio Lower Upper
149 100
167 26.8 22.1 33.1
279 3.7 3.2 4.8

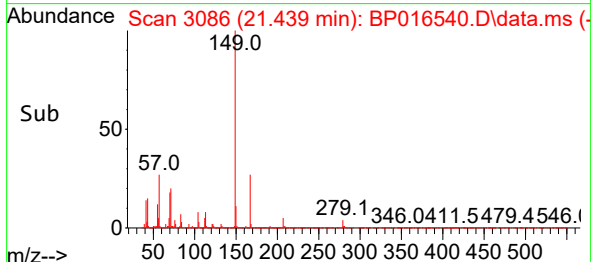

#87
Chrysene
Concen: 4.964 ng/ul
RT: 21.616 min Scan# 3116
Delta R.T. 0.000 min
Lab File: BP016540.D
Acq: 10 Aug 2023 10:17

Tgt Ion:228 Resp: 893500
Ion Ratio Lower Upper
228 100
226 30.2 24.2 36.4
229 19.7 16.0 24.0





#89

Di-n-octyl phthalate

Concen: 4.801 ng/ul

RT: 22.427 min Scan# 31

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17





Instrument :

BNA_P

ClientSampleId :

SSTD005618

Tgt Ion:149 Resp: 826843

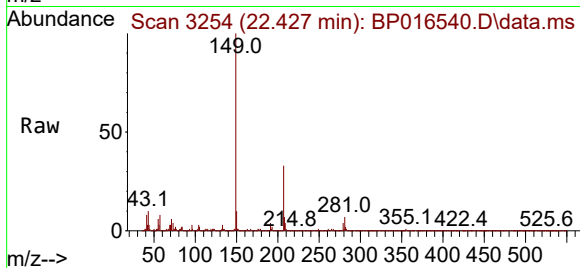

#90

Benzo(b)fluoranthene

Concen: 4.754 ng/ul

RT: 23.357 min Scan# 3412

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:252 Resp: 871857


Ion Ratio Lower Upper

252 100

253 22.1 17.6 26.4

125 11.1 8.6 13.0

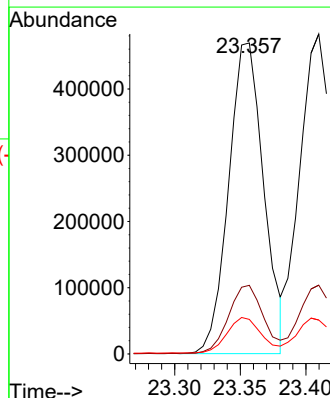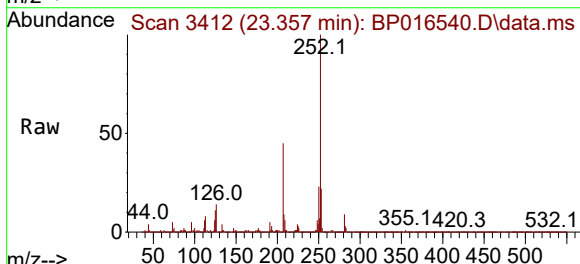



#91

Benzo(k)fluoranthene

Concen: 4.767 ng/ul

RT: 23.410 min Scan# 3421

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:252 Resp: 878984

Ion Ratio Lower Upper

252 100

253 21.5 17.7 26.5

125 10.6 8.8 13.2

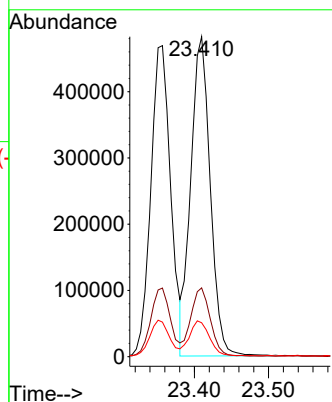

#93

Benzo(a)pyrene

Concen: 4.658 ng/ul

RT: 24.045 min Scan# 3529

Delta R.T. 0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:252 Resp: 800268


Ion Ratio Lower Upper

252 100

253 21.9 18.0 27.0

125 12.6 10.0 15.0





#94

Indeno(1,2,3-cd)pyrene

Concen: 4.452 ng/ul

RT: 26.915 min Scan# 4017

Delta R.T. -0.000 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618





Tgt Ion:276 Resp: 887640

Ion Ratio Lower Upper

276 100

138 24.5 18.6 27.8

277 23.1 19.7 29.5

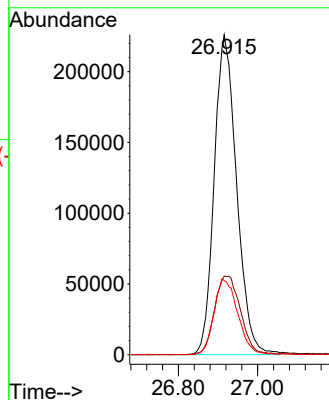

#95

Dibenzo(a,h)anthracene

Concen: 4.463 ng/ul

RT: 26.945 min Scan# 4022

Delta R.T. -0.006 min

Lab File: BP016540.D

Acq: 10 Aug 2023 10:17




Tgt Ion:278 Resp: 741126


Ion Ratio Lower Upper

278 100

139 16.8 13.9 20.9

279 23.1 18.8 28.2

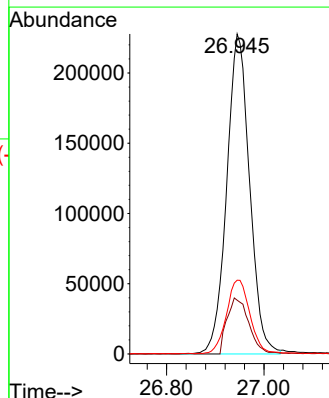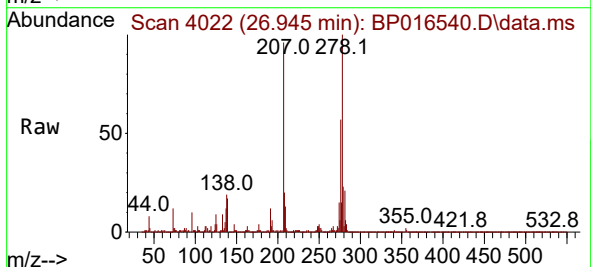



#96

Benzo(g,h,i)perylene

Concen: 4.412 ng/ul

RT: 27.780 min Scan# 41

Delta R.T. 0.000 min

Lab File: BP016540.D


Acq: 10 Aug 2023 10:17

Instrument :

BNA_P

ClientSampleId :

SSTD005618



Tgt Ion:276 Resp: 693647

Ion Ratio Lower Upper

276 100

138 23.4 18.3 27.5

277 22.7 19.1 28.7

