

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016541.D
 Acq On : 10 Aug 2023 10:51
 Operator : MA/JU
 Sample : SSTD01019
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010619

Quant Time: Aug 10 16:48:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 10 14:05:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	314376	20.000	ng/u1	0.00
20) Naphthalene-d8	10.893	136	1347331	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.710	164	813976	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.481	188	1766875	20.000	ng/u1	0.00
79) Chrysene-d12	21.575	240	1635416	20.000	ng/u1	0.00
88) Perylene-d12	24.169	264	1717626	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	32019	3.957	ng/uL	0.00
4) Pyridine-d5	3.834	84	206669	9.166	ng/u1	0.00
7) Phenol-d5	7.199	99	234118	8.959	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	156506	9.735	ng/u1	0.00
11) 2-Chlorophenol-d4	7.581	132	183731	9.056	ng/u1	0.00
15) 4-Methylphenol-d8	8.763	113	183762	8.776	ng/u1	0.00
21) Nitrobenzene-d5	9.258	128	84046	8.706	ng/u1	0.00
24) 2-Nitrophenol-d4	9.975	143	73042	7.799	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.499	165	163945	8.698	ng/u1	0.00
31) 4-Chloroaniline-d4	11.046	131	267911	9.261	ng/u1	0.00
46) Dimethylphthalate-d6	14.122	166	543268	9.305	ng/u1	0.00
49) Acenaphthylene-d8	14.410	160	622098	9.275	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	87680	7.661	ng/u1	0.00
60) Fluorene-d10	15.704	176	480984	9.657	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	52729	6.297	ng/u1	0.00
73) Anthracene-d10	17.581	188	733065	9.639	ng/u1	0.00
81) Pyrene-d10	19.810	212	845005	9.384	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.992	264	756619	9.181	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.434	88	32364	3.815	ng/uL	98
5) Pyridine	3.858	79	218586	9.445	ng/u1	99
6) Benzaldehyde	7.216	77	161792	11.935	ng/u1	95
8) Phenol	7.222	94	257005	9.363	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.493	93	217229	9.688	ng/u1	99
12) 2-Chlorophenol	7.611	128	195225	9.261	ng/u1	97
13) 2-Methylphenol	8.493	108	185602	9.029	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.575	45	166403	6.016	ng/u1	98
16) Acetophenone	8.910	105	320128	9.872	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.875	70	151490	9.208	ng/u1	97
18) 4-Methylphenol	8.828	108	201929	9.068	ng/u1	95
19) Hexachloroethane	9.140	117	81044	9.325	ng/u1	99
22) Nitrobenzene	9.299	77	227658	9.270	ng/u1	95
23) Isophorone	9.816	82	406497	8.832	ng/u1	98
25) 2-Nitrophenol	10.005	139	90412	8.367	ng/u1	95
26) 2,4-Dimethylphenol	10.040	107	215875	9.273	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.305	93	284793	9.389	ng/u1	100
29) 2,4-Dichlorophenol	10.528	162	175155	9.106	ng/u1	99
30) Naphthalene	10.946	128	675358	9.741	ng/u1	99
32) 4-Chloroaniline	11.069	127	273768	9.624	ng/u1	100
33) Hexachlorobutadiene	11.181	225	115039	9.502	ng/u1	99
34) Caprolactam	11.869	113	49680	7.218	ng/u1	92
35) 4-Chloro-3-methylphenol	12.163	107	181259	8.659	ng/u1	99
36) 2-Methylnaphthalene	12.546	142	438790	9.485	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016541.D
 Acq On : 10 Aug 2023 10:51
 Operator : MA/JU
 Sample : SSTD01019
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010619

Quant Time: Aug 10 16:48:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 10 14:05:43 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.763	142	444450	9.566	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.893	216	228010	9.586	ng/ul	99
40) Hexachlorocyclopentadiene	12.846	237	116630	8.036	ng/ul	99
41) 2,4,6-Trichlorophenol	13.140	196	123123	8.408	ng/ul	98
42) 2,4,5-Trichlorophenol	13.204	196	141342	8.843	ng/ul	99
43) 1,1'-Biphenyl	13.546	154	589081	9.764	ng/ul	98
44) 2-Chloronaphthalene	13.593	162	464753	9.797	ng/ul	99
45) 2-Nitroaniline	13.816	65	101335	8.085	ng/ul	93
47) Dimethylphthalate	14.169	163	556690	9.419	ng/ul	99
48) 2,6-Dinitrotoluene	14.304	165	85195	7.845	ng/ul	90
50) Acenaphthylene	14.440	152	740749	9.554	ng/ul	98
51) 3-Nitroaniline	14.645	138	98720	8.622	ng/ul	98
52) Acenaphthene	14.775	153	497850	9.716	ng/ul	100
53) 2,4-Dinitrophenol	14.840	184	29024	4.971	ng/ul	93
55) 4-Nitrophenol	14.922	109	71840	8.518	ng/ul	93
56) Dibenzofuran	15.110	168	697466	9.931	ng/ul	100
57) 2,4-Dinitrotoluene	15.087	165	126911	8.073	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.322	232	112777	8.535	ng/ul	97
59) Diethylphthalate	15.522	149	545795	9.324	ng/ul	98
61) Fluorene	15.763	166	563992	9.950	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.751	204	275019	9.886	ng/ul	98
63) 4-Nitroaniline	15.810	138	93378	9.015	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.834	198	61208	6.644	ng/ul#	92
67) N-Nitrosodiphenylamine	15.975	169	457991	9.532	ng/ul	99
68) 4-Bromophenyl-phenylether	16.657	248	158186	9.258	ng/ul	97
69) Hexachlorobenzene	16.739	284	188703	9.399	ng/ul	99
70) Atrazine	16.928	200	149169	8.781	ng/ul	99
71) Pentachlorophenol	17.098	266	91937	7.518	ng/ul	95
72) Phenanthrene	17.522	178	901138	9.879	ng/ul	99
74) Anthracene	17.616	178	889704	9.774	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.504	216	237446	9.606	ng/uL	98
76) Pentachlorobenzene	15.004	250	214340	9.644	ng/uL	99
77) Carbazole	17.892	167	790109	10.019	ng/ul	99
78) Di-n-butylphthalate	18.410	149	874804	9.055	ng/ul	98
80) Fluoranthene	19.481	202	1006632	9.418	ng/ul	99
82) Pyrene	19.839	202	1078547	9.698	ng/ul	99
83) Butylbenzylphthalate	20.698	149	358331	8.255	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.492	252	310697	8.752	ng/ul	99
85) Benzo(a)anthracene	21.557	228	1049661	9.587	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.439	149	502421	8.169	ng/ul	100
87) Chrysene	21.616	228	992757	9.794	ng/ul	99
89) Di-n-octyl phthalate	22.427	149	840365	8.820	ng/ul	100
90) Benzo(b)fluoranthene	23.357	252	951249	9.377	ng/ul	99
91) Benzo(k)fluoranthene	23.410	252	985160	9.659	ng/ul	99
93) Benzo(a)pyrene	24.045	252	897607	9.445	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.915	276	1027968	9.320	ng/ul	97
95) Dibenzo(a,h)anthracene	26.945	278	864721	9.412	ng/ul	100
96) Benzo(g,h,i)perylene	27.774	276	815596	9.378	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
Data File : BP016541.D
Acq On : 10 Aug 2023 10:51
Operator : MA/JU
Sample : SSTD01019
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010619

Quant Time: Aug 10 16:48:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 10 14:05:43 2023
Response via : Initial Calibration




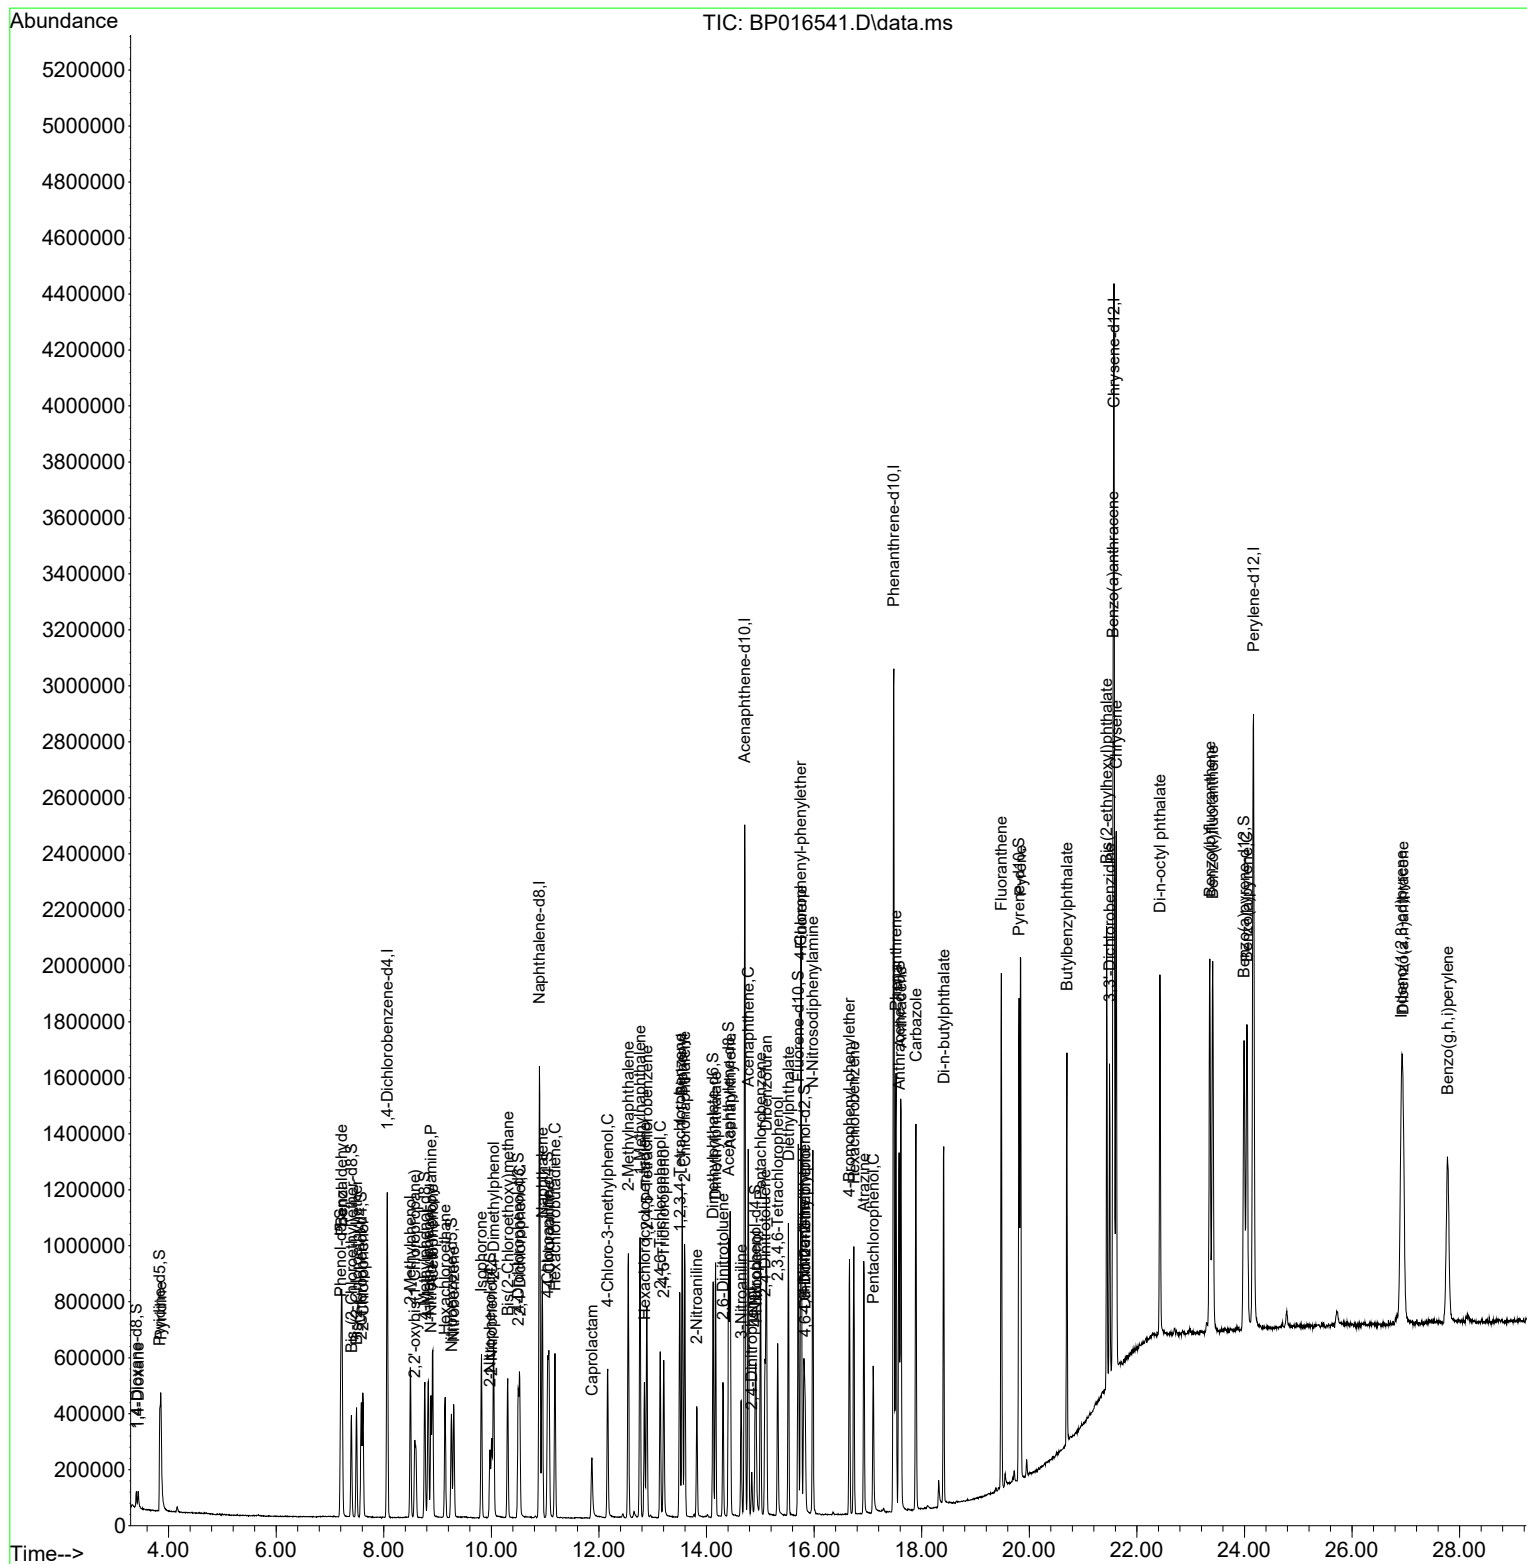




#2
1,4-Dioxane
Concen: 3.815 ng/uL
RT: 3.434 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion: 88 Resp: 32364
Ion Ratio Lower Upper
88 100
43 26.9 20.1 30.1
58 67.5 55.1 82.7

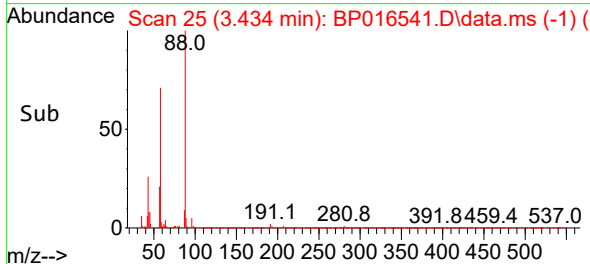

#5
Pyridine
Concen: 9.445 ng/uL
RT: 3.858 min Scan# 97
Delta R.T. 0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion: 79 Resp: 218586
Ion Ratio Lower Upper
79 100
52 65.5 52.9 79.3
51 31.8 24.6 37.0


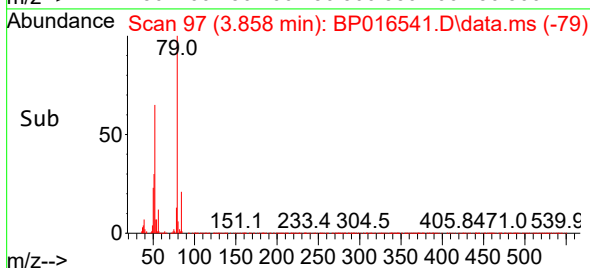
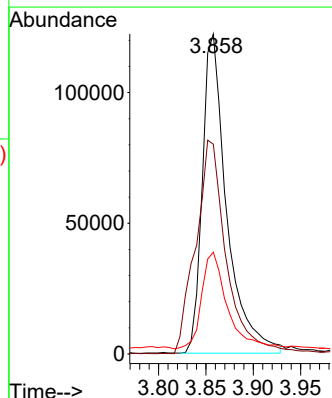
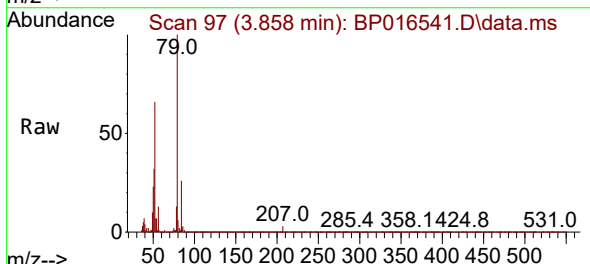




#6
Benzaldehyde
Concen: 11.935 ng/ul
RT: 7.216 min Scan# 668
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion: 77 Resp: 161792
Ion Ratio Lower Upper
77 100
105 97.3 79.6 119.4
106 88.8 76.5 114.7



#8
Phenol
Concen: 9.363 ng/ul
RT: 7.222 min Scan# 669
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion: 94 Resp: 257005
Ion Ratio Lower Upper
94 100
65 26.0 20.7 31.1
66 33.4 26.7 40.1

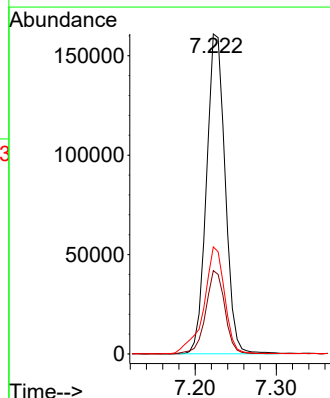







#10
 Bis(2-Chloroethyl)ether
 Concen: 9.688 ng/ul
 RT: 7.493 min Scan# 715
 Delta R.T. -0.000 min
 Lab File: BP016541.D
 Acq: 10 Aug 2023 10:51

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010619

Tgt Ion: 93 Resp: 217229




Ion	Ratio	Lower	Upper
93	100		
63	70.6	57.0	85.6
95	32.6	26.0	39.0

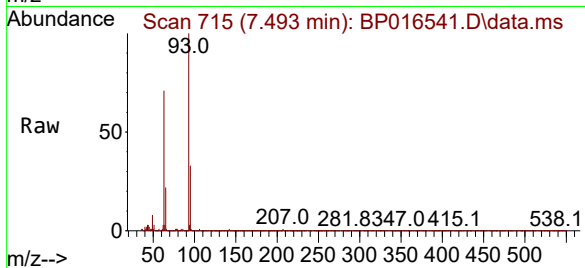


#12
 2-Chlorophenol
 Concen: 9.261 ng/ul
 RT: 7.611 min Scan# 735
 Delta R.T. -0.006 min
 Lab File: BP016541.D
 Acq: 10 Aug 2023 10:51

Tgt Ion: 128 Resp: 195225

Ion	Ratio	Lower	Upper
128	100		
64	45.9	34.7	52.1
130	31.1	25.9	38.9

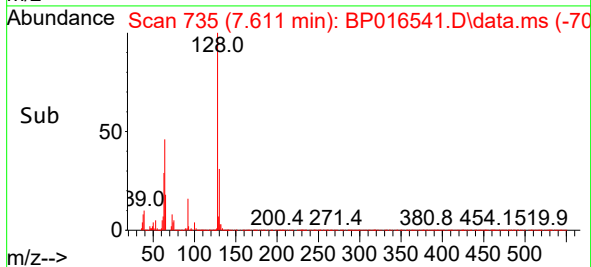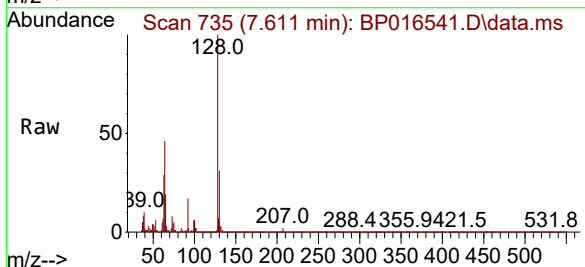



#13

2-Methylphenol

Concen: 9.029 ng/ul

RT: 8.493 min Scan# 886

Delta R.T. -0.006 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :





SSTD010619

Tgt Ion:108 Resp: 185602

Ion Ratio Lower Upper

108 100

107 88.5 71.9 107.9

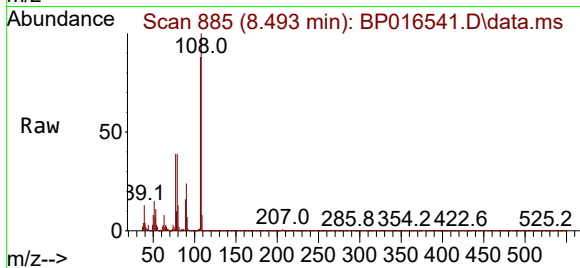

#14

2,2'-oxybis(1-Chloropropane)

Concen: 6.016 ng/ul

RT: 8.575 min Scan# 899

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion: 45 Resp: 166403


Ion Ratio Lower Upper

45 100

77 15.1 12.9 19.3

79 11.3 9.2 13.8




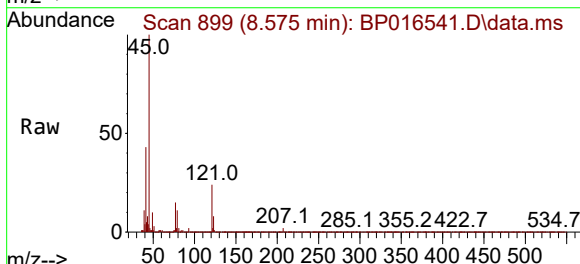




#16
Acetophenone
Concen: 9.872 ng/ul
RT: 8.910 min Scan# 910
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:105 Resp: 320128
Ion Ratio Lower Upper
105 100
77 75.8 61.0 91.4
51 23.3 18.7 28.1



#17
N-Nitroso-di-n-propylamine
Concen: 9.208 ng/ul
RT: 8.875 min Scan# 950
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion: 70 Resp: 151490
Ion Ratio Lower Upper
70 100
42 52.4 39.9 59.9
101 9.9 7.9 11.9
130 20.3 16.6 25.0









#18
4-Methylphenol
Concen: 9.068 ng/ul
RT: 8.828 min Scan# 942
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:108 Resp: 201929
Ion Ratio Lower Upper
108 100
107 106.6 89.5 134.3



#19
Hexachloroethane
Concen: 9.325 ng/ul
RT: 9.140 min Scan# 995
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:117 Resp: 81044
Ion Ratio Lower Upper
117 100
201 96.1 77.2 115.8
199 63.8 49.2 73.8









#22
Nitrobenzene
Concen: 9.270 ng/ul
RT: 9.299 min Scan# 1022
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion: 77 Resp: 227658
Ion Ratio Lower Upper
77 100
123 41.8 36.4 54.6
65 13.1 10.3 15.5

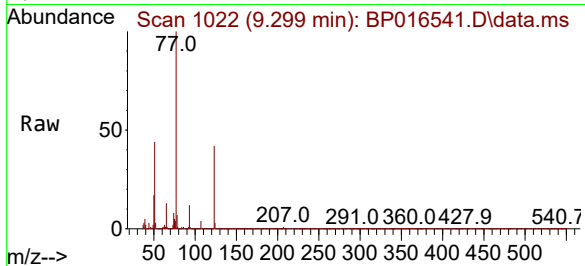

#23
Isophorone
Concen: 8.832 ng/ul
RT: 9.816 min Scan# 1110
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion: 82 Resp: 406497
Ion Ratio Lower Upper
82 100
95 6.9 5.4 8.0
138 16.2 13.6 20.4

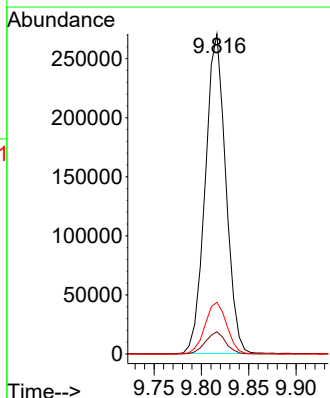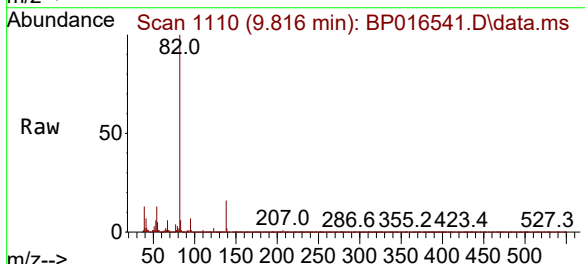



#25

2-Nitrophenol

Concen: 8.367 ng/ul

RT: 10.005 min Scan# 1142

Delta R.T. -0.006 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:139 Resp: 90412

Ion Ratio Lower Upper

139 100

65 52.4 38.9 58.3

109 31.5 23.1 34.7

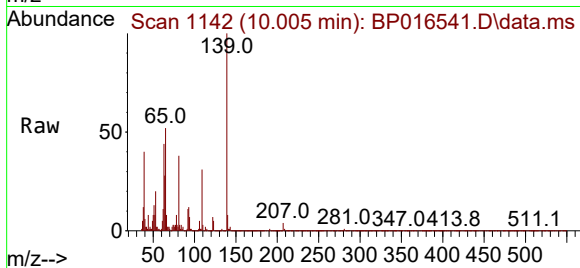

#26

2,4-Dimethylphenol

Concen: 9.273 ng/ul

RT: 10.040 min Scan# 1148

Delta R.T. -0.006 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:107 Resp: 215875


Ion Ratio Lower Upper

107 100

121 51.7 40.2 60.4

122 87.6 69.2 103.8


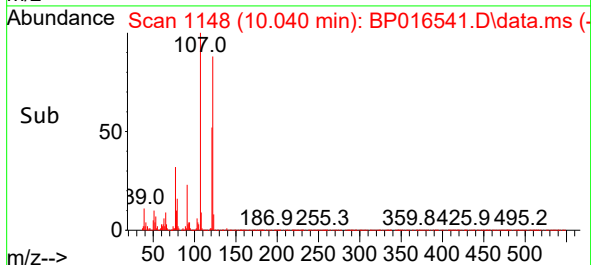
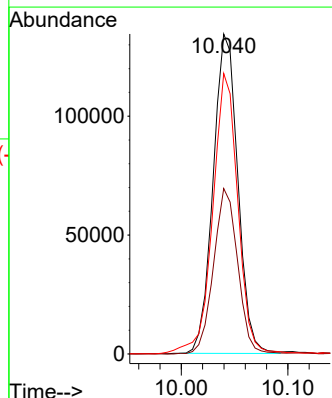
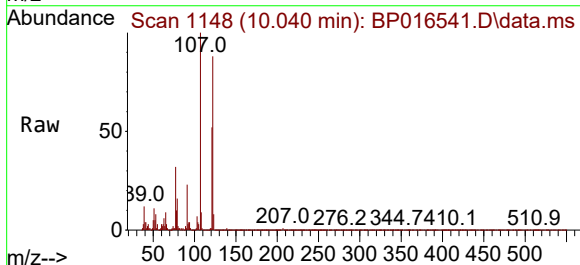




#27
Bis(2-Chloroethoxy)methane
Concen: 9.389 ng/ul
RT: 10.305 min Scan# 1193
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion: 93 Resp: 284793
Ion Ratio Lower Upper
93 100
95 32.8 26.0 39.0
123 11.5 9.0 13.6

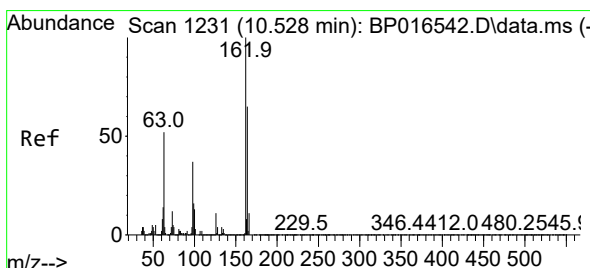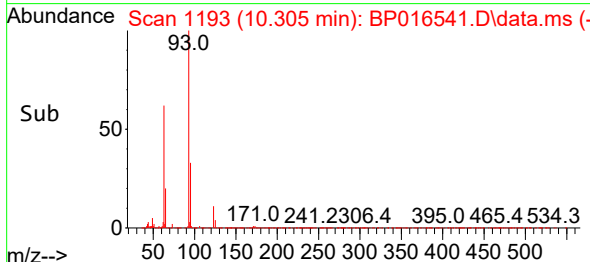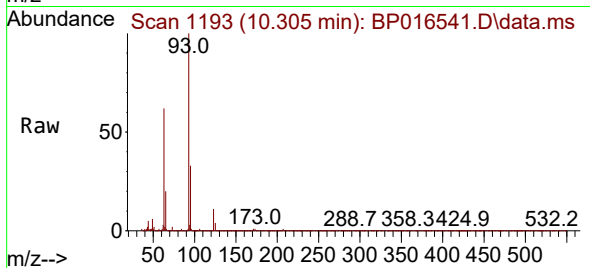

#29
2,4-Dichlorophenol
Concen: 9.106 ng/ul
RT: 10.528 min Scan# 1231
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion: 162 Resp: 175155
Ion Ratio Lower Upper
162 100
164 64.6 52.5 78.7
98 35.8 29.4 44.2


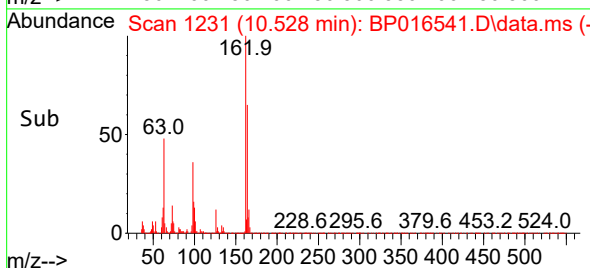

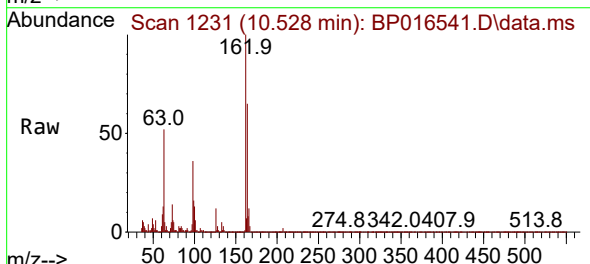




#30
Naphthalene
Concen: 9.741 ng/ul
RT: 10.946 min Scan# 1302
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:128 Resp: 675358
Ion Ratio Lower Upper
128 100
129 11.2 8.7 13.1
127 13.2 10.7 16.1

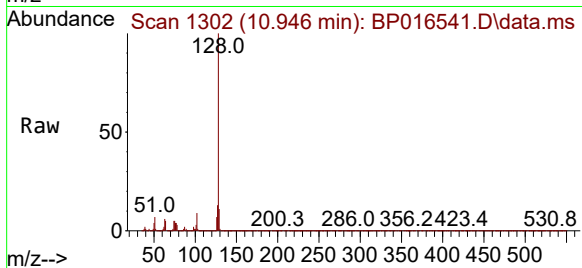

#32
4-Chloroaniline
Concen: 9.624 ng/ul
RT: 11.069 min Scan# 1323
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:127 Resp: 273768
Ion Ratio Lower Upper
127 100
129 32.4 25.8 38.6




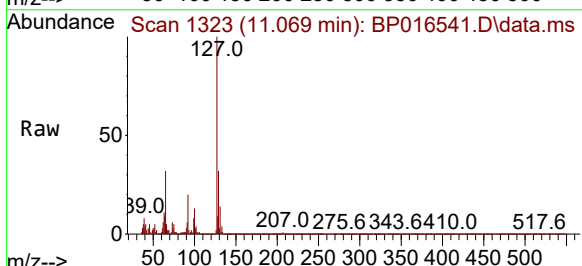




#33
Hexachlorobutadiene
Concen: 9.502 ng/ul
RT: 11.181 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:225 Resp: 115039
Ion Ratio Lower Upper
225 100
223 62.6 50.4 75.6
227 63.5 51.5 77.3



#34
Caprolactam
Concen: 7.218 ng/ul
RT: 11.869 min Scan# 1459
Delta R.T. -0.012 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:113 Resp: 49680
Ion Ratio Lower Upper
113 100
55 142.7 123.0 184.4
56 106.2 90.9 136.3









#35
4-Chloro-3-methylphenol
Concen: 8.659 ng/ul
RT: 12.163 min Scan# 1509
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:107 Resp: 181259
Ion Ratio Lower Upper
107 100
144 26.7 20.7 31.1
142 79.3 64.0 96.0

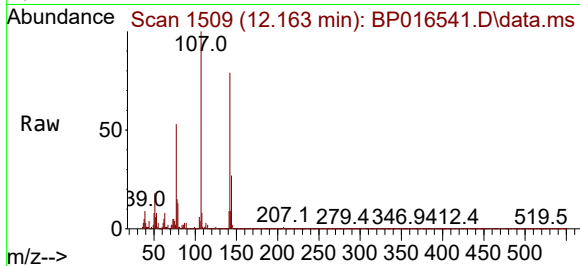

#36
2-Methylnaphthalene
Concen: 9.485 ng/ul
RT: 12.546 min Scan# 1574
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:142 Resp: 438790
Ion Ratio Lower Upper
142 100
141 88.2 71.7 107.5




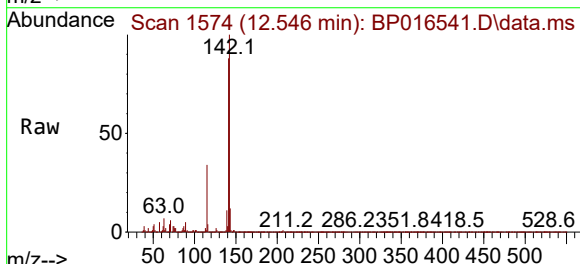




#37
1-Methylnaphthalene
Concen: 9.566 ng/ul
RT: 12.763 min Scan# 1611
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:142 Resp: 444450
Ion Ratio Lower Upper
142 100
141 92.1 73.2 109.8
116 3.6 3.0 4.4

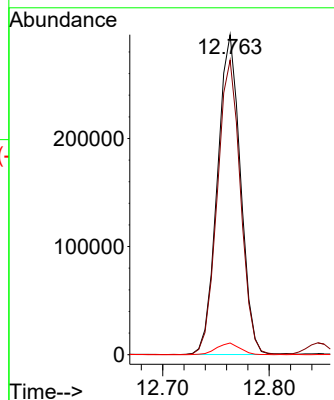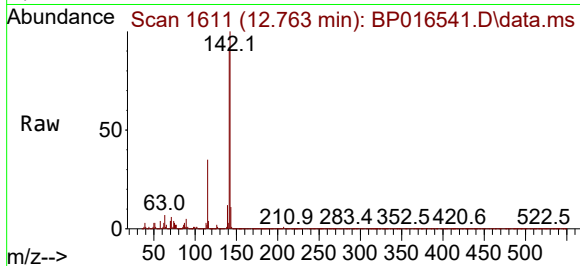

#39
1,2,4,5-Tetrachlorobenzene
Concen: 9.586 ng/ul
RT: 12.893 min Scan# 1633
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:216 Resp: 228010
Ion Ratio Lower Upper
216 100
214 79.2 62.6 94.0
179 21.4 16.6 25.0
108 17.4 13.8 20.8

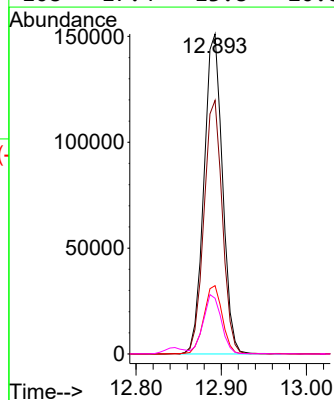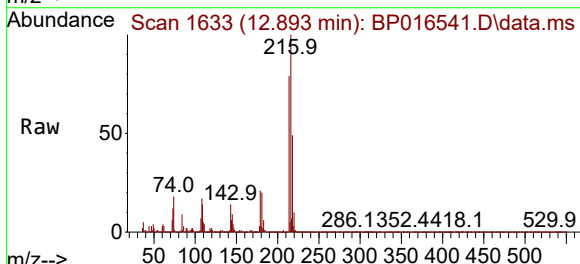



#40

Hexachlorocyclopentadiene

Concen: 8.036 ng/ul

RT: 12.846 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:237 Resp: 116630

Ion Ratio Lower Upper

237 100

235 62.5 49.3 73.9

272 13.1 10.7 16.1



#41

2,4,6-Trichlorophenol

Concen: 8.408 ng/ul

RT: 13.140 min Scan# 1675

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:196 Resp: 123123


Ion Ratio Lower Upper

196 100

198 97.2 76.3 114.5

200 29.6 25.3 37.9


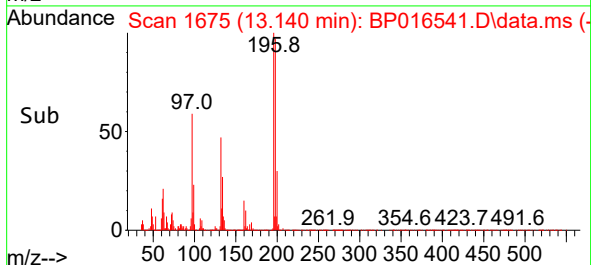

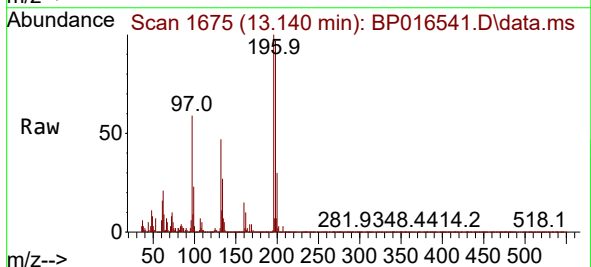




#42
2,4,5-Trichlorophenol
Concen: 8.843 ng/ul
RT: 13.204 min Scan# 1686
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:196 Resp: 141342
Ion Ratio Lower Upper
196 100
198 93.8 75.7 113.5
200 31.3 24.6 37.0

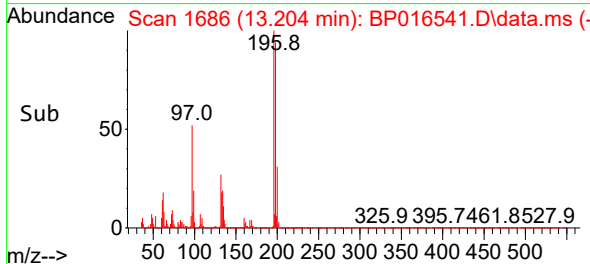

#43
1,1'-Biphenyl
Concen: 9.764 ng/ul
RT: 13.546 min Scan# 1744
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:154 Resp: 589081
Ion Ratio Lower Upper
154 100
153 40.7 31.7 47.5
76 14.6 11.3 16.9


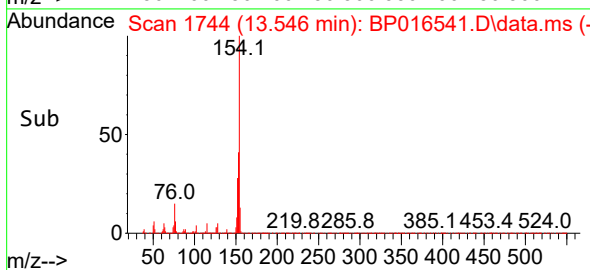

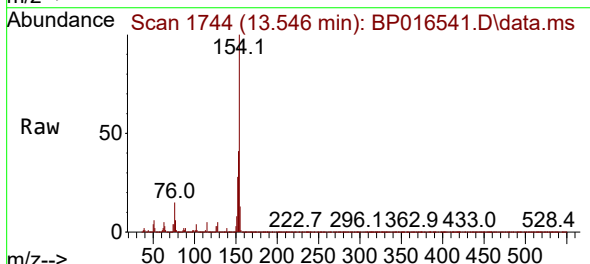




#44
2-Chloronaphthalene
Concen: 9.797 ng/ul
RT: 13.593 min Scan# 1752
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument : BNA_P
ClientSampleId : SSTD010619


Tgt Ion:162 Resp: 464753
Ion Ratio Lower Upper
162 100
164 32.5 26.6 40.0
127 38.9 31.2 46.8

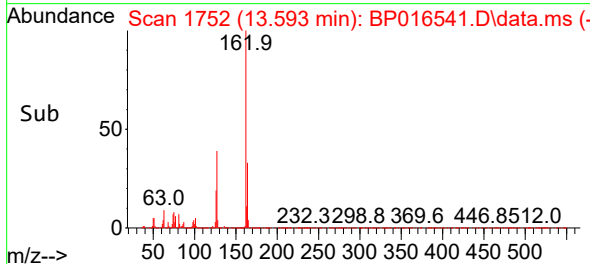

#45
2-Nitroaniline
Concen: 8.085 ng/ul
RT: 13.816 min Scan# 1790
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion: 65 Resp: 101335
Ion Ratio Lower Upper
65 100
92 74.6 58.0 87.0
138 100.5 88.6 132.8


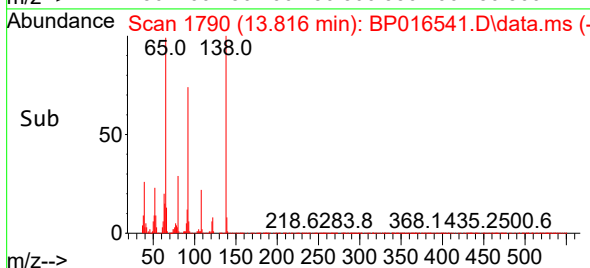
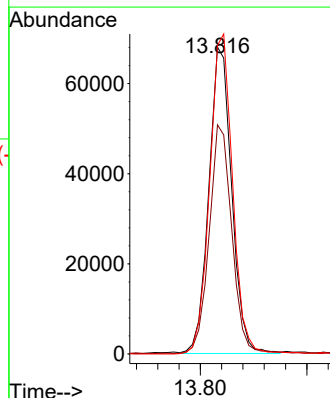
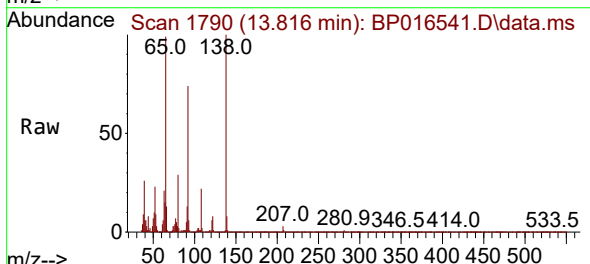




#47
Dimethylphthalate
Concen: 9.419 ng/ul
RT: 14.169 min Scan# 1850
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:163 Resp: 556690
Ion Ratio Lower Upper
163 100
194 4.2 3.2 4.8
164 9.8 8.1 12.1



#48
2,6-Dinitrotoluene
Concen: 7.845 ng/ul
RT: 14.304 min Scan# 1873
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:165 Resp: 85195
Ion Ratio Lower Upper
165 100
89 66.6 46.4 69.6
121 23.1 16.8 25.2









#50
Acenaphthylene
Concen: 9.554 ng/ul
RT: 14.440 min Scan# 1896
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:152 Resp: 740749
Ion Ratio Lower Upper
152 100
151 20.5 15.7 23.5
153 12.8 10.6 16.0

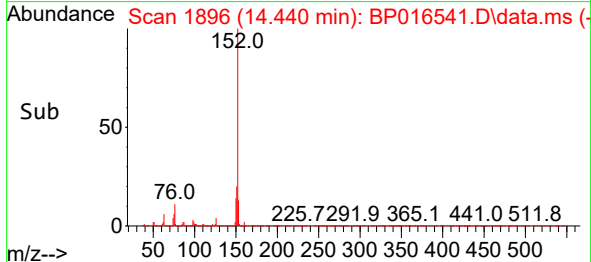

#51
3-Nitroaniline
Concen: 8.622 ng/ul
RT: 14.645 min Scan# 1931
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:138 Resp: 98720
Ion Ratio Lower Upper
138 100
108 13.9 9.4 14.2
92 117.6 95.0 142.6


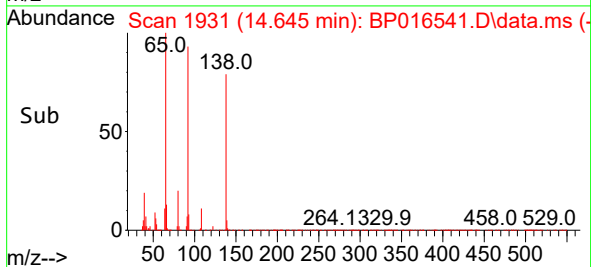

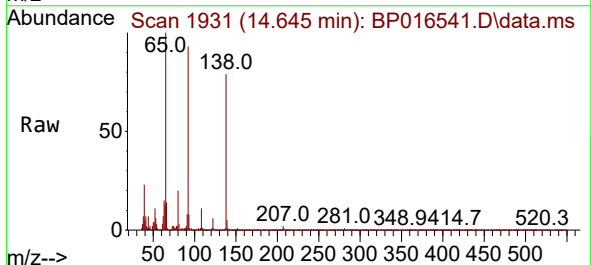




#52
Acenaphthene
Concen: 9.716 ng/ul
RT: 14.775 min Scan# 1953
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:153 Resp: 497850
Ion Ratio Lower Upper
153 100
152 47.6 38.6 58.0
154 88.7 71.0 106.6

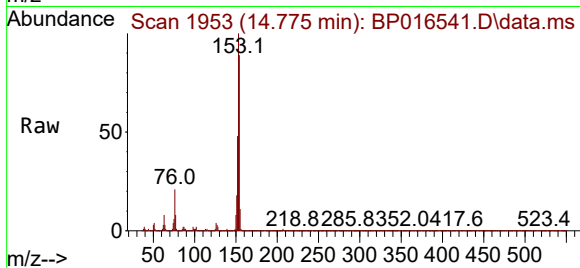

#53
2,4-Dinitrophenol
Concen: 4.971 ng/ul
RT: 14.840 min Scan# 1964
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:184 Resp: 29024
Ion Ratio Lower Upper
184 100
63 78.1 54.3 81.5
154 63.2 50.7 76.1




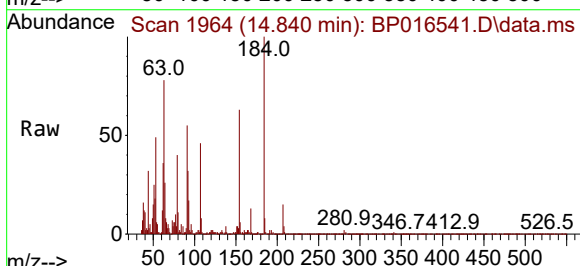




#55
4-Nitrophenol
Concen: 8.518 ng/ul
RT: 14.922 min Scan# 1978
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:109 Resp: 71840
Ion Ratio Lower Upper
109 100
139 129.4 109.4 164.0
65 122.6 105.4 158.2

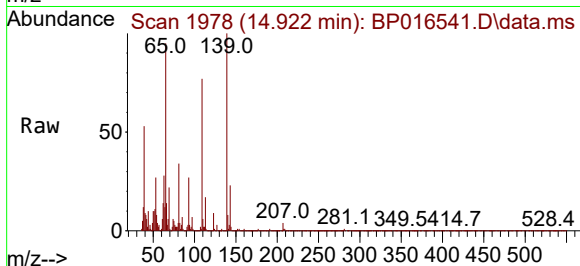

#56
Dibenzofuran
Concen: 9.931 ng/ul
RT: 15.110 min Scan# 2010
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:168 Resp: 697466
Ion Ratio Lower Upper
168 100
139 36.9 29.4 44.0




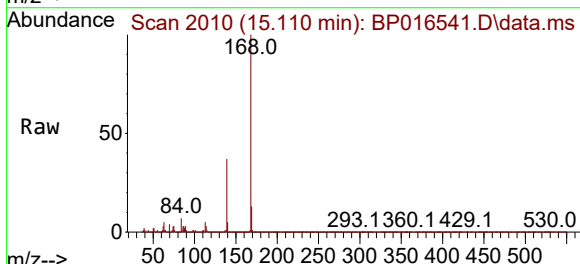




#57
2,4-Dinitrotoluene
Concen: 8.073 ng/ul
RT: 15.087 min Scan# 2006
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:165 Resp: 126911
Ion Ratio Lower Upper
165 100
63 44.4 35.3 52.9
182 2.9 2.0 3.0

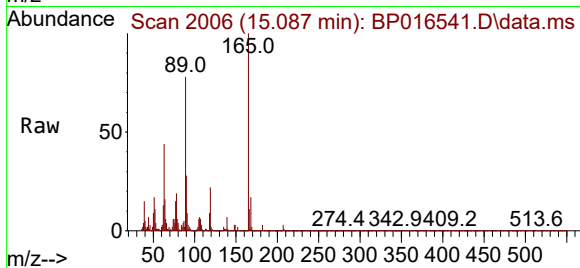

#58
2,3,4,6-Tetrachlorophenol
Concen: 8.535 ng/ul
RT: 15.322 min Scan# 2046
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:232 Resp: 112777
Ion Ratio Lower Upper
232 100
131 49.4 37.2 55.8
130 2.6 1.9 2.9
166 32.9 26.2 39.4


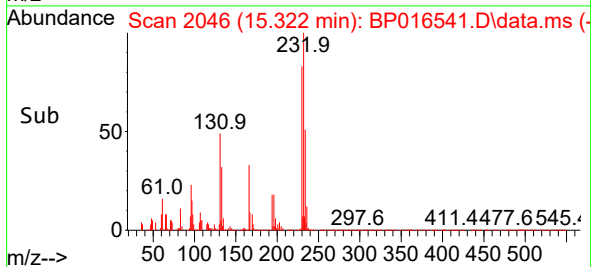

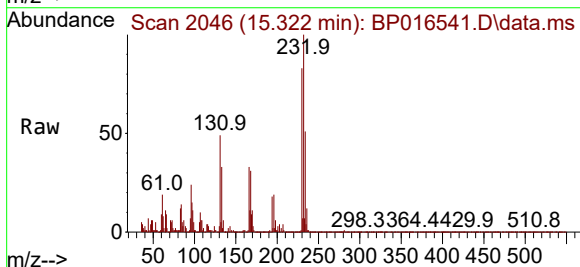




#59
Diethylphthalate
Concen: 9.324 ng/ul
RT: 15.522 min Scan# 2081
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:149 Resp: 545795
Ion Ratio Lower Upper
149 100
177 21.5 18.2 27.2
150 12.2 9.8 14.8



#61
Fluorene
Concen: 9.950 ng/ul
RT: 15.763 min Scan# 2121
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:166 Resp: 563992
Ion Ratio Lower Upper
166 100
165 96.9 77.3 115.9
167 13.0 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 9.886 ng/ul
RT: 15.751 min Scan# 2119
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:204 Resp: 275019
Ion Ratio Lower Upper
204 100
206 33.5 26.4 39.6
141 59.3 48.6 73.0

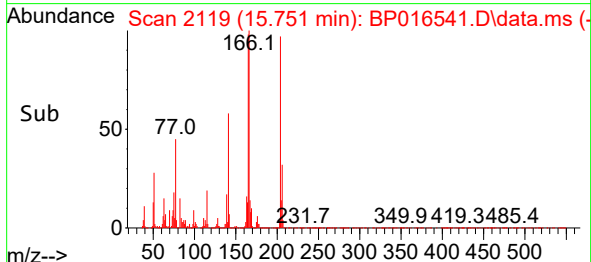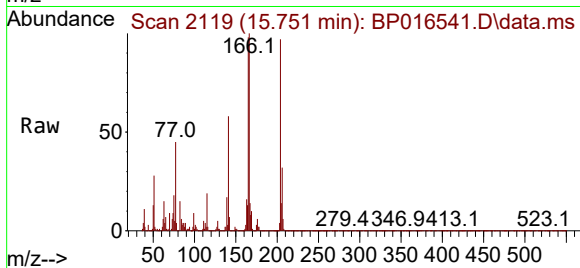

#63
4-Nitroaniline
Concen: 9.015 ng/ul
RT: 15.810 min Scan# 2129
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:138 Resp: 93378
Ion Ratio Lower Upper
138 100
92 54.7 42.2 63.4
108 87.8 64.0 96.0




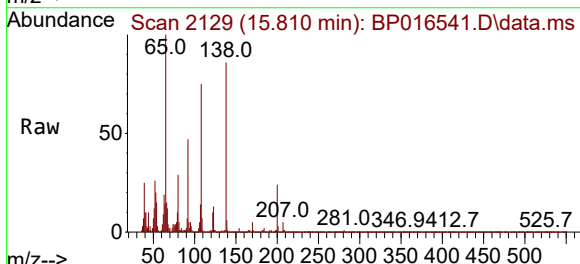




#66
4,6-Dinitro-2-methylphenol
Concen: 6.644 ng/ul
RT: 15.834 min Scan# 2133
Delta R.T. -0.006 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:198 Resp: 61208
Ion Ratio Lower Upper
198 100
182 6.9 3.8 5.8#
77 29.7 20.5 30.7

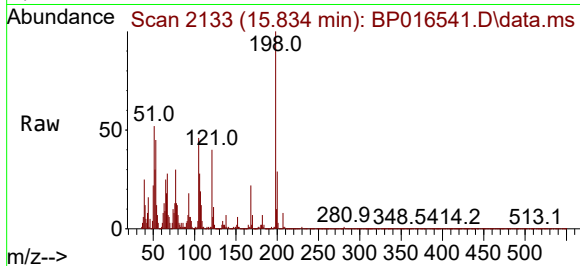

#67
N-Nitrosodiphenylamine
Concen: 9.532 ng/ul
RT: 15.975 min Scan# 2157
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:169 Resp: 457991
Ion Ratio Lower Upper
169 100
168 65.3 53.0 79.6
167 36.4 29.0 43.6









#68
4-Bromophenyl-phenylether
Concen: 9.258 ng/ul
RT: 16.657 min Scan# 211
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51




Instrument :
BNA_P
ClientSampleId :
SSTD010619


Tgt Ion:248 Resp: 158186
Ion Ratio Lower Upper
248 100
250 98.4 78.2 117.4
141 77.8 58.4 87.6



#69
Hexachlorobenzene
Concen: 9.399 ng/ul
RT: 16.739 min Scan# 2287
Delta R.T. -0.000 min
Lab File: BP016541.D
Acq: 10 Aug 2023 10:51

Tgt Ion:284 Resp: 188703
Ion Ratio Lower Upper
284 100
142 35.5 28.6 42.8
249 31.3 24.6 37.0

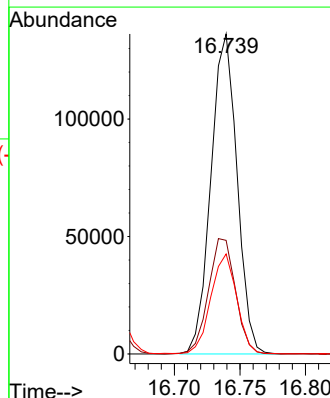



#70

Atrazine

Concen: 8.781 ng/ul

RT: 16.928 min Scan# 2319

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:200 Resp: 149169

Ion Ratio Lower Upper

200 100

173 26.2 21.4 32.2

215 47.0 38.0 57.0

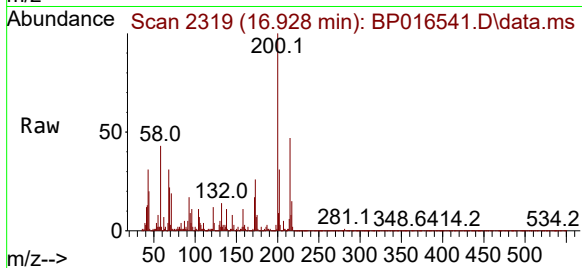

#71

Pentachlorophenol

Concen: 7.518 ng/ul

RT: 17.098 min Scan# 2348

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:266 Resp: 91937


Ion Ratio Lower Upper

266 100

264 61.6 51.4 77.2

268 60.0 51.6 77.4

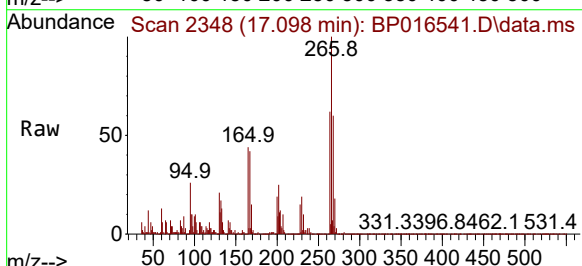



#72

Phenanthrene

Concen: 9.879 ng/ul

RT: 17.522 min Scan# 2420

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:178 Resp: 901138

Ion Ratio Lower Upper

178 100

179 15.3 12.6 18.8

176 19.3 15.5 23.3



#74

Anthracene

Concen: 9.774 ng/ul

RT: 17.616 min Scan# 2436

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:178 Resp: 889704


Ion Ratio Lower Upper

178 100

179 15.3 12.3 18.5

176 18.6 15.0 22.4





#75

1,2,3,4-Tetrachlorobenzene

Concen: 9.606 ng/uL

RT: 13.504 min Scan# 1737

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:216 Resp: 237446

Ion Ratio Lower Upper

216 100

214 75.5 61.8 92.8

218 47.4 38.9 58.3



#76

Pentachlorobenzene

Concen: 9.644 ng/uL

RT: 15.004 min Scan# 1992

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:250 Resp: 214340


Ion Ratio Lower Upper

250 100

248 64.0 51.2 76.8

252 64.0 50.2 75.2









#77
 Carbazole
 Concen: 10.019 ng/ul
 RT: 17.892 min Scan# 2483
 Delta R.T. -0.000 min
 Lab File: BP016541.D
 Acq: 10 Aug 2023 10:51




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010619


Tgt Ion:167 Resp: 790109
 Ion Ratio Lower Upper
 167 100
 166 21.8 17.0 25.6
 139 12.7 10.1 15.1

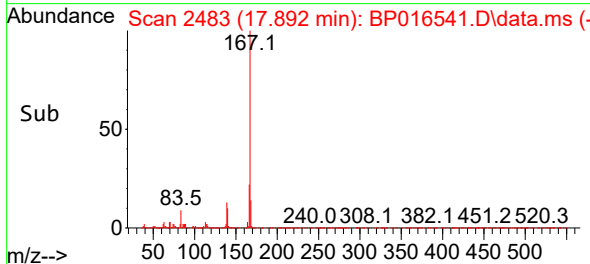

#78
 Di-n-butylphthalate
 Concen: 9.055 ng/ul
 RT: 18.410 min Scan# 2571
 Delta R.T. 0.006 min
 Lab File: BP016541.D
 Acq: 10 Aug 2023 10:51

Tgt Ion:149 Resp: 874804
 Ion Ratio Lower Upper
 149 100
 150 8.6 7.6 11.4
 104 5.2 4.3 6.5

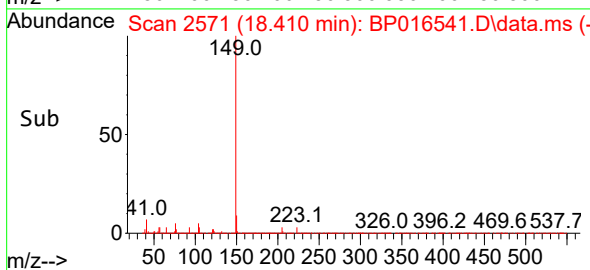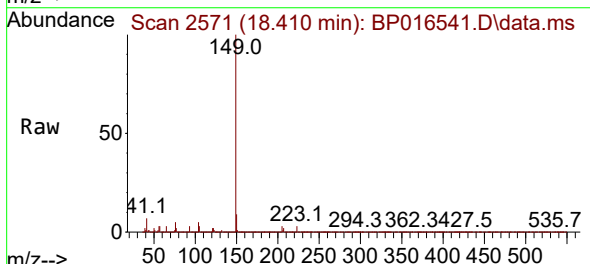



#80

Fluoranthene

Concen: 9.418 ng/ul

RT: 19.481 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:202 Resp: 1006632

Ion Ratio Lower Upper

202 100

101 11.9 9.9 14.9

100 9.0 7.5 11.3

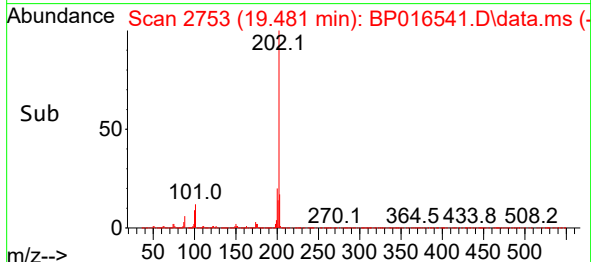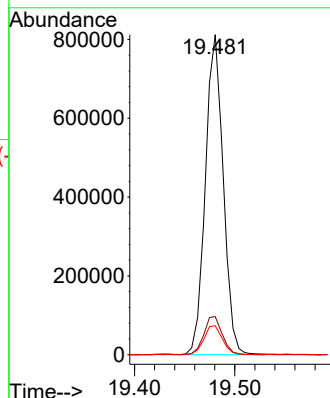

#82

Pyrene

Concen: 9.698 ng/ul

RT: 19.839 min Scan# 2814

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:202 Resp: 1078547


Ion Ratio Lower Upper

202 100

101 13.9 11.3 16.9

100 11.8 9.2 13.8





#83

Butylbenzylphthalate

Concen: 8.255 ng/ul

RT: 20.698 min Scan# 2960

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:149 Resp: 358331

Ion Ratio Lower Upper

149 100

91 74.7 58.5 87.7

206 20.1 16.5 24.7

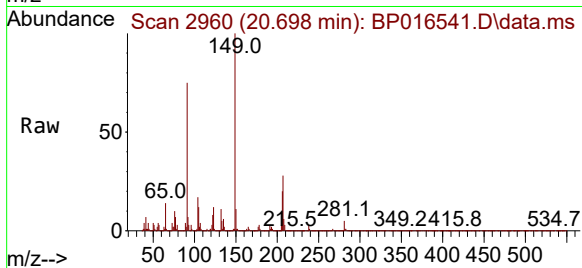

#84

3,3'-Dichlorobenzidine

Concen: 8.752 ng/ul

RT: 21.492 min Scan# 3095

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:252 Resp: 310697


Ion Ratio Lower Upper

252 100

254 64.2 51.8 77.8

126 12.0 9.7 14.5

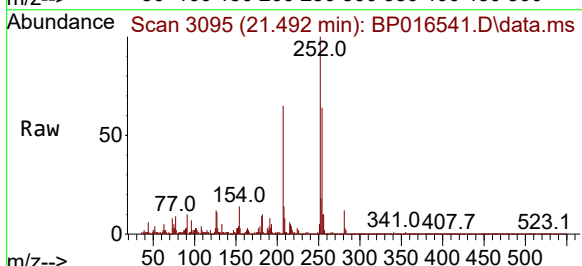



#85

Benzo(a)anthracene

Concen: 9.587 ng/ul

RT: 21.557 min Scan# 3106

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:228 Resp: 1049661

Ion Ratio Lower Upper

228 100

229 19.2 15.6 23.4

226 26.1 21.8 32.6

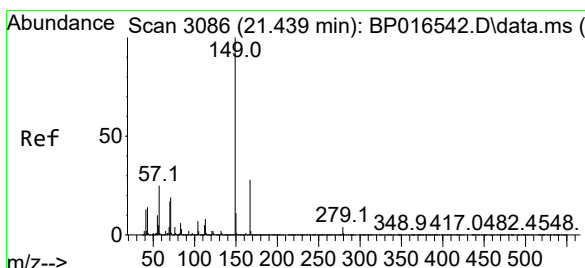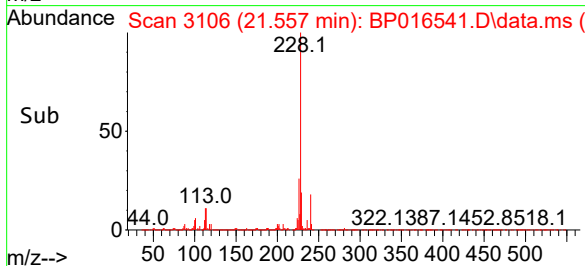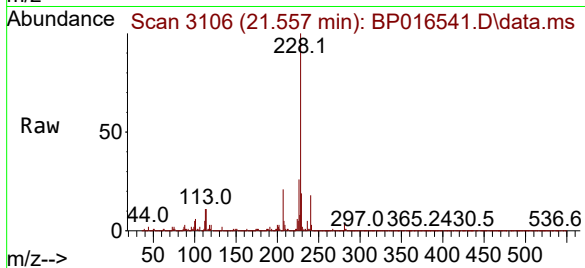

#86

Bis(2-ethylhexyl)phthalate

Concen: 8.169 ng/ul

RT: 21.439 min Scan# 3086

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:149 Resp: 502421


Ion Ratio Lower Upper

149 100

167 27.3 22.1 33.1

279 4.0 3.2 4.8

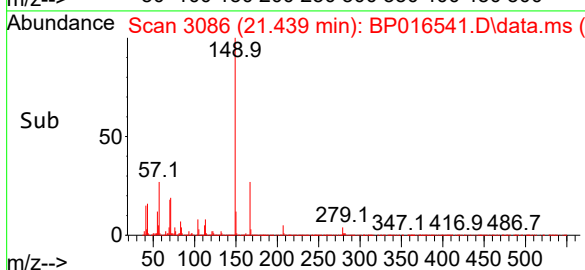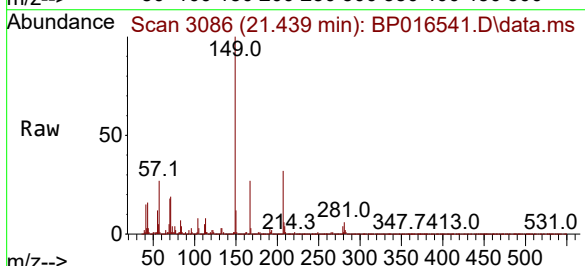



#87

Chrysene

Concen: 9.794 ng/ul

RT: 21.616 min Scan# 3116

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:228 Resp: 992757

Ion Ratio Lower Upper

228 100

226 29.5 24.2 36.4

229 19.6 16.0 24.0



#89

Di-n-octyl phthalate

Concen: 8.820 ng/ul




RT: 22.427 min Scan# 3254


Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Tgt Ion:149 Resp: 840365





#90

Benzo(b)fluoranthene

Concen: 9.377 ng/ul

RT: 23.357 min Scan# 3412

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:252 Resp: 951249

Ion Ratio Lower Upper

252 100

253 22.5 17.6 26.4

125 11.2 8.6 13.0

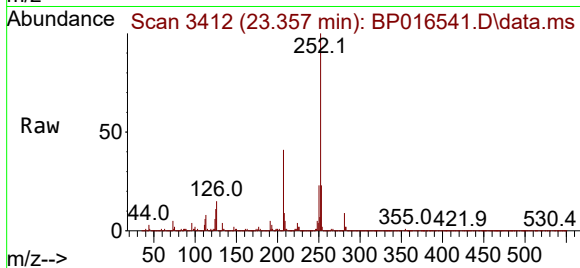

#91

Benzo(k)fluoranthene

Concen: 9.659 ng/ul

RT: 23.410 min Scan# 3421

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:252 Resp: 985160


Ion Ratio Lower Upper

252 100

253 21.9 17.7 26.5

125 11.6 8.8 13.2

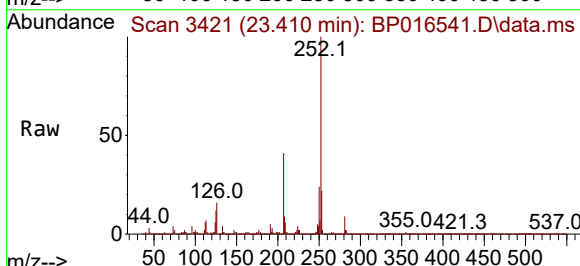



#93

Benzo(a)pyrene

Concen: 9.445 ng/ul

RT: 24.045 min Scan# 3529

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51

Instrument :

BNA_P

ClientSampleId :

SSTD010619





Tgt Ion:252 Resp: 897607

Ion Ratio Lower Upper

252 100

253 22.8 18.0 27.0

125 12.2 10.0 15.0



#94

Indeno(1,2,3-cd)pyrene

Concen: 9.320 ng/ul

RT: 26.915 min Scan# 4017

Delta R.T. -0.000 min

Lab File: BP016541.D

Acq: 10 Aug 2023 10:51




Tgt Ion:276 Resp: 1027968


Ion Ratio Lower Upper

276 100

138 24.9 18.6 27.8

277 23.3 19.7 29.5









#95
 Dibenzo(a,h)anthracene
 Concen: 9.412 ng/ul
 RT: 26.945 min Scan# 4023
 Delta R.T. -0.006 min
 Lab File: BP016541.D
 Acq: 10 Aug 2023 10:51

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010619

Tgt Ion:278 Resp: 864721
 Ion Ratio Lower Upper
 278 100
 139 17.1 13.9 20.9
 279 23.5 18.8 28.2



#96
 Benzo(g,h,i)perylene
 Concen: 9.378 ng/ul
 RT: 27.774 min Scan# 4163
 Delta R.T. -0.006 min
 Lab File: BP016541.D
 Acq: 10 Aug 2023 10:51

Tgt Ion:276 Resp: 815596
 Ion Ratio Lower Upper
 276 100
 138 23.1 18.3 27.5
 277 23.6 19.1 28.7

