

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016550.D
 Acq On : 10 Aug 2023 15:59
 Operator : MA/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020679

Quant Time: Aug 11 03:41:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 11 03:00:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	443925	20.000	ng/u1	0.00
20) Naphthalene-d8	10.893	136	1950016	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.710	164	1215889	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.481	188	2676444	20.000	ng/u1	0.00
79) Chrysene-d12	21.574	240	2496860	20.000	ng/u1	0.00
88) Perylene-d12	24.163	264	2760906	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	94682	8.286	ng/uL	0.00
4) Pyridine-d5	3.834	84	671211	21.081	ng/u1	0.00
7) Phenol-d5	7.199	99	781334	21.173	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	494014	21.762	ng/u1	0.00
11) 2-Chlorophenol-d4	7.581	132	618930	21.605	ng/u1	0.00
15) 4-Methylphenol-d8	8.763	113	642691	21.737	ng/u1	0.00
21) Nitrobenzene-d5	9.257	128	305279	21.848	ng/u1	0.00
24) 2-Nitrophenol-d4	9.975	143	298167	21.996	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.499	165	591436	21.681	ng/u1	0.00
31) 4-Chloroaniline-d4	11.046	131	917120	21.903	ng/u1	0.00
46) Dimethylphthalate-d6	14.122	166	1842591	21.128	ng/u1	0.00
49) Acenaphthylene-d8	14.410	160	2176419	21.723	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	367955	21.521	ng/u1	0.00
60) Fluorene-d10	15.704	176	1585621	21.311	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	255681	20.156	ng/u1	0.00
73) Anthracene-d10	17.581	188	2481963	21.545	ng/u1	0.00
81) Pyrene-d10	19.810	212	2936657	21.361	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.992	264	2831796	21.378	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.434	88	99088	8.272	ng/uL	98
5) Pyridine	3.852	79	693779	21.244	ng/u1	99
6) Benzaldehyde	7.216	77	495424	25.881	ng/u1	95
8) Phenol	7.228	94	824972	21.283	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.493	93	679164	21.450	ng/u1	99
12) 2-Chlorophenol	7.610	128	636963	21.399	ng/u1	97
13) 2-Methylphenol	8.499	108	619271	21.335	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.575	45	865937	22.166	ng/u1	99
16) Acetophenone	8.910	105	1033576	22.572	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.881	70	525221	22.607	ng/u1	98
18) 4-Methylphenol	8.828	108	680218	21.631	ng/u1	98
19) Hexachloroethane	9.140	117	257875	21.013	ng/u1	100
22) Nitrobenzene	9.304	77	771208	21.697	ng/u1	100
23) Isophorone	9.816	82	1448274	21.741	ng/u1	100
25) 2-Nitrophenol	10.010	139	348031	22.253	ng/u1	99
26) 2,4-Dimethylphenol	10.046	107	731276	21.705	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.304	93	929415	21.171	ng/u1	100
29) 2,4-Dichlorophenol	10.528	162	600874	21.583	ng/u1	99
30) Naphthalene	10.946	128	2128816	21.216	ng/u1	99
32) 4-Chloroaniline	11.075	127	906235	22.011	ng/u1	99
33) Hexachlorobutadiene	11.181	225	369843	21.107	ng/u1	99
34) Caprolactam	11.881	113	204004	21.329	ng/u1	98
35) 4-Chloro-3-methylphenol	12.163	107	675369	22.292	ng/u1	99
36) 2-Methylnaphthalene	12.545	142	1440701	21.517	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016550.D
 Acq On : 10 Aug 2023 15:59
 Operator : MA/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020679

Quant Time: Aug 11 03:41:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 11 03:00:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.763	142	1462741	21.753	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.893	216	728554	20.506	ng/ul	98
40) Hexachlorocyclopentadiene	12.845	237	428395	19.761	ng/ul	99
41) 2,4,6-Trichlorophenol	13.140	196	470665	21.517	ng/ul	98
42) 2,4,5-Trichlorophenol	13.204	196	509351	21.334	ng/ul	99
43) 1,1'-Biphenyl	13.551	154	1891554	20.989	ng/ul	100
44) 2-Chloronaphthalene	13.598	162	1490786	21.037	ng/ul	99
45) 2-Nitroaniline	13.822	65	418237	22.340	ng/ul	98
47) Dimethylphthalate	14.169	163	1866132	21.137	ng/ul	99
48) 2,6-Dinitrotoluene	14.310	165	354693	21.866	ng/ul	96
50) Acenaphthylene	14.440	152	2486931	21.473	ng/ul	100
51) 3-Nitroaniline	14.645	138	385826	22.559	ng/ul	98
52) Acenaphthene	14.775	153	1599525	20.897	ng/ul	100
53) 2,4-Dinitrophenol	14.839	184	160802	18.439	ng/ul	97
55) 4-Nitrophenol	14.922	109	279519	22.188	ng/ul	97
56) Dibenzofuran	15.110	168	2222998	21.189	ng/ul	99
57) 2,4-Dinitrotoluene	15.087	165	525774	22.390	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.322	232	430127	21.791	ng/ul	98
59) Diethylphthalate	15.528	149	1873363	21.428	ng/ul	99
61) Fluorene	15.763	166	1804793	21.315	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.751	204	873901	21.031	ng/ul	100
63) 4-Nitroaniline	15.810	138	375143	24.273	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.839	198	292682	20.972	ng/ul	98
67) N-Nitrosodiphenylamine	15.975	169	1540381	21.165	ng/ul	100
68) 4-Bromophenyl-phenylether	16.657	248	543968	21.016	ng/ul	99
69) Hexachlorobenzene	16.739	284	635736	20.903	ng/ul	98
70) Atrazine	16.928	200	559735	21.753	ng/ul	99
71) Pentachlorophenol	17.098	266	381961	20.619	ng/ul	99
72) Phenanthrene	17.522	178	2923214	21.155	ng/ul	100
74) Anthracene	17.616	178	2973602	21.566	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.504	216	771351	20.600	ng/ul	99
76) Pentachlorobenzene	15.004	250	697623	20.722	ng/ul	99
77) Carbazole	17.892	167	2729118	22.846	ng/ul	99
78) Di-n-butylphthalate	18.404	149	3281769	22.425	ng/ul	99
80) Fluoranthene	19.480	202	3435367	21.053	ng/ul	99
82) Pyrene	19.839	202	3582015	21.097	ng/ul	100
83) Butylbenzylphthalate	20.692	149	1462939	22.074	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.492	252	1182020	21.808	ng/ul	99
85) Benzo(a)anthracene	21.557	228	3549854	21.236	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.439	149	2080990	22.163	ng/ul	100
87) Chrysene	21.616	228	3296296	21.299	ng/ul	100
89) Di-n-octyl phthalate	22.427	149	3561864	23.257	ng/ul	100
90) Benzo(b)fluoranthene	23.351	252	3427039	21.016	ng/ul	100
91) Benzo(k)fluoranthene	23.410	252	3458670	21.095	ng/ul	100
93) Benzo(a)pyrene	24.045	252	3256727	21.318	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.915	276	3730665	21.043	ng/ul	99
95) Dibenzo(a,h)anthracene	26.945	278	3118781	21.119	ng/ul	99
96) Benzo(g,h,i)perylene	27.780	276	2918005	20.873	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed

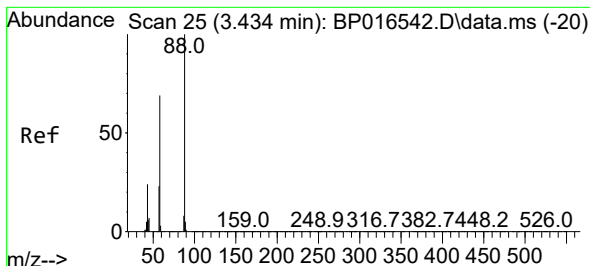

#2
 1,4-Dioxane
 Concen: 8.272 ng/uL
 RT: 3.434 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP016550.D
 Acq: 10 Aug 2023 15:59




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020679


Tgt Ion: 88 Resp: 99088
 Ion Ratio Lower Upper
 88 100
 43 26.3 20.1 30.1
 58 67.5 55.1 82.7

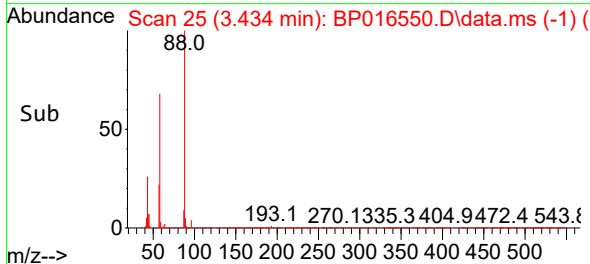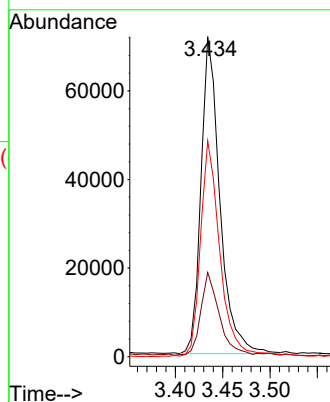

#5
 Pyridine
 Concen: 21.244 ng/uL
 RT: 3.852 min Scan# 96
 Delta R.T. -0.000 min
 Lab File: BP016550.D
 Acq: 10 Aug 2023 15:59

Tgt Ion: 79 Resp: 693779
 Ion Ratio Lower Upper
 79 100
 52 67.3 52.9 79.3
 51 31.5 24.6 37.0




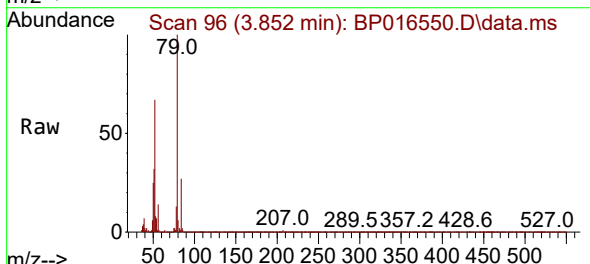




#6
Benzaldehyde
Concen: 25.881 ng/ul
RT: 7.216 min Scan# 60
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion: 77 Resp: 495424
Ion Ratio Lower Upper
77 100
105 95.0 79.6 119.4
106 91.0 76.5 114.7

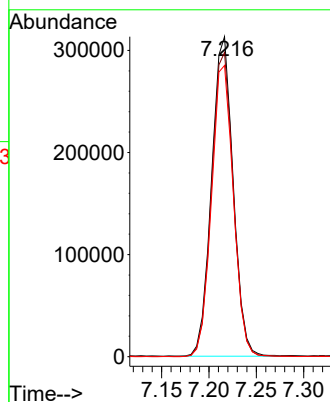

#8
Phenol
Concen: 21.283 ng/ul
RT: 7.228 min Scan# 670
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion: 94 Resp: 824972
Ion Ratio Lower Upper
94 100
65 26.1 20.7 31.1
66 33.8 26.7 40.1









#10
Bis(2-Chloroethyl)ether
Concen: 21.450 ng/ul
RT: 7.493 min Scan# 715
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion: 93 Resp: 679164
Ion Ratio Lower Upper
93 100
63 72.3 57.0 85.6
95 32.4 26.0 39.0



#12
2-Chlorophenol
Concen: 21.399 ng/ul
RT: 7.610 min Scan# 735
Delta R.T. -0.006 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:128 Resp: 636963
Ion Ratio Lower Upper
128 100
64 46.2 34.7 52.1
130 32.3 25.9 38.9



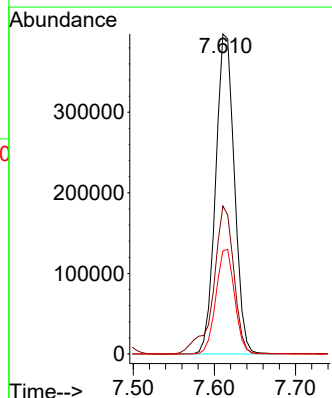





#13
2-Methylphenol
Concen: 21.335 ng/ul
RT: 8.499 min Scan# 886
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:108 Resp: 619271
Ion Ratio Lower Upper
108 100
107 89.5 71.9 107.9

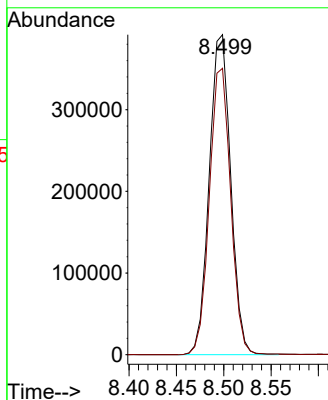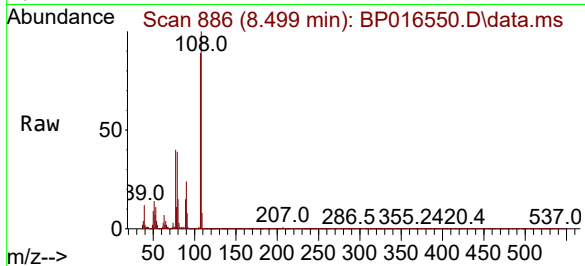

#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.166 ng/ul
RT: 8.575 min Scan# 899
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion: 45 Resp: 865937
Ion Ratio Lower Upper
45 100
77 16.8 12.9 19.3
79 11.6 9.2 13.8



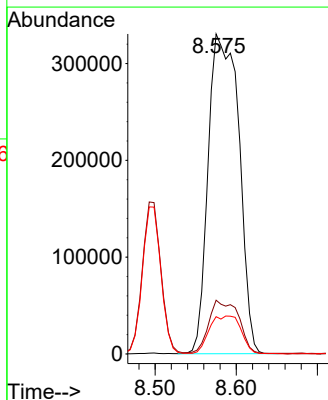
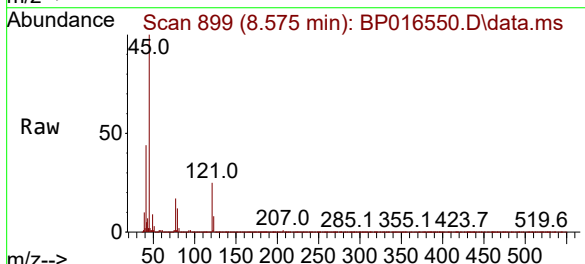




#16
Acetophenone
Concen: 22.572 ng/ul
RT: 8.910 min Scan# 910
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:105 Resp: 1033576
Ion Ratio Lower Upper
105 100
77 77.3 61.0 91.4
51 24.0 18.7 28.1



#17
N-Nitroso-di-n-propylamine
Concen: 22.607 ng/ul
RT: 8.881 min Scan# 951
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion: 70 Resp: 525221
Ion Ratio Lower Upper
70 100
42 51.6 39.9 59.9
101 10.0 7.9 11.9
130 19.5 16.6 25.0









#18
4-Methylphenol
Concen: 21.631 ng/ul
RT: 8.828 min Scan# 942
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:108 Resp: 680218
Ion Ratio Lower Upper
108 100
107 114.0 89.5 134.3



#19
Hexachloroethane
Concen: 21.013 ng/ul
RT: 9.140 min Scan# 995
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:117 Resp: 257875
Ion Ratio Lower Upper
117 100
201 96.9 77.2 115.8
199 61.4 49.2 73.8









#22
Nitrobenzene
Concen: 21.697 ng/ul
RT: 9.304 min Scan# 1023
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion: 77 Resp: 771208
Ion Ratio Lower Upper
77 100
123 45.5 36.4 54.6
65 12.4 10.3 15.5



#23
Isophorone
Concen: 21.741 ng/ul
RT: 9.816 min Scan# 1110
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion: 82 Resp: 1448274
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.0
138 16.8 13.6 20.4









#25
2-Nitrophenol
Concen: 22.253 ng/ul
RT: 10.010 min Scan# 1143
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:139 Resp: 348031
Ion Ratio Lower Upper
139 100
65 48.6 38.9 58.3
109 30.1 23.1 34.7



#26
2,4-Dimethylphenol
Concen: 21.705 ng/ul
RT: 10.046 min Scan# 1149
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:107 Resp: 731276
Ion Ratio Lower Upper
107 100
121 50.1 40.2 60.4
122 85.2 69.2 103.8


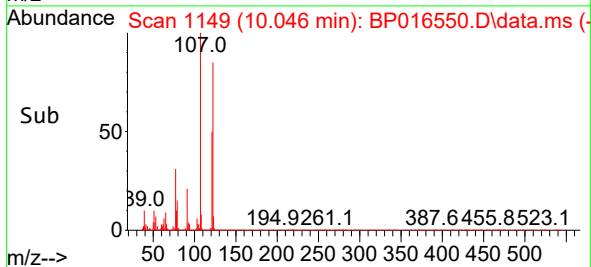

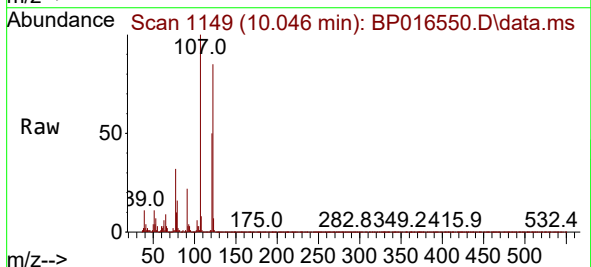


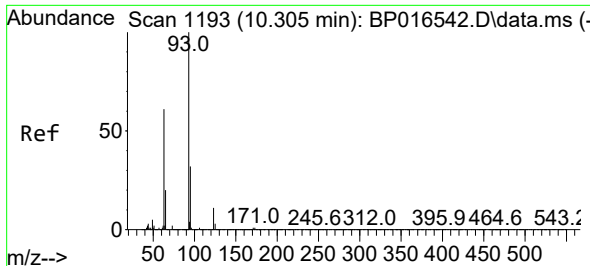

#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.171 ng/ul
 RT: 10.304 min Scan# 1193
 Delta R.T. -0.000 min
 Lab File: BP016550.D
 Acq: 10 Aug 2023 15:59




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020679


Tgt Ion: 93 Resp: 929415
 Ion Ratio Lower Upper
 93 100
 95 32.6 26.0 39.0
 123 11.1 9.0 13.6

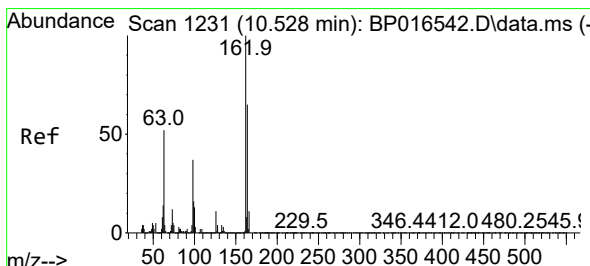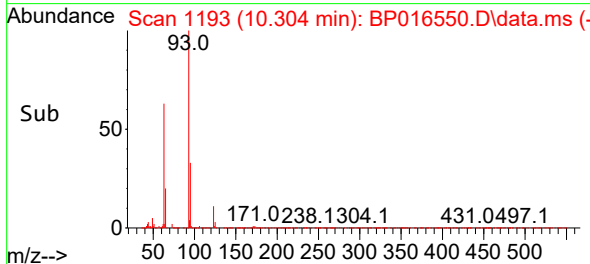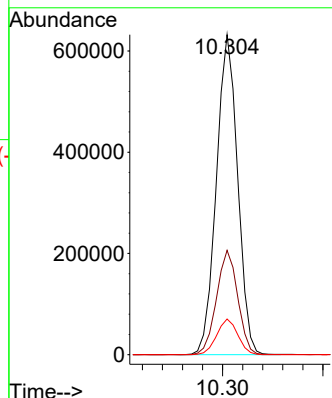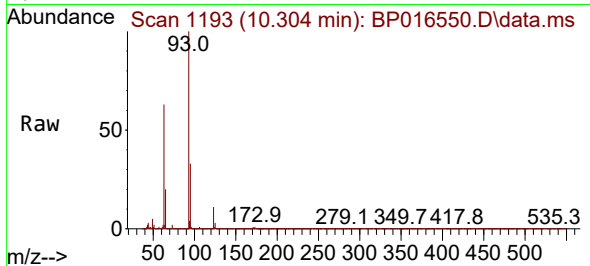

#29
 2,4-Dichlorophenol
 Concen: 21.583 ng/ul
 RT: 10.528 min Scan# 1231
 Delta R.T. -0.000 min
 Lab File: BP016550.D
 Acq: 10 Aug 2023 15:59

Tgt Ion:162 Resp: 600874
 Ion Ratio Lower Upper
 162 100
 164 65.1 52.5 78.7
 98 37.8 29.4 44.2




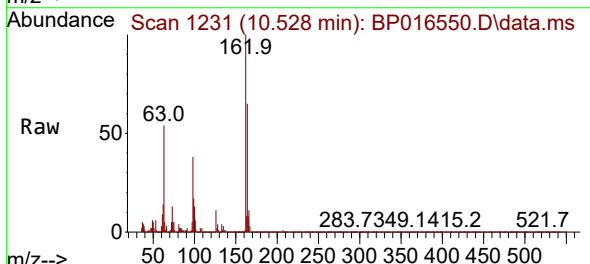




#30
Naphthalene
Concen: 21.216 ng/ul
RT: 10.946 min Scan# 1302
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:128 Resp: 2128816
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 12.9 10.7 16.1



#32
4-Chloroaniline
Concen: 22.011 ng/ul
RT: 11.075 min Scan# 1324
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:127 Resp: 906235
Ion Ratio Lower Upper
127 100
129 32.5 25.8 38.6






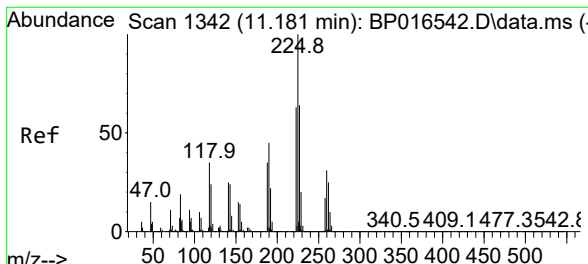


#33
 Hexachlorobutadiene
 Concen: 21.107 ng/ul
 RT: 11.181 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BP016550.D
 Acq: 10 Aug 2023 15:59

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020679

Tgt Ion:225 Resp: 369843




Ion	Ratio	Lower	Upper
225	100		
223	62.9	50.4	75.6
227	63.5	51.5	77.3

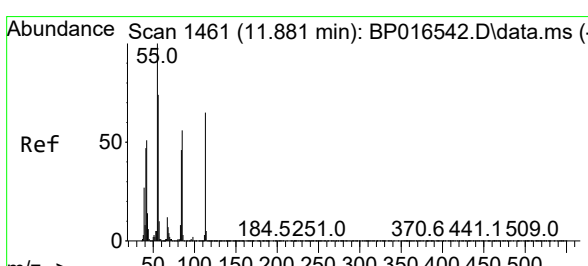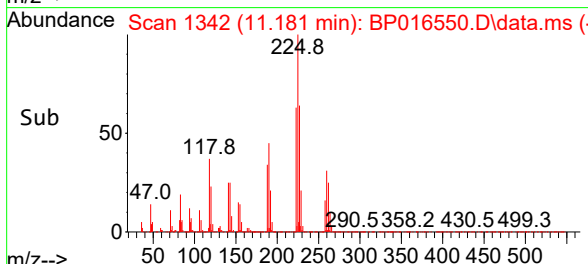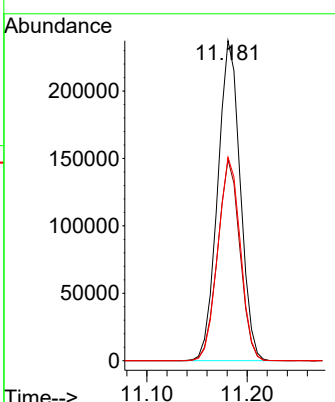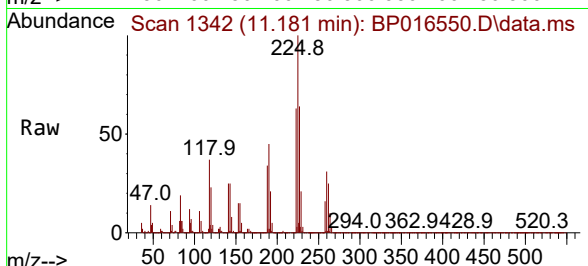


#34
 Caprolactam
 Concen: 21.329 ng/ul
 RT: 11.881 min Scan# 1461
 Delta R.T. -0.000 min
 Lab File: BP016550.D
 Acq: 10 Aug 2023 15:59

Tgt Ion:113 Resp: 204004

Ion	Ratio	Lower	Upper
113	100		
55	155.8	123.0	184.4
56	116.8	90.9	136.3


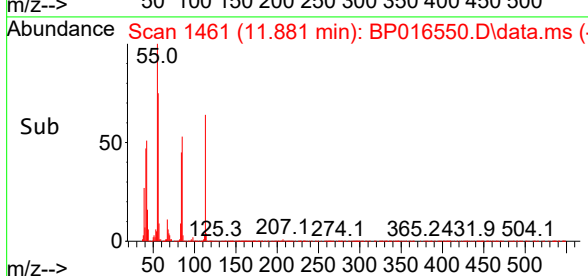
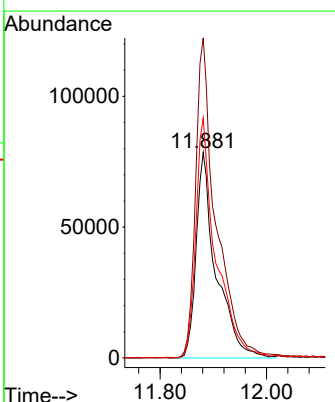
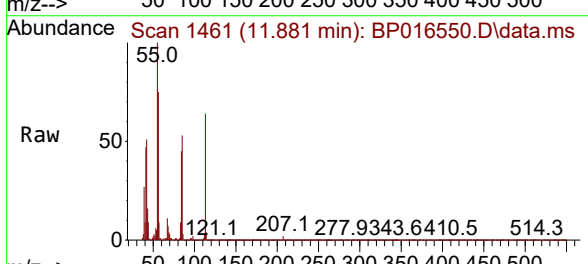




#35
4-Chloro-3-methylphenol
Concen: 22.292 ng/ul
RT: 12.163 min Scan# 1509
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:107 Resp: 675369
Ion Ratio Lower Upper
107 100
144 25.3 20.7 31.1
142 79.6 64.0 96.0

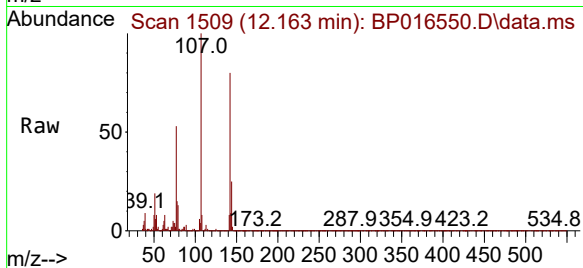

#36
2-Methylnaphthalene
Concen: 21.517 ng/ul
RT: 12.545 min Scan# 1574
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:142 Resp: 1440701
Ion Ratio Lower Upper
142 100
141 89.0 71.7 107.5

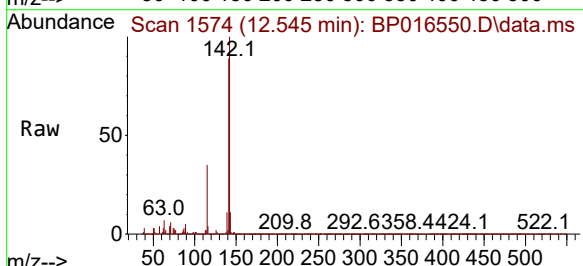



#37

1-Methylnaphthalene

Concen: 21.753 ng/ul

RT: 12.763 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:142 Resp: 1462741

Ion Ratio Lower Upper

142 100

141 92.1 73.2 109.8

116 3.7 3.0 4.4

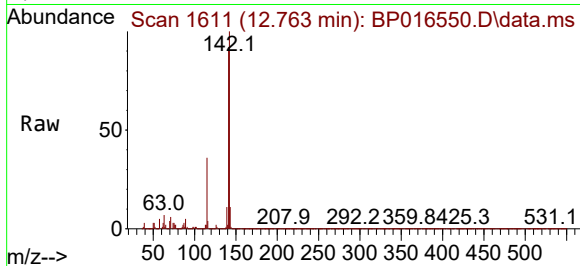

#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.506 ng/ul

RT: 12.893 min Scan# 1633

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Tgt Ion:216 Resp: 728554




Ion Ratio Lower Upper


216 100

214 79.9 62.6 94.0

179 21.1 16.6 25.0

108 18.3 13.8 20.8

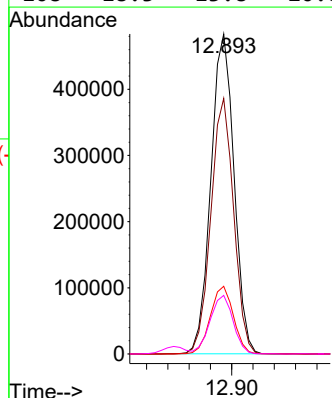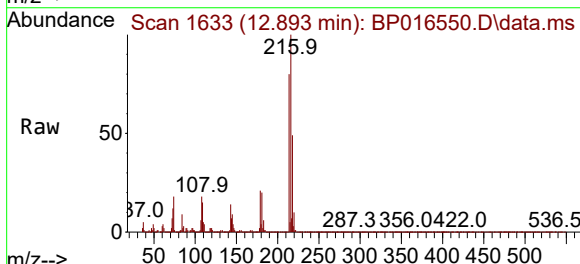



#40

Hexachlorocyclopentadiene

Concen: 19.761 ng/ul

RT: 12.845 min Scan# 1625

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:237 Resp: 428395

Ion Ratio Lower Upper

237 100

235 61.9 49.3 73.9

272 12.8 10.7 16.1



#41

2,4,6-Trichlorophenol

Concen: 21.517 ng/ul

RT: 13.140 min Scan# 1675

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:196 Resp: 470665


Ion Ratio Lower Upper

196 100

198 97.3 76.3 114.5

200 31.0 25.3 37.9









#42
2,4,5-Trichlorophenol
Concen: 21.334 ng/ul
RT: 13.204 min Scan# 1
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:196 Resp: 509351
Ion Ratio Lower Upper
196 100
198 95.6 75.7 113.5
200 30.3 24.6 37.0



#43
1,1'-Biphenyl
Concen: 20.989 ng/ul
RT: 13.551 min Scan# 1745
Delta R.T. 0.006 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:154 Resp: 1891554
Ion Ratio Lower Upper
154 100
153 39.8 31.7 47.5
76 13.7 11.3 16.9



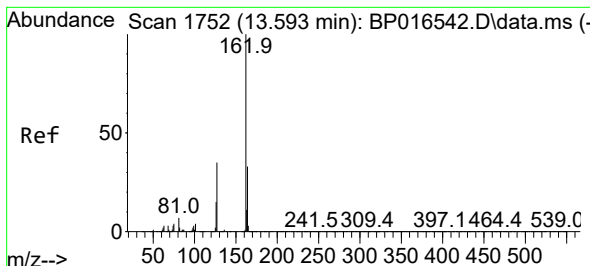

#44

2-Chloronaphthalene

Concen: 21.037 ng/ul

RT: 13.598 min Scan# 1752

Delta R.T. 0.006 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:162 Resp: 1490786

Ion Ratio Lower Upper

162 100

164 33.1 26.6 40.0

127 38.3 31.2 46.8

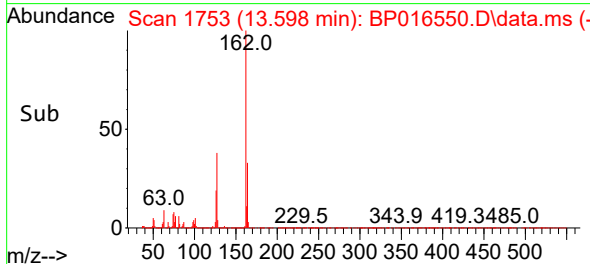

#45

2-Nitroaniline

Concen: 22.340 ng/ul

RT: 13.822 min Scan# 1791

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion: 65 Resp: 418237


Ion Ratio Lower Upper

65 100

92 74.2 58.0 87.0

138 108.9 88.6 132.8


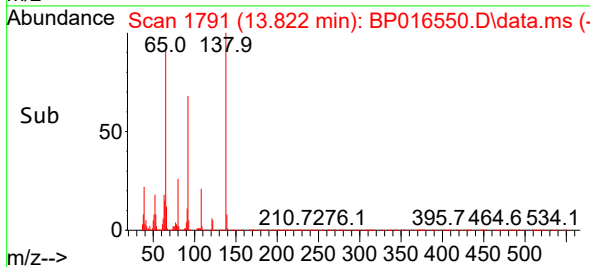

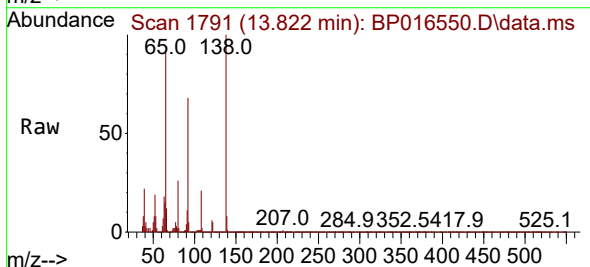




#47
Dimethylphthalate
Concen: 21.137 ng/ul
RT: 14.169 min Scan# 1850
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:163 Resp: 1866132
Ion Ratio Lower Upper
163 100
194 4.1 3.2 4.8
164 10.4 8.1 12.1

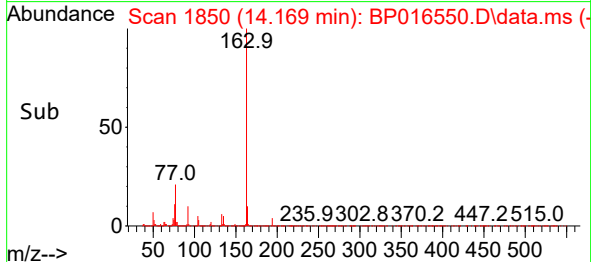

#48
2,6-Dinitrotoluene
Concen: 21.866 ng/ul
RT: 14.310 min Scan# 1874
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:165 Resp: 354693
Ion Ratio Lower Upper
165 100
89 61.1 46.4 69.6
121 22.7 16.8 25.2









#50
Acenaphthylene
Concen: 21.473 ng/ul
RT: 14.440 min Scan# 1896
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:152 Resp: 2486931
Ion Ratio Lower Upper
152 100
151 19.4 15.7 23.5
153 13.4 10.6 16.0



#51
3-Nitroaniline
Concen: 22.559 ng/ul
RT: 14.645 min Scan# 1931
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:138 Resp: 385826
Ion Ratio Lower Upper
138 100
108 11.3 9.4 14.2
92 121.5 95.0 142.6









#52
Acenaphthene
Concen: 20.897 ng/ul
RT: 14.775 min Scan# 1953
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:153 Resp: 1599525
Ion Ratio Lower Upper
153 100
152 47.6 38.6 58.0
154 88.8 71.0 106.6



#53
2,4-Dinitrophenol
Concen: 18.439 ng/ul
RT: 14.839 min Scan# 1964
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:184 Resp: 160802
Ion Ratio Lower Upper
184 100
63 69.3 54.3 81.5
154 60.5 50.7 76.1









#55
4-Nitrophenol
Concen: 22.188 ng/ul
RT: 14.922 min Scan# 1978
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:109 Resp: 279519
Ion Ratio Lower Upper
109 100
139 138.9 109.4 164.0
65 137.7 105.4 158.2



#56
Dibenzofuran
Concen: 21.189 ng/ul
RT: 15.110 min Scan# 2010
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:168 Resp: 2222998
Ion Ratio Lower Upper
168 100
139 37.2 29.4 44.0









#57
2,4-Dinitrotoluene
Concen: 22.390 ng/ul
RT: 15.087 min Scan# 2006
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:165 Resp: 525774
Ion Ratio Lower Upper
165 100
63 45.1 35.3 52.9
182 2.8 2.0 3.0



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.791 ng/ul
RT: 15.322 min Scan# 2046
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:232 Resp: 430127
Ion Ratio Lower Upper
232 100
131 48.6 37.2 55.8
130 2.3 1.9 2.9
166 32.7 26.2 39.4


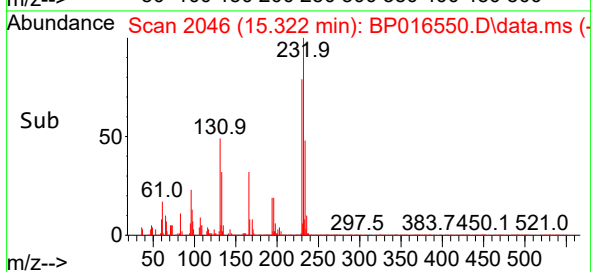






#59
Diethylphthalate
Concen: 21.428 ng/ul
RT: 15.528 min Scan# 2081
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:149 Resp: 1873363
Ion Ratio Lower Upper
149 100
177 22.3 18.2 27.2
150 12.5 9.8 14.8



#61
Fluorene
Concen: 21.315 ng/ul
RT: 15.763 min Scan# 2121
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:166 Resp: 1804793
Ion Ratio Lower Upper
166 100
165 97.5 77.3 115.9
167 13.0 10.7 16.1



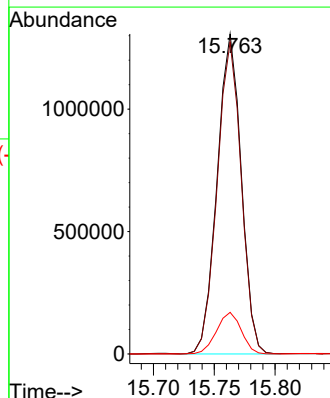





#62
4-Chlorophenyl-phenylether
Concen: 21.031 ng/ul
RT: 15.751 min Scan# 2119
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:204 Resp: 873901
Ion Ratio Lower Upper
204 100
206 33.2 26.4 39.6
141 60.5 48.6 73.0



#63
4-Nitroaniline
Concen: 24.273 ng/ul
RT: 15.810 min Scan# 2129
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:138 Resp: 375143
Ion Ratio Lower Upper
138 100
92 54.8 42.2 63.4
108 85.7 64.0 96.0



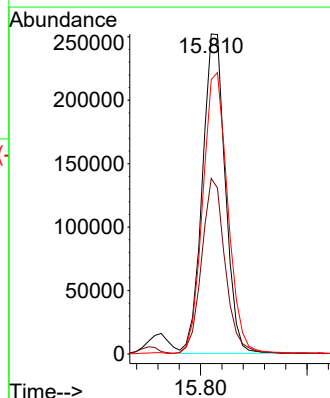





#66
4,6-Dinitro-2-methylphenol
Concen: 20.972 ng/ul
RT: 15.839 min Scan# 2134
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:198 Resp: 292682
Ion Ratio Lower Upper
198 100
182 4.0 3.8 5.8
77 26.7 20.5 30.7

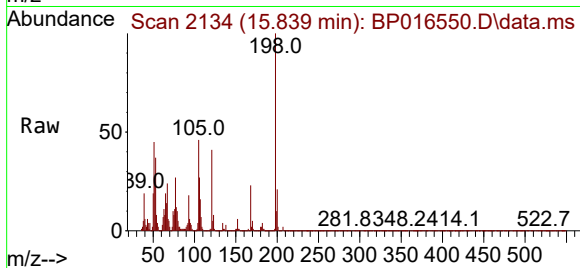

#67
N-Nitrosodiphenylamine
Concen: 21.165 ng/ul
RT: 15.975 min Scan# 2157
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:169 Resp: 1540381
Ion Ratio Lower Upper
169 100
168 66.3 53.0 79.6
167 36.4 29.0 43.6



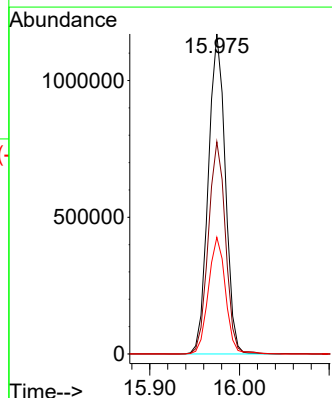
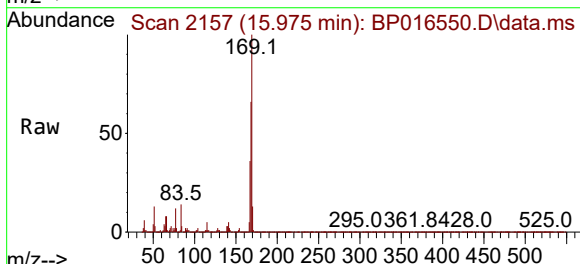




#68
4-Bromophenyl-phenylether
Concen: 21.016 ng/ul
RT: 16.657 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:248 Resp: 543968
Ion Ratio Lower Upper
248 100
250 98.6 78.2 117.4
141 72.4 58.4 87.6



#69
Hexachlorobenzene
Concen: 20.903 ng/ul
RT: 16.739 min Scan# 2287
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:284 Resp: 635736
Ion Ratio Lower Upper
284 100
142 33.9 28.6 42.8
249 31.2 24.6 37.0





#70

Atrazine

Concen: 21.753 ng/ul

RT: 16.928 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:200 Resp: 559735

Ion Ratio Lower Upper

200 100

173 28.1 21.4 32.2

215 48.0 38.0 57.0

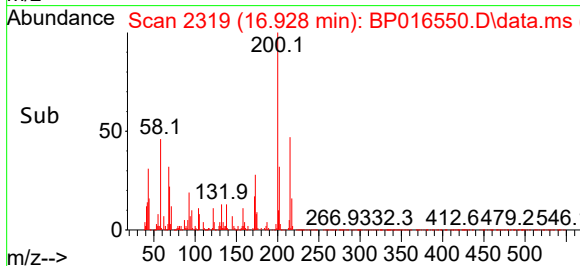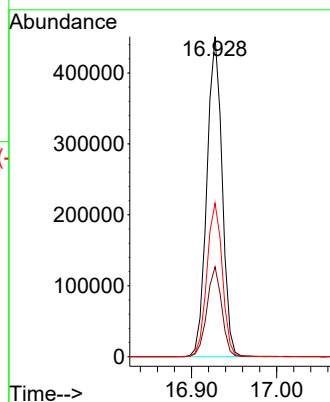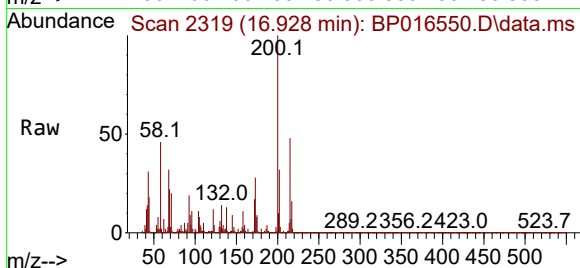

#71

Pentachlorophenol

Concen: 20.619 ng/ul

RT: 17.098 min Scan# 2348

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:266 Resp: 381961


Ion Ratio Lower Upper

266 100

264 63.1 51.4 77.2

268 64.4 51.6 77.4


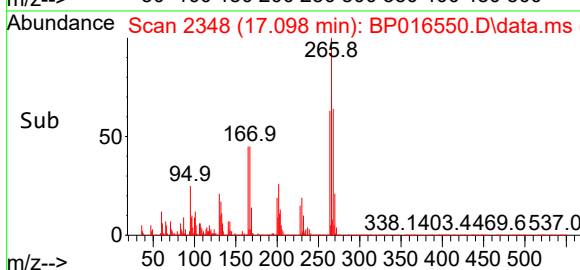

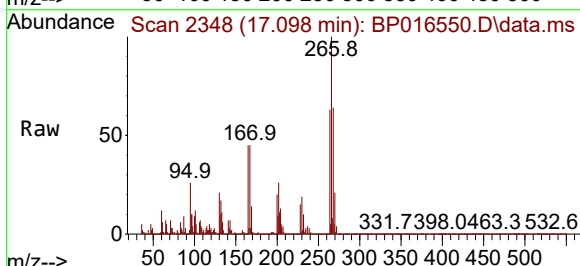




#72
Phenanthrene
Concen: 21.155 ng/ul
RT: 17.522 min Scan# 2420
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:178 Resp: 2923214
Ion Ratio Lower Upper
178 100
179 15.5 12.6 18.8
176 19.3 15.5 23.3



#74
Anthracene
Concen: 21.566 ng/ul
RT: 17.616 min Scan# 2436
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:178 Resp: 2973602
Ion Ratio Lower Upper
178 100
179 15.2 12.3 18.5
176 18.3 15.0 22.4





#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.600 ng/uL

RT: 13.504 min Scan# 1737

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:216 Resp: 771351

Ion Ratio Lower Upper

216 100

214 79.2 61.8 92.8

218 48.6 38.9 58.3

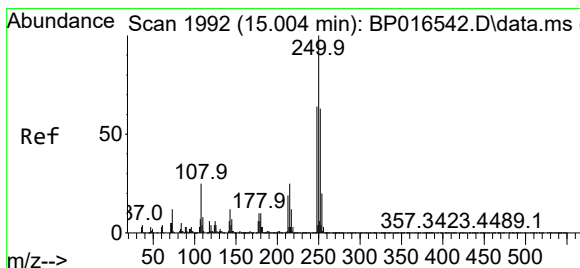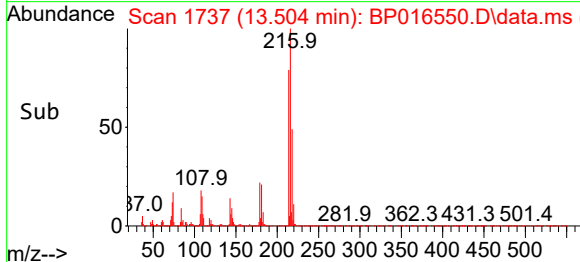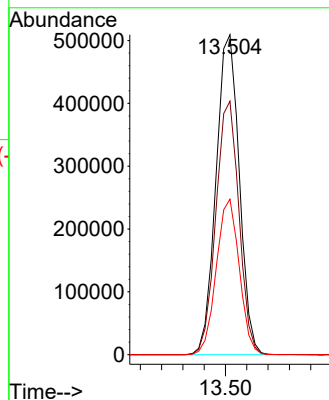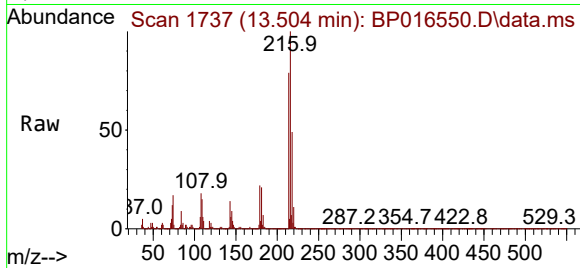

#76

Pentachlorobenzene

Concen: 20.722 ng/uL

RT: 15.004 min Scan# 1992

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:250 Resp: 697623


Ion Ratio Lower Upper

250 100

248 63.3 51.2 76.8

252 63.8 50.2 75.2

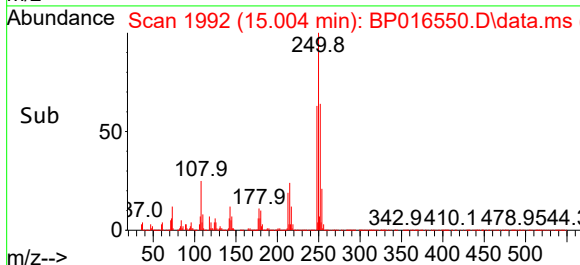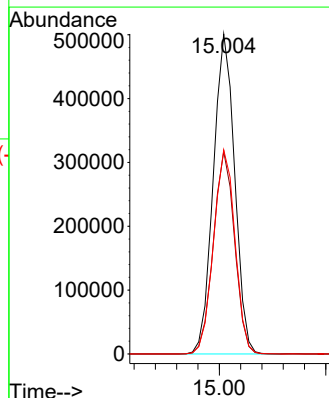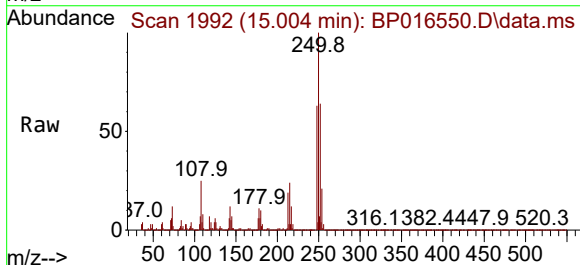



#77

Carbazole

Concen: 22.846 ng/ul

RT: 17.892 min Scan# 2483

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:167 Resp: 2729118

Ion Ratio Lower Upper

167 100

166 21.5 17.0 25.6

139 13.1 10.1 15.1

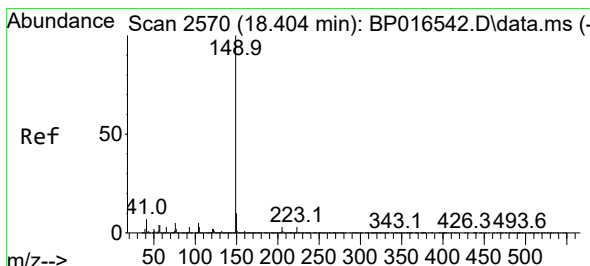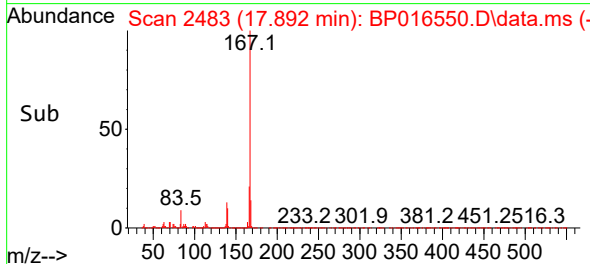

#78

Di-n-butylphthalate

Concen: 22.425 ng/ul

RT: 18.404 min Scan# 2570

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:149 Resp: 3281769


Ion Ratio Lower Upper

149 100

150 9.3 7.6 11.4

104 5.2 4.3 6.5

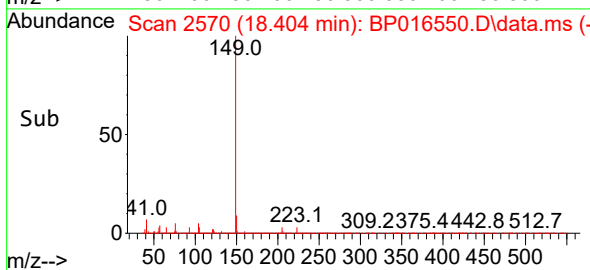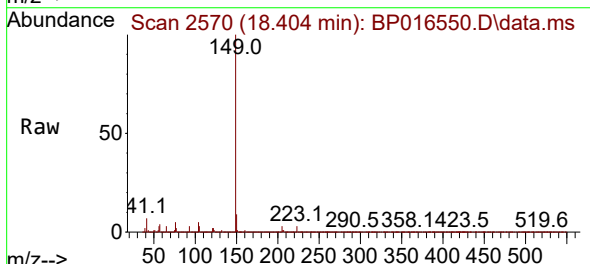



#80

Fluoranthene

Concen: 21.053 ng/ul

RT: 19.480 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:202 Resp: 3435367

Ion Ratio Lower Upper

202 100

101 12.1 9.9 14.9

100 9.2 7.5 11.3



#82

Pyrene

Concen: 21.097 ng/ul

RT: 19.839 min Scan# 2814

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:202 Resp: 3582015


Ion Ratio Lower Upper

202 100

101 14.1 11.3 16.9

100 11.6 9.2 13.8









#83
Butylbenzylphthalate
Concen: 22.074 ng/ul
RT: 20.692 min Scan# 2960
Delta R.T. -0.006 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:149 Resp: 1462939
Ion Ratio Lower Upper
149 100
91 76.3 58.5 87.7
206 19.5 16.5 24.7

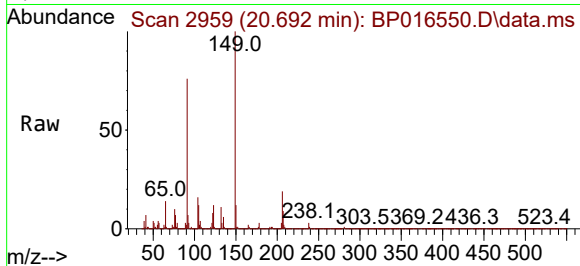

#84
3,3'-Dichlorobenzidine
Concen: 21.808 ng/ul
RT: 21.492 min Scan# 3095
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:252 Resp: 1182020
Ion Ratio Lower Upper
252 100
254 63.9 51.8 77.8
126 11.7 9.7 14.5

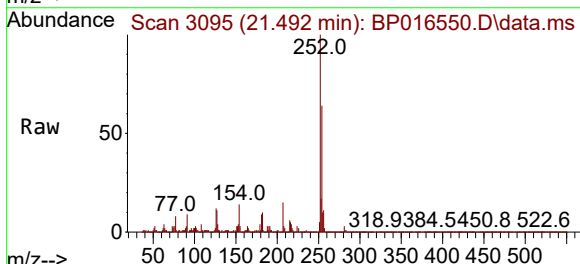



#85

Benzo(a)anthracene

Concen: 21.236 ng/ul

RT: 21.557 min Scan# 3106

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:228 Resp: 3549854

Ion Ratio Lower Upper

228 100

229 19.6 15.6 23.4

226 27.2 21.8 32.6



#86

Bis(2-ethylhexyl)phthalate

Concen: 22.163 ng/ul

RT: 21.439 min Scan# 3086

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:149 Resp: 2080990


Ion Ratio Lower Upper

149 100

167 27.7 22.1 33.1

279 4.4 3.2 4.8







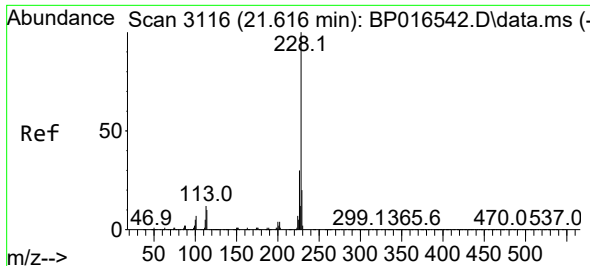

#87
Chrysene
Concen: 21.299 ng/ul
RT: 21.616 min Scan# 3116
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59




Instrument :
BNA_P
ClientSampleId :
SSTD020679


Tgt Ion:228 Resp: 3296296
Ion Ratio Lower Upper
228 100
226 30.5 24.2 36.4
229 19.7 16.0 24.0

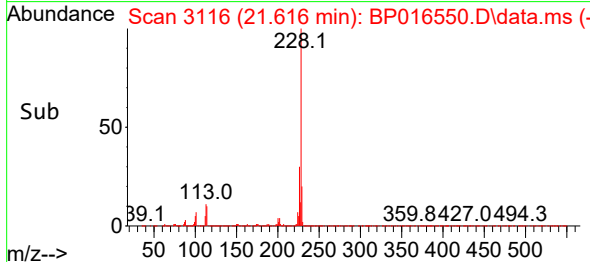

#89
Di-n-octyl phthalate
Concen: 23.257 ng/ul
RT: 22.427 min Scan# 3254
Delta R.T. -0.000 min
Lab File: BP016550.D
Acq: 10 Aug 2023 15:59

Tgt Ion:149 Resp: 3561864

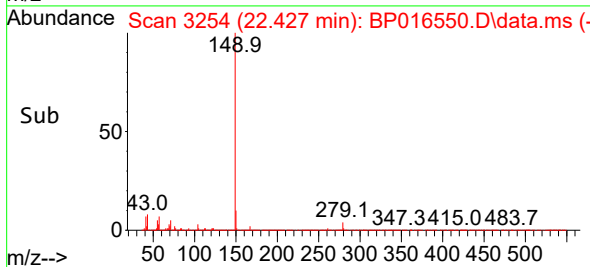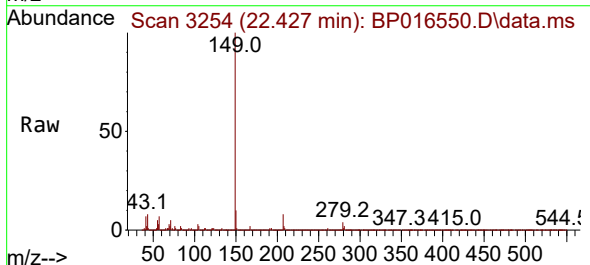



#90

Benzo(b)fluoranthene

Concen: 21.016 ng/ul

RT: 23.351 min Scan# 3412

Delta R.T. -0.006 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:252 Resp: 3427039

Ion Ratio Lower Upper

252 100

253 22.3 17.6 26.4

125 10.8 8.6 13.0



#91

Benzo(k)fluoranthene

Concen: 21.095 ng/ul

RT: 23.410 min Scan# 3421

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:252 Resp: 3458670


Ion Ratio Lower Upper

252 100

253 21.9 17.7 26.5

125 10.8 8.8 13.2





#93

Benzo(a)pyrene

Concen: 21.318 ng/ul

RT: 24.045 min Scan# 3529

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:252 Resp: 3256727

Ion Ratio Lower Upper

252 100

253 22.0 18.0 27.0

125 11.8 10.0 15.0



#94

Indeno(1,2,3-cd)pyrene

Concen: 21.043 ng/ul

RT: 26.915 min Scan# 4017

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59




Tgt Ion:276 Resp: 3730665


Ion Ratio Lower Upper

276 100

138 22.9 18.6 27.8

277 24.3 19.7 29.5

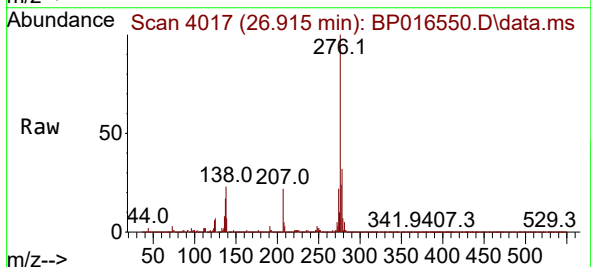



#95

Dibenzo(a,h)anthracene

Concen: 21.119 ng/ul

RT: 26.945 min Scan# 4023

Delta R.T. -0.006 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Instrument :

BNA_P

ClientSampleId :

SSTD020679





Tgt Ion:278 Resp: 3118781

Ion Ratio Lower Upper

278 100

139 17.0 13.9 20.9

279 23.8 18.8 28.2

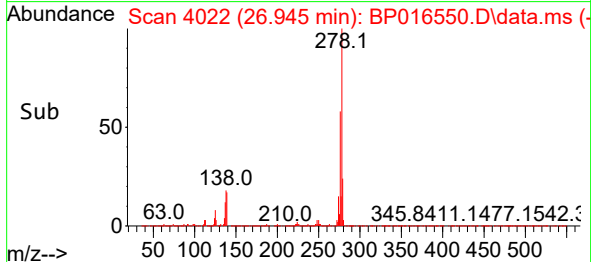

#96

Benzo(g,h,i)perylene

Concen: 20.873 ng/ul

RT: 27.780 min Scan# 4164

Delta R.T. -0.000 min

Lab File: BP016550.D

Acq: 10 Aug 2023 15:59

Tgt Ion:276 Resp: 2918005

Ion Ratio Lower Upper

276 100

138 22.7 18.3 27.5

277 23.1 19.1 28.7

