

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
 Data File : BP016547.D
 Acq On : 10 Aug 2023 14:16
 Operator : MA/JU
 Sample : PB154647BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK647

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	15	19	31	rVB	112868	164371	1.25%	0.114%
2	3.834	89	93	114	rBV	1455885	2369652	18.09%	1.647%
3	4.158	144	148	156	rVB	36210	56482	0.43%	0.039%
4	5.675	399	406	410	rBV7	6715	13115	0.10%	0.009%
5	7.199	657	665	673	rBV	1890726	2912672	22.24%	2.025%
6	7.399	690	699	708	rBV	1574695	2392533	18.27%	1.663%
7	7.581	722	730	739	rBV	1806598	2854877	21.80%	1.985%
8	8.064	804	812	822	rBV	2559505	4107201	31.36%	2.855%
9	8.764	923	931	940	rBV	2268457	3624151	27.67%	2.519%
10	9.258	1007	1015	1026	rBV	1767083	2818442	21.52%	1.959%
11	9.975	1128	1137	1146	rBV	1370004	2184842	16.68%	1.519%
12	10.499	1218	1226	1242	rBV	2164717	3545121	27.07%	2.464%
13	10.893	1285	1293	1302	rBV	3722782	6317875	48.24%	4.392%
14	11.046	1310	1319	1334	rBV	2321326	3887738	29.68%	2.703%
15	12.469	1555	1561	1567	rBV	45596	71416	0.55%	0.050%
16	13.563	1742	1747	1751	rVB5	11341	19061	0.15%	0.013%
17	13.675	1760	1766	1773	rVB7	7385	15026	0.11%	0.010%
18	14.122	1835	1842	1856	rBV	4147102	5701023	43.53%	3.963%
19	14.410	1884	1891	1905	rBV	4674164	6782938	51.79%	4.715%
20	14.710	1935	1942	1956	rBV	5801790	8683981	66.30%	6.037%
21	14.904	1968	1975	1990	rBV	2090860	3066758	23.41%	2.132%
22	15.704	2104	2111	2125	rBV	6003992	8601526	65.67%	5.979%
23	15.822	2125	2131	2146	rVV	1717012	2355775	17.99%	1.638%
24	15.940	2148	2151	2156	rVB2	27346	39464	0.30%	0.027%
25	16.493	2239	2245	2250	rVB8	7310	13337	0.10%	0.009%
26	17.140	2351	2355	2361	rBV8	8480	13458	0.10%	0.009%
27	17.263	2372	2376	2382	rVB	17899	25811	0.20%	0.018%
28	17.481	2405	2413	2423	rBV	7506355	10857724	82.90%	7.548%
29	17.581	2423	2430	2446	rVV	6845016	9755655	74.48%	6.782%
30	18.316	2551	2555	2564	rBV4	62184	118791	0.91%	0.083%
31	19.381	2732	2736	2741	rBV2	91317	119426	0.91%	0.083%
32	19.445	2743	2747	2752	rBV	82887	120864	0.92%	0.084%
33	19.551	2762	2765	2771	rBV7	28680	52490	0.40%	0.036%
34	19.810	2803	2809	2819	rBV	8890820	11917204	90.99%	8.284%
35	21.575	3103	3109	3118	rBV	9313677	12291268	93.84%	8.544%
36	23.992	3512	3520	3531	rBV2	5981561	12881794	98.35%	8.955%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
Data File : BP016547.D
Acq On : 10 Aug 2023 14:16
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
Title : SVOA CALIBRATION

37 24.169 3541 3550 3560 rVB 5890627 13097684 100.00% 9.105%




Sum of corrected areas: 143851546

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
Data File : BP016547.D
Acq On : 10 Aug 2023 14:16
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

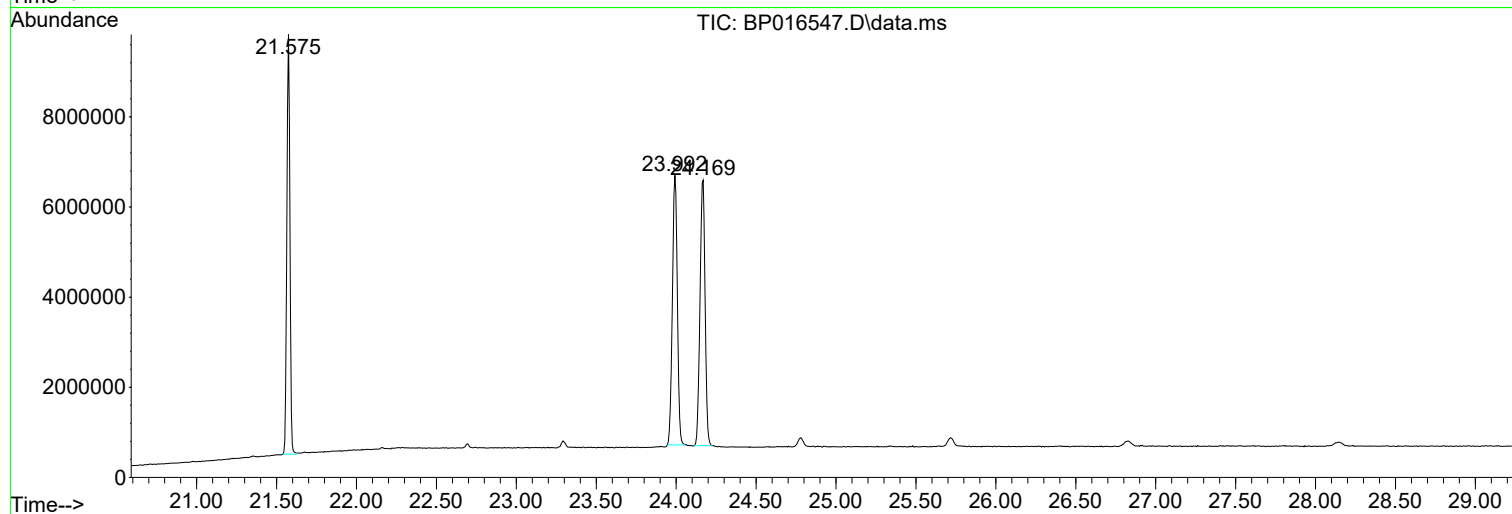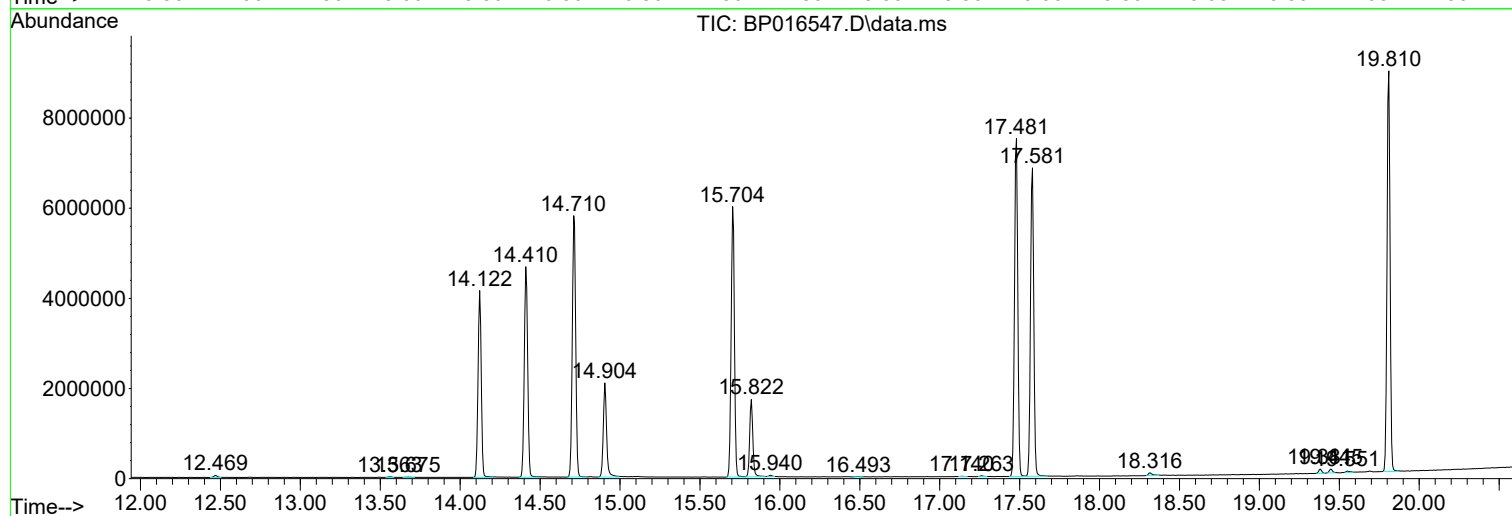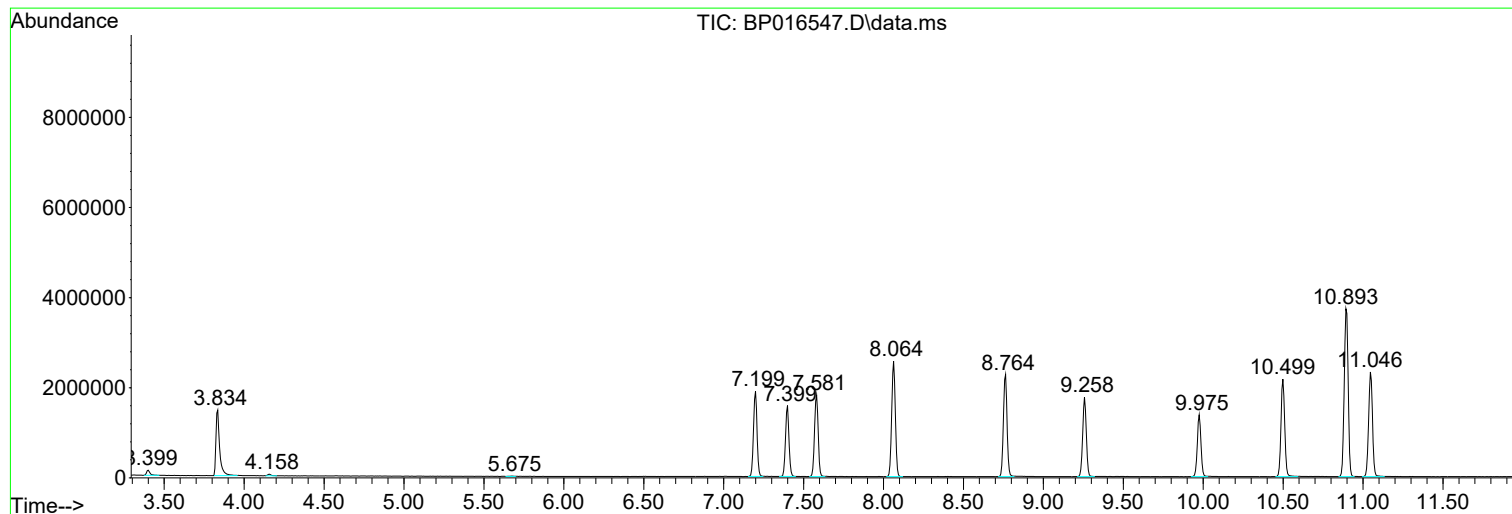

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
Data File : BP016547.D
Acq On : 10 Aug 2023 14:16
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081023\
Data File : BP016547.D
Acq On : 10 Aug 2023 14:16
Operator : MA/JU
Sample : PB154647BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------