
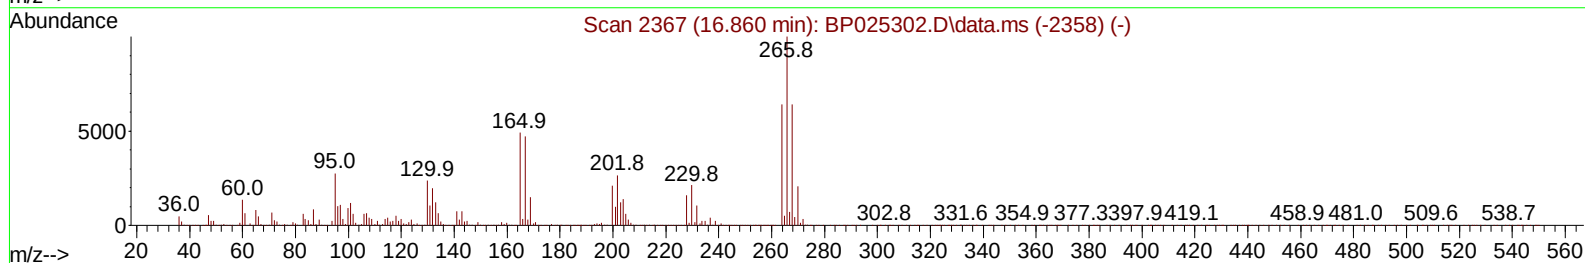
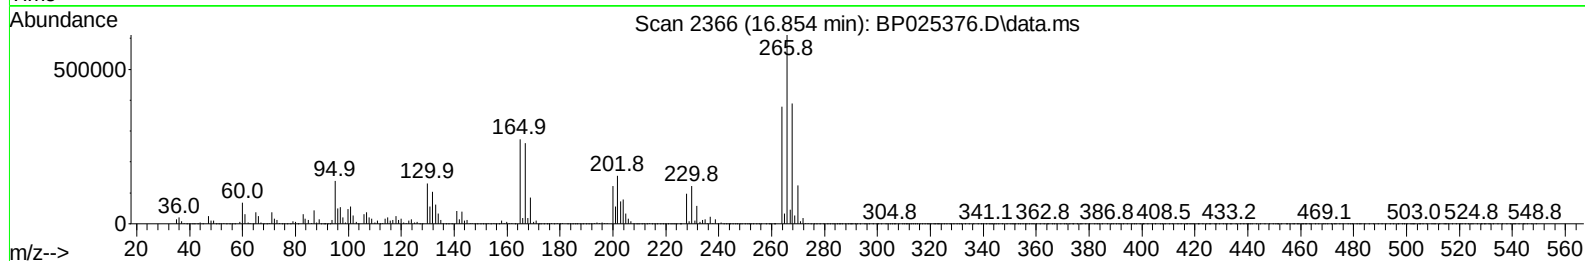


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081325\
Data File : BP025376.D
Acq On : 13 Aug 2025 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 10:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

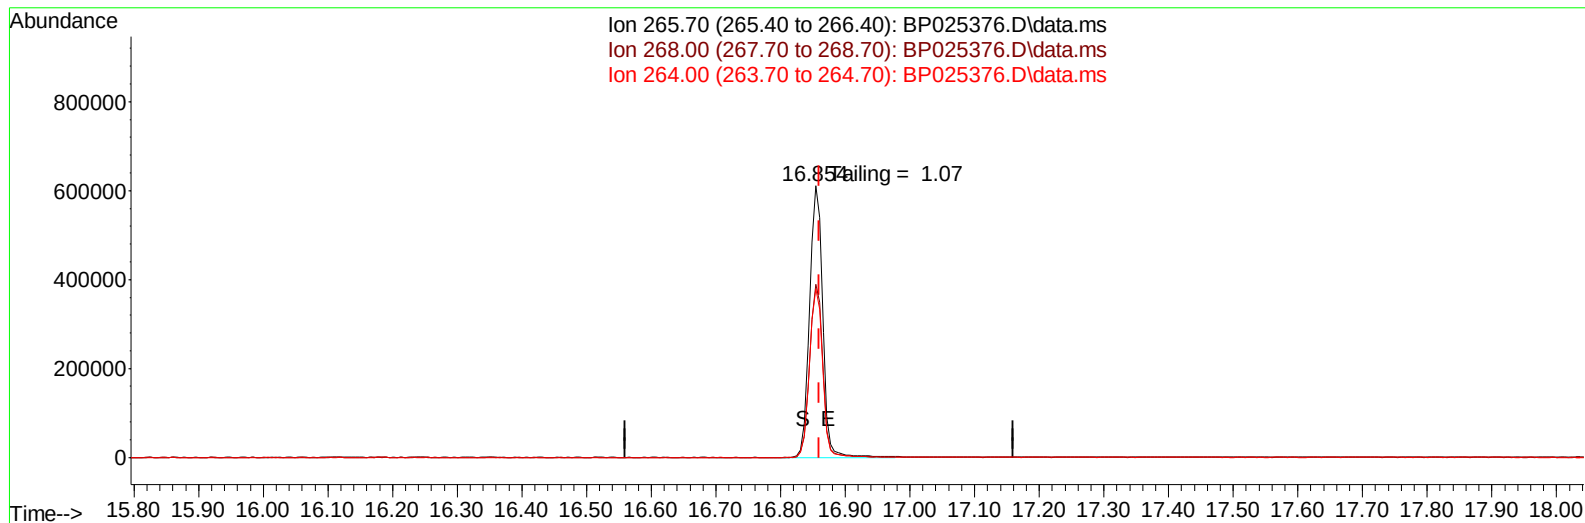

TIC: BP025376.D\data.ms

(70) Pentachlorophenol (C)




16.854min (-0.006) 72054.22 ng

response 872257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.77
264.00	63.90	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081325\
Data File : BP025376.D
Acq On : 13 Aug 2025 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 10:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

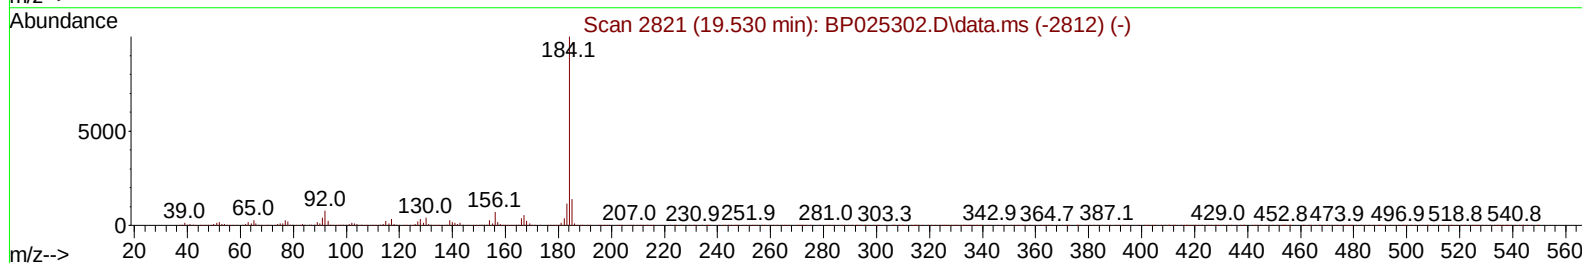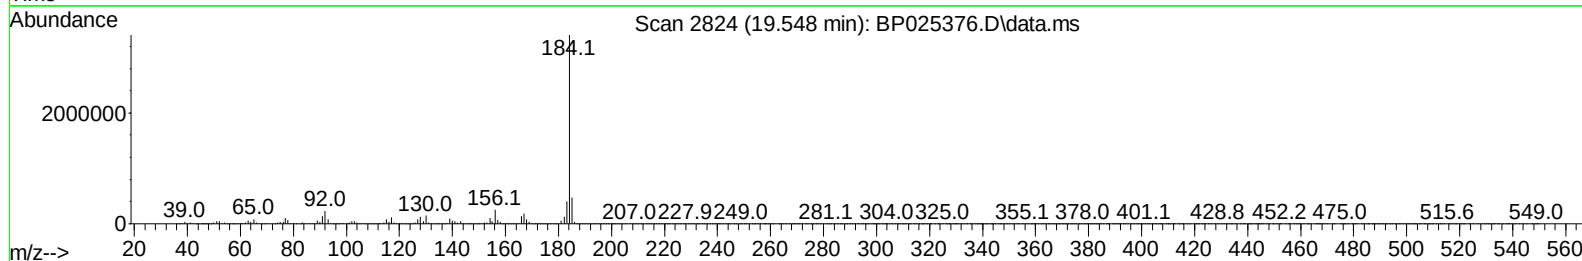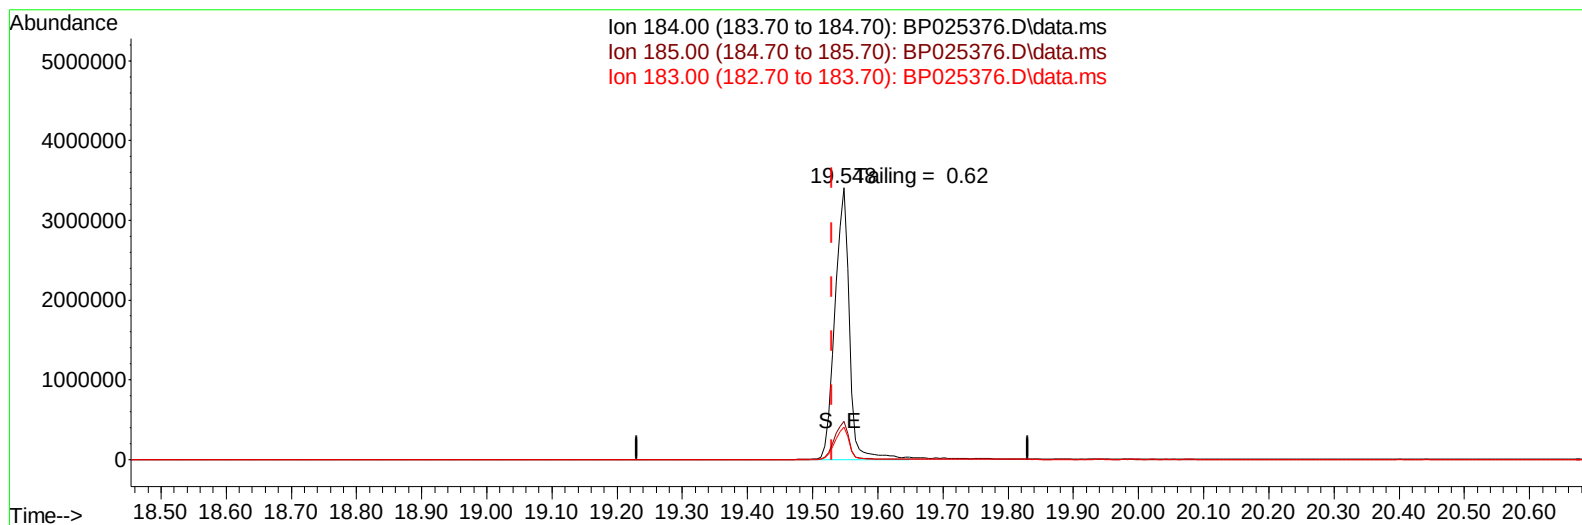

TIC: BP025376.D\data.ms

(77) Benzidine**19.548min (+ 0.018) 57458.25 ng****response 5292761**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.00
183.00	11.50	11.99
0.00	0.00	0.00