

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
 Data File : BP016560.D
 Acq On : 14 Aug 2023 14:25
 Operator : MA/JU
 Sample : PB154773BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK773

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	14	18	30	rVB	77112	121206	1.44%	0.128%
2	3.828	88	92	111	rBV	996638	1737434	20.66%	1.828%
3	4.158	144	148	152	rBV	21928	32584	0.39%	0.034%
4	7.199	658	665	675	rBV	1311459	2096451	24.93%	2.205%
5	7.393	690	698	708	rBV	1073514	1709613	20.33%	1.798%
6	7.575	722	729	742	rBV	1252946	2008752	23.89%	2.113%
7	8.063	804	812	820	rVB	1752830	2767622	32.91%	2.911%
8	8.757	923	930	944	rBV	1584948	2526319	30.04%	2.658%
9	9.257	1006	1015	1025	rBV	1238951	2030717	24.15%	2.136%
10	9.975	1124	1137	1148	rBV	932902	1538411	18.29%	1.618%
11	10.499	1218	1226	1242	rBV	1410980	2392016	28.44%	2.516%
12	10.893	1285	1293	1306	rBV	2646223	4329156	51.48%	4.554%
13	11.046	1310	1319	1333	rBV	1590255	2709516	32.22%	2.850%
14	12.469	1554	1561	1566	rBV2	29924	45892	0.55%	0.048%
15	13.557	1741	1746	1755	rBV2	23544	40489	0.48%	0.043%
16	13.675	1762	1766	1772	rVB8	5460	10877	0.13%	0.011%
17	14.122	1835	1842	1851	rBV	2646026	3762910	44.75%	3.958%
18	14.410	1883	1891	1904	rBV	3121788	4472137	53.18%	4.704%
19	14.710	1935	1942	1955	rBV	4011370	5824569	69.26%	6.127%
20	14.904	1968	1975	1993	rBV	1264055	2005366	23.85%	2.110%
21	15.704	2104	2111	2123	rBV	4059054	5654953	67.25%	5.949%
22	15.816	2125	2130	2146	rVV	995294	1469644	17.48%	1.546%
23	15.939	2147	2151	2160	rVB2	21305	40375	0.48%	0.042%
24	17.263	2371	2376	2382	rBV2	12080	19088	0.23%	0.020%
25	17.475	2406	2412	2422	rBV	5112971	7288816	86.68%	7.667%
26	17.575	2423	2429	2446	rVB2	4475873	6235697	74.15%	6.560%
27	18.322	2553	2556	2557	rBV3	9451	10727	0.13%	0.011%
28	19.380	2732	2736	2741	rVB3	53355	67124	0.80%	0.071%
29	19.445	2744	2747	2750	rVB	42654	51201	0.61%	0.054%
30	19.804	2802	2808	2817	rBV	5690856	7468082	88.81%	7.856%
31	21.569	3103	3108	3115	rBV2	5990607	8141449	96.81%	8.564%
32	23.986	3511	3519	3535	rVB2	3830899	8044208	95.66%	8.462%
33	24.157	3540	3548	3563	rVB	3821678	8409343	100.00%	8.846%




Sum of corrected areas: 95062744

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016560.D
Acq On : 14 Aug 2023 14:25
Operator : MA/JU
Sample : PB154773BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

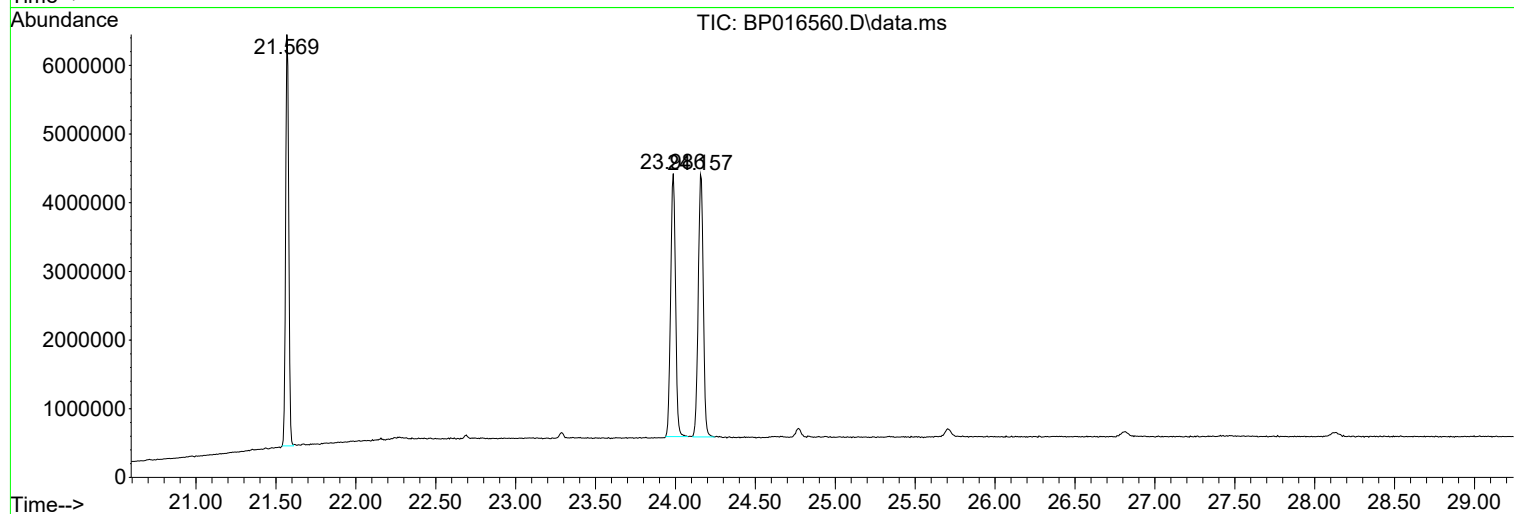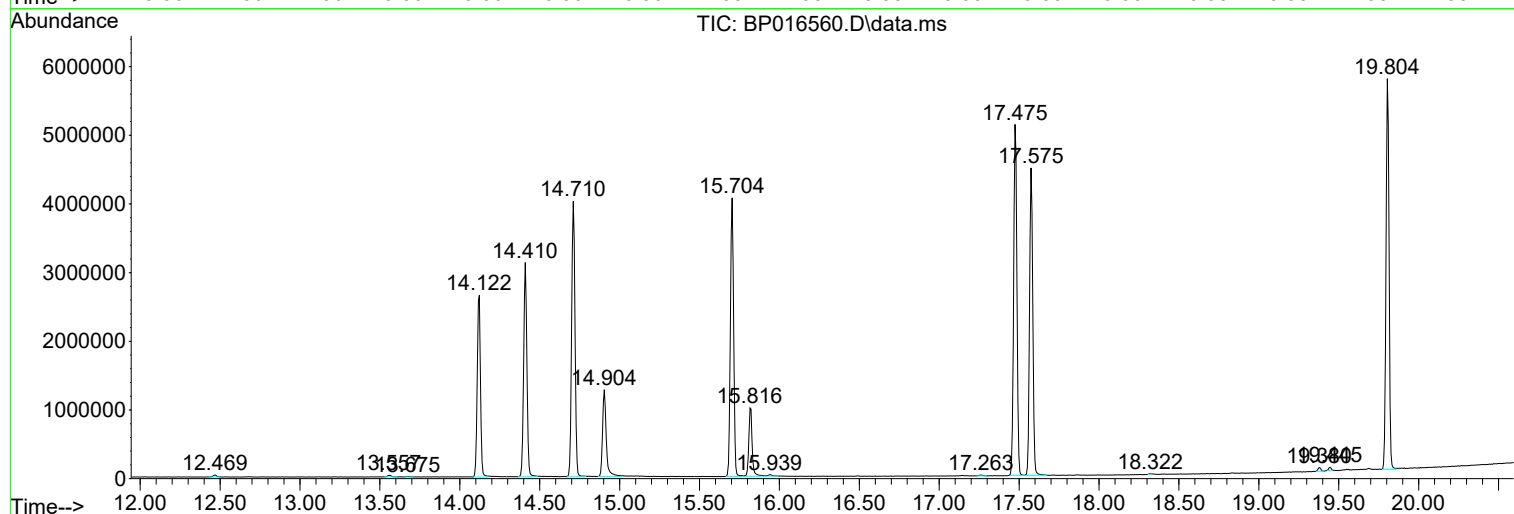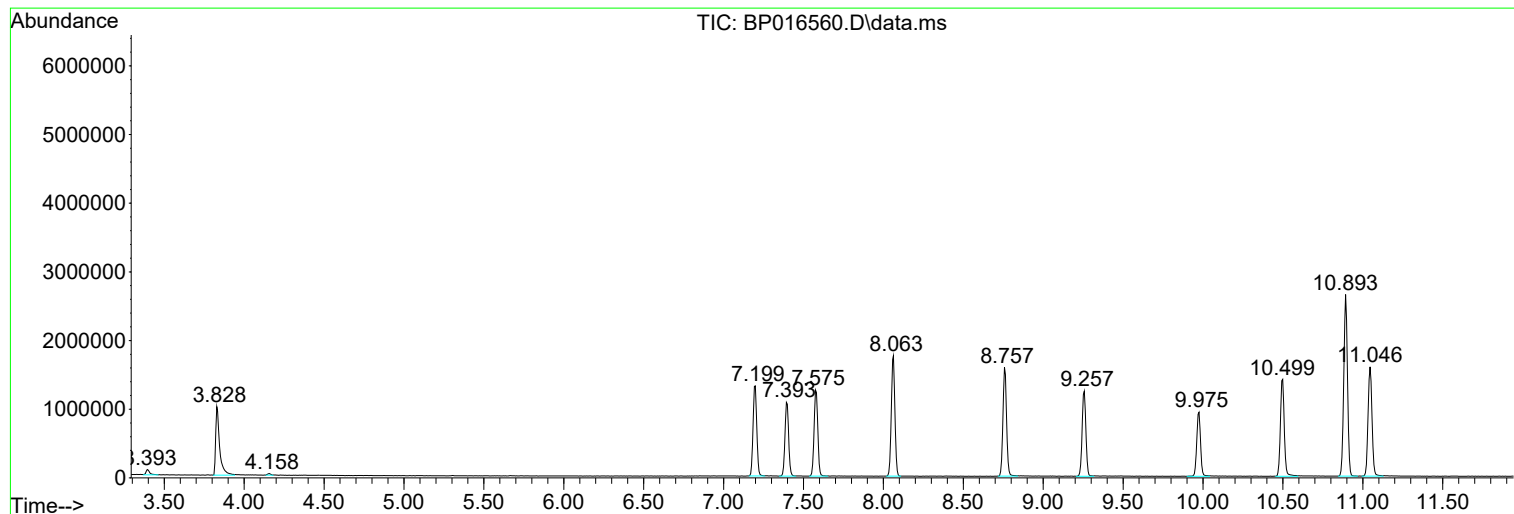

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016560.D
Acq On : 14 Aug 2023 14:25
Operator : MA/JU
Sample : PB154773BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016560.D
Acq On : 14 Aug 2023 14:25
Operator : MA/JU
Sample : PB154773BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------