

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
 Data File : BP016572.D
 Acq On : 14 Aug 2023 21:49
 Operator : MA/JU
 Sample : PB154810BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	15	19	30	rVB	127562	191773	1.82%	0.140%
2	3.834	88	93	111	rBV	1735322	2833664	26.88%	2.069%
3	4.152	143	147	154	rVB	40543	64998	0.62%	0.047%
4	5.305	340	343	348	rVB7	6241	11671	0.11%	0.009%
5	7.199	657	665	678	rBV	2188361	3448106	32.71%	2.517%
6	7.393	689	698	708	rBV	1761093	2762994	26.21%	2.017%
7	7.575	722	729	743	rBV	2076547	3346033	31.74%	2.443%
8	8.063	803	812	820	rBV	2799998	4523855	42.91%	3.302%
9	8.763	923	931	943	rBV	2536867	4167765	39.53%	3.042%
10	9.258	1007	1015	1029	rBV	2012545	3301460	31.32%	2.410%
11	9.975	1124	1137	1147	rBV	1615131	2662207	25.25%	1.943%
12	10.499	1217	1226	1238	rBV	2388379	4031002	38.24%	2.943%
13	10.893	1285	1293	1303	rBV	4166646	6857628	65.05%	5.006%
14	11.046	1311	1319	1331	rBV	2533134	4283937	40.63%	3.127%
15	12.469	1554	1561	1566	rVB	47320	72370	0.69%	0.053%
16	12.687	1593	1598	1602	rBV8	5978	10871	0.10%	0.008%
17	13.557	1739	1746	1753	rBV2	41337	67111	0.64%	0.049%
18	13.669	1759	1765	1771	rBV9	8430	17839	0.17%	0.013%
19	14.122	1835	1842	1856	rBV	4115161	5686024	53.93%	4.151%
20	14.410	1884	1891	1906	rBV	4859614	7046491	66.84%	5.144%
21	14.710	1934	1942	1951	rBV	6095313	8873580	84.17%	6.478%
22	14.904	1968	1975	1996	rBV	2014153	3095385	29.36%	2.260%
23	15.704	2104	2111	2122	rBV	5967319	8492998	80.56%	6.200%
24	15.816	2124	2130	2143	rVV	1326945	1940067	18.40%	1.416%
25	15.940	2147	2151	2161	rVB2	31241	54443	0.52%	0.040%
26	17.134	2352	2354	2361	rVB8	9966	16176	0.15%	0.012%
27	17.257	2371	2375	2381	rVB2	18046	27816	0.26%	0.020%
28	17.475	2405	2412	2421	rBV	7374099	10542652	100.00%	7.696%
29	17.575	2423	2429	2444	rVB2	6471432	9086514	86.19%	6.633%
30	17.857	2474	2477	2481	rBV2	8633	12931	0.12%	0.009%
31	18.316	2551	2555	2562	rBV6	21181	45425	0.43%	0.033%
32	19.380	2732	2736	2740	rBV	78636	104434	0.99%	0.076%
33	19.445	2744	2747	2751	rVB	74418	92909	0.88%	0.068%
34	19.804	2802	2808	2816	rBV	7732297	10335151	98.03%	7.545%
35	21.569	3103	3108	3119	rVB2	7830627	10305800	97.75%	7.523%
36	23.986	3511	3519	3530	rVB2	4334757	9382926	89.00%	6.849%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016572.D
Acq On : 14 Aug 2023 21:49
Operator : MA/JU
Sample : PB154810BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Title : SVOA CALIBRATION

37	24.157	3541	3548	3558	rVB	4254524	9190176	87.17%	6.709%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 136987182

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016572.D
Acq On : 14 Aug 2023 21:49
Operator : MA/JU
Sample : PB154810BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

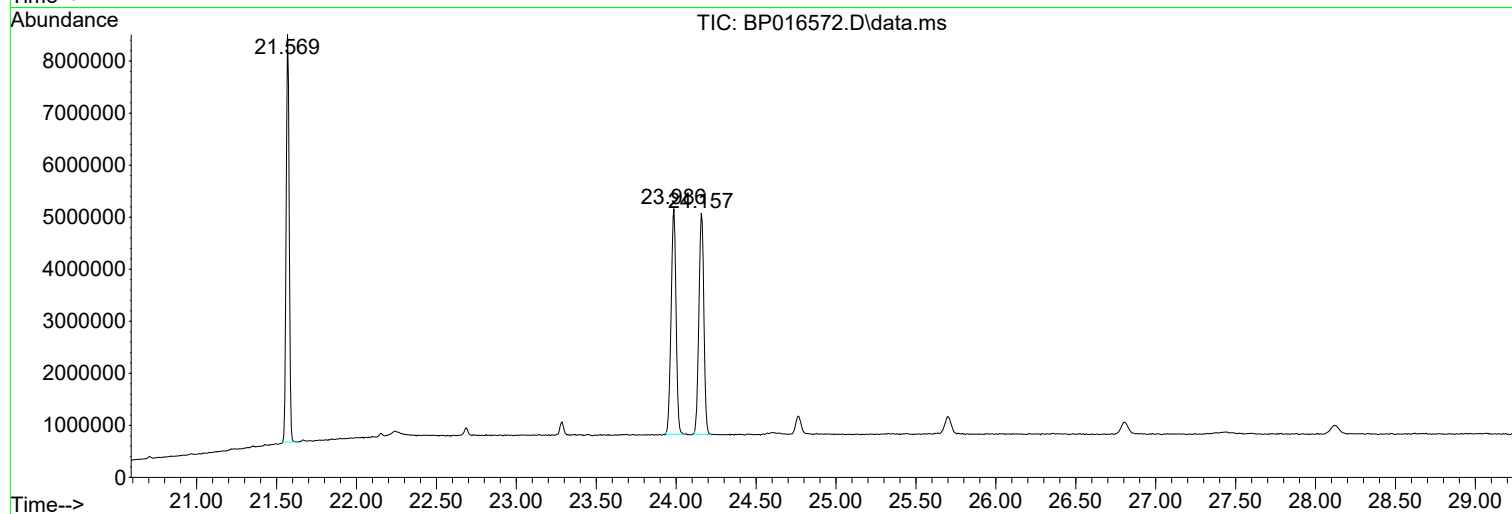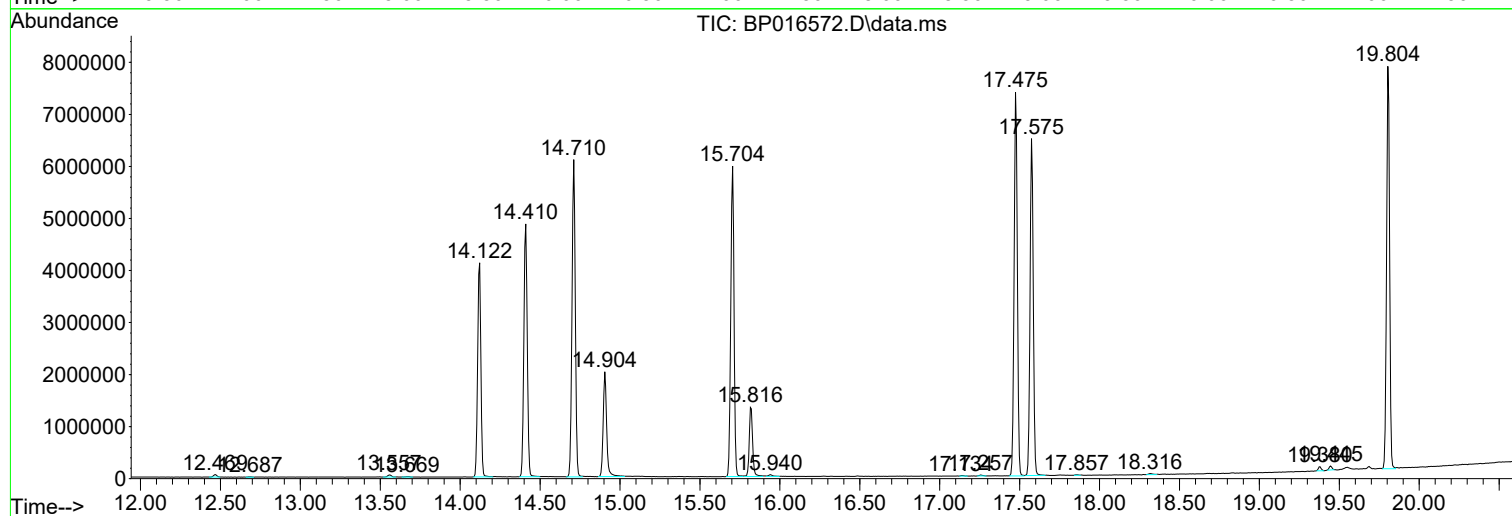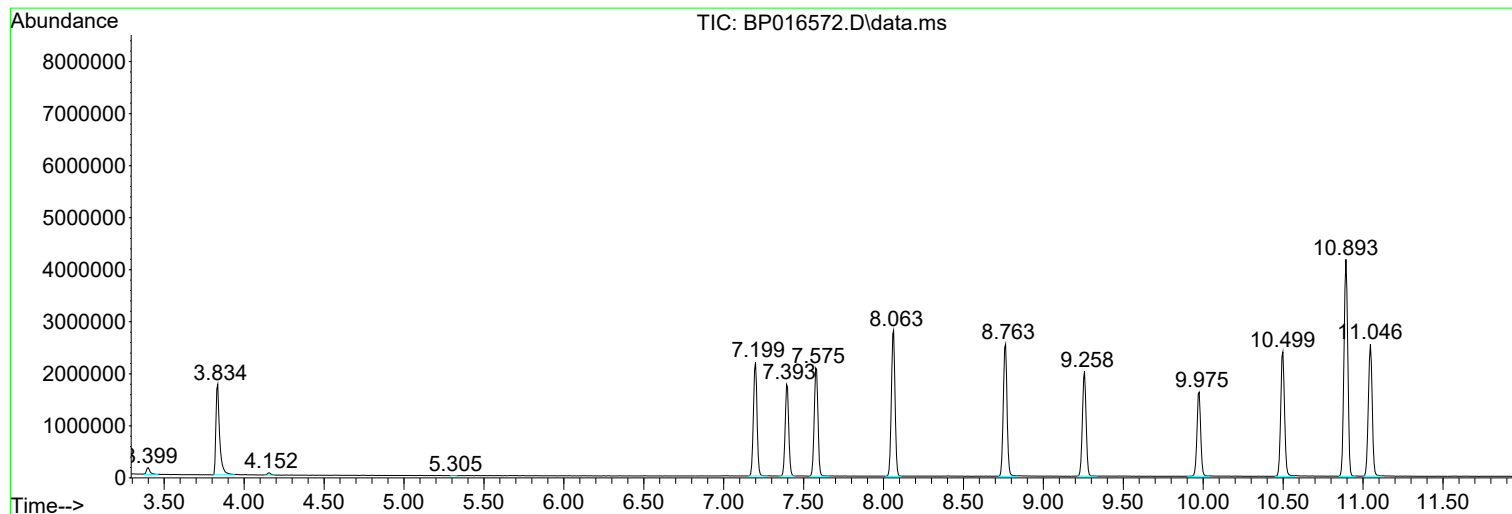

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016572.D
Acq On : 14 Aug 2023 21:49
Operator : MA/JU
Sample : PB154810BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016572.D
Acq On : 14 Aug 2023 21:49
Operator : MA/JU
Sample : PB154810BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------