

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
 Data File : BP016577.D
 Acq On : 15 Aug 2023 00:40
 Operator : MA/JU
 Sample : 03965-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	15	19	28	rVB	48711	77698	1.13%	0.108%
2	3.840	92	94	108	rBV2	50811	98506	1.43%	0.136%
3	3.952	109	113	116	rVB2	19093	24877	0.36%	0.034%
4	4.040	122	128	138	rVB	89076	145443	2.12%	0.201%
5	4.158	143	148	154	rVB	26734	41590	0.61%	0.058%
6	4.540	209	213	223	rBV6	15440	32408	0.47%	0.045%
7	4.740	244	247	253	rVB4	12426	17137	0.25%	0.024%
8	4.881	267	271	278	rBV7	6222	9621	0.14%	0.013%
9	4.987	287	289	296	rVB6	5451	8174	0.12%	0.011%
10	5.093	303	307	318	rVB	64074	100873	1.47%	0.140%
11	5.217	324	328	331	rVB6	5797	9427	0.14%	0.013%
12	5.687	401	408	412	rBV3	9998	21400	0.31%	0.030%
13	6.005	461	462	469	rVB7	7068	8034	0.12%	0.011%
14	6.499	542	546	553	rBV10	5108	10635	0.15%	0.015%
15	7.193	655	664	679	rBV	868724	1425756	20.75%	1.973%
16	7.393	691	698	706	rBV	748818	1135806	16.53%	1.572%
17	7.575	721	729	739	rBV	857296	1362881	19.83%	1.886%
18	7.652	739	742	752	rVB3	14374	28819	0.42%	0.040%
19	7.858	773	777	781	rBV3	6947	13103	0.19%	0.018%
20	8.058	804	811	825	rBV	1689091	2707652	39.40%	3.748%
21	8.758	923	930	939	rBV	945004	1477745	21.50%	2.045%
22	8.905	949	955	961	rVB	84993	142289	2.07%	0.197%
23	9.252	1006	1014	1027	rBV	827261	1369018	19.92%	1.895%
24	9.375	1031	1035	1040	rVB8	7861	13751	0.20%	0.019%
25	9.487	1048	1054	1061	rVB6	9906	18242	0.27%	0.025%
26	9.969	1128	1136	1148	rBV	633287	1033179	15.03%	1.430%
27	10.081	1150	1155	1159	rBV7	7809	14604	0.21%	0.020%
28	10.334	1193	1198	1205	rVB8	11144	19428	0.28%	0.027%
29	10.493	1217	1225	1236	rBV	980004	1627945	23.69%	2.253%
30	10.893	1284	1293	1300	rBV	2441397	4138700	60.22%	5.728%
31	11.046	1311	1319	1336	rBV	812881	1432091	20.84%	1.982%
32	11.428	1380	1384	1391	rBV10	6539	13710	0.20%	0.019%
33	11.634	1415	1419	1425	rBV9	9384	17749	0.26%	0.025%
34	11.705	1425	1431	1434	rVV7	6534	10868	0.16%	0.015%
35	12.281	1527	1529	1537	rVB9	4472	7302	0.11%	0.010%
36	12.463	1556	1560	1569	rVB2	19766	35462	0.52%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
 Data File : BP016577.D
 Acq On : 15 Aug 2023 00:40
 Operator : MA/JU
 Sample : 03965-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

37	13.046	1654	1659	1663	rVB7	8159	14419	0.21%	0.020%
38	13.287	1697	1700	1707	rVB7	8634	14348	0.21%	0.020%
39	13.475	1726	1732	1737	rBV4	11048	17294	0.25%	0.024%
40	13.557	1740	1746	1752	rVB2	82992	131338	1.91%	0.182%
41	13.651	1757	1762	1764	rVV5	5835	11080	0.16%	0.015%
42	13.893	1795	1803	1809	rBV5	8880	17664	0.26%	0.024%
43	14.028	1821	1826	1831	rBV7	15105	25903	0.38%	0.036%
44	14.116	1834	1841	1856	rVV	1842806	2467434	35.90%	3.415%
45	14.316	1872	1875	1879	rBV6	5613	8747	0.13%	0.012%
46	14.410	1884	1891	1910	rVV	1974538	3023672	44.00%	4.185%
47	14.546	1912	1914	1919	rVB6	6993	9767	0.14%	0.014%
48	14.710	1935	1942	1953	rBV	3640079	5416878	78.82%	7.497%
49	14.904	1968	1975	1992	rBV	641313	1052359	15.31%	1.457%
50	15.087	2002	2006	2009	rBV4	23636	37284	0.54%	0.052%
51	15.134	2009	2014	2029	rVB2	111147	191759	2.79%	0.265%
52	15.451	2065	2068	2071	rBV5	6481	8819	0.13%	0.012%
53	15.704	2102	2111	2118	rBV	2611099	3809395	55.43%	5.273%
54	15.816	2125	2130	2138	rBV	425714	588278	8.56%	0.814%
55	15.940	2148	2151	2157	rVB6	10694	13324	0.19%	0.018%
56	16.040	2166	2168	2174	rVB6	5713	8792	0.13%	0.012%
57	16.357	2219	2222	2226	rBV6	6377	10457	0.15%	0.014%
58	16.992	2326	2330	2333	rBV5	12309	19954	0.29%	0.028%
59	17.257	2372	2375	2379	rBV2	7490	12931	0.19%	0.018%
60	17.340	2385	2389	2393	rBV7	9354	16429	0.24%	0.023%
61	17.475	2405	2412	2417	rBV	4618215	6523122	94.92%	9.029%
62	17.516	2417	2419	2423	rVV	138750	167373	2.44%	0.232%
63	17.575	2423	2429	2439	rVV	2881827	4086306	59.46%	5.656%
64	17.651	2439	2442	2448	rVB3	61459	81701	1.19%	0.113%
65	17.734	2453	2456	2459	rVV	13138	14107	0.21%	0.020%
66	18.057	2507	2511	2514	rVB4	15067	22931	0.33%	0.032%
67	18.098	2514	2518	2521	rBV3	29802	36949	0.54%	0.051%
68	18.310	2550	2554	2562	rBV2	311019	522211	7.60%	0.723%
69	18.398	2567	2569	2574	rVB	61534	73869	1.07%	0.102%
70	18.522	2584	2590	2593	rBV5	36436	85210	1.24%	0.118%
71	18.875	2646	2650	2653	rBV4	61570	77283	1.12%	0.107%
72	19.475	2748	2752	2756	rBV	339144	386297	5.62%	0.535%
73	19.545	2760	2764	2771	rBV2	126944	194335	2.83%	0.269%
74	19.804	2802	2808	2819	rBV	3836049	5440979	79.17%	7.531%
75	21.228	3046	3050	3056	rBV2	402604	603235	8.78%	0.835%
76	21.569	3102	3108	3113	rBV	5031022	6872188	100.00%	9.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016577.D
Acq On : 15 Aug 2023 00:40
Operator : MA/JU
Sample : 03965-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48L1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Title : SVOA CALIBRATION

77	23.974	3511	3517	3536	rVB2	2168514	5020264	73.05%	6.949%
78	24.151	3540	3547	3564	rVB	2971609	6460555	94.01%	8.942%




Sum of corrected areas: 72249163

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016577.D
Acq On : 15 Aug 2023 00:40
Operator : MA/JU
Sample : 03965-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48L1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

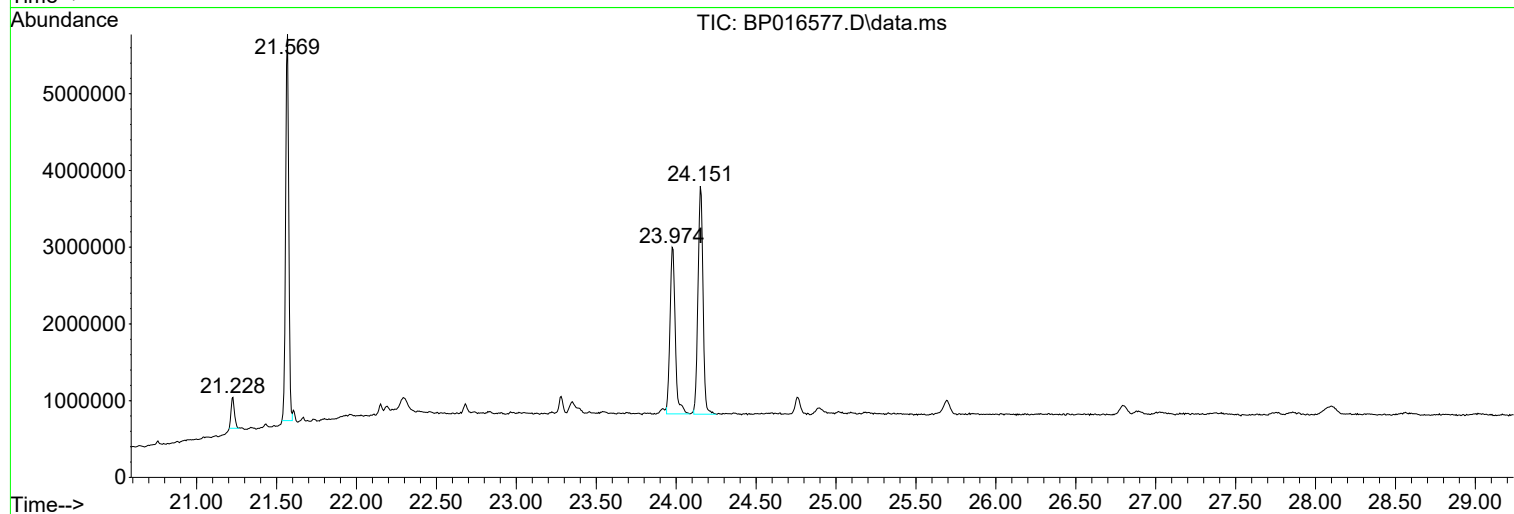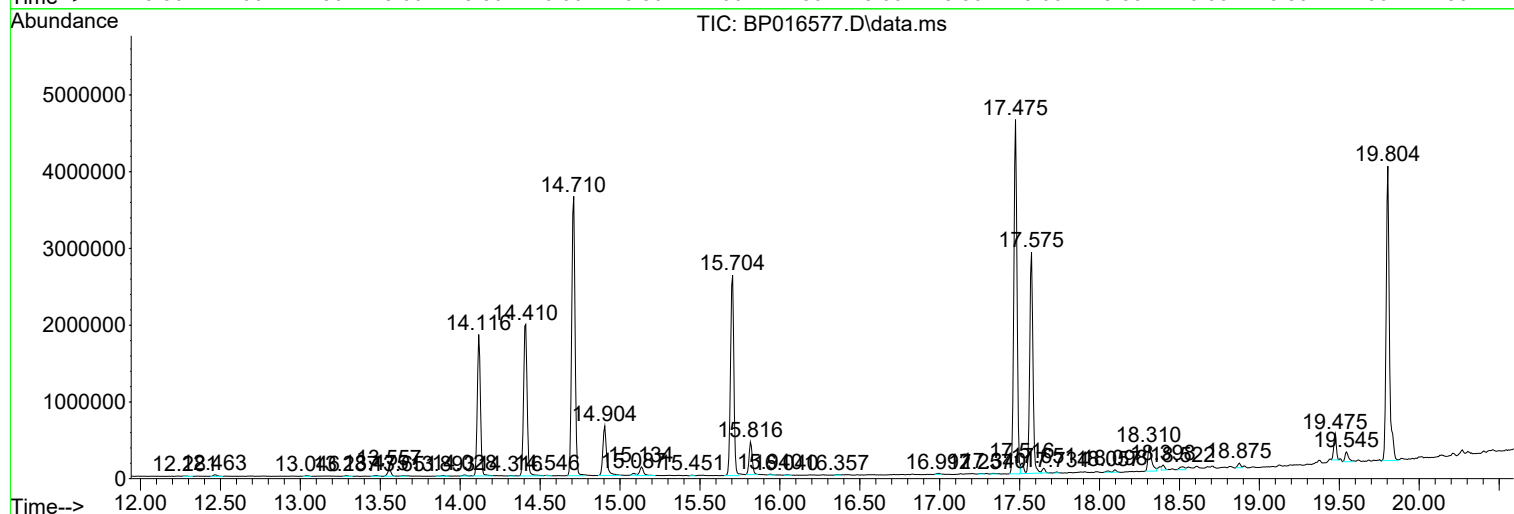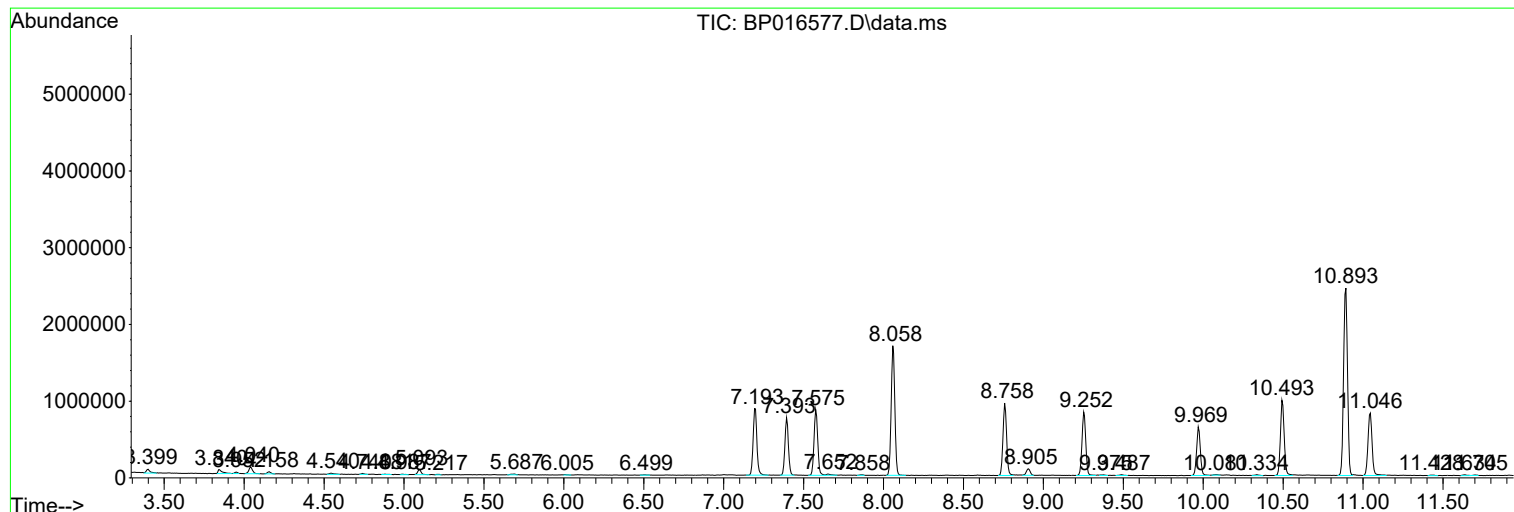

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016577.D
Acq On : 15 Aug 2023 00:40
Operator : MA/JU
Sample : 03965-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48L1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081423\
Data File : BP016577.D
Acq On : 15 Aug 2023 00:40
Operator : MA/JU
Sample : 03965-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48L1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------