

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
 Data File : BP016608.D
 Acq On : 16 Aug 2023 18:07
 Operator : MA/JU
 Sample : 03967-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48K4

Quant Time: Aug 17 00:47:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 14 18:26:05 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.057	152	375584	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	1753116	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164	1137131	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	2584465	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	2347284	20.000	ng/ul	-0.01
88) Perylene-d12	24.151	264	2365877	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	35956	3.638	ng/uL	0.00
4) Pyridine-d5	3.840	84	34708	1.154	ng/ul	0.00
7) Phenol-d5	7.193	99	550196	15.890	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	360316	15.799	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	397025	15.964	ng/ul	0.00
15) 4-Methylphenol-d8	8.757	113	412235	14.973	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	202429	16.410	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	203990	17.411	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	378577	16.420	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	364178	9.206	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	1371747	16.678	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	1548745	16.683	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	223983	13.368	ng/ul	0.00
60) Fluorene-d10	15.698	176	1206928	17.213	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	126869	10.319	ng/ul	0.00
73) Anthracene-d10	17.569	188	1861596	16.652	ng/ul	0.00
81) Pyrene-d10	19.798	212	2326126	18.913	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	1957865	17.268	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.904	105	168779	3.796	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.427	149	98597	1.088	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
Data File : BP016608.D
Acq On : 16 Aug 2023 18:07
Operator : MA/JU
Sample : 03967-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48K4

Quant Time: Aug 17 00:47:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 14 18:26:05 2023
Response via : Initial Calibration




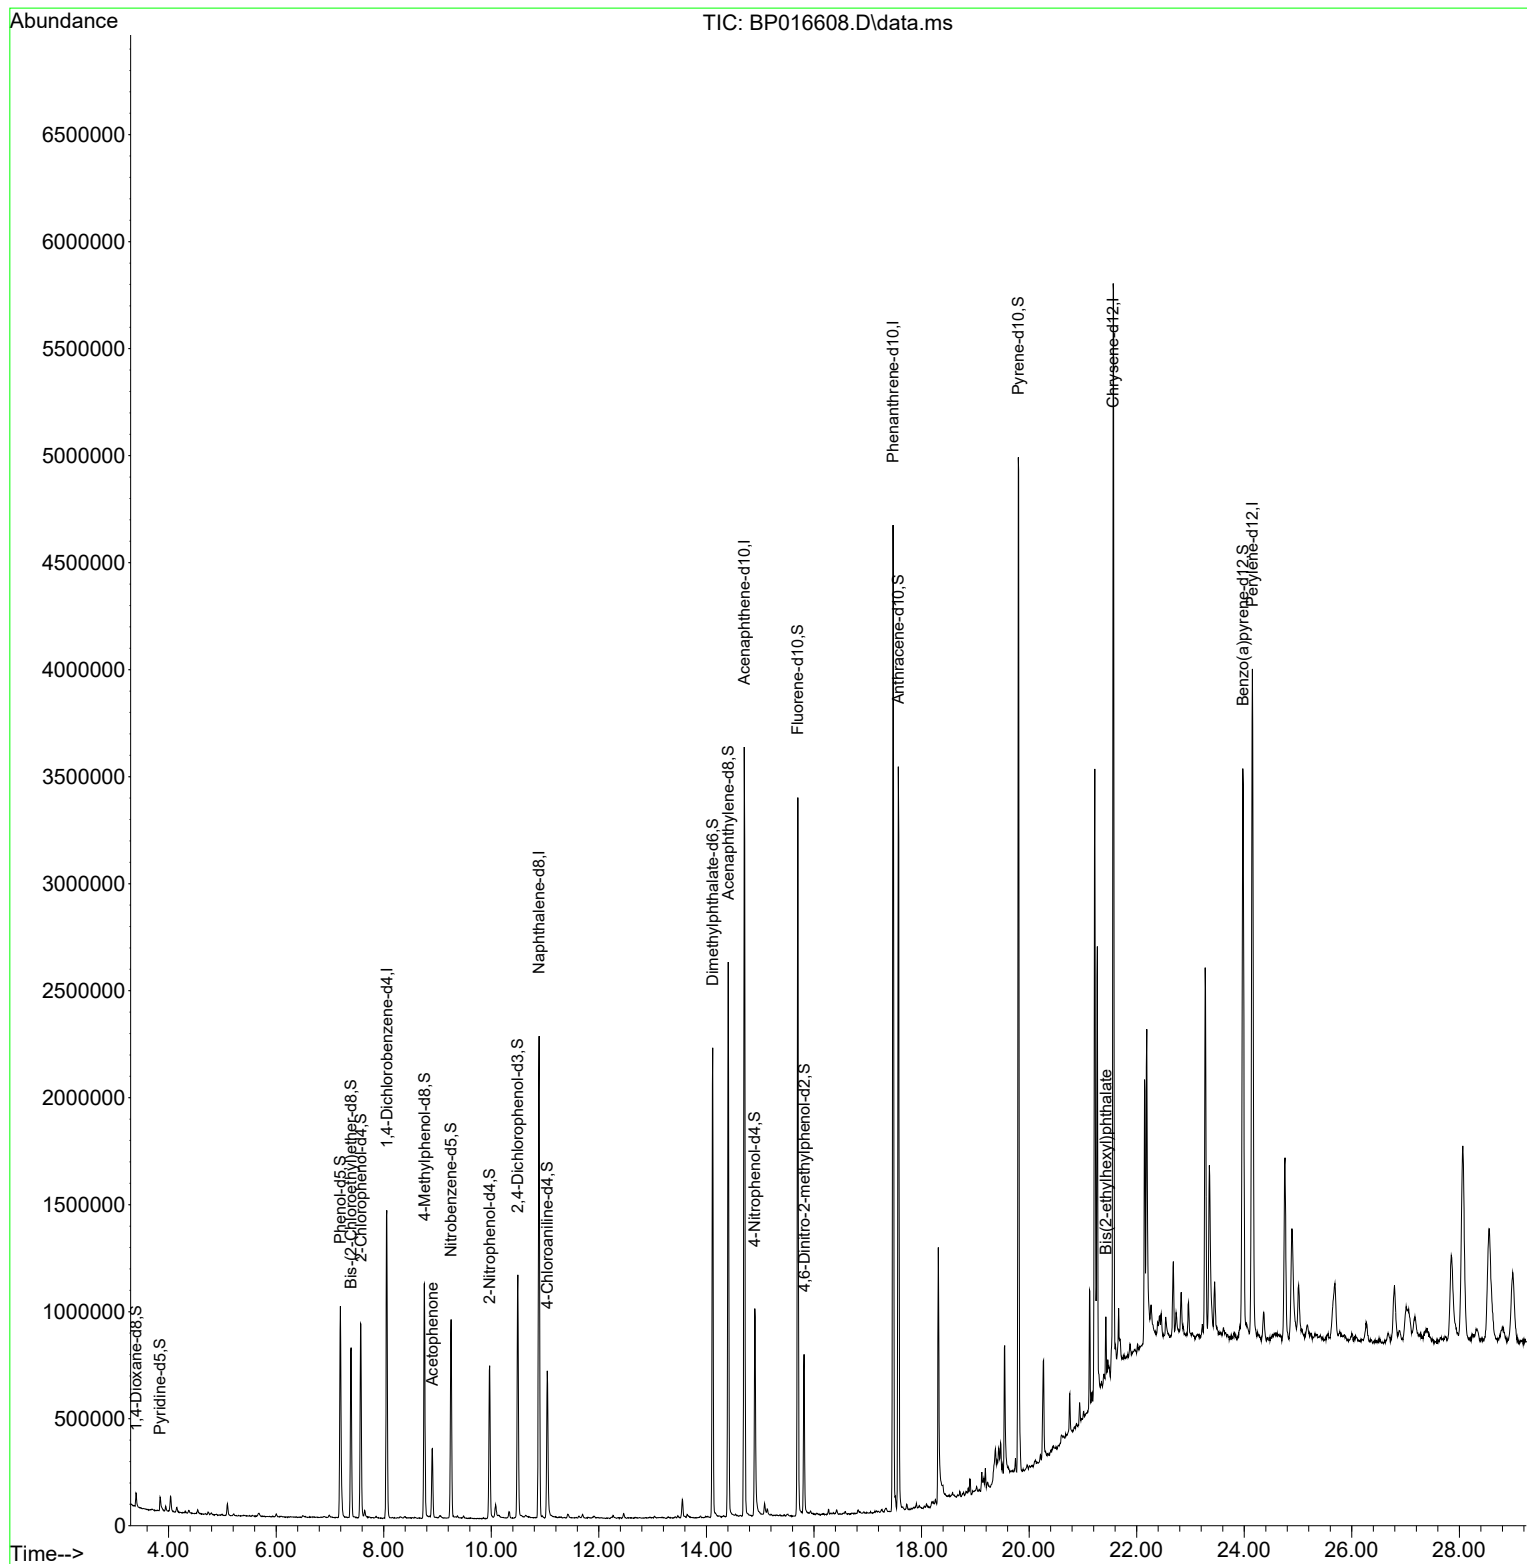


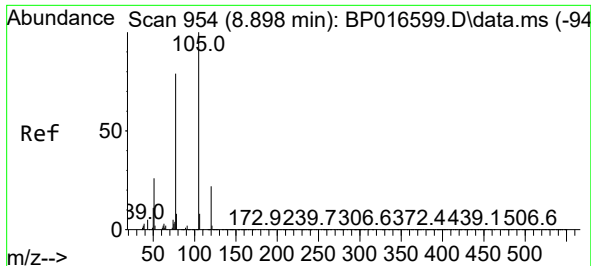

#16
Acetophenone
Concen: 3.796 ng/ul
RT: 8.904 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP016608.D
Acq: 16 Aug 2023 18:07

Instrument :
BNA_P
ClientSampleId :
A48K4

Tgt Ion:105 Resp: 168779
Ion Ratio Lower Upper
105 100
77 80.2 64.4 96.6
51 27.3 21.2 31.8

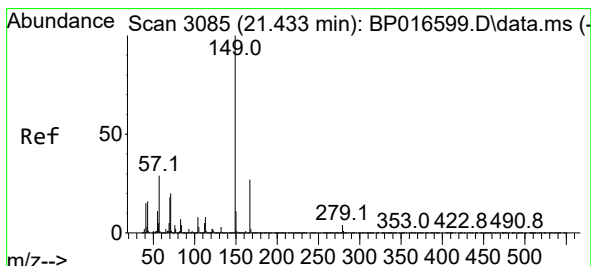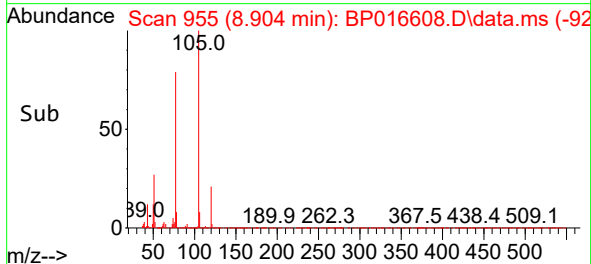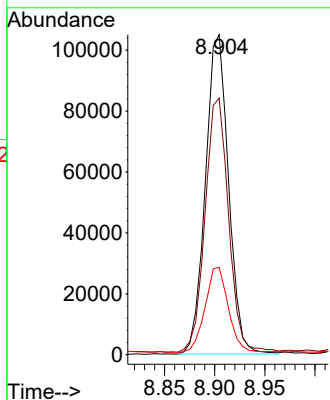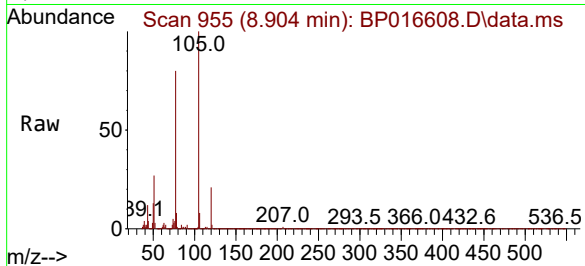

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.088 ng/ul
RT: 21.427 min Scan# 3084
Delta R.T. -0.006 min
Lab File: BP016608.D
Acq: 16 Aug 2023 18:07

Tgt Ion:149 Resp: 98597
Ion Ratio Lower Upper
149 100
167 27.2 20.9 31.3
279 3.7 2.6 4.0

