

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
 Data File : BP016610.D
 Acq On : 16 Aug 2023 19:15
 Operator : MA/JU
 Sample : 03967-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48L7

Quant Time: Aug 17 00:48:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 14 18:26:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.057	152	450243	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	2076351	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164	1362805	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	3104822	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	2959704	20.000	ng/ul	-0.01
88) Perylene-d12	24.151	264	3117473	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	27612	2.330	ng/uL	0.00
4) Pyridine-d5	3.840	84	33619	0.933	ng/ul	0.00
7) Phenol-d5	7.193	99	418786	10.089	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	283353	10.364	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	308895	10.361	ng/ul	-0.01
15) 4-Methylphenol-d8	8.752	113	286138	8.669	ng/ul	-0.01
21) Nitrobenzene-d5	9.252	128	159651	10.928	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	159449	11.491	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	291992	10.693	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	380750	8.126	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	1109834	11.259	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	1242121	11.164	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	162150	8.075	ng/ul	0.00
60) Fluorene-d10	15.698	176	986732	11.742	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	93354	6.320	ng/ul	0.00
73) Anthracene-d10	17.569	188	1536565	11.441	ng/ul	0.00
81) Pyrene-d10	19.798	212	2006518	12.938	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	1842737	12.334	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.899	105	65730	1.233	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
Data File : BP016610.D
Acq On : 16 Aug 2023 19:15
Operator : MA/JU
Sample : 03967-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48L7


Quant Time: Aug 17 00:48:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 14 18:26:05 2023
Response via : Initial Calibration

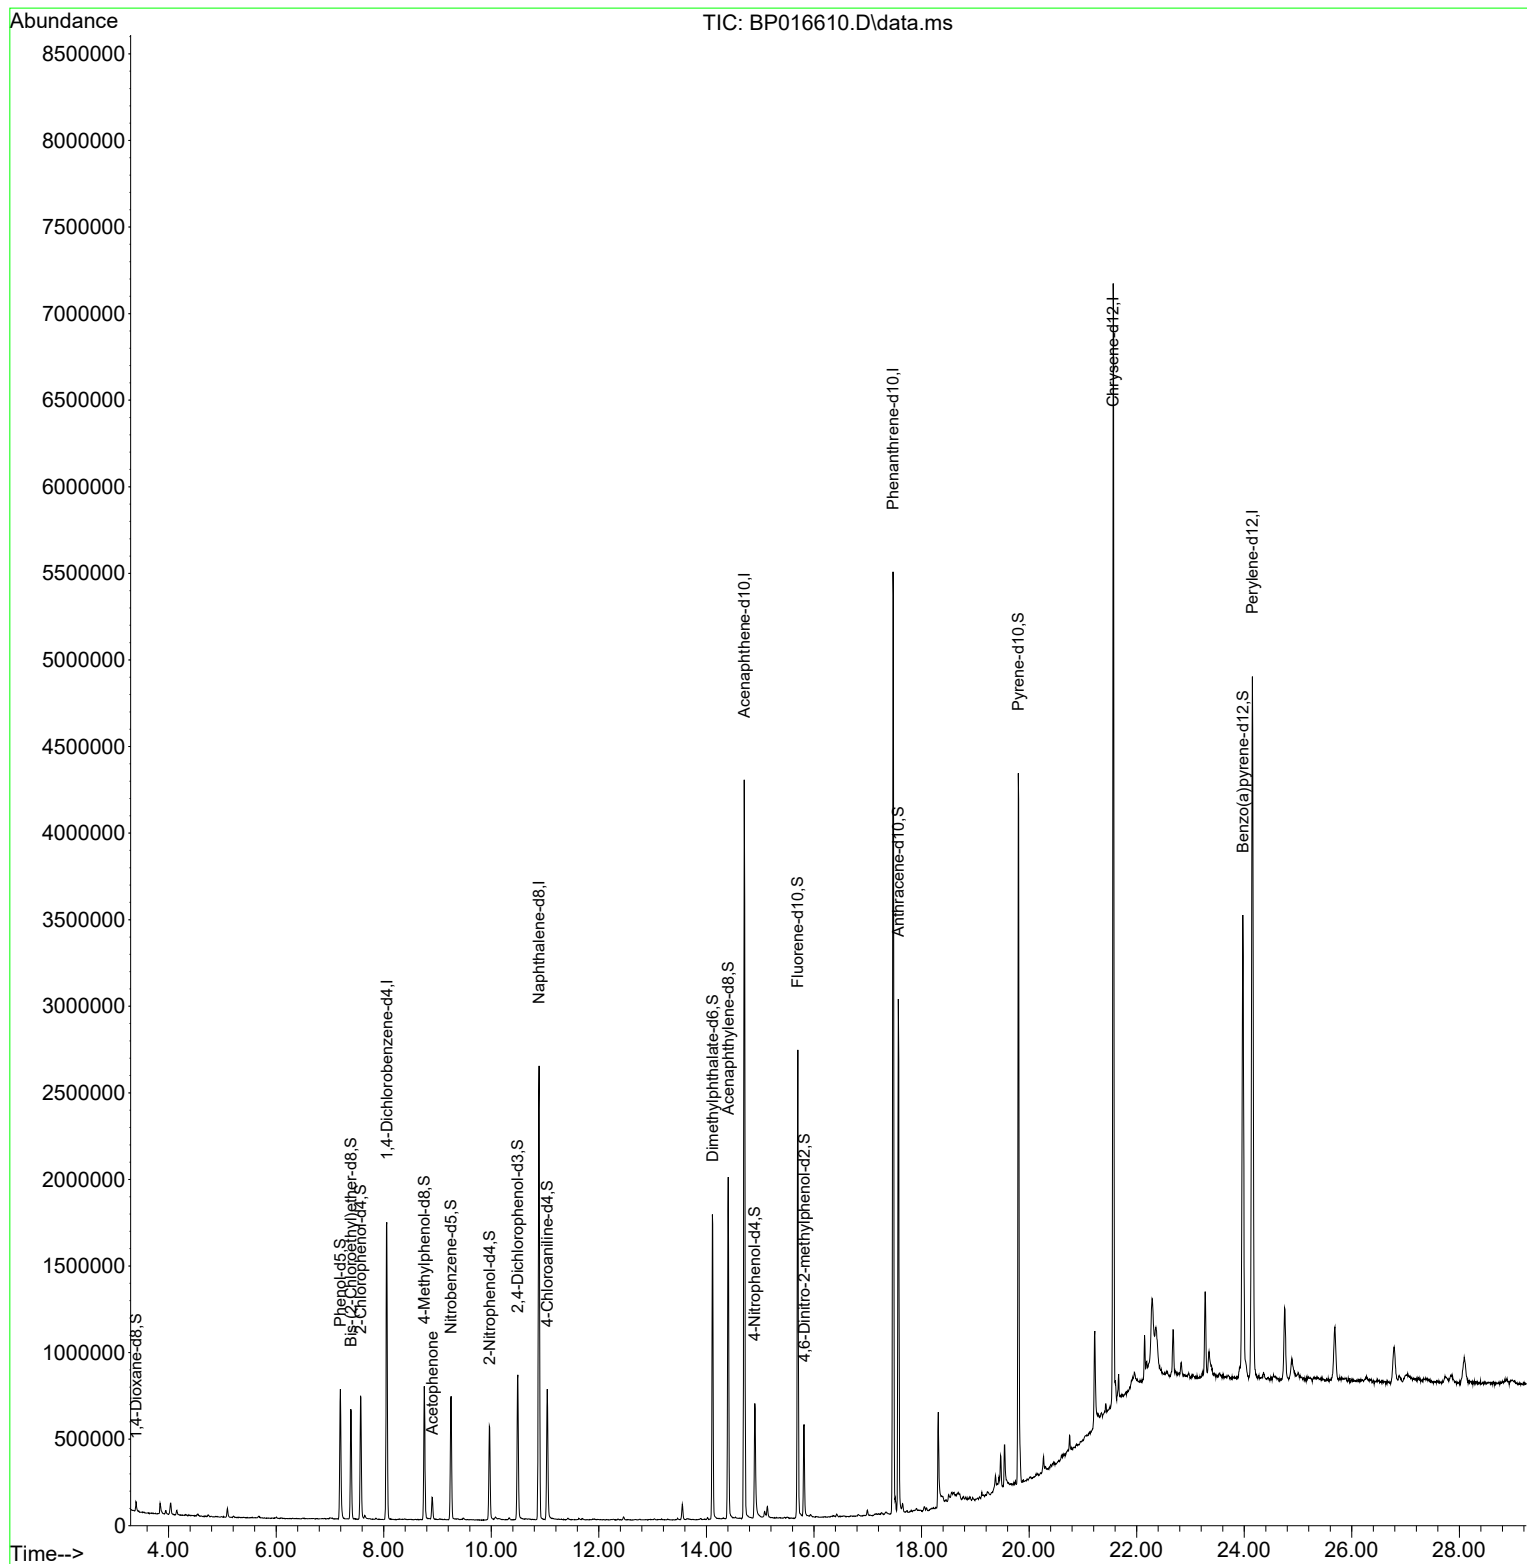

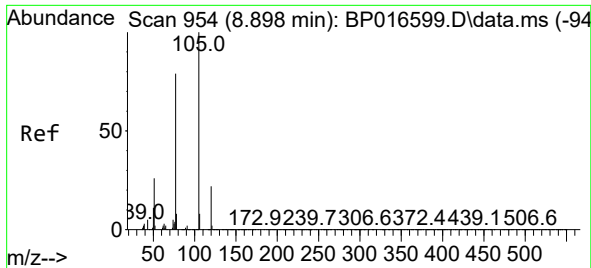

#16
Acetophenone
Concen: 1.233 ng/ul
RT: 8.899 min Scan# 91
Delta R.T. -0.012 min
Lab File: BP016610.D
Acq: 16 Aug 2023 19:15

Instrument :
BNA_P
ClientSampleId :
A48L7

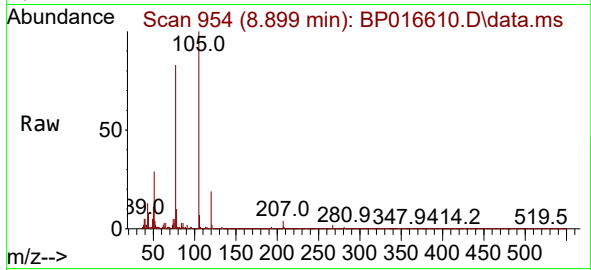

Tgt Ion:	105	Resp:	65730
Ion	Ratio	Lower	Upper
105	100		
77	83.4	64.4	96.6
51	28.6	21.2	31.8

