




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
 Data File : BP016619.D
 Acq On : 17 Aug 2023 00:55
 Operator : MA/JU
 Sample : 03967-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48M3

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:43:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/17/2023
 Supervised By :mohammad ahmed 08/17/2023

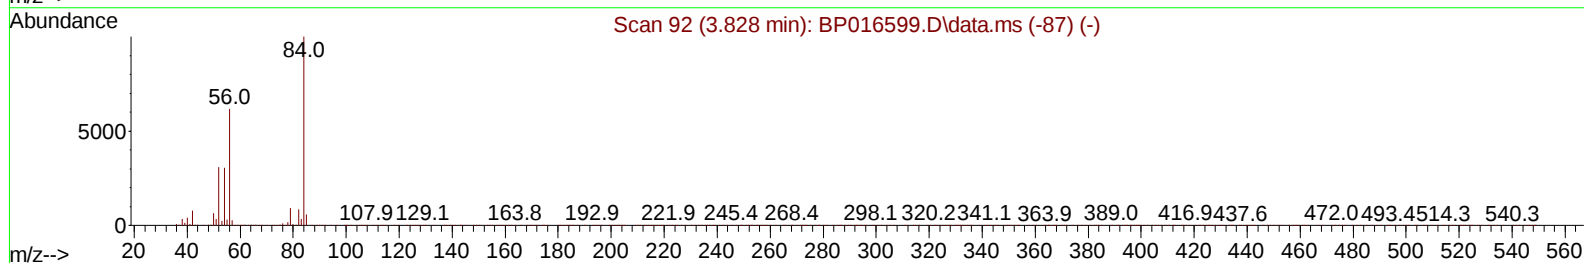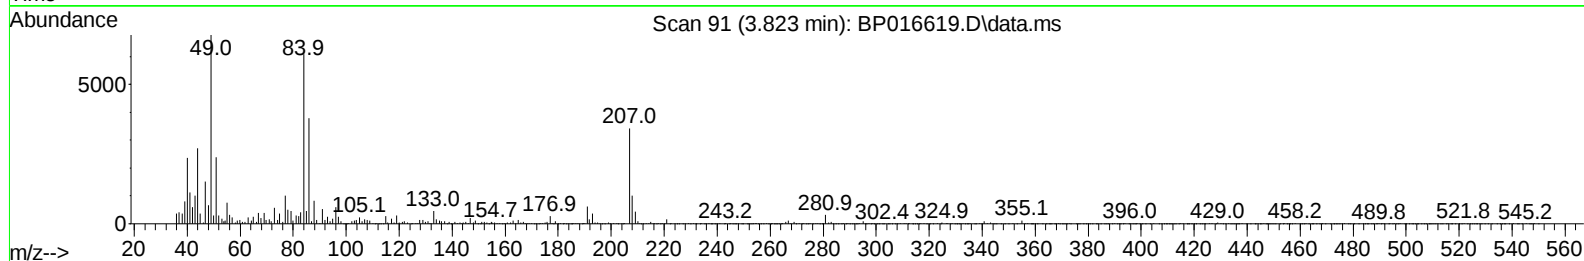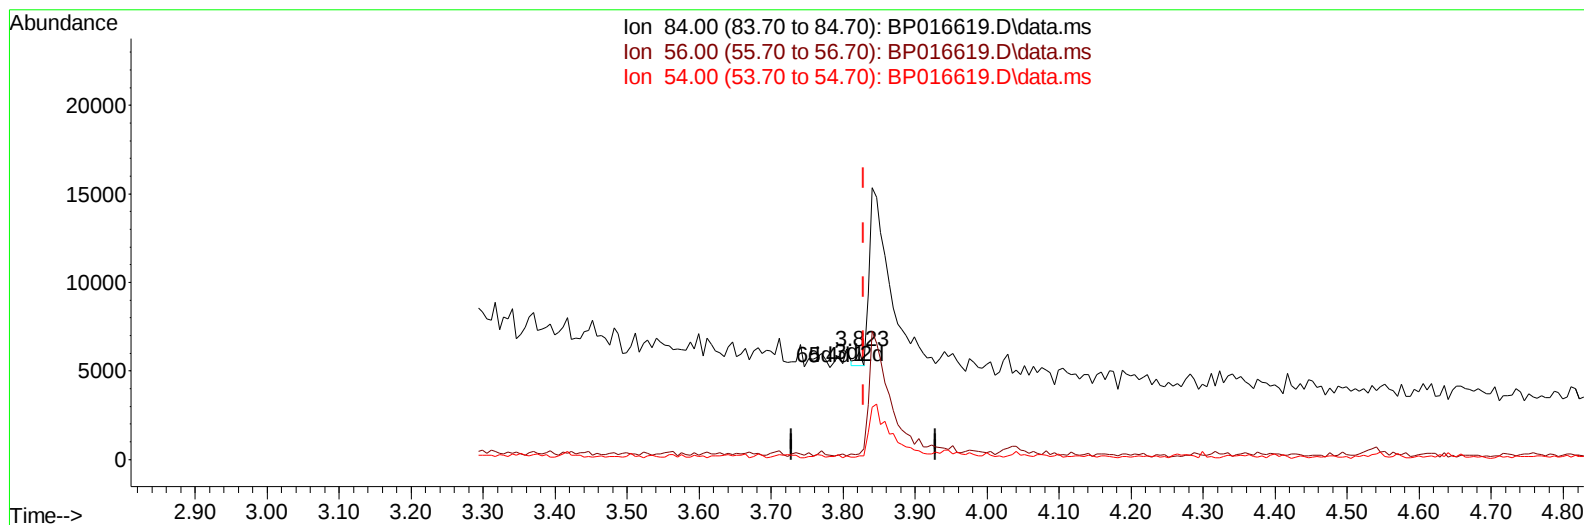

TIC: BP016619.D\data.ms

(4) Pyridine-d5 (S)

3.823min (-0.006) 0.01 ng/u1

response 402

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.90	5.37#
54.00	30.30	3.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
 Data File : BP016619.D
 Acq On : 17 Aug 2023 00:55
 Operator : MA/JU
 Sample : 03967-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48M3

Manual IntegrationsAPPROVED

Quant Time: Aug 17 01:43:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/17/2023
 Supervised By :mohammad ahmed 08/17/2023

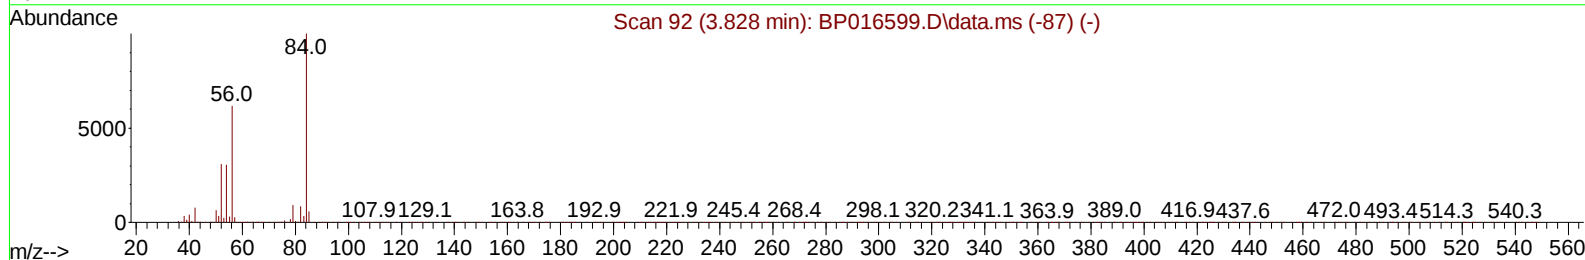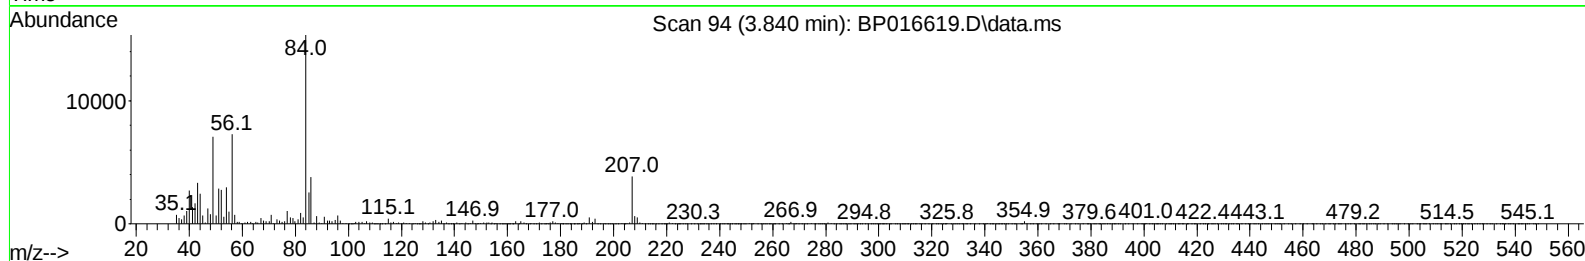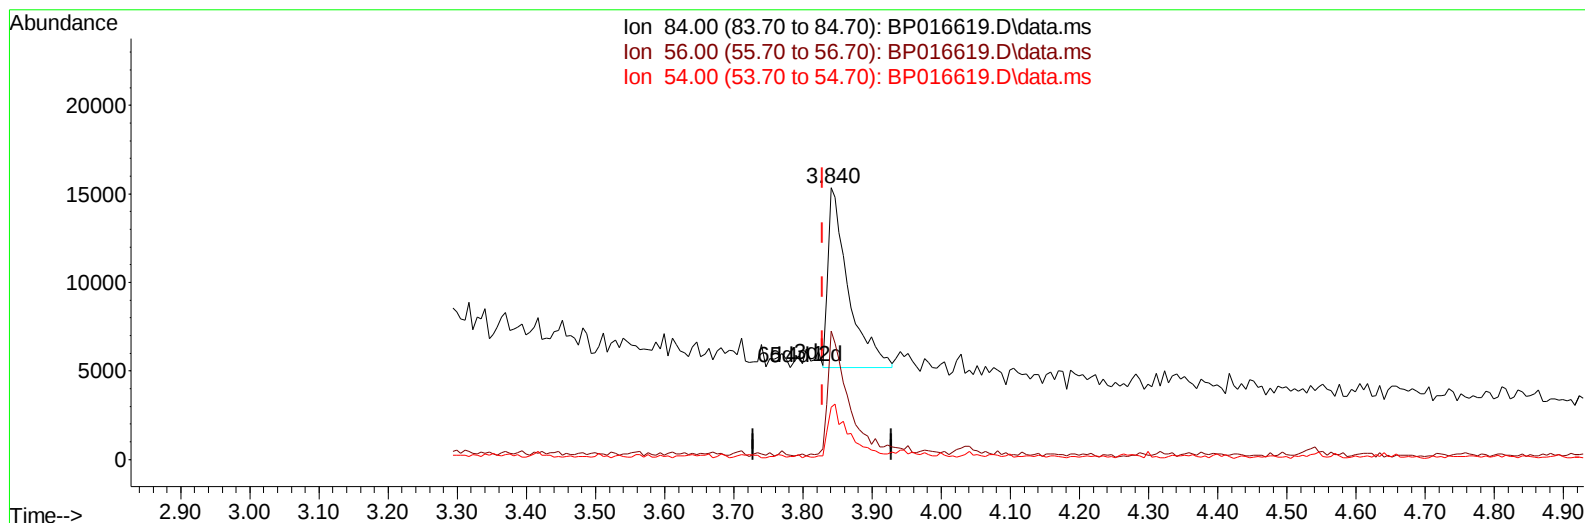

TIC: BP016619.D\data.ms

(4) Pyridine-d5 (S)

3.840min (+ 0.012) 0.76 ng/ul m

response 20704

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.90	47.40#
54.00	30.30	19.25#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
 Data File : BP016619.D
 Acq On : 17 Aug 2023 00:55
 Operator : MA/JU
 Sample : 03967-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48M3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/17/2023
 Supervised By :mohammad ahmed 08/17/2023

Quant Time: Aug 17 01:45:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.052	152		338774	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136		1601341	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164		1033465	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188		2423733	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240		2515179	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264		2813991	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.393	96		20673	2.319	ng/uL	0.00
4) Pyridine-d5	3.840	84		20704m	0.763	ng/ul	0.01
7) Phenol-d5	7.193	99		313559	10.040	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67		219057	10.649	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132		232145	10.348	ng/ul	0.00
15) 4-Methylphenol-d8	8.752	113		202036	8.135	ng/ul	0.00
21) Nitrobenzene-d5	9.252	128		120590	10.702	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143		116234	10.861	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.493	165		220588	10.474	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131		221958	6.142	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166		817043	10.930	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160		914530	10.839	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143		125816	8.262	ng/ul	0.00
60) Fluorene-d10	15.693	176		742463	11.651	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200		71830	6.230	ng/ul	0.00
73) Anthracene-d10	17.569	188		1176186	11.219	ng/ul	0.00
81) Pyrene-d10	19.798	212		1574400	11.946	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.969	264		1578196	11.703	ng/ul	0.00
Target Compounds							
						Qvalue	
16) Acetophenone	8.899	105		108953	2.717	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
Data File : BP016619.D
Acq On : 17 Aug 2023 00:55
Operator : MA/JU
Sample : 03967-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48M3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/17/2023
Supervised By :mohammad ahmed 08/17/2023

Quant Time: Aug 17 01:45:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

