

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
 Data File : BP016609.D
 Acq On : 16 Aug 2023 18:41
 Operator : MA/JU
 Sample : 03967-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48K5

Quant Time: Aug 17 01:18:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 14 18:26:05 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.057	152	333576	20.000	ng/u1	0.00
20) Naphthalene-d8	10.887	136	1555125	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.704	164	1012386	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.469	188	2364638	20.000	ng/u1	0.00
79) Chrysene-d12	21.563	240	2343169	20.000	ng/u1	-0.01
88) Perylene-d12	24.151	264	2514034	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	21217	2.417	ng/uL	0.00
4) Pyridine-d5	3.840	84	25085	0.939	ng/u1	0.00
7) Phenol-d5	7.193	99	323059	10.505	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	215419	10.635	ng/u1	0.00
11) 2-Chlorophenol-d4	7.575	132	235467	10.660	ng/u1	0.00
15) 4-Methylphenol-d8	8.757	113	243027	9.939	ng/u1	0.00
21) Nitrobenzene-d5	9.251	128	116604	10.656	ng/u1	0.00
24) 2-Nitrophenol-d4	9.969	143	119453	11.494	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.493	165	222976	10.902	ng/u1	0.00
31) 4-Chloroaniline-d4	11.040	131	207207	5.905	ng/u1	0.00
46) Dimethylphthalate-d6	14.116	166	823141	11.241	ng/u1	0.00
49) Acenaphthylene-d8	14.404	160	917494	11.101	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	126440	8.476	ng/u1	0.00
60) Fluorene-d10	15.698	176	734671	11.769	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	68691	6.106	ng/u1	0.00
73) Anthracene-d10	17.569	188	1131034	11.058	ng/u1	0.00
81) Pyrene-d10	19.798	212	1471270	11.983	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	1348840	11.195	ng/u1	-0.01
Target Compounds						
16) Acetophenone	8.899	105	134323	3.402	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
Data File : BP016609.D
Acq On : 16 Aug 2023 18:41
Operator : MA/JU
Sample : 03967-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48K5


Quant Time: Aug 17 01:18:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 14 18:26:05 2023
Response via : Initial Calibration

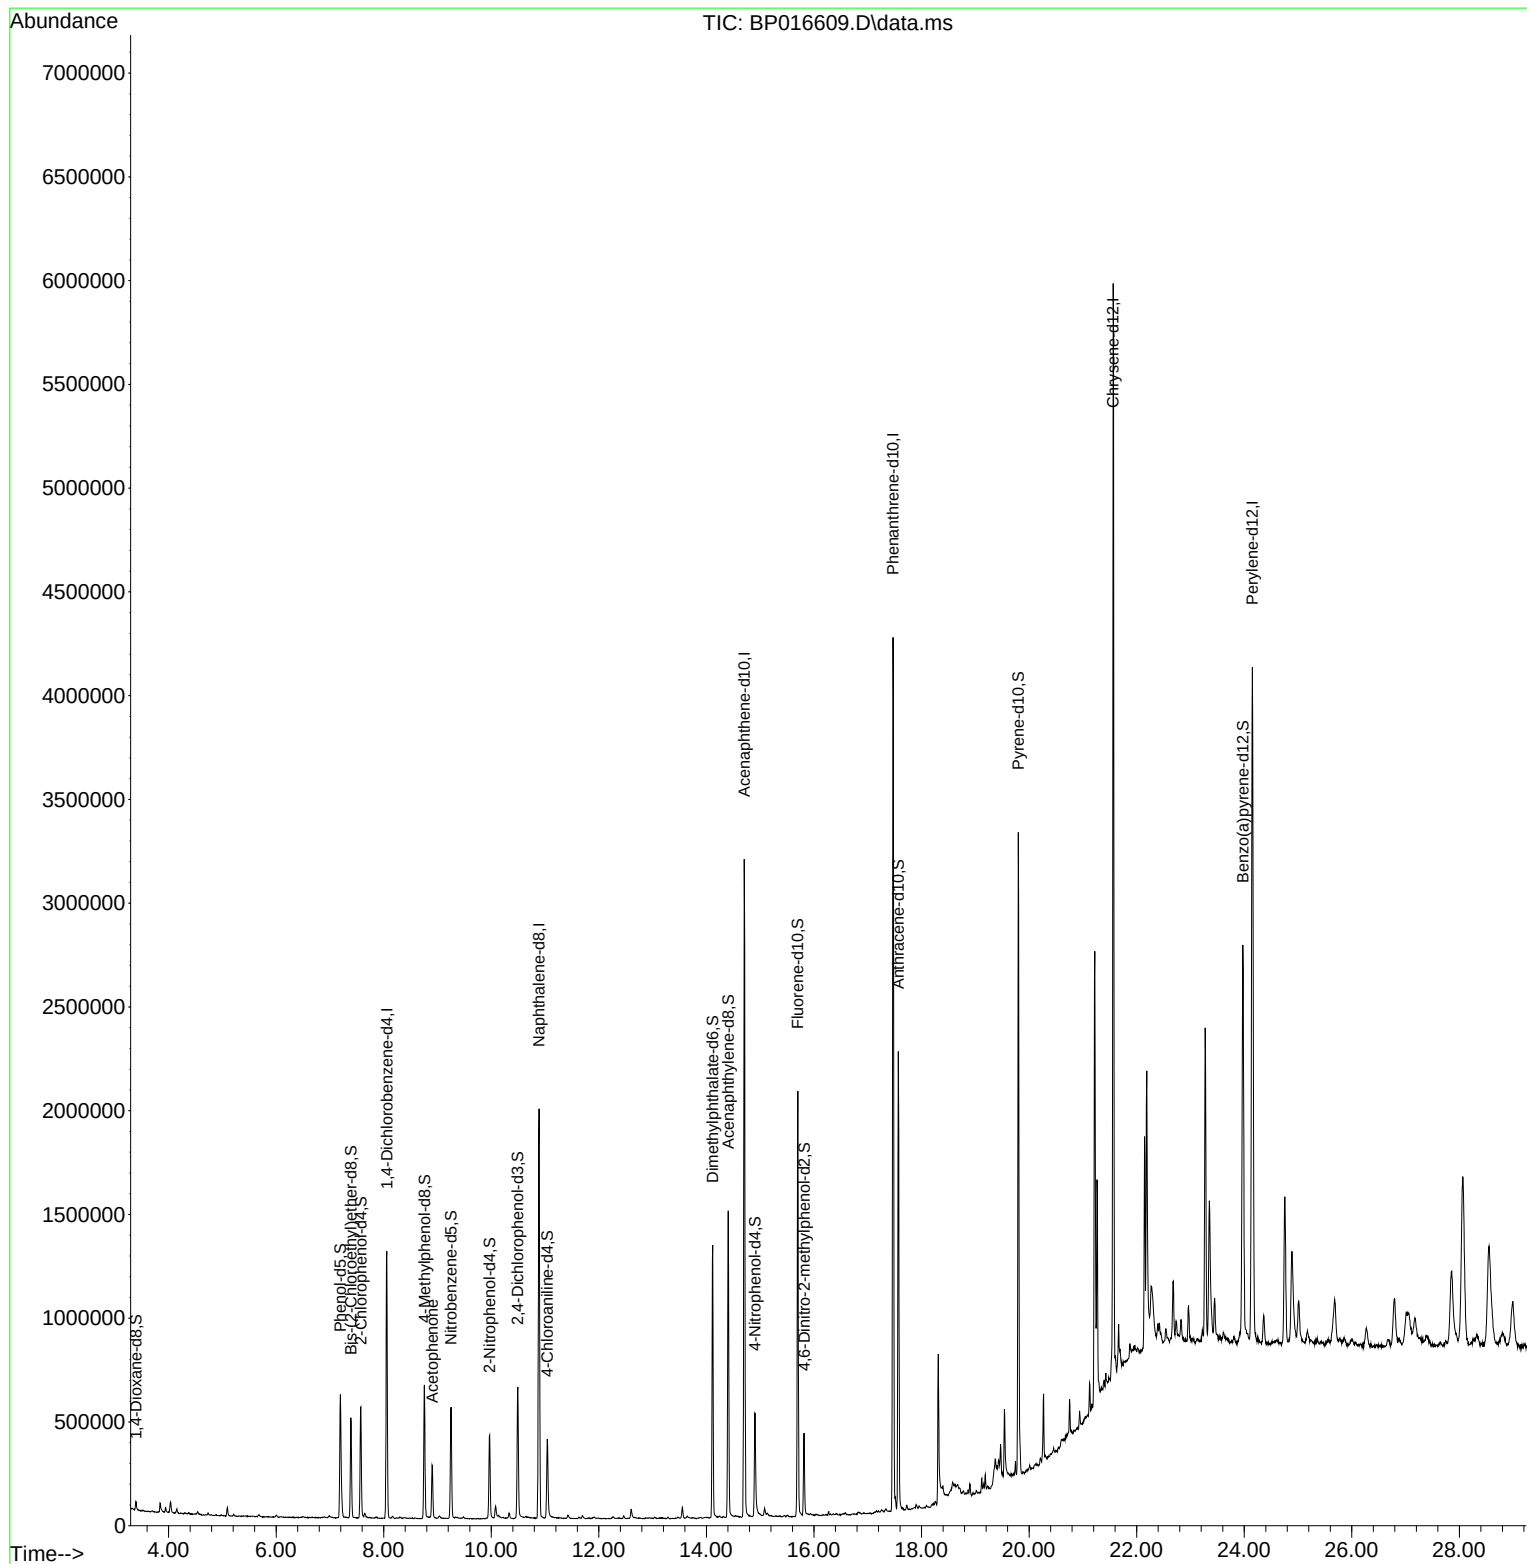

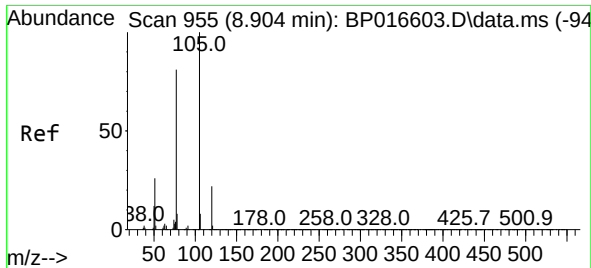

#16
 Acetophenone
 Concen: 3.402 ng/ul
 RT: 8.899 min Scan# 91
 Delta R.T. -0.012 min
 Lab File: BP016609.D
 Acq: 16 Aug 2023 18:41

Instrument :
 BNA_P
 ClientSampleId :
 A48K5

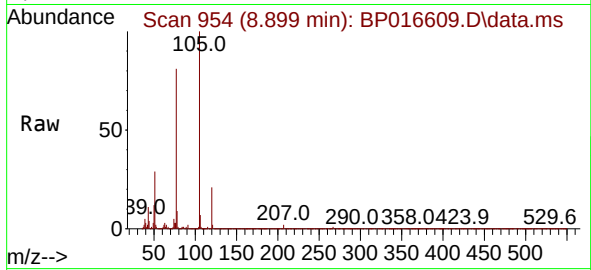

Tgt Ion:105 Resp: 134323
 Ion Ratio Lower Upper
 105 100
 77 81.5 64.4 96.6
 51 28.7 21.2 31.8

