

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
 Data File : BP016623.D
 Acq On : 17 Aug 2023 03:11
 Operator : MA/JU
 Sample : 03967-21
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48M9

Quant Time: Aug 17 04:28:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	169030	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	792762	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.698	164	546550	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1416967	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	1705259	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	2058648	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	14913	3.352	ng/uL	0.00
4) Pyridine-d5	3.846	84	13839	1.023	ng/ul	0.02
7) Phenol-d5	7.193	99	239287	15.355	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	165792	16.153	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	172463	15.408	ng/ul	0.00
15) 4-Methylphenol-d8	8.752	113	182323	14.714	ng/ul	0.00
21) Nitrobenzene-d5	9.246	128	90609	16.244	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	84086	15.871	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	162534	15.589	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	228793	12.790	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	667340	16.881	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	737740	16.534	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	98710	12.257	ng/ul	0.00
60) Fluorene-d10	15.692	176	616398	18.290	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	52707	7.819	ng/ul	0.00
73) Anthracene-d10	17.569	188	1077092	17.573	ng/ul	0.00
81) Pyrene-d10	19.798	212	1472770	16.483	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	1752296	17.761	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.905	105	35777	1.788	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081623\
Data File : BP016623.D
Acq On : 17 Aug 2023 03:11
Operator : MA/JU
Sample : 03967-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48M9

Quant Time: Aug 17 04:28:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

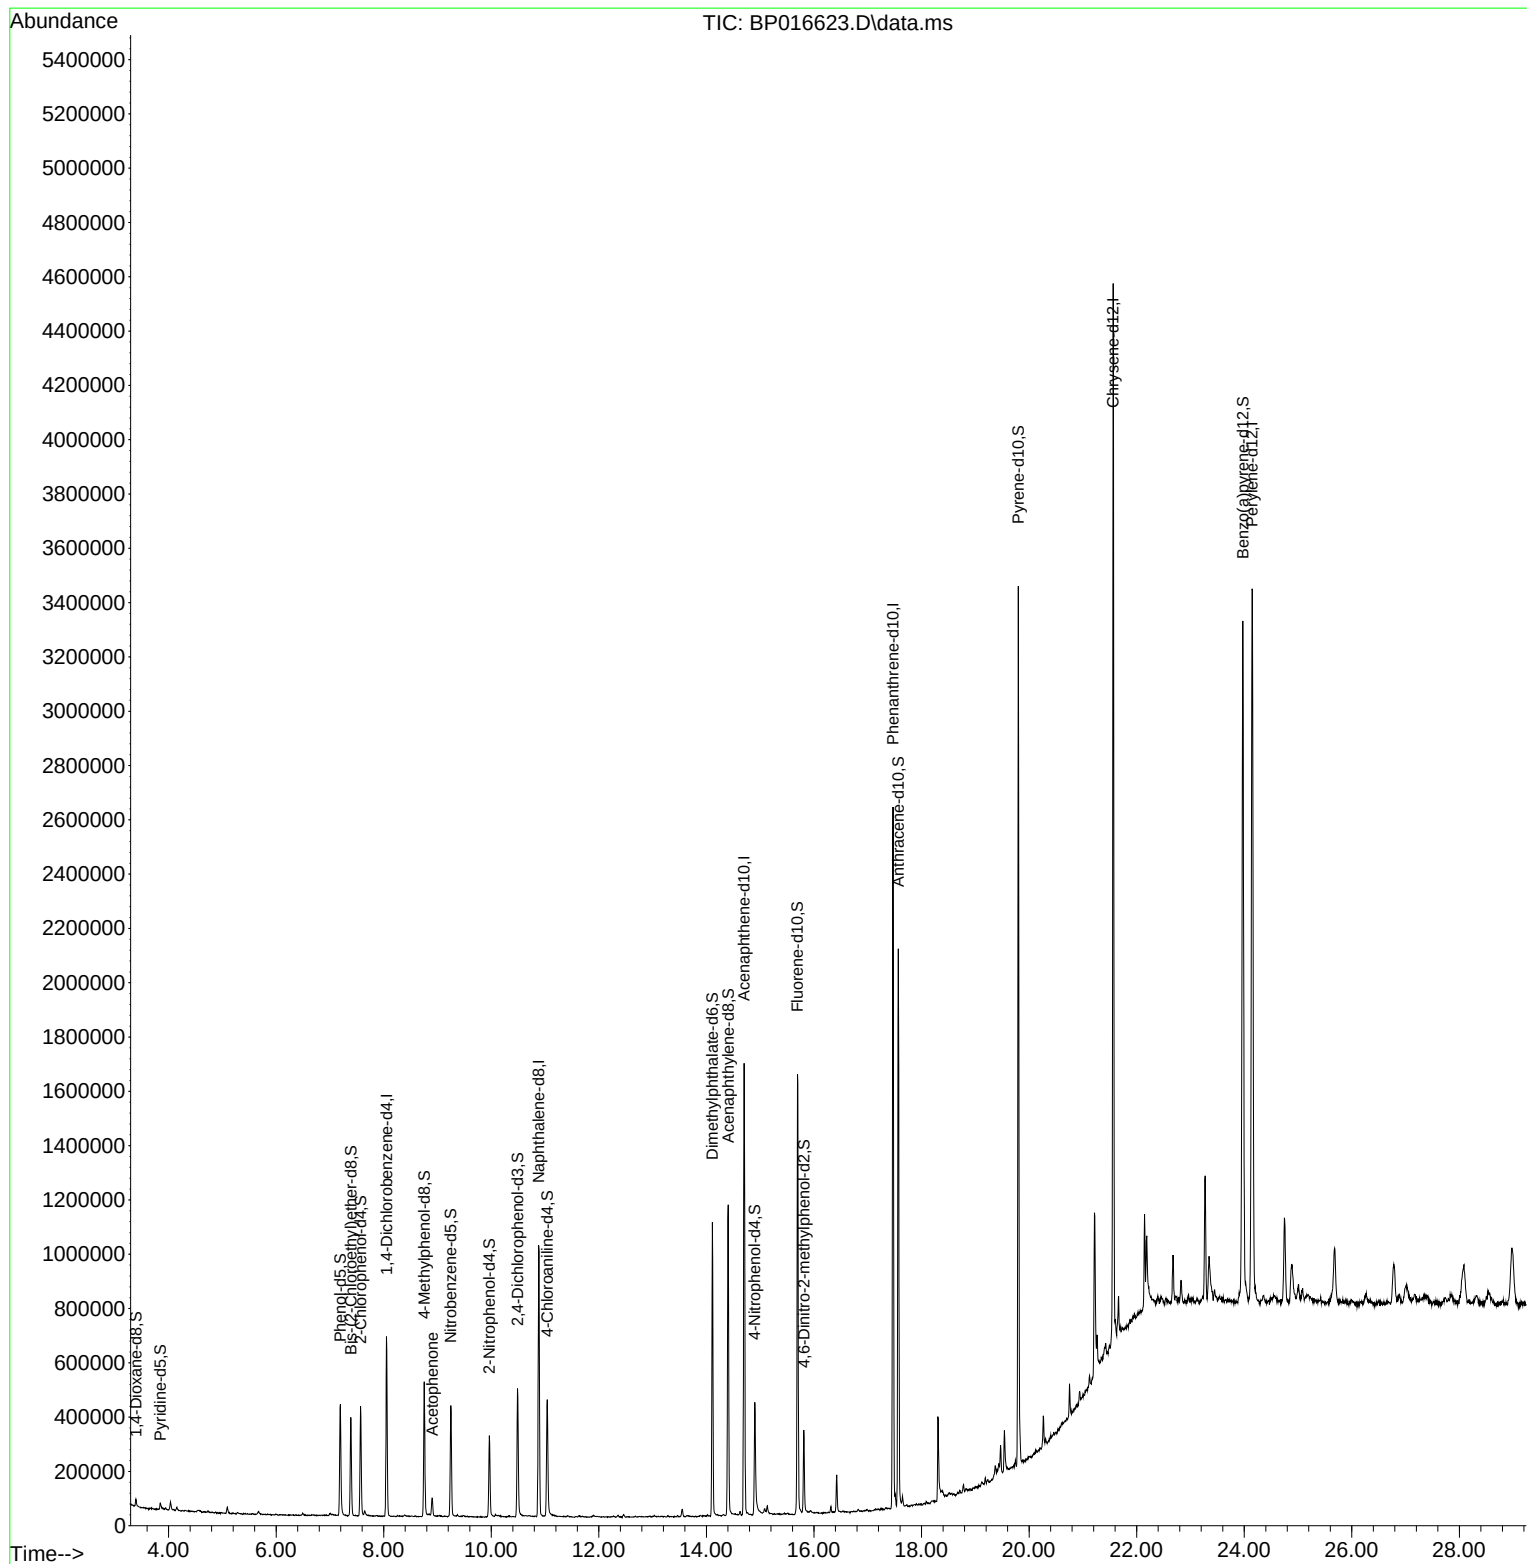

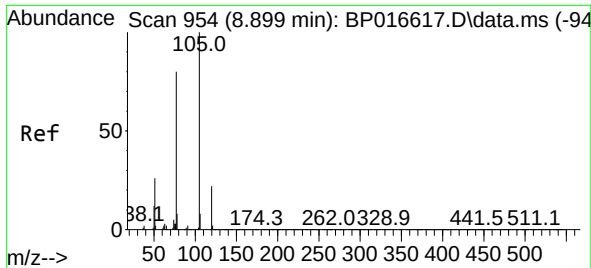

#16
 Acetophenone
 Concen: 1.788 ng/ul
 RT: 8.905 min Scan# 91
 Delta R.T. 0.006 min
 Lab File: BP016623.D
 Acq: 17 Aug 2023 03:11

Instrument :
 BNA_P
 ClientSampleId :
 A48M9

Tgt Ion:	105	Resp:	35777
Ion	Ratio	Lower	Upper
105	100		
77	83.9	64.4	96.6
51	28.7	21.2	31.8

