
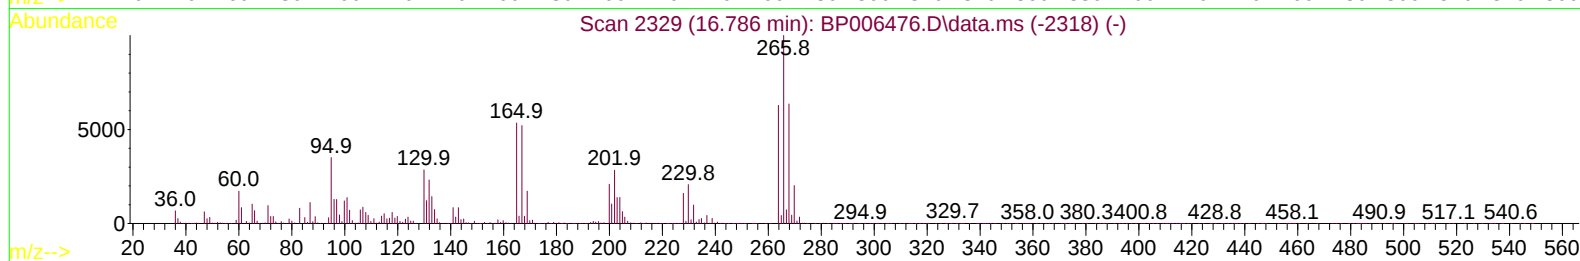
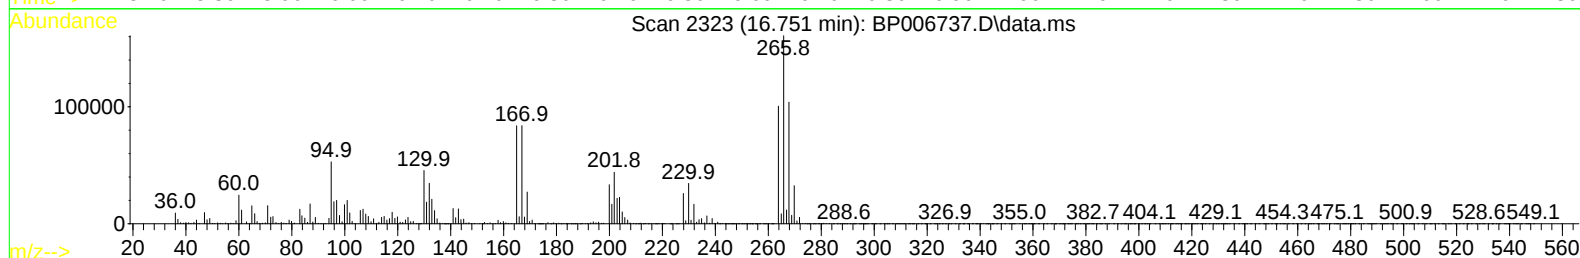


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006737.D
 Acq On : 18 Aug 2021 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 12:04:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 18:17:59 2021
 Response via : Initial Calibration

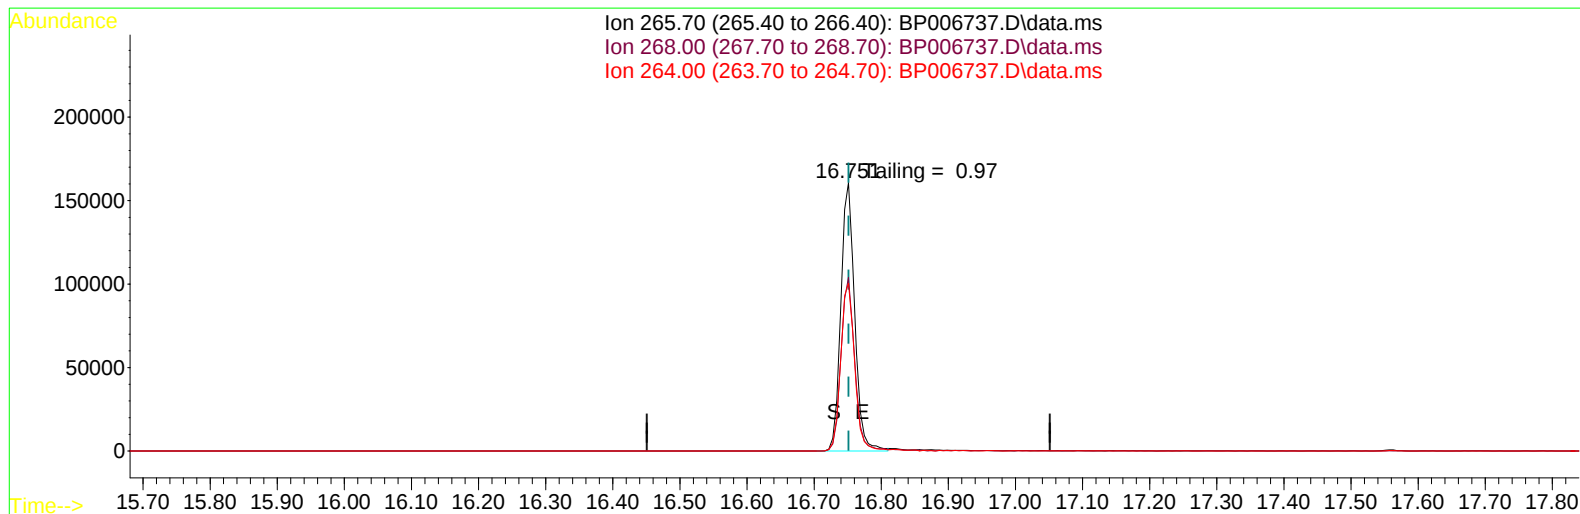

TIC: BP006737.D\data.ms

(70) Pentachlorophenol (C)




16.751min (+ 0.000) 1675779.11 ng

response 232188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.72
264.00	62.90	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006737.D
 Acq On : 18 Aug 2021 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 12:04:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 18:17:59 2021
 Response via : Initial Calibration

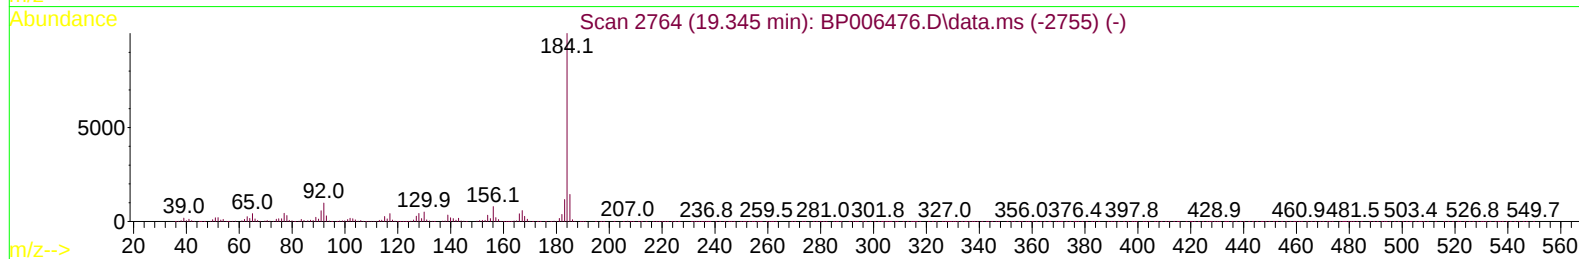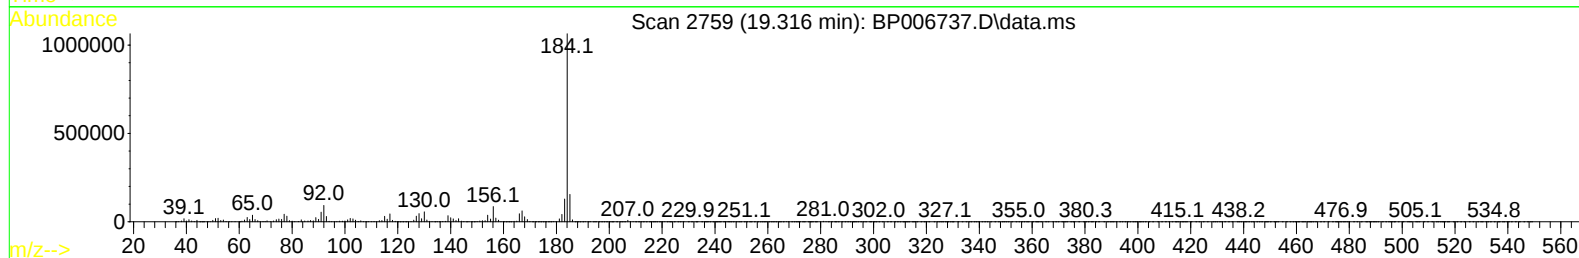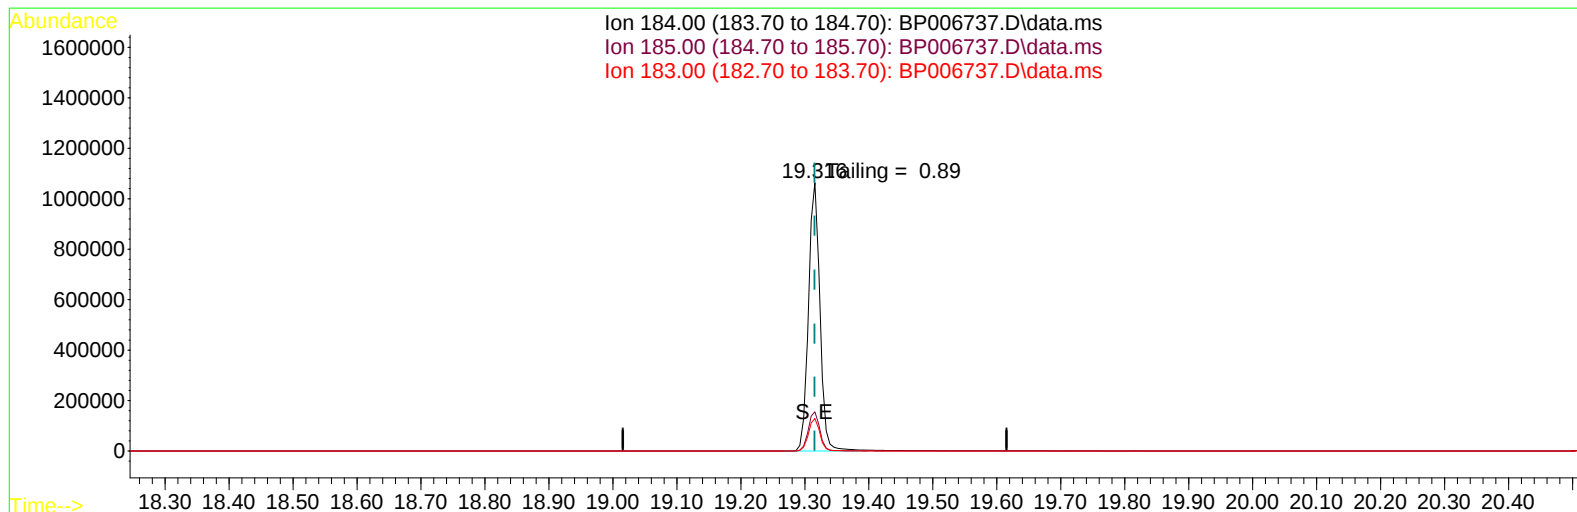

TIC: BP006737.D\data.ms

(77) Benzidine

19.316min (+ 0.000) 228781.44 ng

response 1345345

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.59
183.00	11.90	12.10
0.00	0.00	0.00