
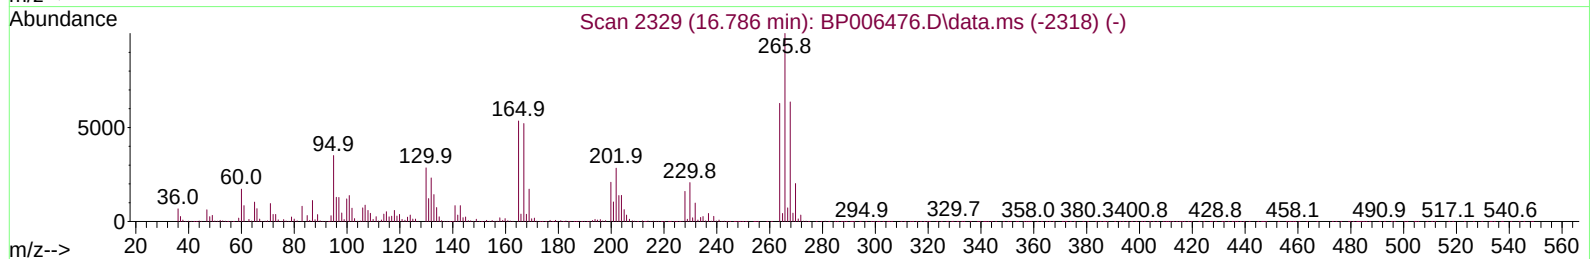
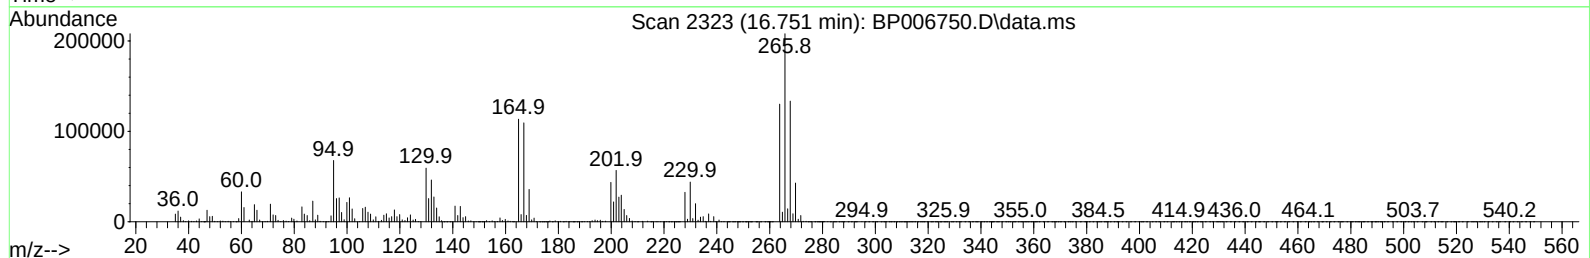


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081821\  
Data File : BP006750.D  
Acq On : 18 Aug 2021 18:17  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:17:22 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 16 18:17:59 2021  
Response via : Initial Calibration

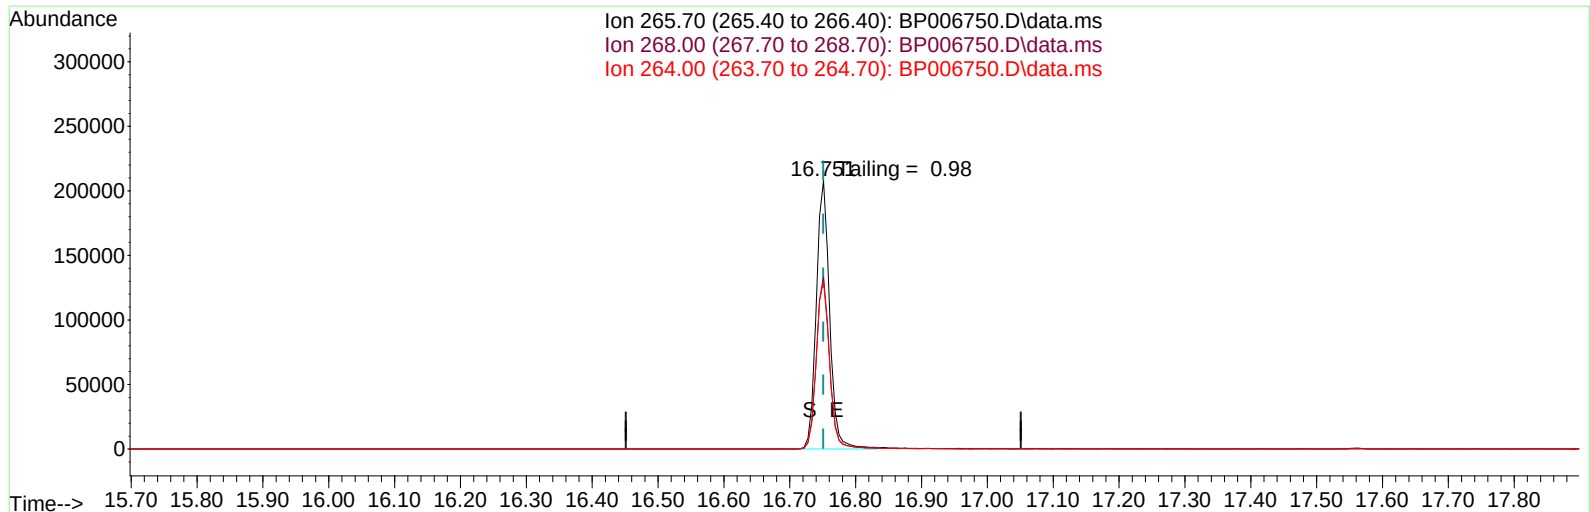

TIC: BP006750.D\data.ms

**(70) Pentachlorophenol (C)**




16.751min (+ 0.000) 229374.78 ng

response 293975

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 64.17  |
| 264.00 | 62.90  | 62.53  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081821\  
 Data File : BP006750.D  
 Acq On : 18 Aug 2021 18:17  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:17:22 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP080321.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 16 18:17:59 2021  
 Response via : Initial Calibration

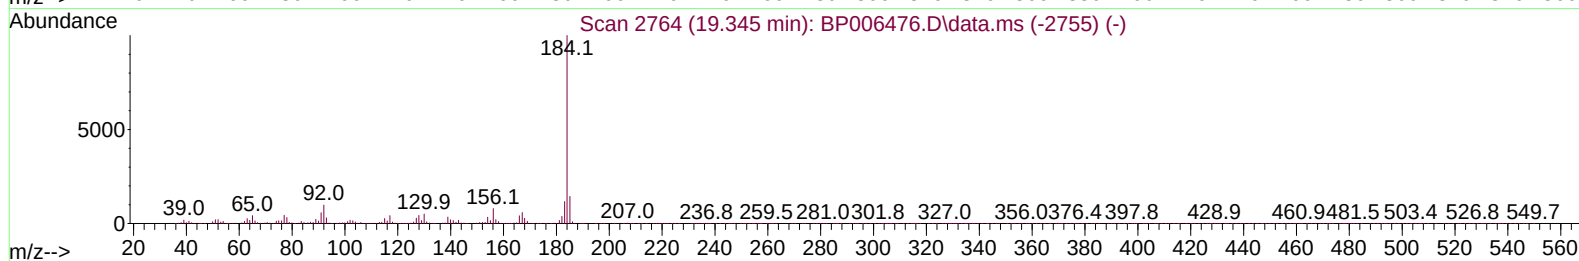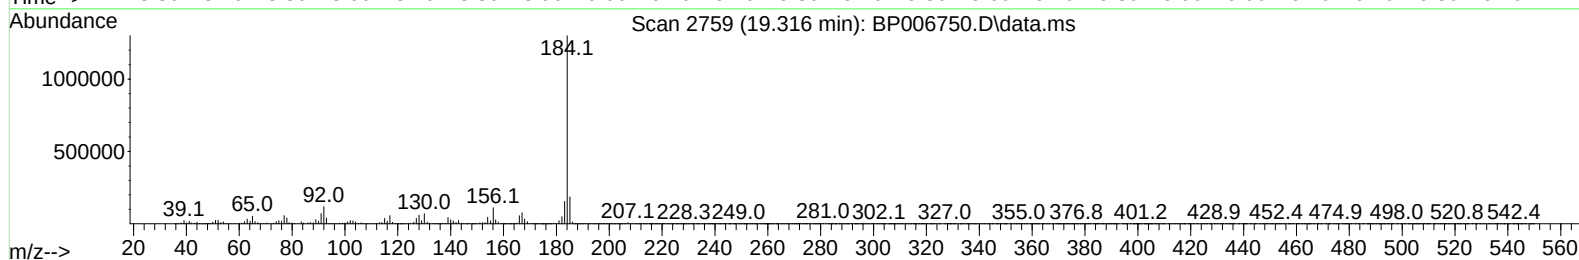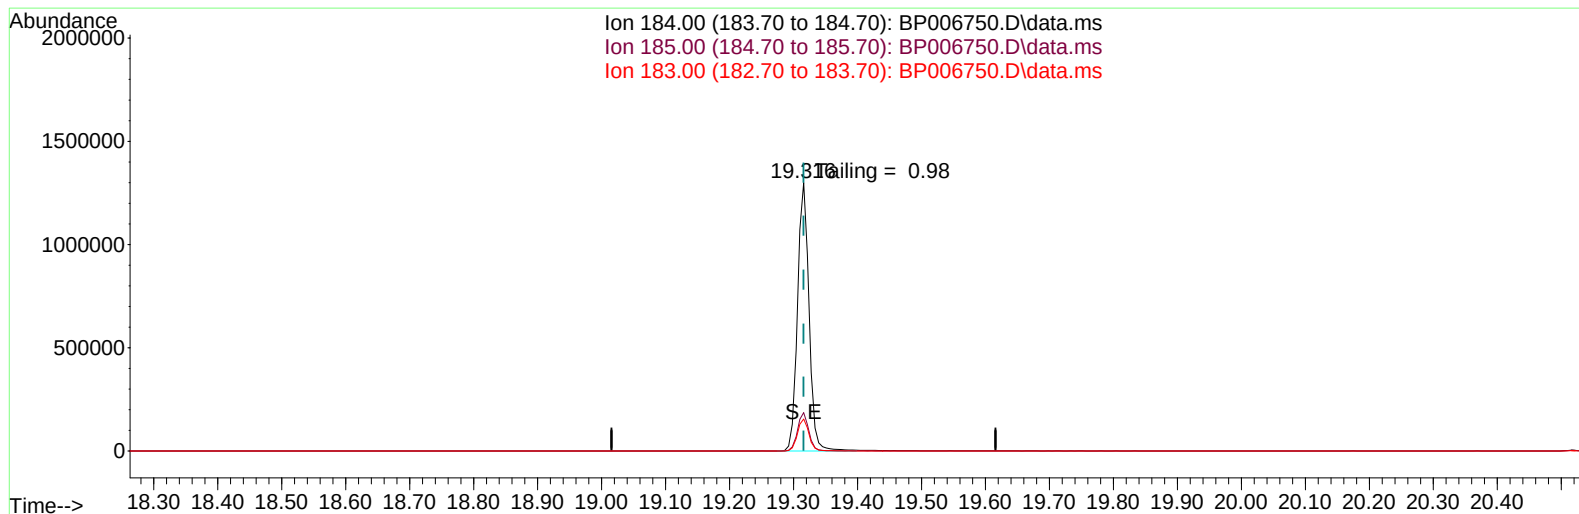

TIC: BP006750.D\data.ms

**(77) Benzidine**

19.316min (+ 0.000) 564119.53 ng

response 1637473

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.70  | 14.32  |
| 183.00 | 11.90  | 11.94  |
| 0.00   | 0.00   | 0.00   |