

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006739.D
 Acq On : 18 Aug 2021 11:34
 Operator : CG/JU
 Sample : PB138447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB138447BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	297	300	306	rVB	76220	108833	1.07%	0.240%
2	5.305	371	377	389	rVB	3457192	4839865	47.80%	10.683%
3	6.887	639	646	657	rBV	3182872	4910544	48.50%	10.839%
4	7.699	778	784	791	rBV	603027	932871	9.21%	2.059%
5	8.857	974	981	991	rBV	1979891	3251208	32.11%	7.176%
6	10.481	1250	1257	1268	rVB	783561	1291591	12.76%	2.851%
7	12.963	1671	1679	1693	rBV	4498470	6612181	65.30%	14.595%
8	14.339	1906	1913	1922	rBV	1084922	1598916	15.79%	3.529%
9	15.839	2161	2168	2183	rBV	3659954	5210967	51.47%	11.502%
10	17.098	2376	2382	2394	rVB	1363047	1903530	18.80%	4.202%
11	19.680	2816	2821	2827	rBV	8229031	10125101	100.00%	22.349%
12	20.169	2900	2904	2914	rBV3	62158	123163	1.22%	0.272%
13	21.204	3075	3080	3086	rBV	1712947	2076435	20.51%	4.583%
14	21.333	3098	3102	3106	rBV	97162	150604	1.49%	0.332%
15	23.515	3467	3473	3484	rVB2	1137245	2168679	21.42%	4.787%




Sum of corrected areas: 45304488

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006739.D
Acq On : 18 Aug 2021 11:34
Operator : CG/JU
Sample : PB138447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

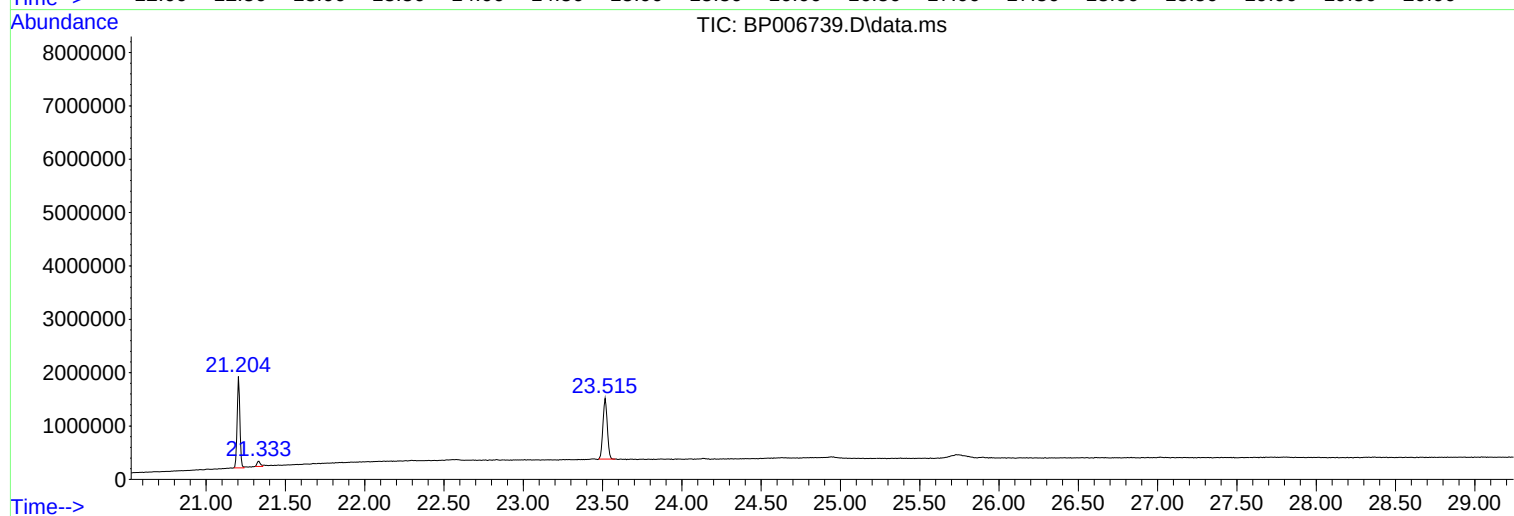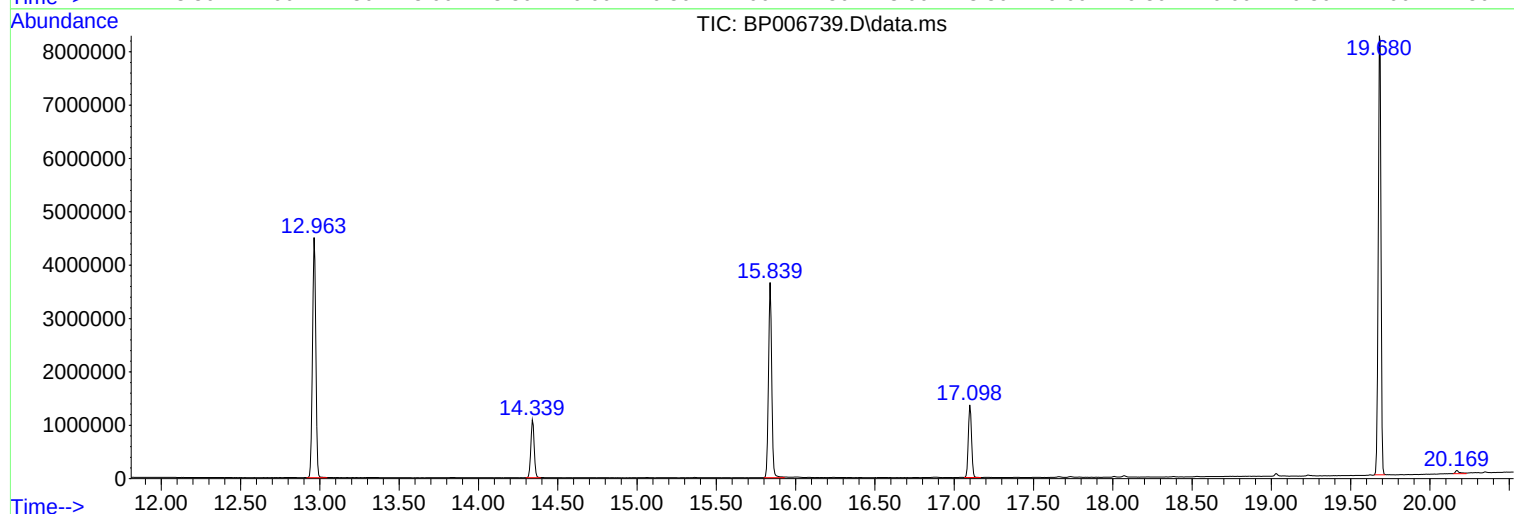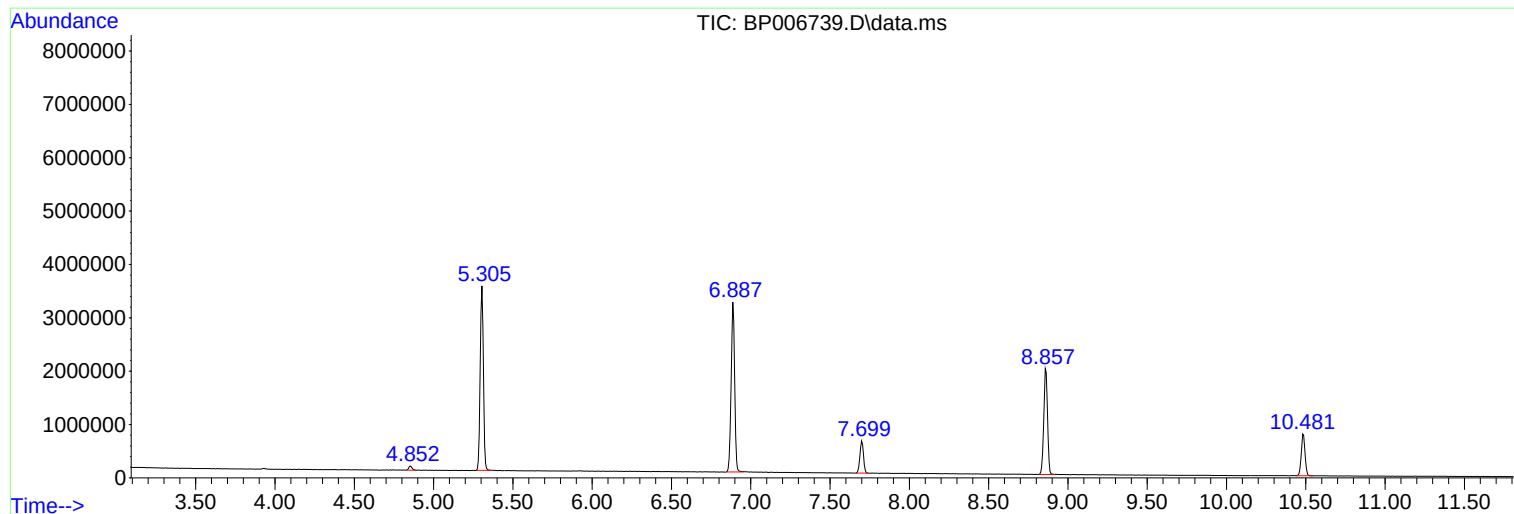

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006739.D
Acq On : 18 Aug 2021 11:34
Operator : CG/JU
Sample : PB138447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006739.D
Acq On : 18 Aug 2021 11:34
Operator : CG/JU
Sample : PB138447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------