

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006741.D
 Acq On : 18 Aug 2021 12:57
 Operator : CG/JU
 Sample : M3398-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-10-FD-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	305	rVB	177987	233904	3.08%	0.230%
2	5.305	371	377	389	rVB	2791874	3960170	52.08%	3.891%
3	6.887	639	646	656	rBV	2662718	4067879	53.50%	3.996%
4	7.699	778	784	792	rVB	585929	914066	12.02%	0.898%
5	8.858	974	981	991	rBV	1656859	2690159	35.38%	2.643%
6	10.287	1217	1224	1231	rBV	183364	356909	4.69%	0.351%
7	10.487	1251	1258	1266	rVB	742429	1261006	16.58%	1.239%
8	12.963	1672	1679	1689	rBV	3593288	5313721	69.88%	5.220%
9	13.428	1751	1758	1759	rBV	52749	78976	1.04%	0.078%
10	13.534	1766	1776	1778	rBV	187630	476454	6.27%	0.468%
11	13.693	1801	1803	1804	rBV	140372	115951	1.52%	0.114%
12	13.728	1807	1809	1811	rVV	148660	169687	2.23%	0.167%
13	13.793	1818	1820	1825	rVB	269350	277984	3.66%	0.273%
14	14.346	1908	1914	1927	rVB	997654	1573807	20.70%	1.546%
15	14.657	1949	1967	1968	rBV	72999	206859	2.72%	0.203%
16	15.181	2051	2056	2064	rBV	90289	137289	1.81%	0.135%
17	15.840	2159	2168	2179	rBV	3123049	4359872	57.34%	4.283%
18	16.516	2276	2283	2293	rBV6	47429	108732	1.43%	0.107%
19	17.104	2369	2383	2387	rBV	1380125	2420119	31.83%	2.378%
20	17.792	2495	2500	2505	rBV3	101487	151510	1.99%	0.149%
21	18.022	2529	2539	2568	rBV	2700619	4591896	60.39%	4.511%
22	18.281	2579	2583	2589	rBV2	114260	157550	2.07%	0.155%
23	18.904	2678	2689	2701	rBV2	1497118	4349177	57.20%	4.273%
24	19.063	2713	2716	2721	rBV	117401	151082	1.99%	0.148%
25	19.116	2721	2725	2726	rBV2	128698	150640	1.98%	0.148%
26	19.139	2726	2729	2737	rVB2	132246	250426	3.29%	0.246%
27	19.263	2742	2750	2770	rVB	4564285	6993721	91.98%	6.871%
28	19.686	2816	2822	2827	rBV	6299993	7603932	100.00%	7.470%
29	19.986	2865	2873	2883	rVB	2360473	4712994	61.98%	4.630%
30	20.310	2925	2928	2932	rBV	95281	126397	1.66%	0.124%
31	20.822	3008	3015	3024	rBV	2765540	5699022	74.95%	5.599%
32	20.945	3032	3036	3042	rBV2	262864	418567	5.50%	0.411%
33	20.998	3043	3045	3050	rVB	137740	154145	2.03%	0.151%
34	21.210	3076	3081	3085	rBV	1563754	2081638	27.38%	2.045%
35	21.545	3131	3138	3148	rBV	3085230	5673862	74.62%	5.574%
36	21.822	3182	3185	3187	rBV2	97835	114837	1.51%	0.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006741.D
Acq On : 18 Aug 2021 12:57
Operator : CG/JU
Sample : M3398-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-10-FD-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	22.328	3262	3271	3279	rBV	2361338	5995899	78.85%	5.890%
38	22.433	3283	3289	3301	rVV2	851873	2371192	31.18%	2.330%
39	22.551	3304	3309	3326	rVB4	629410	1656736	21.79%	1.628%
40	23.198	3410	3419	3428	rBV	1748314	4328726	56.93%	4.253%
41	23.522	3468	3474	3485	rVB2	1216192	2353674	30.95%	2.312%
42	24.210	3583	3591	3605	rVB	978416	2999440	39.45%	2.947%
43	25.045	3726	3733	3753	rVB6	685044	2741687	36.06%	2.693%
44	25.380	3783	3790	3802	rVB	704924	2162745	28.44%	2.125%
45	26.221	3926	3933	3948	rVB	851093	2925427	38.47%	2.874%
46	26.757	4017	4024	4047	rVB2	548283	2149102	28.26%	2.111%




Sum of corrected areas: 101789568

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006741.D
Acq On : 18 Aug 2021 12:57
Operator : CG/JU
Sample : M3398-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-10-FD-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

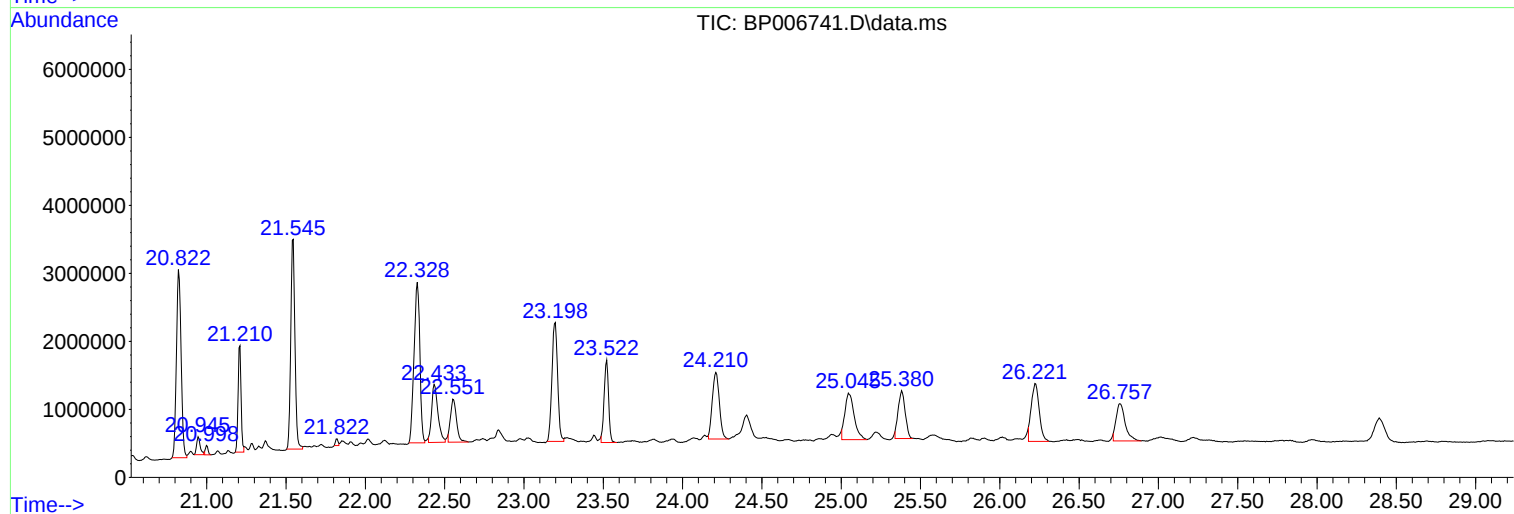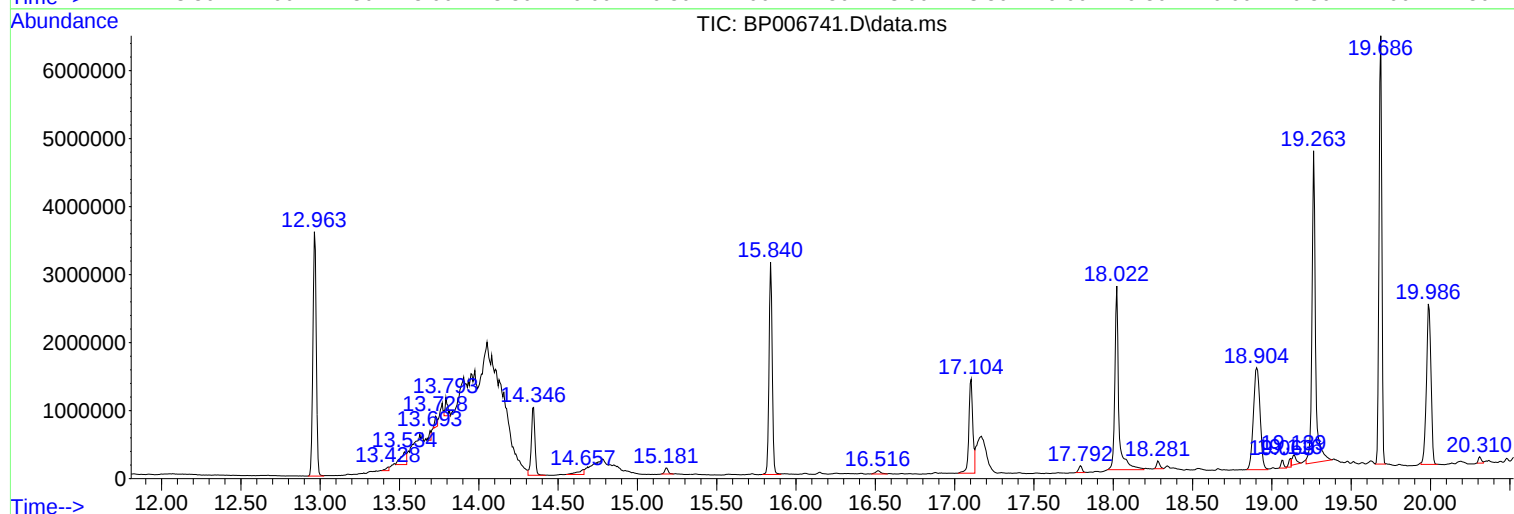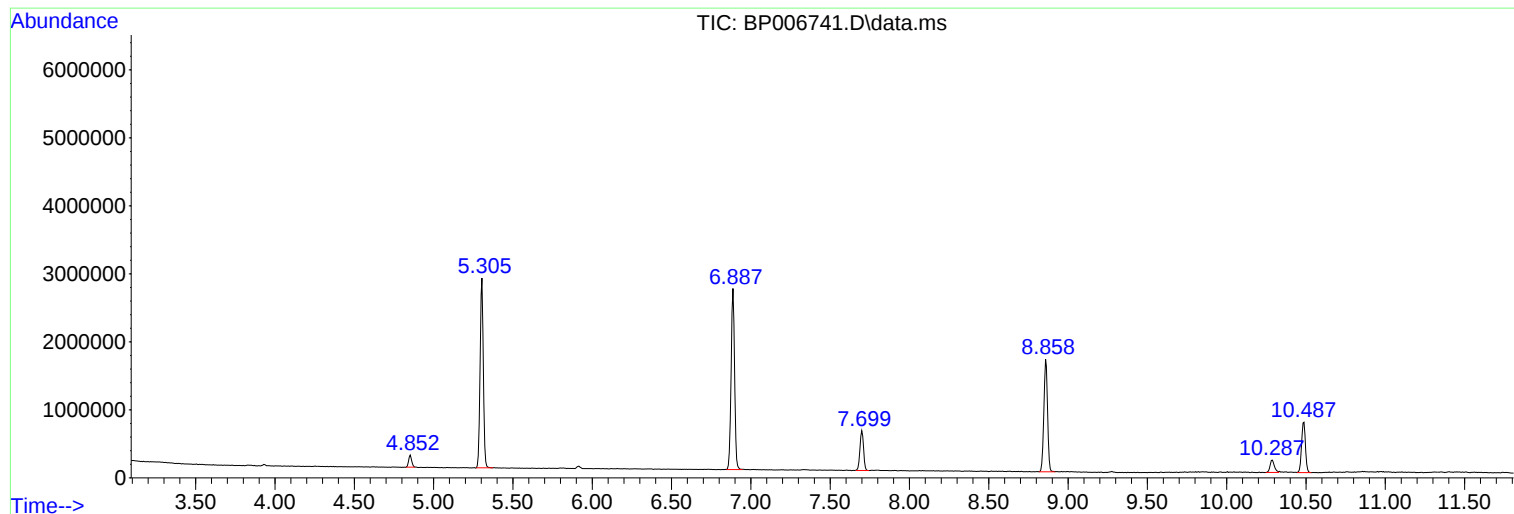

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006741.D
Acq On : 18 Aug 2021 12:57
Operator : CG/JU
Sample : M3398-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-10-FD-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006741.D
Acq On : 18 Aug 2021 12:57
Operator : CG/JU
Sample : M3398-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-10-FD-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------