

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006754.D
 Acq On : 18 Aug 2021 20:34
 Operator : CG/JU
 Sample : M3435-21
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-26-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	297	300	308	rVB	69398	103527	1.51%	0.250%
2	5.305	371	377	386	rVB	2501871	3591844	52.33%	8.673%
3	6.887	639	646	662	rVB	2406777	3793589	55.27%	9.160%
4	7.699	778	784	792	rVB	651807	998157	14.54%	2.410%
5	8.858	974	981	994	rBV	1546440	2456294	35.79%	5.931%
6	10.281	1216	1223	1238	rBV	922385	1632057	23.78%	3.941%
7	10.481	1250	1257	1267	rVB	866428	1412275	20.58%	3.410%
8	12.963	1669	1679	1694	rBV	3476317	4986733	72.66%	12.041%
9	13.252	1721	1728	1737	rBV	170899	296772	4.32%	0.717%
10	14.340	1903	1913	1921	rBV	1245810	1746384	25.45%	4.217%
11	15.840	2157	2168	2178	rBV	2601874	3823277	55.71%	9.232%
12	17.098	2376	2382	2388	rBV	1405489	1967477	28.67%	4.751%
13	17.792	2496	2500	2506	rBV	165115	190320	2.77%	0.460%
14	18.010	2532	2537	2544	rBV	175986	258448	3.77%	0.624%
15	18.934	2690	2694	2698	rVB	443765	500018	7.29%	1.207%
16	19.063	2712	2716	2721	rBV	124517	132483	1.93%	0.320%
17	19.251	2744	2748	2757	rVB	63657	91475	1.33%	0.221%
18	19.681	2815	2821	2826	rBV	5842843	6863361	100.00%	16.572%
19	19.992	2868	2874	2877	rBV2	47138	75252	1.10%	0.182%
20	20.939	3031	3035	3043	rBV	408994	732563	10.67%	1.769%
21	21.204	3075	3080	3085	rBV	1734314	2112096	30.77%	5.100%
22	21.328	3098	3101	3105	rBV	96738	127396	1.86%	0.308%
23	21.816	3180	3184	3186	rBV	155456	196324	2.86%	0.474%
24	21.845	3186	3189	3195	rVB	196841	332691	4.85%	0.803%
25	22.833	3352	3357	3362	rVB	324372	481218	7.01%	1.162%
26	23.516	3467	3473	3483	rVB2	1146924	2221785	32.37%	5.365%
27	23.769	3514	3516	3525	rVB3	185069	291428	4.25%	0.704%




Sum of corrected areas: 41415244

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006754.D
Acq On : 18 Aug 2021 20:34
Operator : CG/JU
Sample : M3435-21
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-26-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

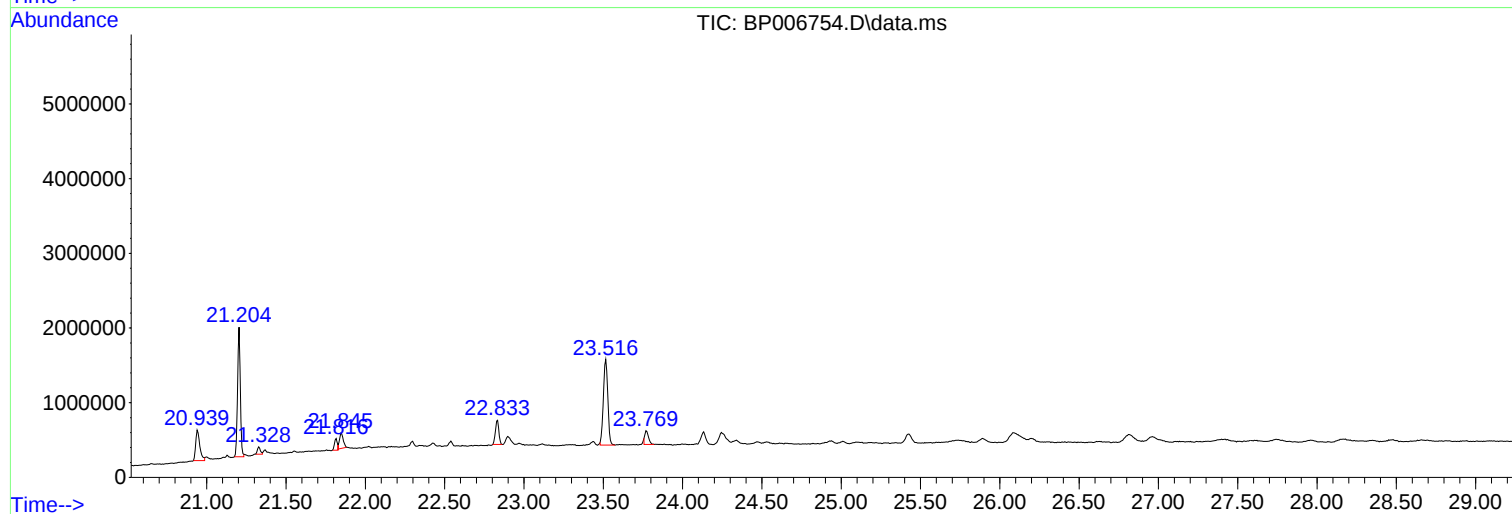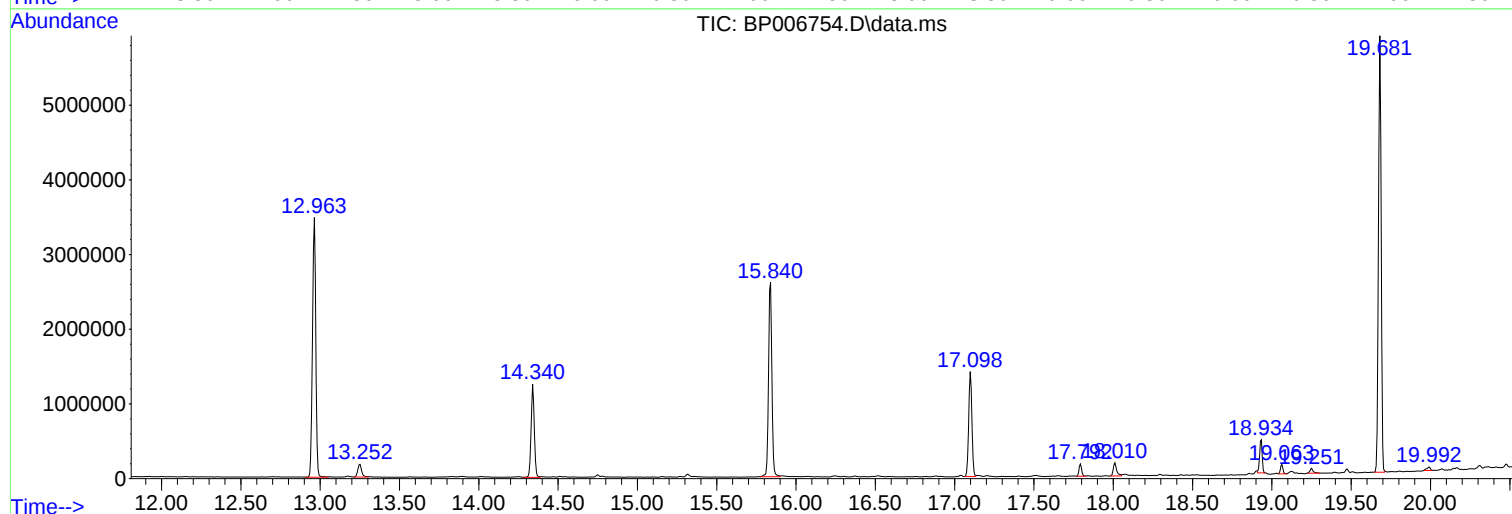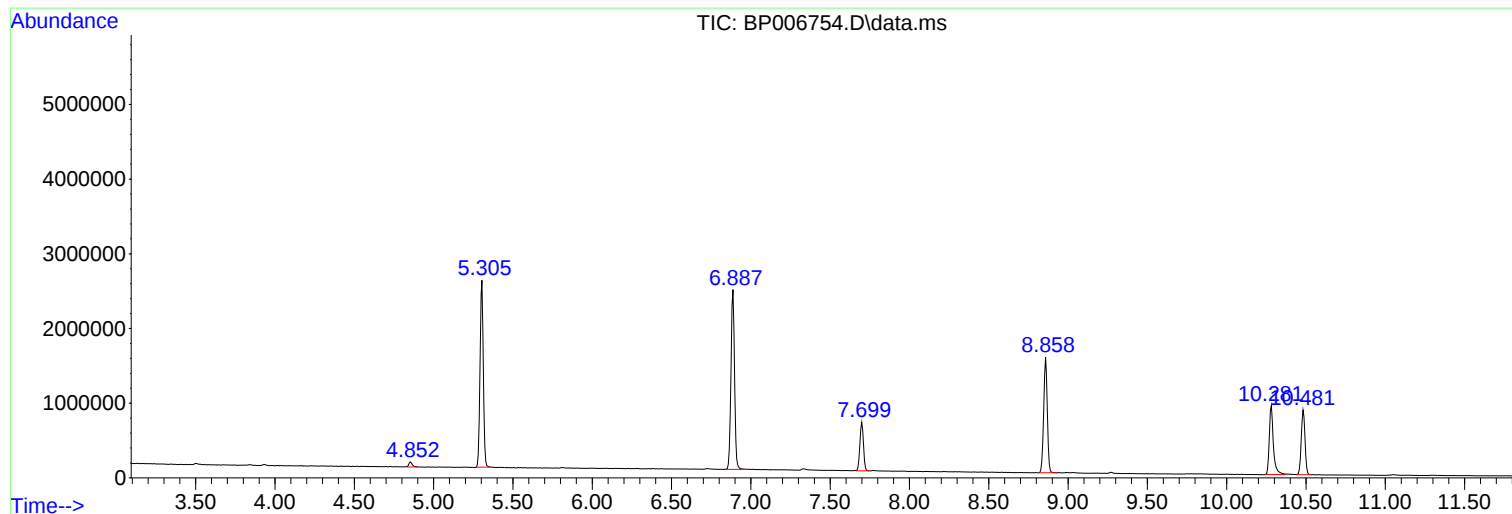

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006754.D
Acq On : 18 Aug 2021 20:34
Operator : CG/JU
Sample : M3435-21
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-26-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006754.D
Acq On : 18 Aug 2021 20:34
Operator : CG/JU
Sample : M3435-21
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-26-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------