

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006755.D
 Acq On : 18 Aug 2021 21:08
 Operator : CG/JU
 Sample : M3419-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-08-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	309	rVB	211452	296506	4.52%	0.830%
2	5.305	371	377	387	rVB	2197660	3184344	48.53%	8.918%
3	6.887	639	646	657	rBV	2145944	3374177	51.43%	9.449%
4	7.699	778	784	791	rVB	670148	1015466	15.48%	2.844%
5	8.858	974	981	994	rVB	1405356	2285982	34.84%	6.402%
6	10.281	1217	1223	1235	rBV	250470	492837	7.51%	1.380%
7	10.481	1250	1257	1269	rVB	887522	1452576	22.14%	4.068%
8	12.963	1672	1679	1693	rBV	3278797	4728807	72.07%	13.243%
9	14.340	1906	1913	1925	rBV	1242533	1796260	27.38%	5.030%
10	15.840	2157	2168	2187	rBV	2296606	3405509	51.91%	9.537%
11	17.098	2375	2382	2394	rBV	1456593	2045313	31.17%	5.728%
12	17.792	2495	2500	2504	rBV	57909	67776	1.03%	0.190%
13	18.010	2532	2537	2543	rBV	70141	109830	1.67%	0.308%
14	19.681	2815	2821	2832	rBV	5704944	6560991	100.00%	18.374%
15	20.945	3031	3036	3042	rBV3	156375	299603	4.57%	0.839%
16	21.204	3075	3080	3087	rBV	1734951	2156816	32.87%	6.040%
17	21.327	3098	3101	3105	rBV	93342	126732	1.93%	0.355%
18	23.516	3466	3473	3483	rVB2	1204883	2308221	35.18%	6.464%




Sum of corrected areas: 35707746

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006755.D
Acq On : 18 Aug 2021 21:08
Operator : CG/JU
Sample : M3419-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

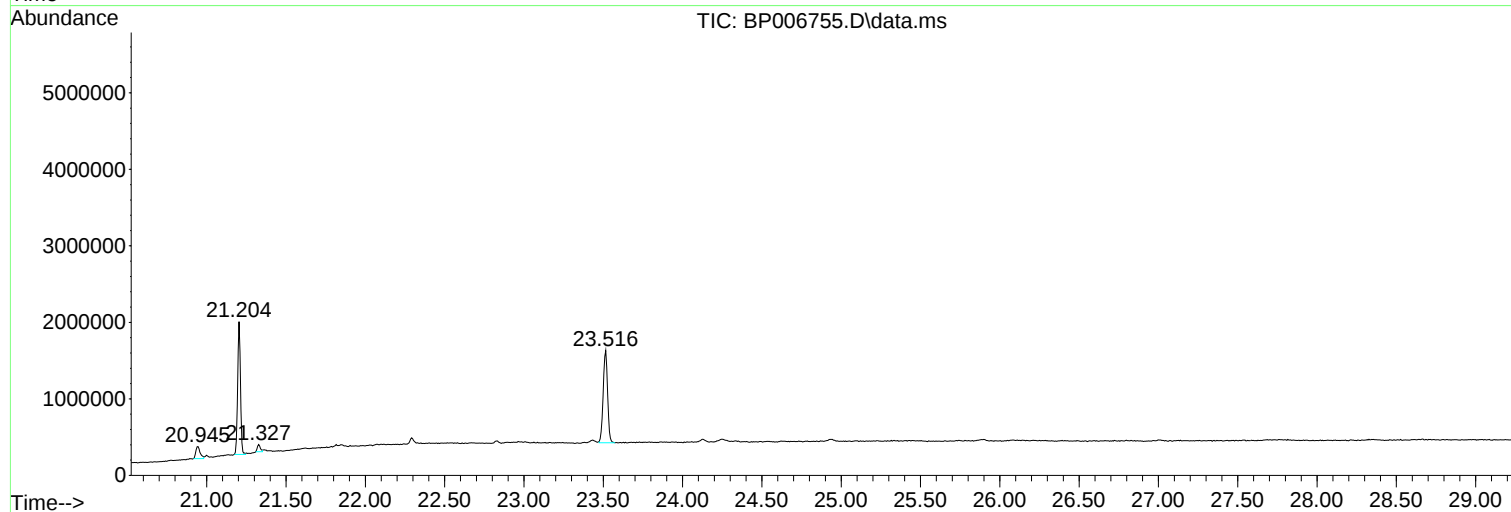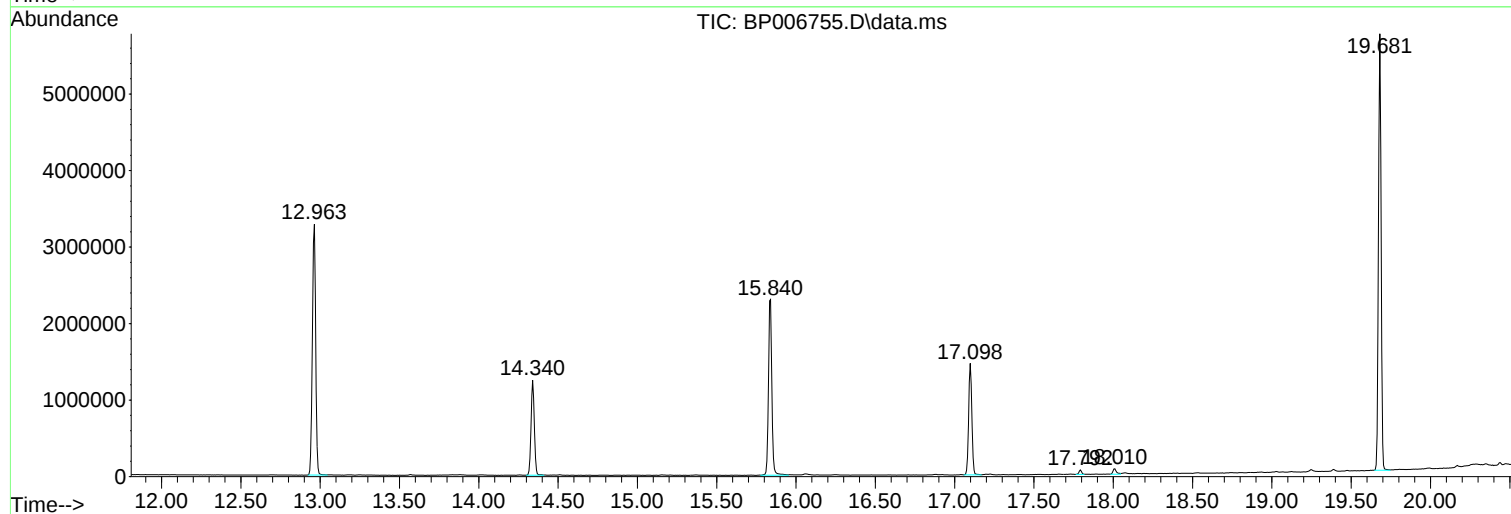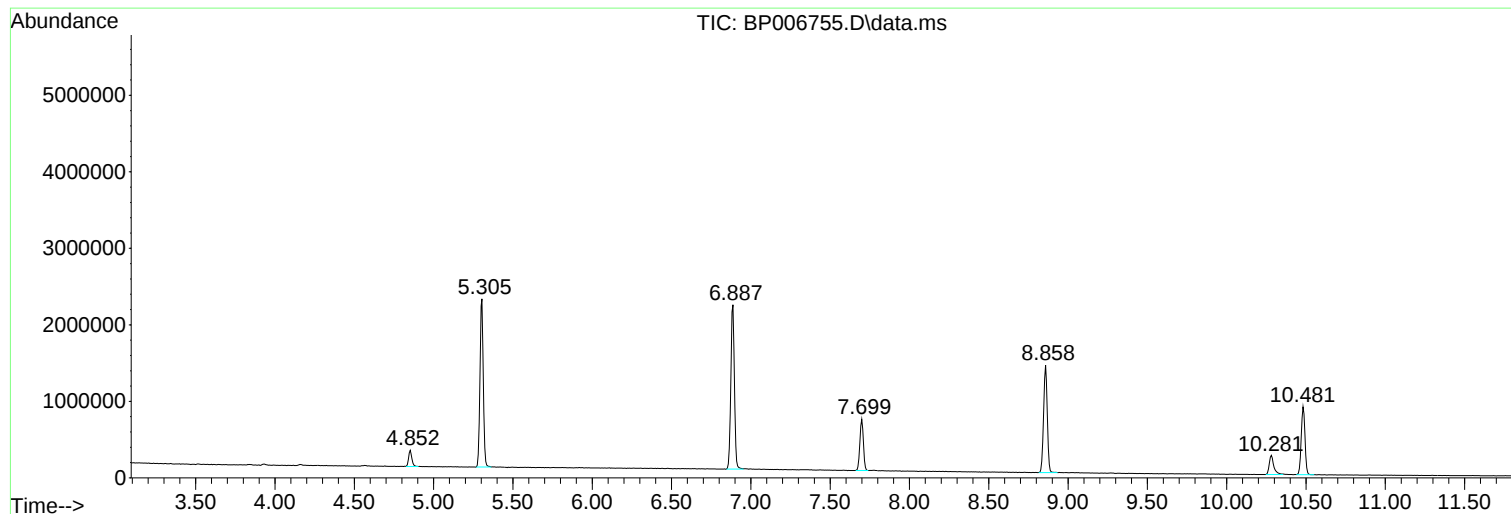

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006755.D
Acq On : 18 Aug 2021 21:08
Operator : CG/JU
Sample : M3419-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006755.D
Acq On : 18 Aug 2021 21:08
Operator : CG/JU
Sample : M3419-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc