

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006756.D
 Acq On : 18 Aug 2021 21:42
 Operator : CG/JU
 Sample : M3435-25
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-28-0003

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	297	300	307	rVB	55298	82388	1.23%	0.206%
2	5.305	371	377	392	rVB	2698849	3830490	57.34%	9.595%
3	6.887	639	646	659	rBV	2547956	3975004	59.50%	9.957%
4	7.699	778	784	790	rVB	640982	984138	14.73%	2.465%
5	8.857	974	981	990	rVB	1611556	2592552	38.81%	6.494%
6	9.904	1154	1159	1165	rVB	73376	119273	1.79%	0.299%
7	10.281	1218	1223	1239	rVB2	45320	111403	1.67%	0.279%
8	10.481	1250	1257	1266	rVB	857699	1405578	21.04%	3.521%
9	12.963	1671	1679	1690	rBV	3488529	5119658	76.63%	12.824%
10	13.657	1790	1797	1804	rBV	244091	342443	5.13%	0.858%
11	14.340	1907	1913	1920	rVB	1178122	1702561	25.48%	4.265%
12	15.839	2153	2168	2188	rBV	2619712	3983488	59.63%	9.978%
13	17.098	2375	2382	2388	rBV	1442024	1936791	28.99%	4.851%
14	17.951	2522	2527	2533	rBV2	120746	174916	2.62%	0.438%
15	18.010	2533	2537	2545	rBV	252612	341015	5.10%	0.854%
16	19.251	2744	2748	2759	rVB	101314	136070	2.04%	0.341%
17	19.680	2815	2821	2827	rBV	5850341	6680730	100.00%	16.735%
18	20.939	3031	3035	3042	rBV2	235006	421849	6.31%	1.057%
19	21.204	3075	3080	3086	rBV	1685082	2069046	30.97%	5.183%
20	21.327	3098	3101	3104	rBV	88353	113117	1.69%	0.283%
21	22.427	3284	3288	3295	rVB	186625	253486	3.79%	0.635%
22	22.827	3353	3356	3363	rVB	145875	212901	3.19%	0.533%
23	23.516	3466	3473	3481	rVB2	1117079	2177777	32.60%	5.455%
24	24.127	3572	3577	3585	rVB	565269	1155094	17.29%	2.893%




Sum of corrected areas: 39921768

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006756.D
Acq On : 18 Aug 2021 21:42
Operator : CG/JU
Sample : M3435-25
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-28-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

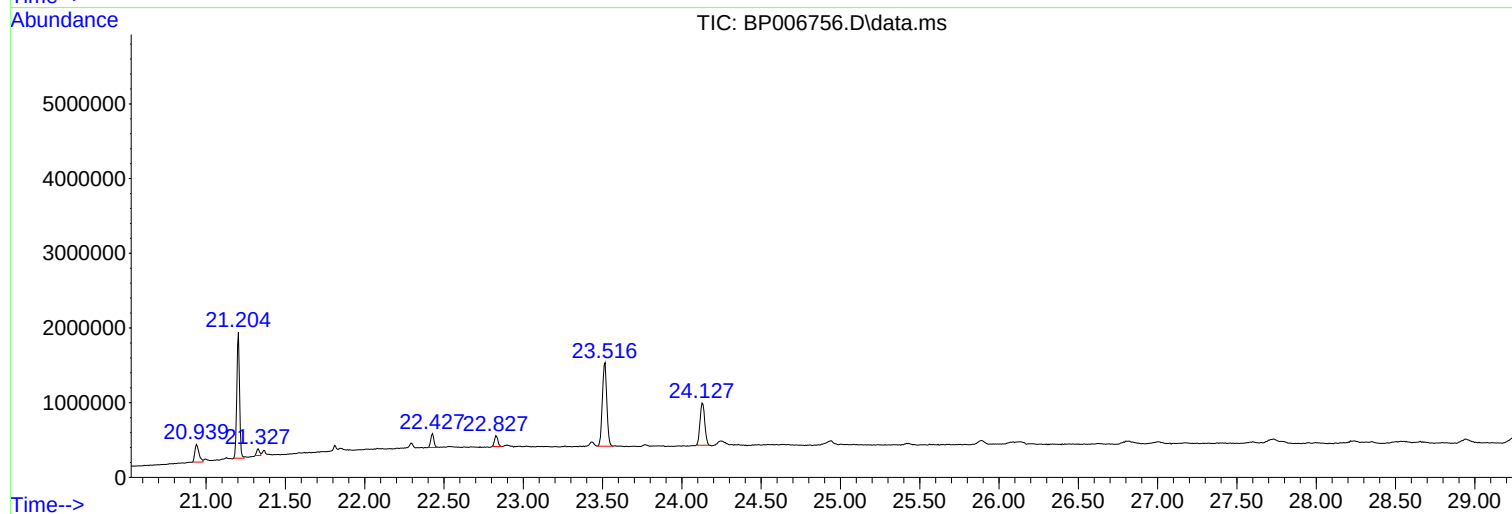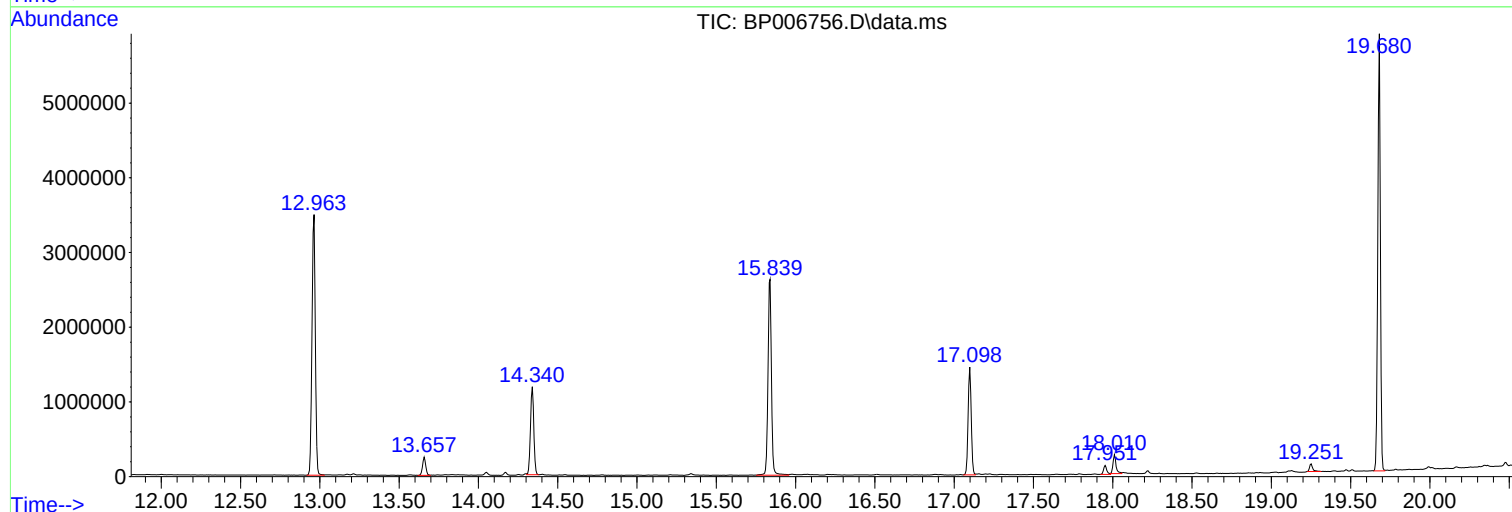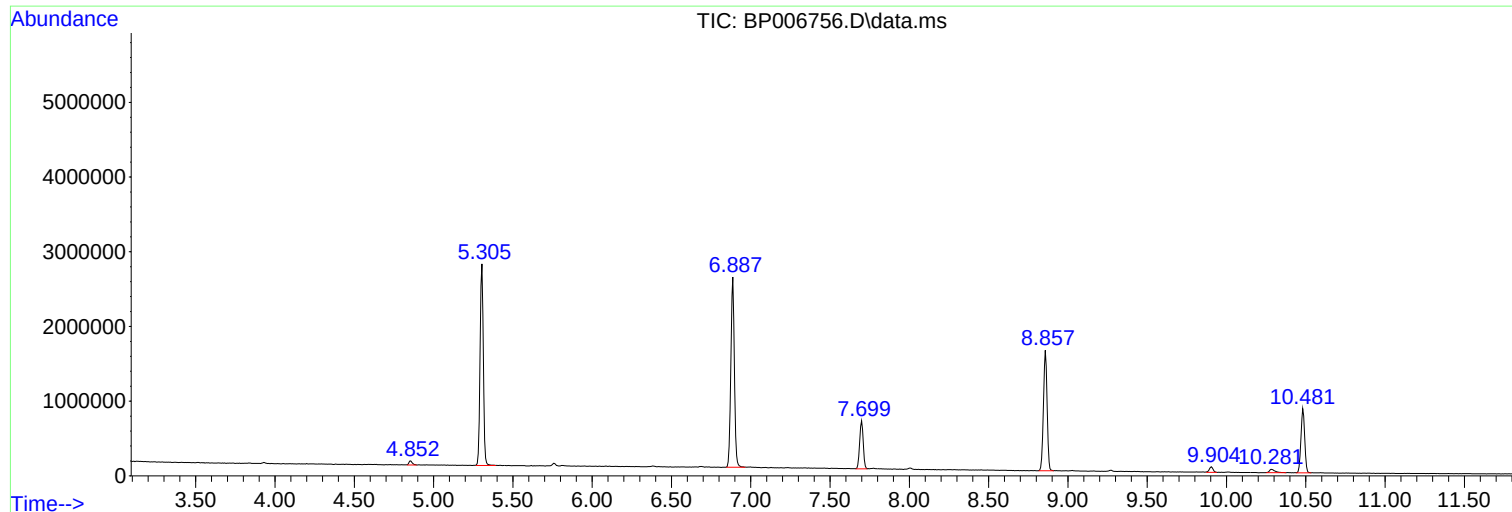

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006756.D
Acq On : 18 Aug 2021 21:42
Operator : CG/JU
Sample : M3435-25
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-28-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006756.D
Acq On : 18 Aug 2021 21:42
Operator : CG/JU
Sample : M3435-25
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-28-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
