

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006757.D
 Acq On : 18 Aug 2021 22:16
 Operator : CG/JU
 Sample : M3435-23
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-26-0306

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.305	371	377	386	rVB	2316513	3374245	64.88%	10.164%
2	6.887	639	646	657	rBV	2209017	3518690	67.66%	10.599%
3	7.699	778	784	793	rVB	612398	959193	18.44%	2.889%
4	8.857	974	981	994	rVB	1438738	2308040	44.38%	6.952%
5	10.281	1218	1223	1238	rVB	92447	195624	3.76%	0.589%
6	10.481	1250	1257	1269	rVB	833288	1363189	26.21%	4.106%
7	12.963	1670	1679	1693	rBV	2972930	4399497	84.60%	13.252%
8	14.340	1905	1913	1923	rBV	1163703	1682913	32.36%	5.069%
9	15.834	2159	2167	2188	rBV	2353448	3471948	66.76%	10.458%
10	17.098	2375	2382	2392	rBV	1369974	1887048	36.29%	5.684%
11	18.010	2531	2537	2543	rBV	128841	193863	3.73%	0.584%
12	19.245	2743	2747	2753	rBV	71600	100521	1.93%	0.303%
13	19.680	2815	2821	2827	rBV	4305503	5200579	100.00%	15.665%
14	20.939	3031	3035	3041	rBV2	134515	228140	4.39%	0.687%
15	21.198	3074	3079	3084	rBV	1626571	2013198	38.71%	6.064%
16	21.327	3097	3101	3104	rBV	97908	139503	2.68%	0.420%
17	23.510	3465	3472	3484	rVB2	1094961	2162052	41.57%	6.513%




Sum of corrected areas: 33198243

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006757.D
Acq On : 18 Aug 2021 22:16
Operator : CG/JU
Sample : M3435-23
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-26-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

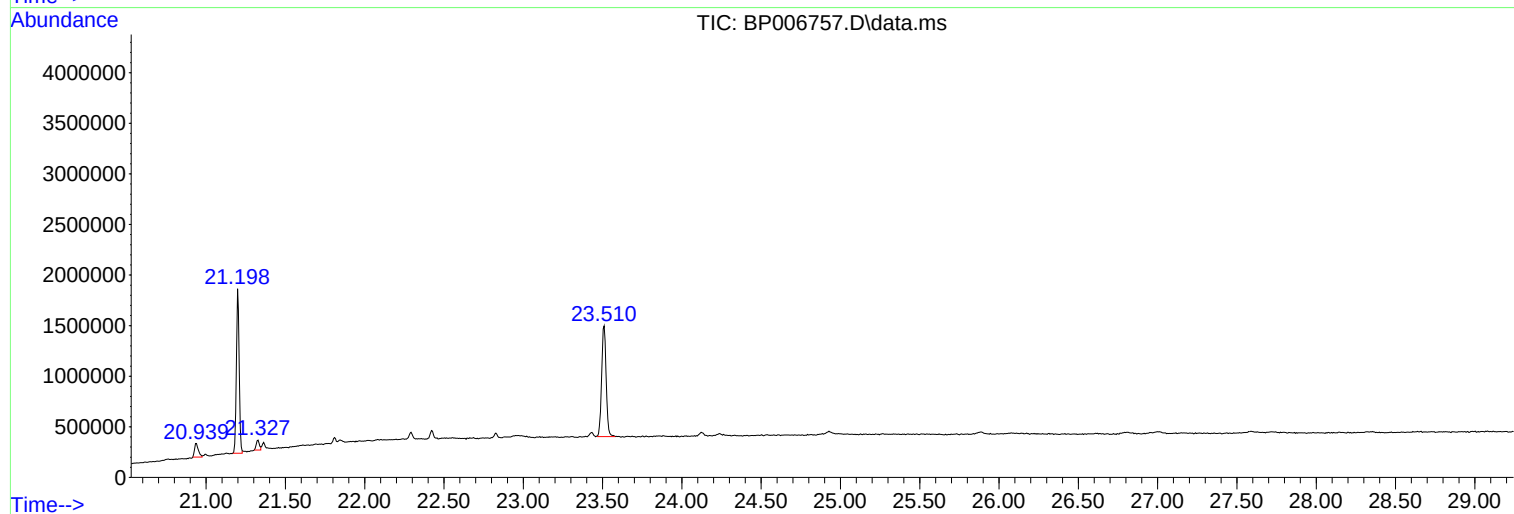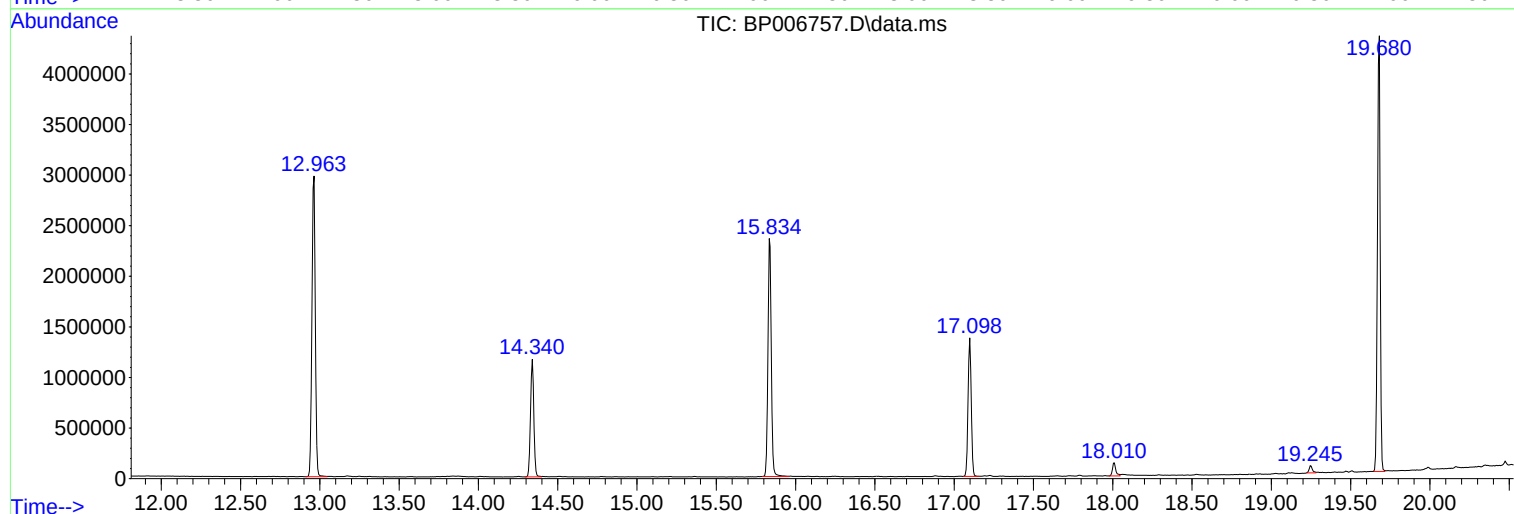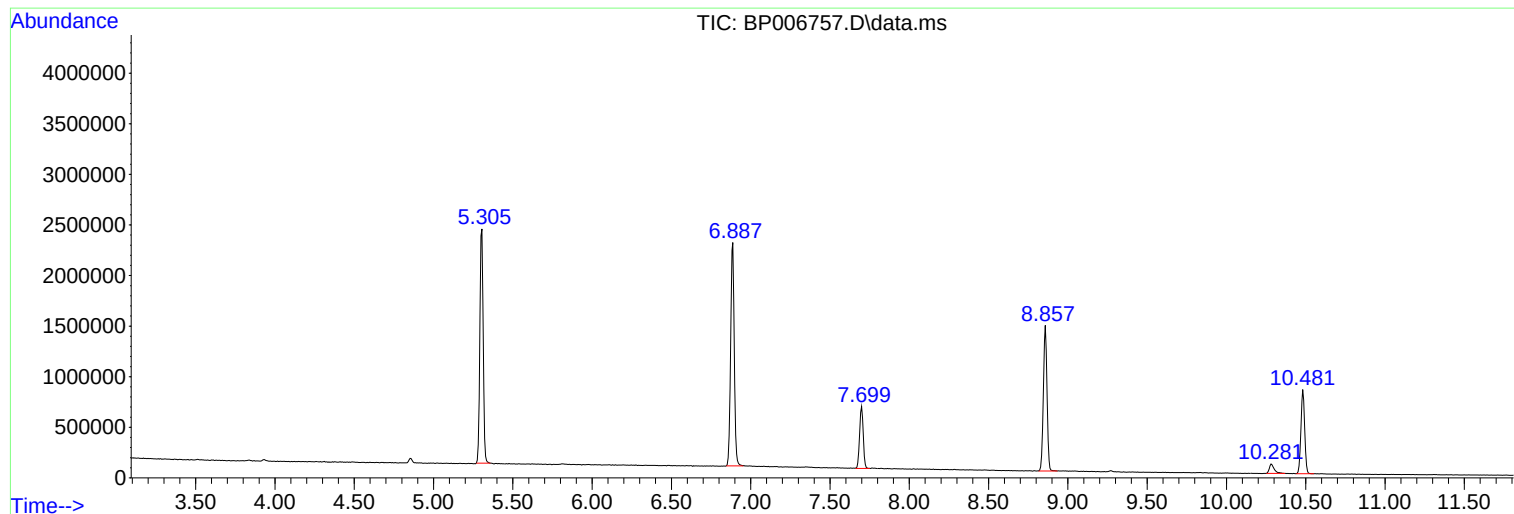

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006757.D
Acq On : 18 Aug 2021 22:16
Operator : CG/JU
Sample : M3435-23
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-26-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006757.D
Acq On : 18 Aug 2021 22:16
Operator : CG/JU
Sample : M3435-23
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-26-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------