

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006758.D
 Acq On : 18 Aug 2021 22:51
 Operator : CG/JU
 Sample : M3419-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-08-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	298	300	306	rVB	43237	52565	1.02%	0.177%
2	5.304	371	377	388	rVB	1763709	2627937	50.99%	8.868%
3	6.881	639	645	658	rBV	1715868	2753905	53.44%	9.293%
4	7.698	778	784	793	rVB	607339	931426	18.07%	3.143%
5	8.857	974	981	991	rBV	1136929	1817127	35.26%	6.132%
6	10.281	1217	1223	1242	rBV	154871	324745	6.30%	1.096%
7	10.481	1250	1257	1264	rVB	799383	1304926	25.32%	4.404%
8	12.963	1671	1679	1694	rBV	2556982	3742962	72.63%	12.631%
9	14.339	1905	1913	1929	rBV	1113345	1623673	31.51%	5.479%
10	15.833	2157	2167	2189	rBV	1885651	2810902	54.54%	9.486%
11	17.098	2375	2382	2394	rBV	1309508	1838533	35.67%	6.204%
12	18.004	2531	2536	2544	rBV	110283	168748	3.27%	0.569%
13	19.245	2743	2747	2753	rBV3	49621	65218	1.27%	0.220%
14	19.680	2815	2821	2826	rBV	4217209	5153680	100.00%	17.391%
15	20.939	3031	3035	3042	rBV3	173846	310919	6.03%	1.049%
16	21.204	3075	3080	3086	rBV	1567132	1945931	37.76%	6.567%
17	21.327	3098	3101	3105	rBV	78814	98914	1.92%	0.334%
18	23.515	3466	3473	3481	rVB2	1076753	2061439	40.00%	6.956%




Sum of corrected areas: 29633550

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006758.D
Acq On : 18 Aug 2021 22:51
Operator : CG/JU
Sample : M3419-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

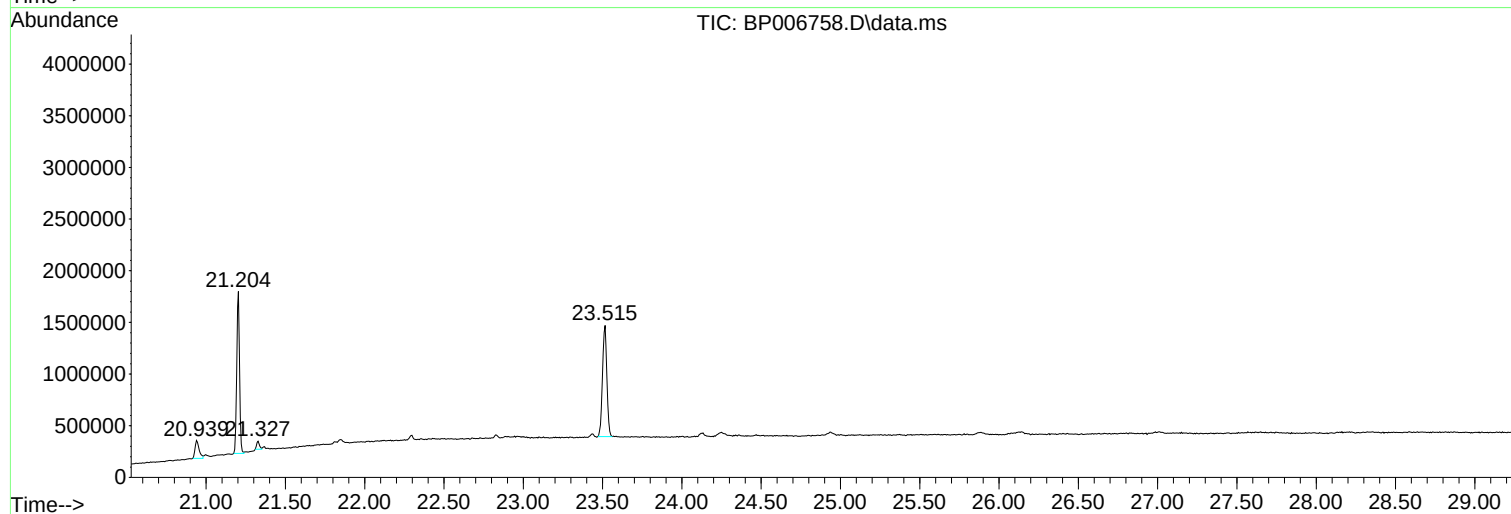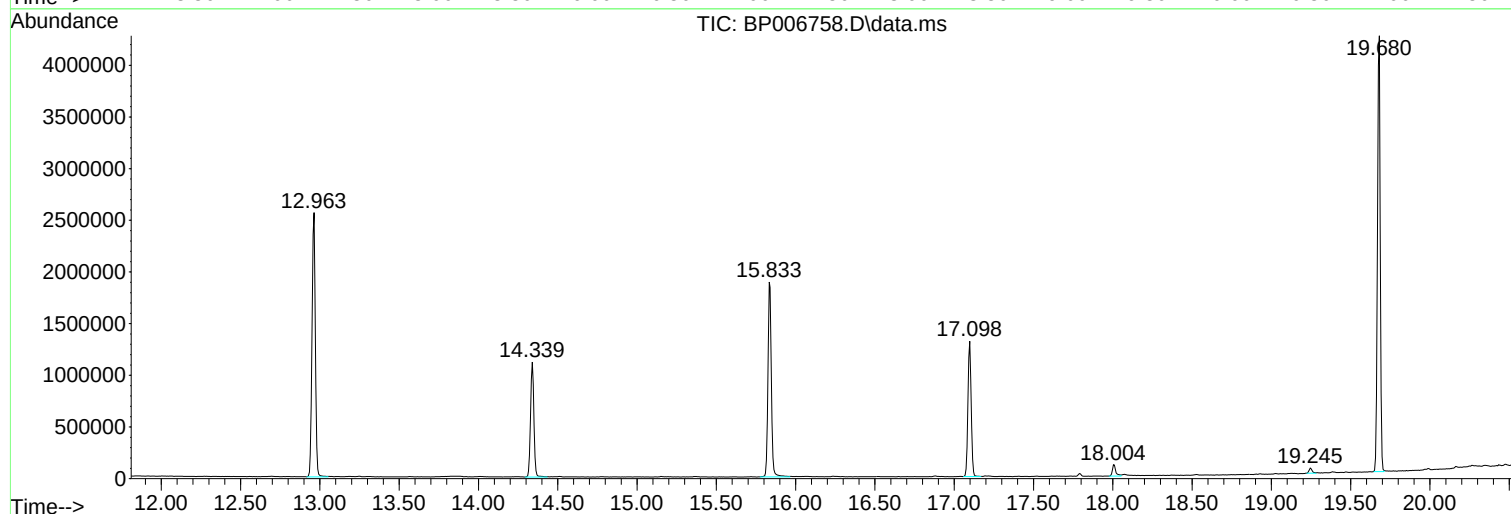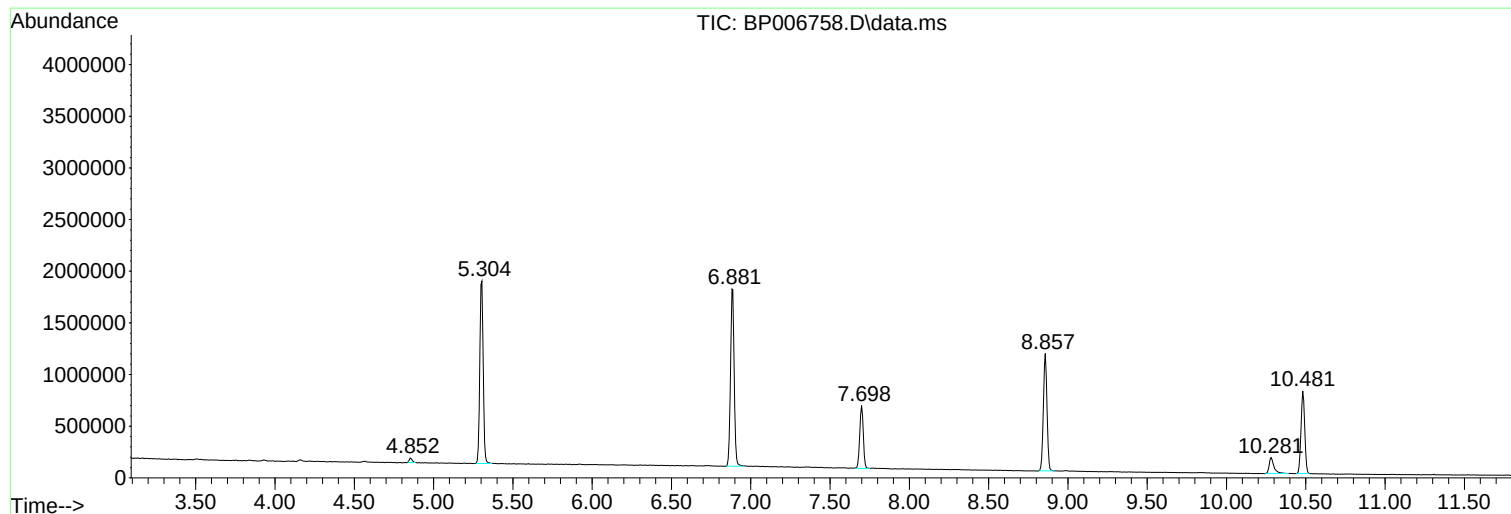

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006758.D
Acq On : 18 Aug 2021 22:51
Operator : CG/JU
Sample : M3419-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006758.D
Acq On : 18 Aug 2021 22:51
Operator : CG/JU
Sample : M3419-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-08-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
