

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006759.D
 Acq On : 18 Aug 2021 23:25
 Operator : CG/JU
 Sample : M3435-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-24-0306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	297	300	309	rVB	77040	113973	1.58%	0.241%
2	5.305	371	377	392	rVB	3429931	4869807	67.35%	10.311%
3	6.887	639	646	657	rBV	3277315	5151069	71.24%	10.906%
4	7.699	778	784	793	rVB	654646	993539	13.74%	2.104%
5	8.857	974	981	993	rVB	2042586	3348754	46.32%	7.090%
6	10.281	1216	1223	1240	rBV	1125366	1974695	27.31%	4.181%
7	10.481	1250	1257	1269	rVB	843254	1409497	19.49%	2.984%
8	12.963	1671	1679	1691	rBV	4169786	5940000	82.15%	12.577%
9	13.245	1721	1727	1736	rBV	174651	286332	3.96%	0.606%
10	14.339	1905	1913	1921	rBV	1200609	1740758	24.08%	3.686%
11	15.839	2153	2168	2180	rBV	3445859	5137816	71.06%	10.878%
12	17.098	2375	2382	2388	rBV	1357441	1945779	26.91%	4.120%
13	17.792	2495	2500	2507	rBV	170042	200450	2.77%	0.424%
14	18.010	2532	2537	2544	rBV	229957	341650	4.73%	0.723%
15	18.927	2689	2693	2698	rVB	435157	470661	6.51%	0.997%
16	19.063	2712	2716	2720	rVB	106404	117995	1.63%	0.250%
17	19.245	2743	2747	2756	rBV	87515	135926	1.88%	0.288%
18	19.680	2815	2821	2831	rBV	6128753	7230262	100.00%	15.309%
19	19.992	2867	2874	2879	rBV3	74615	135146	1.87%	0.286%
20	20.474	2953	2956	2960	rBV	77958	84942	1.17%	0.180%
21	20.939	3031	3035	3042	rBV2	387453	656027	9.07%	1.389%
22	21.204	3075	3080	3085	rBV	1631238	2061432	28.51%	4.365%
23	21.327	3098	3101	3104	rBV	71032	81113	1.12%	0.172%
24	21.363	3104	3107	3111	rVV	95429	107897	1.49%	0.228%
25	21.815	3180	3184	3186	rBV	178817	229184	3.17%	0.485%
26	22.292	3262	3265	3271	rVB	170929	219008	3.03%	0.464%
27	23.509	3466	3472	3487	rVB2	1139179	2246557	31.07%	4.757%




Sum of corrected areas: 47230269

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006759.D
Acq On : 18 Aug 2021 23:25
Operator : CG/JU
Sample : M3435-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-24-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

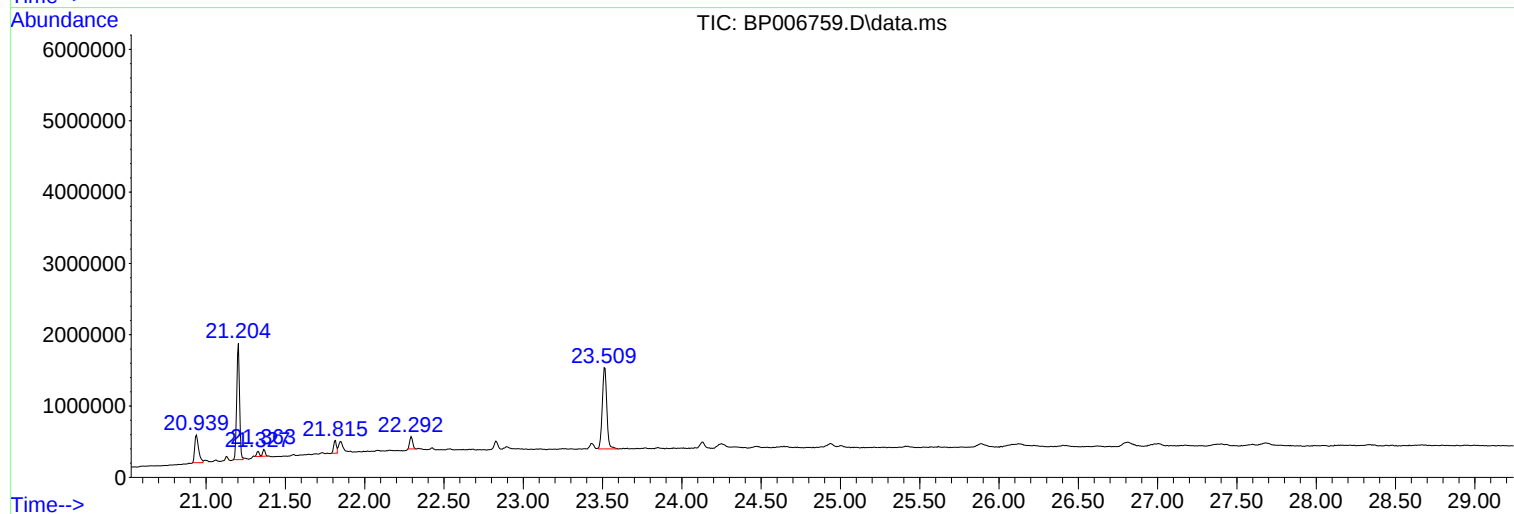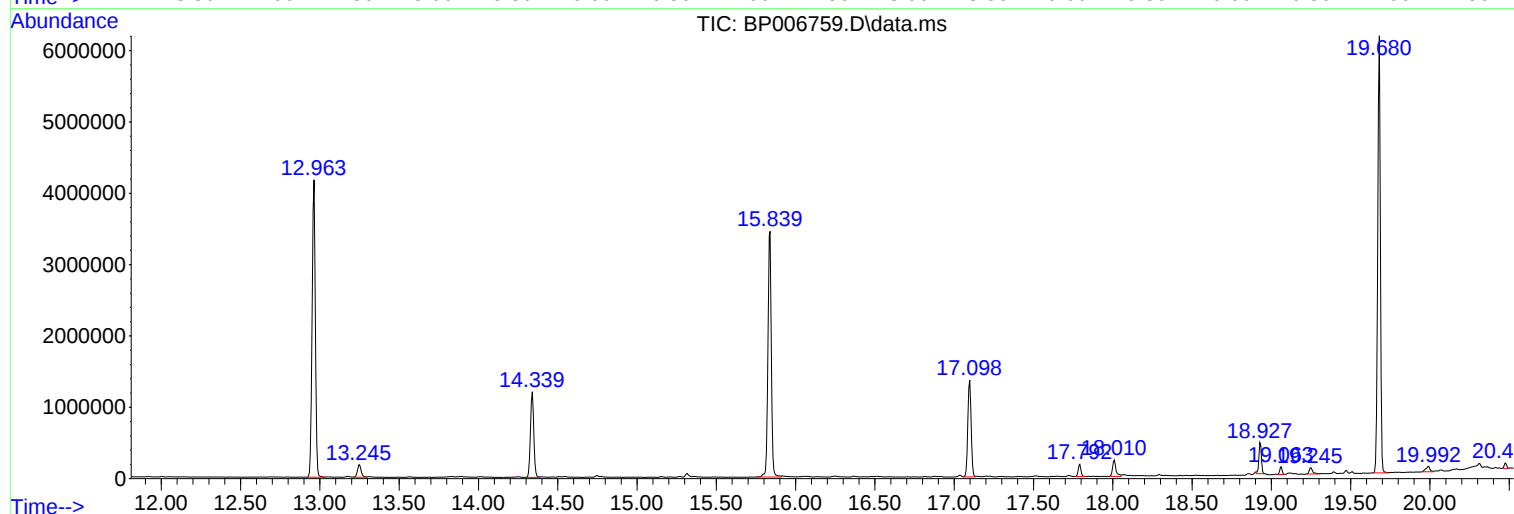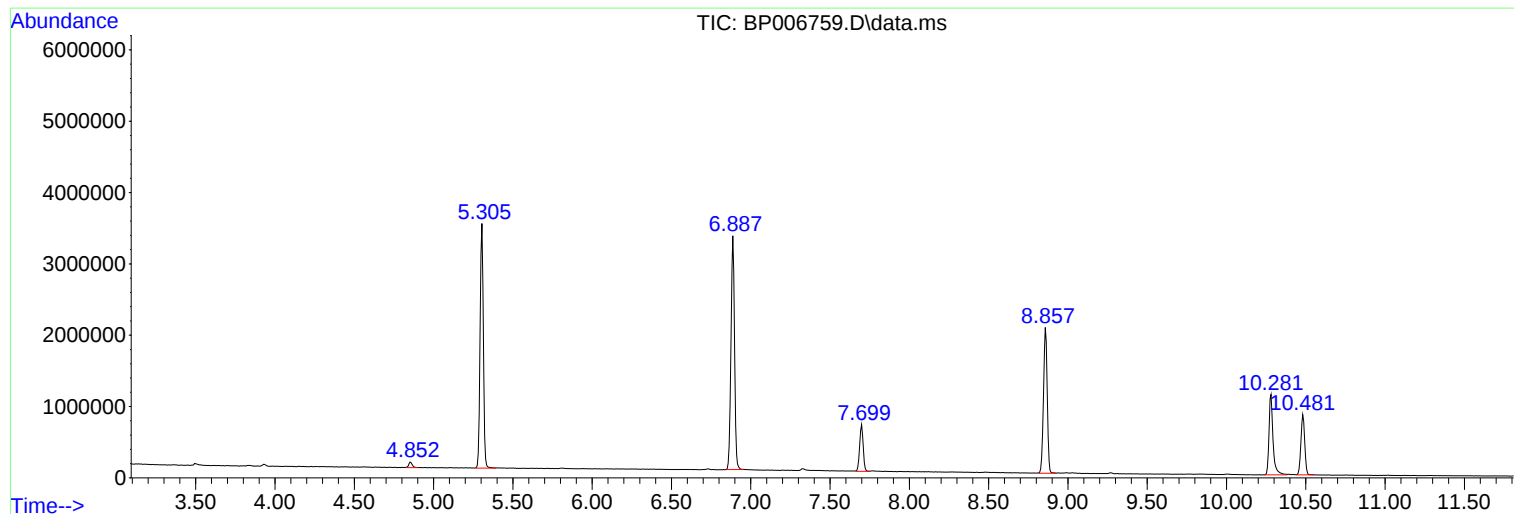

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006759.D
Acq On : 18 Aug 2021 23:25
Operator : CG/JU
Sample : M3435-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-24-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006759.D
Acq On : 18 Aug 2021 23:25
Operator : CG/JU
Sample : M3435-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-24-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------