

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006763.D
 Acq On : 19 Aug 2021 01:41
 Operator : CG/JU
 Sample : M3397-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-06-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	306	rVB	117666	172317	2.81%	0.500%
2	5.299	370	376	388	rVB	2388184	3408542	55.67%	9.886%
3	6.881	639	645	655	rVB	2243736	3497401	57.12%	10.144%
4	7.699	778	784	792	rVB	615220	978399	15.98%	2.838%
5	8.858	974	981	989	rVB	1388885	2299716	37.56%	6.670%
6	10.281	1218	1223	1238	rVB3	43596	101949	1.66%	0.296%
7	10.481	1250	1257	1268	rVB	829480	1379854	22.53%	4.002%
8	12.963	1671	1679	1692	rBV	3042097	4573797	74.70%	13.266%
9	14.340	1905	1913	1922	rBV	1134982	1668209	27.24%	4.838%
10	15.834	2159	2167	2189	rBV	2376390	3470033	56.67%	10.065%
11	17.098	2375	2382	2394	rBV	1273040	1874415	30.61%	5.437%
12	18.004	2532	2536	2545	rBV	153889	231049	3.77%	0.670%
13	19.245	2743	2747	2763	rBV	110665	181379	2.96%	0.526%
14	19.681	2815	2821	2828	rBV	5194379	6123287	100.00%	17.760%
15	20.933	3031	3034	3042	rBV2	113839	194035	3.17%	0.563%
16	21.198	3075	3079	3085	rBV	1568215	2002168	32.70%	5.807%
17	21.327	3098	3101	3104	rBV	62991	74499	1.22%	0.216%
18	21.363	3105	3107	3111	rVB	74642	71962	1.18%	0.209%
19	23.510	3466	3472	3481	rVB2	1131718	2174920	35.52%	6.308%




Sum of corrected areas: 34477931

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006763.D
Acq On : 19 Aug 2021 01:41
Operator : CG/JU
Sample : M3397-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-06-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

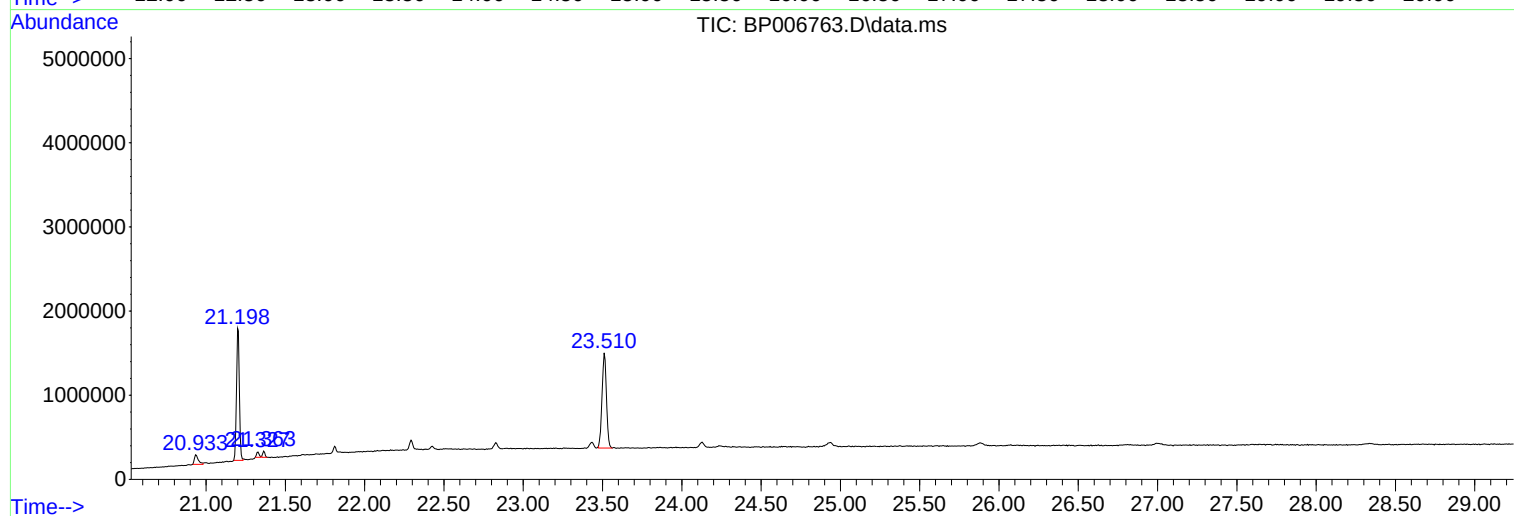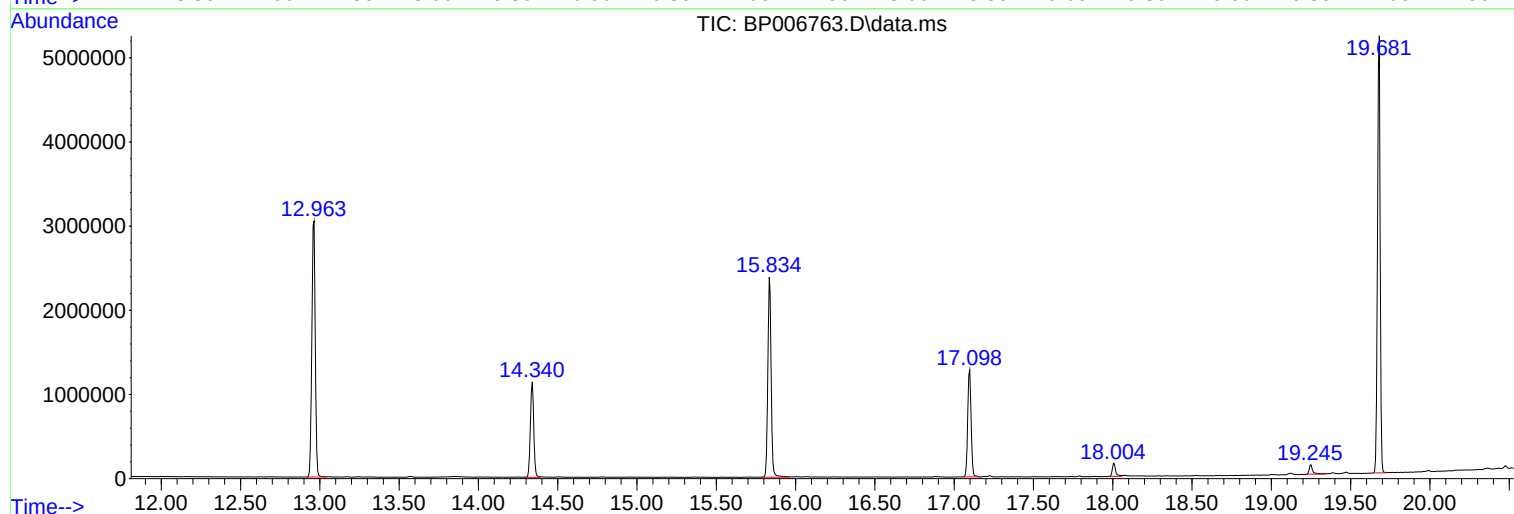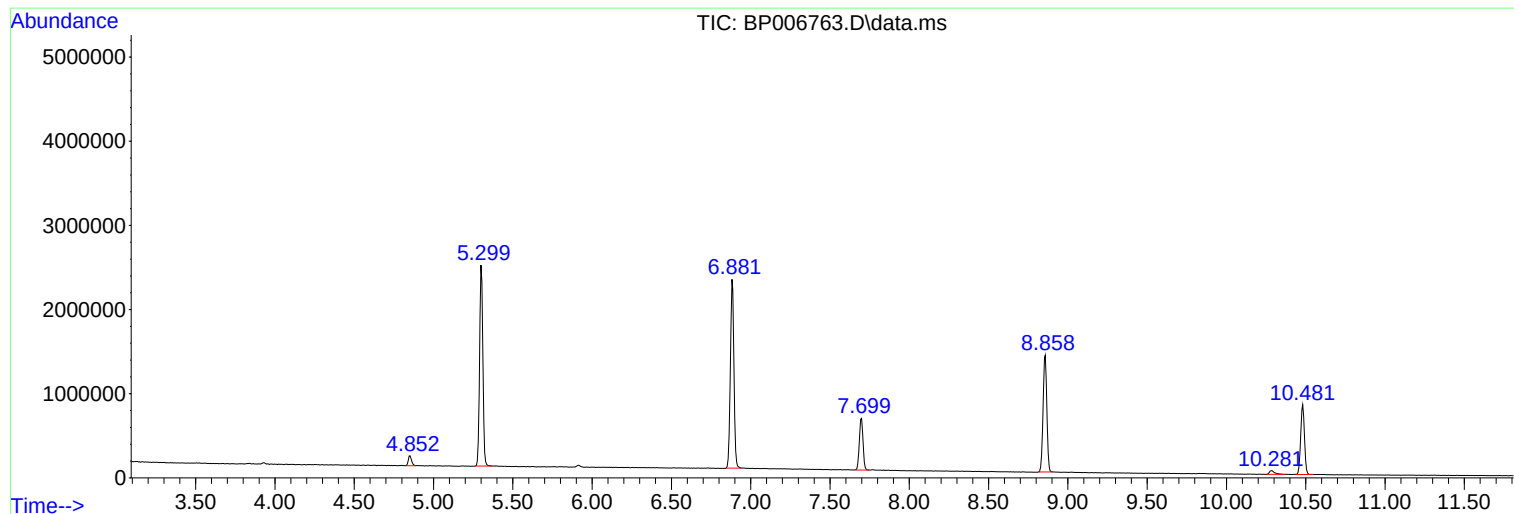

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006763.D
Acq On : 19 Aug 2021 01:41
Operator : CG/JU
Sample : M3397-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-06-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006763.D
Acq On : 19 Aug 2021 01:41
Operator : CG/JU
Sample : M3397-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-06-1015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
