

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006764.D
 Acq On : 19 Aug 2021 02:15
 Operator : CG/JU
 Sample : M3435-37
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-13-EB-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.869	294	303	307	rBV	7970967	12911249	100.00%	19.752%
2	5.305	372	377	408	rBV	1110487	2319283	17.96%	3.548%
3	5.769	452	456	458	rBV	154662	212369	1.64%	0.325%
4	5.799	458	461	478	rVB	503889	771338	5.97%	1.180%
5	6.881	640	645	661	rVB2	771666	1539679	11.93%	2.355%
6	7.005	662	666	676	rVB	83511	146726	1.14%	0.224%
7	7.499	746	750	763	rVB	85529	156908	1.22%	0.240%
8	7.699	777	784	790	rBV	662488	1046440	8.10%	1.601%
9	7.769	790	796	807	rVB3	114981	210986	1.63%	0.323%
10	7.946	821	826	850	rVB	397340	793455	6.15%	1.214%
11	8.522	915	924	929	rBV2	155046	269126	2.08%	0.412%
12	8.799	964	971	975	rBV2	464752	792171	6.14%	1.212%
13	8.857	975	981	992	rVB	2441790	4005836	31.03%	6.128%
14	9.028	1004	1010	1035	rVB2	738529	1457153	11.29%	2.229%
15	9.434	1074	1079	1085	rVB	92727	146311	1.13%	0.224%
16	9.757	1127	1134	1145	rVB3	178049	327045	2.53%	0.500%
17	9.963	1164	1169	1181	rVB2	205108	458839	3.55%	0.702%
18	10.281	1215	1223	1229	rBV4	53468	130029	1.01%	0.199%
19	10.399	1238	1243	1250	rVV4	82824	162394	1.26%	0.248%
20	10.481	1250	1257	1263	rVV	895440	1494315	11.57%	2.286%
21	10.546	1263	1268	1274	rVB3	68779	134000	1.04%	0.205%
22	10.787	1303	1309	1315	rBV4	72037	140506	1.09%	0.215%
23	10.857	1315	1321	1339	rVB	69972	194194	1.50%	0.297%
24	11.040	1344	1352	1358	rBV3	71855	156309	1.21%	0.239%
25	11.134	1363	1368	1377	rVB	191548	323210	2.50%	0.494%
26	11.763	1468	1475	1481	rBV	81625	151765	1.18%	0.232%
27	12.610	1610	1619	1627	rBV	61973	129272	1.00%	0.198%
28	12.698	1627	1634	1639	rVV	153894	294824	2.28%	0.451%
29	12.763	1639	1645	1669	rVB	459647	969651	7.51%	1.483%
30	12.963	1671	1679	1694	rBV	6064359	9160561	70.95%	14.014%
31	13.275	1723	1732	1750	rVB2	63761	169955	1.32%	0.260%
32	14.340	1906	1913	1922	rBV	1259647	1852536	14.35%	2.834%
33	15.175	2047	2055	2062	rVB2	123906	202150	1.57%	0.309%
34	15.592	2122	2126	2129	rBV	98536	135104	1.05%	0.207%
35	15.834	2160	2167	2180	rBV	1556150	2386856	18.49%	3.651%
36	17.098	2375	2382	2392	rBV	1444839	2059791	15.95%	3.151%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006764.D
Acq On : 19 Aug 2021 02:15
Operator : CG/JU
Sample : M3435-37
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-13-EB-04

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.680	2815	2821	2826	rBV	10690873	12726083	98.57%	19.469%
38	20.686	2989	2992	2998	rBV2	93345	135168	1.05%	0.207%
39	21.198	3074	3079	3085	rBV	1715933	2202407	17.06%	3.369%
40	22.286	3261	3264	3271	rVB2	113622	166538	1.29%	0.255%
41	23.510	3465	3472	3481	rVB2	1190142	2324425	18.00%	3.556%




Sum of corrected areas: 65366957

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006764.D
Acq On : 19 Aug 2021 02:15
Operator : CG/JU
Sample : M3435-37
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-13-EB-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

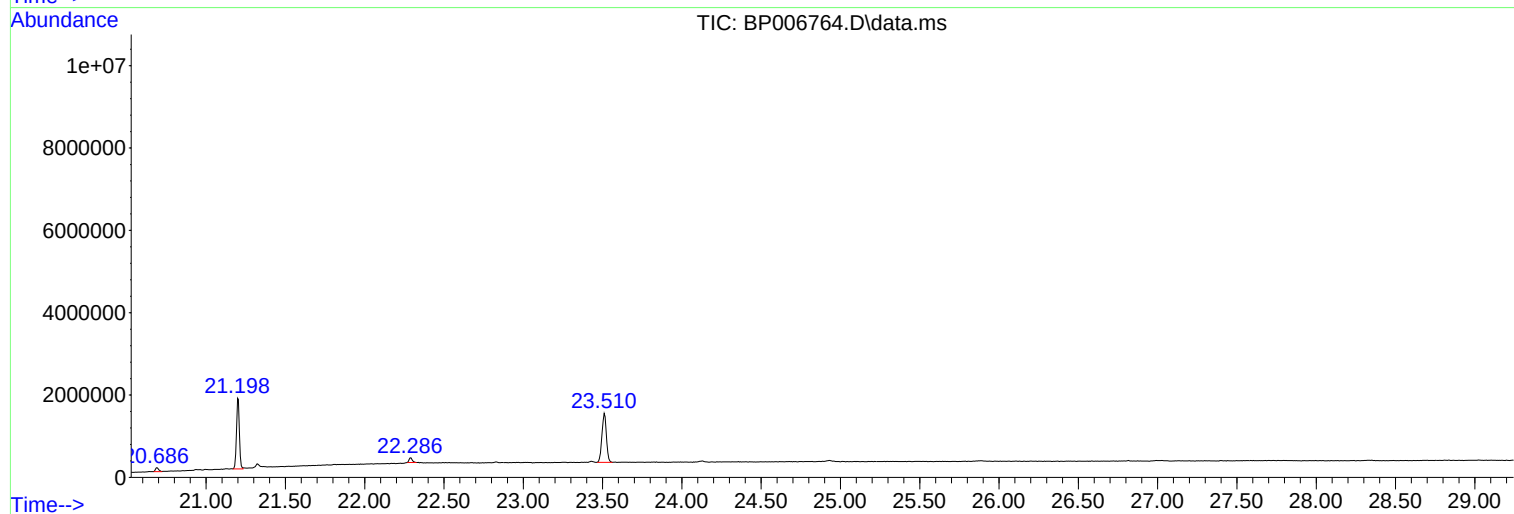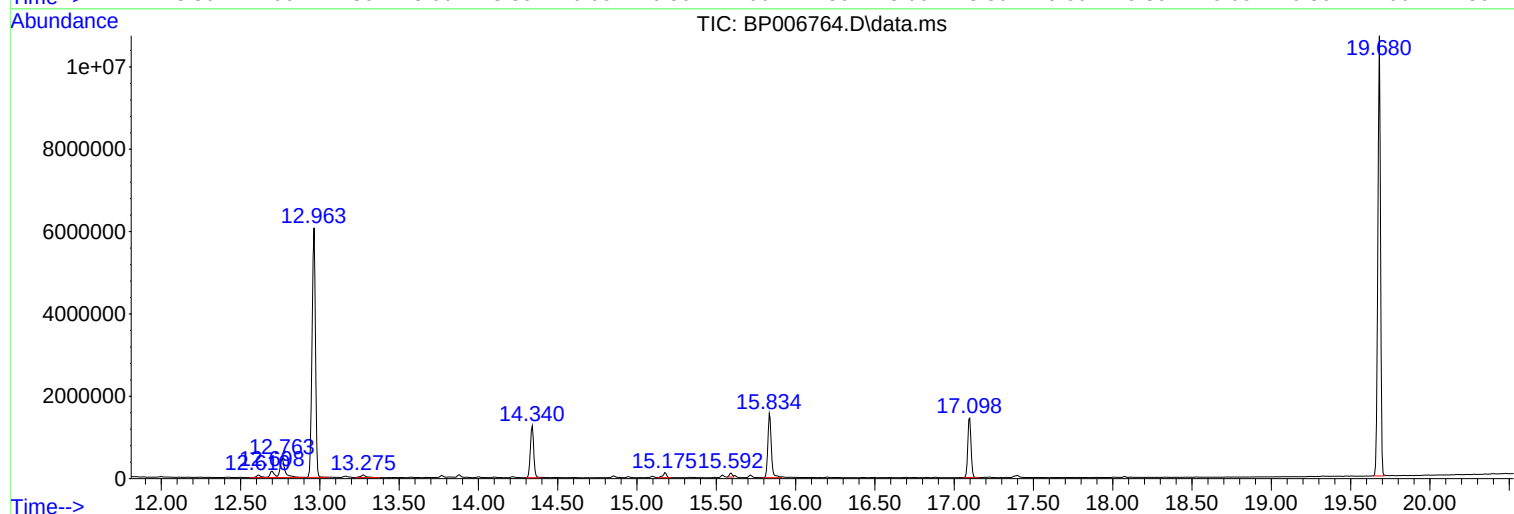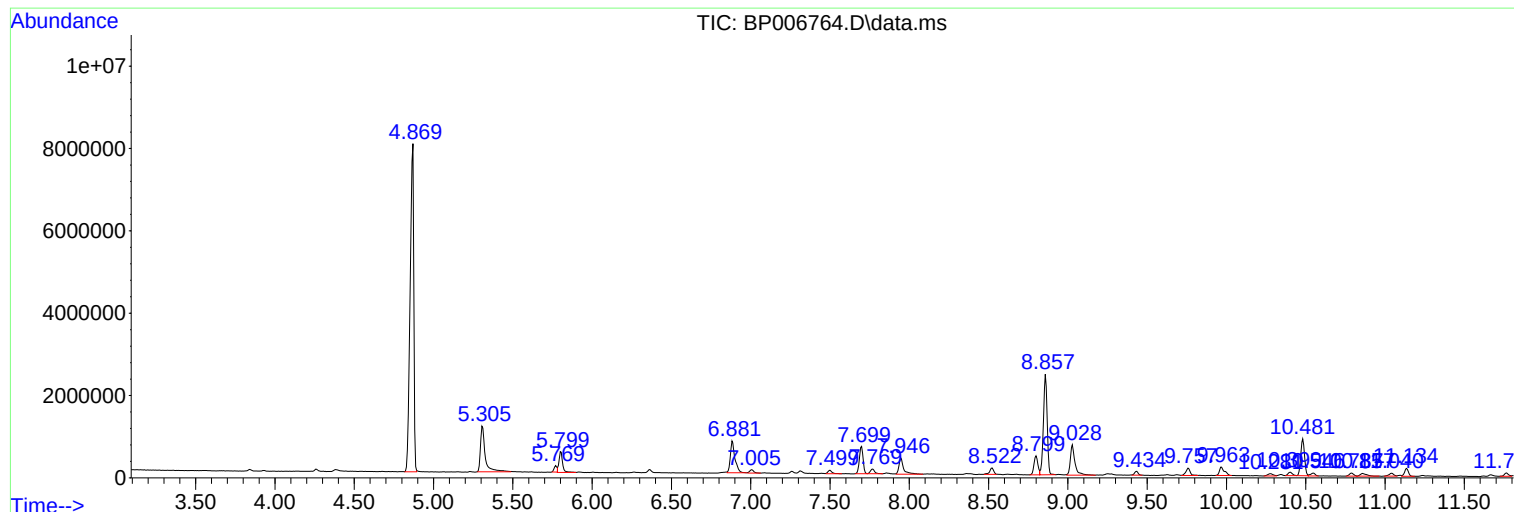

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006764.D
Acq On : 19 Aug 2021 02:15
Operator : CG/JU
Sample : M3435-37
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-13-EB-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006764.D
Acq On : 19 Aug 2021 02:15
Operator : CG/JU
Sample : M3435-37
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-13-EB-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
