

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006765.D
 Acq On : 19 Aug 2021 02:49
 Operator : CG/JU
 Sample : M3435-27
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-28-0306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	297	300	306	rVB	41445	61410	1.11%	0.188%
2	5.299	370	376	387	rVB	2265931	3249344	58.58%	9.934%
3	6.881	639	645	660	rVB	2134661	3389620	61.11%	10.363%
4	7.699	778	784	791	rVB	612670	962894	17.36%	2.944%
5	8.858	974	981	996	rVB	1341263	2200396	39.67%	6.727%
6	10.281	1218	1223	1235	rBV2	35597	85969	1.55%	0.263%
7	10.481	1250	1257	1265	rVB	821141	1353005	24.39%	4.137%
8	12.963	1671	1679	1693	rBV	2867067	4283652	77.23%	13.096%
9	14.340	1906	1913	1928	rBV	1113287	1644188	29.64%	5.027%
10	15.834	2158	2167	2182	rBV	2374989	3348612	60.37%	10.238%
11	17.098	2375	2382	2393	rBV	1277678	1862118	33.57%	5.693%
12	18.004	2531	2536	2546	rBV	116030	170805	3.08%	0.522%
13	19.245	2743	2747	2755	rBV2	62508	86061	1.55%	0.263%
14	19.675	2815	2820	2826	rBV	4939869	5546511	100.00%	16.957%
15	20.933	3030	3034	3043	rBV3	136747	252988	4.56%	0.773%
16	21.198	3074	3079	3084	rBV	1675980	1992730	35.93%	6.092%
17	21.322	3097	3100	3104	rBV	69965	101089	1.82%	0.309%
18	23.510	3465	3472	3481	rVB2	1069438	2117315	38.17%	6.473%




Sum of corrected areas: 32708707

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006765.D
Acq On : 19 Aug 2021 02:49
Operator : CG/JU
Sample : M3435-27
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-28-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

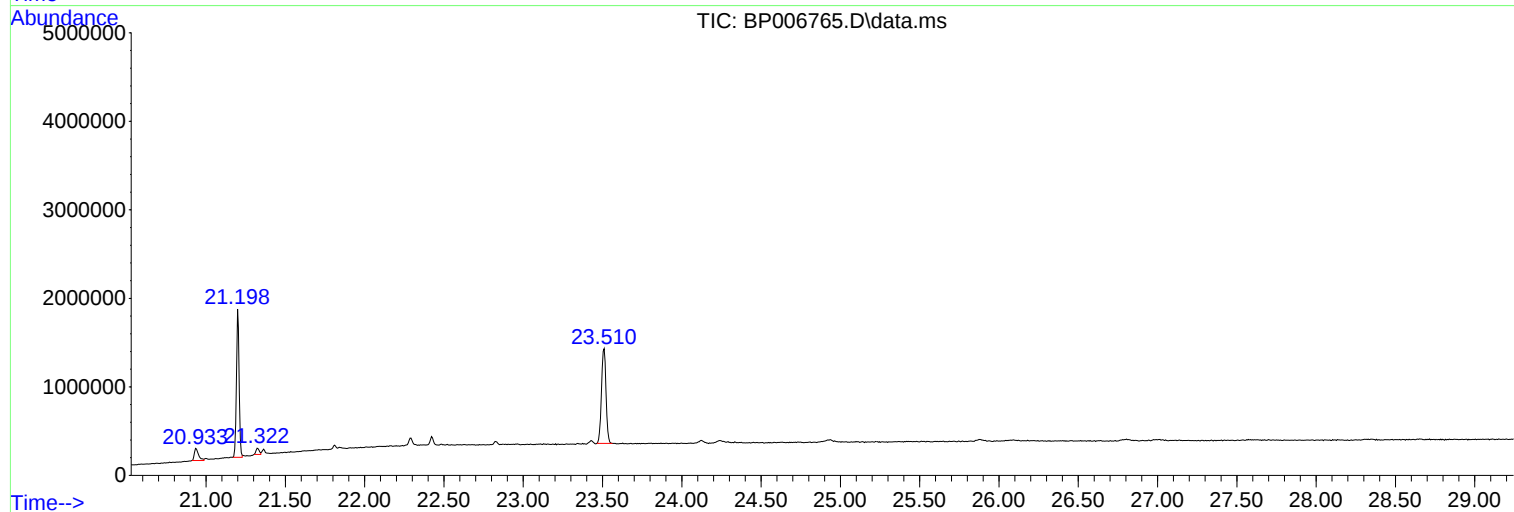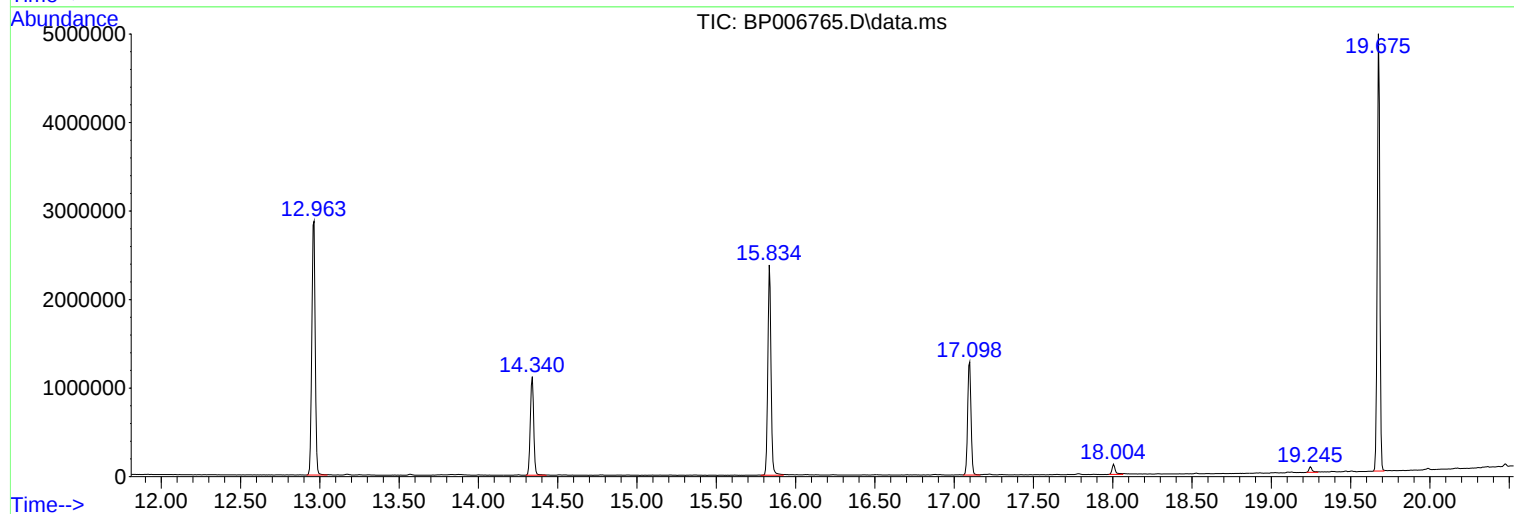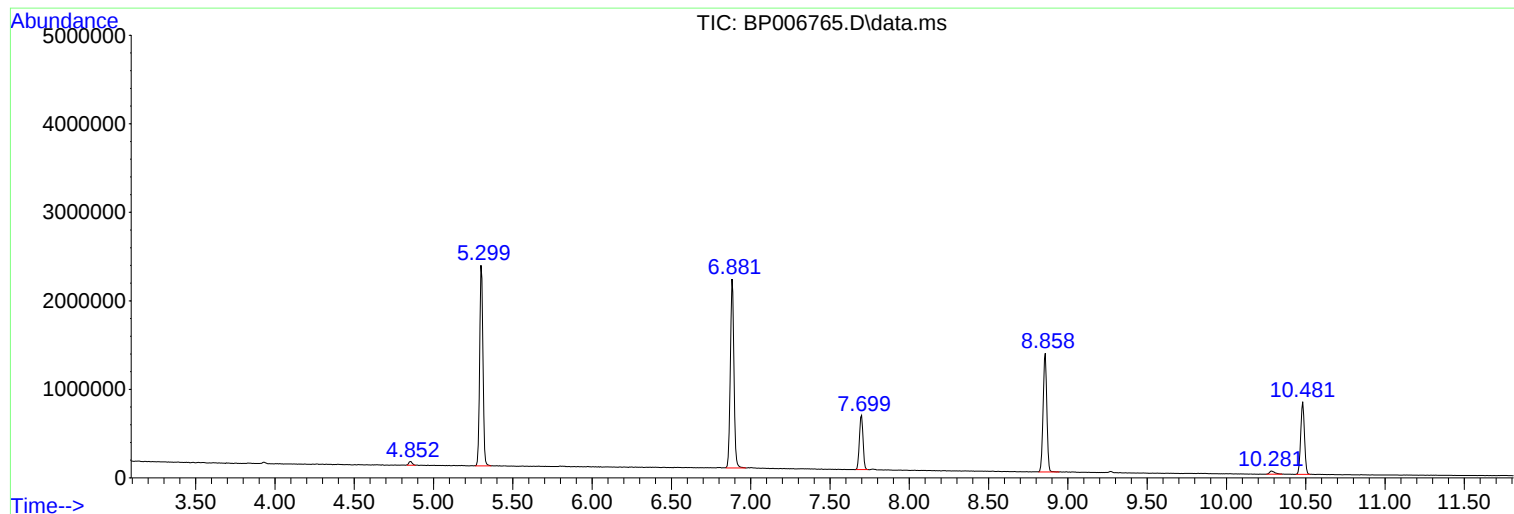

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006765.D
Acq On : 19 Aug 2021 02:49
Operator : CG/JU
Sample : M3435-27
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-28-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006765.D
Acq On : 19 Aug 2021 02:49
Operator : CG/JU
Sample : M3435-27
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-28-0306

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
