

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006766.D
 Acq On : 19 Aug 2021 03:23
 Operator : CG/JU
 Sample : M3435-31
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-10-EB-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	306	rVB	182344	254000	2.13%	0.557%
2	5.299	371	376	385	rBV	1838374	2691188	22.61%	5.905%
3	6.881	639	645	657	rVB	1148988	1786761	15.01%	3.921%
4	7.699	778	784	793	rVB	620204	970461	8.15%	2.129%
5	8.857	974	981	992	rVB	2498967	3991939	33.54%	8.759%
6	10.481	1250	1257	1266	rVB	817842	1355338	11.39%	2.974%
7	12.157	1534	1542	1557	rBV	336734	612478	5.15%	1.344%
8	12.963	1671	1679	1694	rBV	5545103	7997677	67.19%	17.549%
9	14.339	1906	1913	1924	rBV	1112568	1648032	13.85%	3.616%
10	15.839	2159	2168	2189	rBV	4464313	6370086	53.51%	13.977%
11	17.098	2375	2382	2394	rVB	1323242	1874803	15.75%	4.114%
12	19.680	2815	2821	2826	rBV	9978875	11903411	100.00%	26.119%
13	21.198	3075	3079	3086	rBV	1543759	1985555	16.68%	4.357%
14	23.510	3466	3472	3485	rVB2	1051669	2132897	17.92%	4.680%




Sum of corrected areas: 45574626

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006766.D
Acq On : 19 Aug 2021 03:23
Operator : CG/JU
Sample : M3435-31
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-10-EB-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

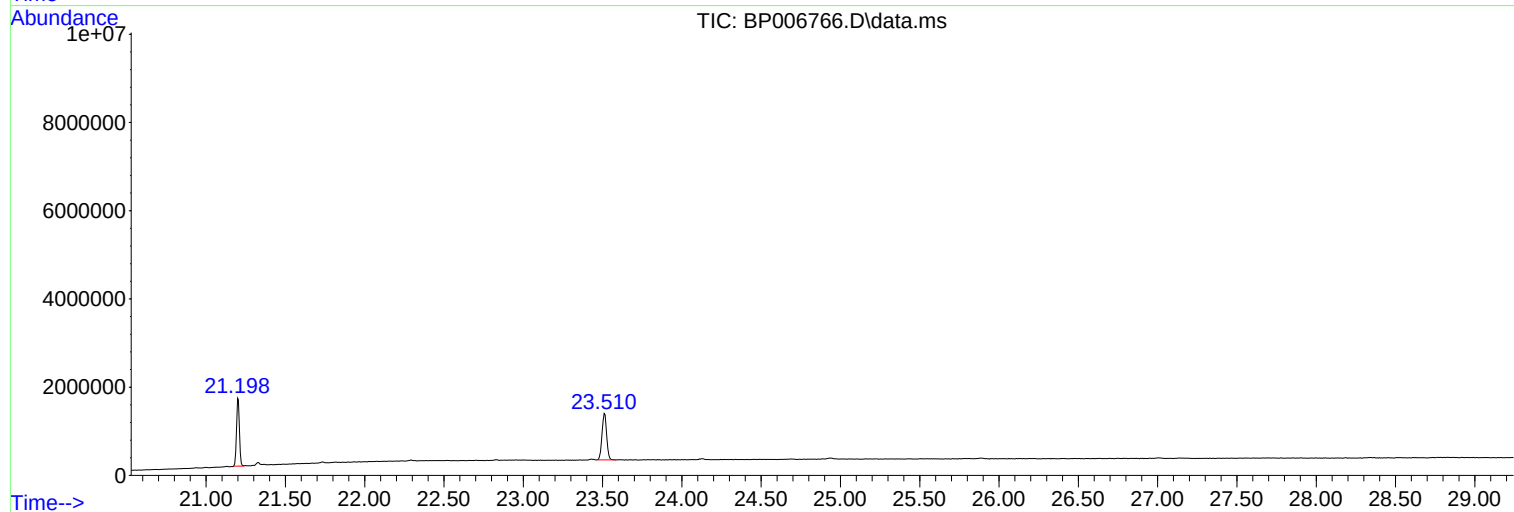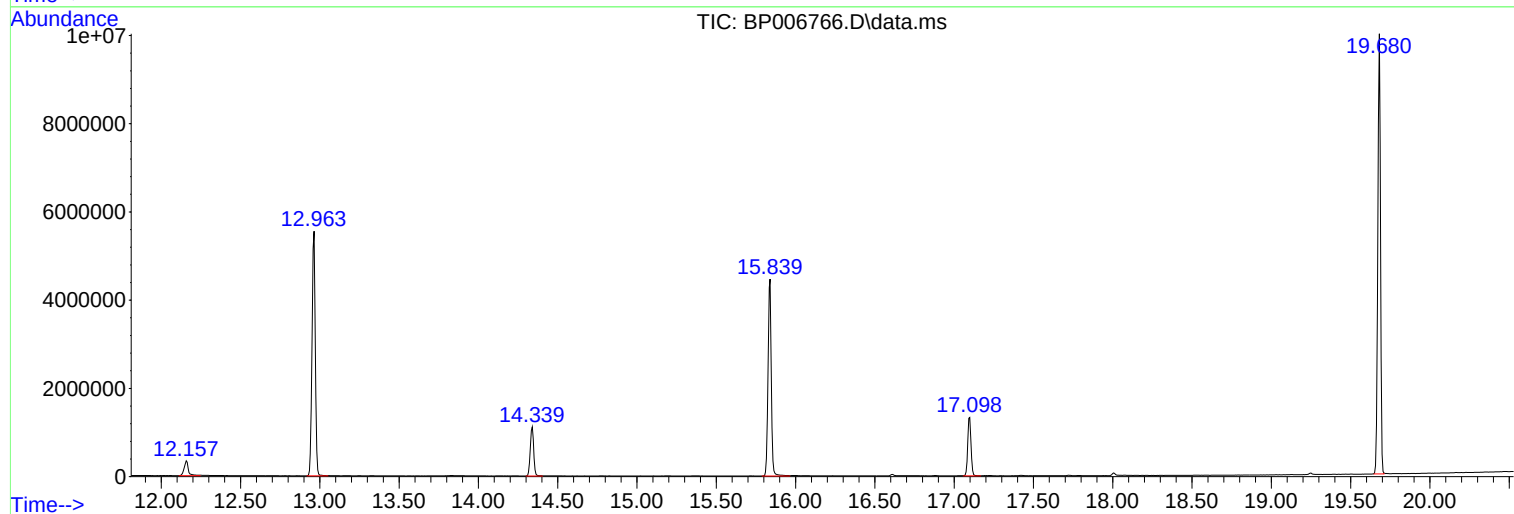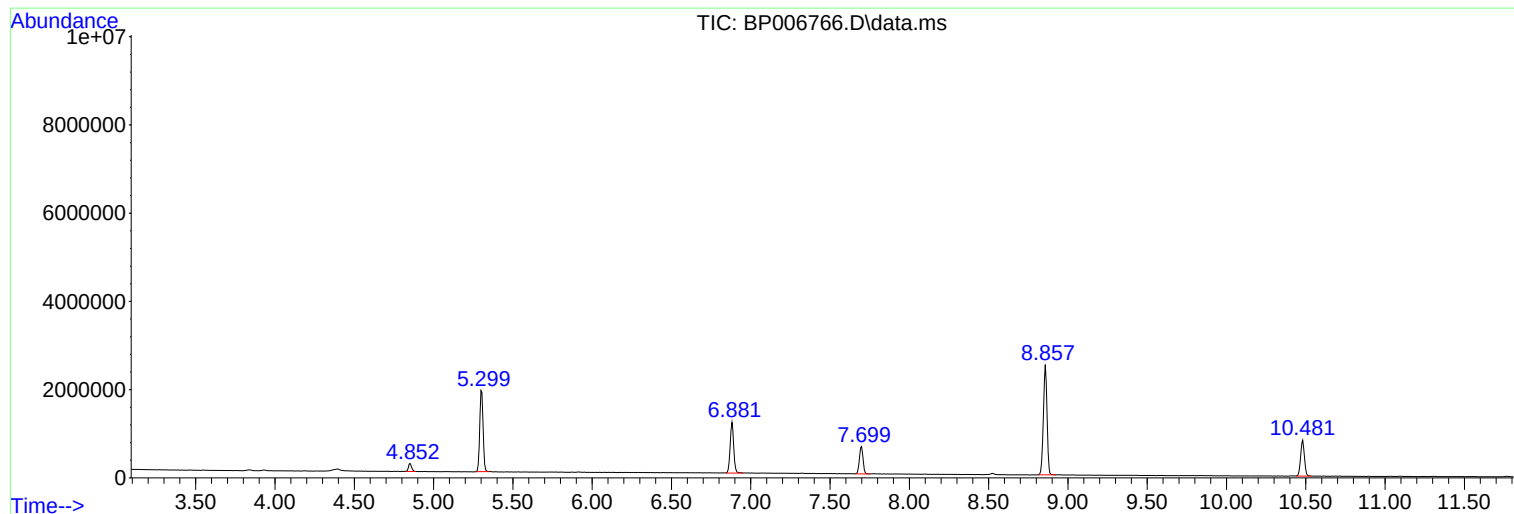

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006766.D
Acq On : 19 Aug 2021 03:23
Operator : CG/JU
Sample : M3435-31
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-10-EB-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006766.D
Acq On : 19 Aug 2021 03:23
Operator : CG/JU
Sample : M3435-31
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-10-EB-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc