

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006767.D
 Acq On : 19 Aug 2021 03:58
 Operator : CG/JU
 Sample : M3435-33
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-11-EB-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	308	rVB	134539	190299	1.68%	0.439%
2	5.299	371	376	387	rVB	1601968	2305383	20.41%	5.319%
3	6.881	639	645	657	rVB	923156	1439589	12.74%	3.322%
4	7.699	778	784	791	rVB	591547	918144	8.13%	2.119%
5	8.858	974	981	991	rVB	2313010	3743214	33.13%	8.637%
6	10.481	1250	1257	1265	rVB	774758	1306596	11.57%	3.015%
7	12.163	1534	1543	1566	rBV	427712	854034	7.56%	1.971%
8	12.963	1670	1679	1694	rBV	5144765	7642770	67.65%	17.635%
9	14.334	1906	1912	1927	rBV	1077284	1633219	14.46%	3.769%
10	15.834	2160	2167	2188	rBV	4141524	6136632	54.32%	14.160%
11	16.610	2293	2299	2314	rBV	81266	142011	1.26%	0.328%
12	17.098	2375	2382	2394	rVB	1273998	1809885	16.02%	4.176%
13	19.680	2815	2821	2826	rBV	9900340	11297612	100.00%	26.068%
14	21.204	3075	3080	3087	rBV	1526541	1901701	16.83%	4.388%
15	23.510	3466	3472	3481	rVB2	1047455	2017276	17.86%	4.655%




Sum of corrected areas: 43338365

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006767.D
Acq On : 19 Aug 2021 03:58
Operator : CG/JU
Sample : M3435-33
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-11-EB-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

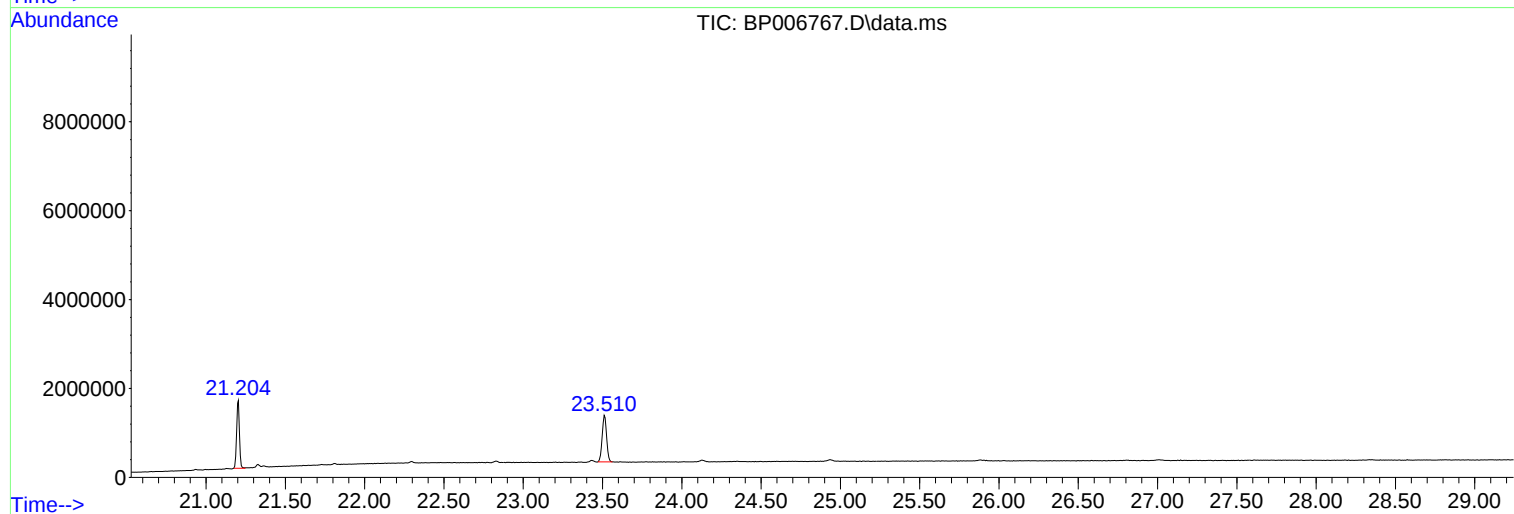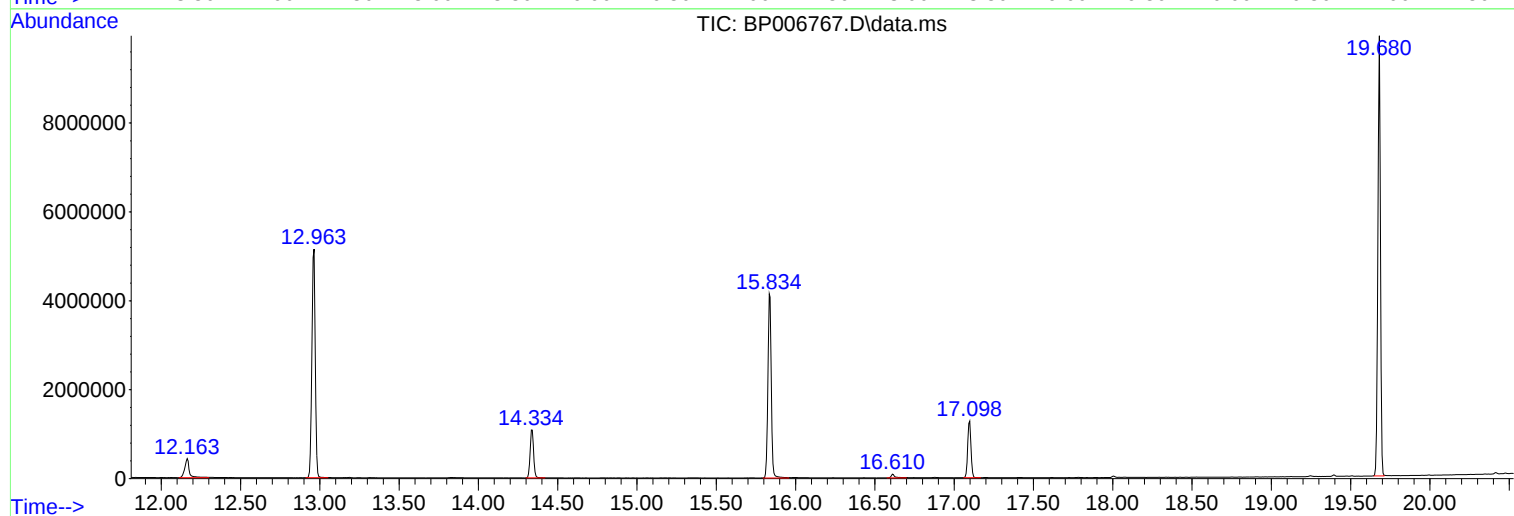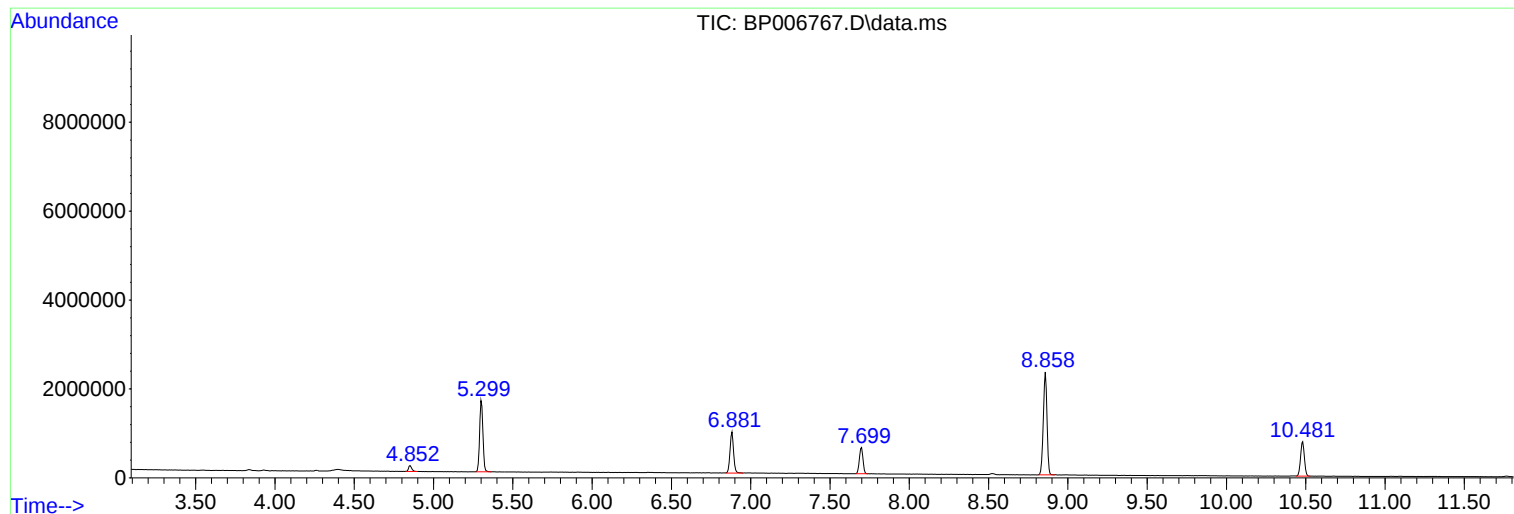

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006767.D
Acq On : 19 Aug 2021 03:58
Operator : CG/JU
Sample : M3435-33
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-11-EB-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006767.D
Acq On : 19 Aug 2021 03:58
Operator : CG/JU
Sample : M3435-33
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-11-EB-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
