

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006768.D
 Acq On : 19 Aug 2021 04:32
 Operator : CG/JU
 Sample : M3435-35
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-12-EB-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.852	296	300	306	rVB	107529	155035	1.52%	0.311%
2	5.299	371	376	386	rVB	1595948	2335010	22.90%	4.681%
3	5.769	451	456	458	rBV	134729	197577	1.94%	0.396%
4	5.799	458	461	472	rVB	425107	614613	6.03%	1.232%
5	6.881	639	645	656	rVB2	977713	1793103	17.59%	3.595%
6	7.699	777	784	790	rBV	591240	941501	9.23%	1.887%
7	7.769	790	796	806	rVB3	88075	160950	1.58%	0.323%
8	7.946	820	826	837	rBV	300489	561850	5.51%	1.126%
9	8.516	919	923	929	rVB2	100428	165326	1.62%	0.331%
10	8.793	964	970	975	rBV2	400786	663371	6.51%	1.330%
11	8.857	975	981	988	rVB	2116402	3440395	33.74%	6.897%
12	9.028	1000	1010	1030	rVB	545056	1104129	10.83%	2.213%
13	9.428	1073	1078	1085	rVB	96361	151285	1.48%	0.303%
14	9.757	1126	1134	1144	rBV2	288982	796901	7.82%	1.597%
15	9.963	1164	1169	1172	rBV	192445	315628	3.10%	0.633%
16	10.281	1215	1223	1231	rBV4	47154	114632	1.12%	0.230%
17	10.398	1238	1243	1250	rVB4	79091	139242	1.37%	0.279%
18	10.481	1250	1257	1263	rVV	812221	1345223	13.19%	2.697%
19	10.546	1263	1268	1275	rVB3	59629	116397	1.14%	0.233%
20	10.787	1303	1309	1315	rVB2	60126	108630	1.07%	0.218%
21	10.857	1315	1321	1329	rBV	54084	133842	1.31%	0.268%
22	11.040	1344	1352	1357	rBV3	59475	110477	1.08%	0.221%
23	11.134	1363	1368	1379	rVB	156435	279060	2.74%	0.559%
24	11.722	1464	1468	1478	rVB	56642	104586	1.03%	0.210%
25	12.610	1611	1619	1626	rBV	72066	122352	1.20%	0.245%
26	12.698	1628	1634	1646	rVV	143441	294506	2.89%	0.590%
27	12.963	1668	1679	1693	rBV	4706222	7368507	72.26%	14.771%
28	13.269	1723	1731	1748	rBV	740170	1186481	11.64%	2.378%
29	13.475	1758	1766	1779	rVB	254098	452954	4.44%	0.908%
30	14.210	1884	1891	1902	rVB	86807	136779	1.34%	0.274%
31	14.339	1905	1913	1923	rBV	1127521	1690956	16.58%	3.390%
32	15.181	2047	2056	2062	rVB2	120420	203422	1.99%	0.408%
33	15.839	2157	2168	2179	rBV	3797860	5449992	53.45%	10.925%
34	17.098	2375	2382	2393	rBV	1323500	1875780	18.40%	3.760%
35	17.780	2492	2498	2507	rBV	723541	857410	8.41%	1.719%
36	19.680	2815	2821	2826	rBV	8566387	10196715	100.00%	20.441%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006768.D
Acq On : 19 Aug 2021 04:32
Operator : CG/JU
Sample : M3435-35
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-EB-03

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.204	3075	3080	3085	rBV	1544870	1939697	19.02%	3.888%
38	22.292	3261	3265	3273	rBV2	125851	202426	1.99%	0.406%
39	23.510	3466	3472	3482	rVB2	1055959	2057887	20.18%	4.125%




Sum of corrected areas: 49884627

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006768.D
Acq On : 19 Aug 2021 04:32
Operator : CG/JU
Sample : M3435-35
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-EB-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

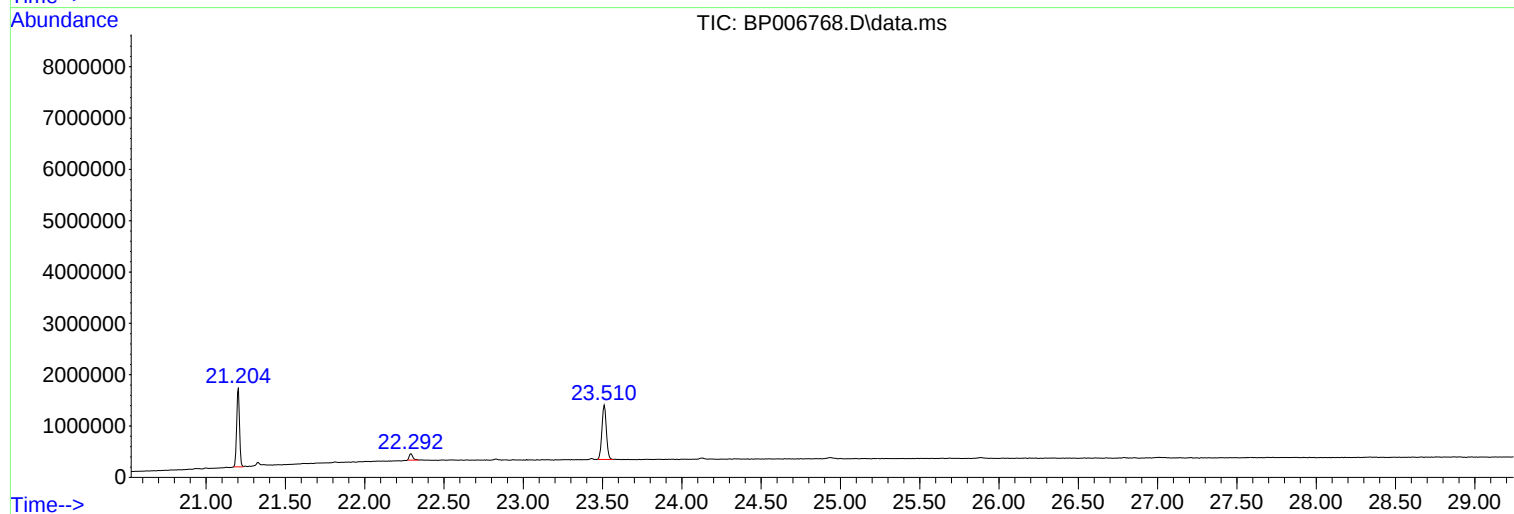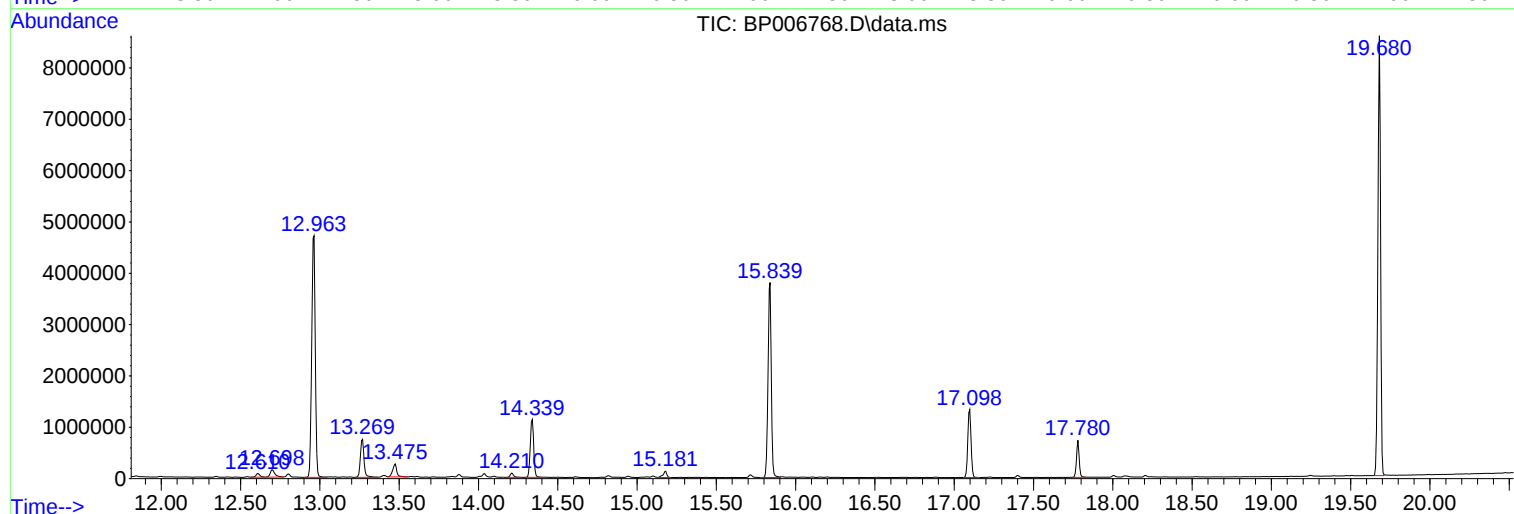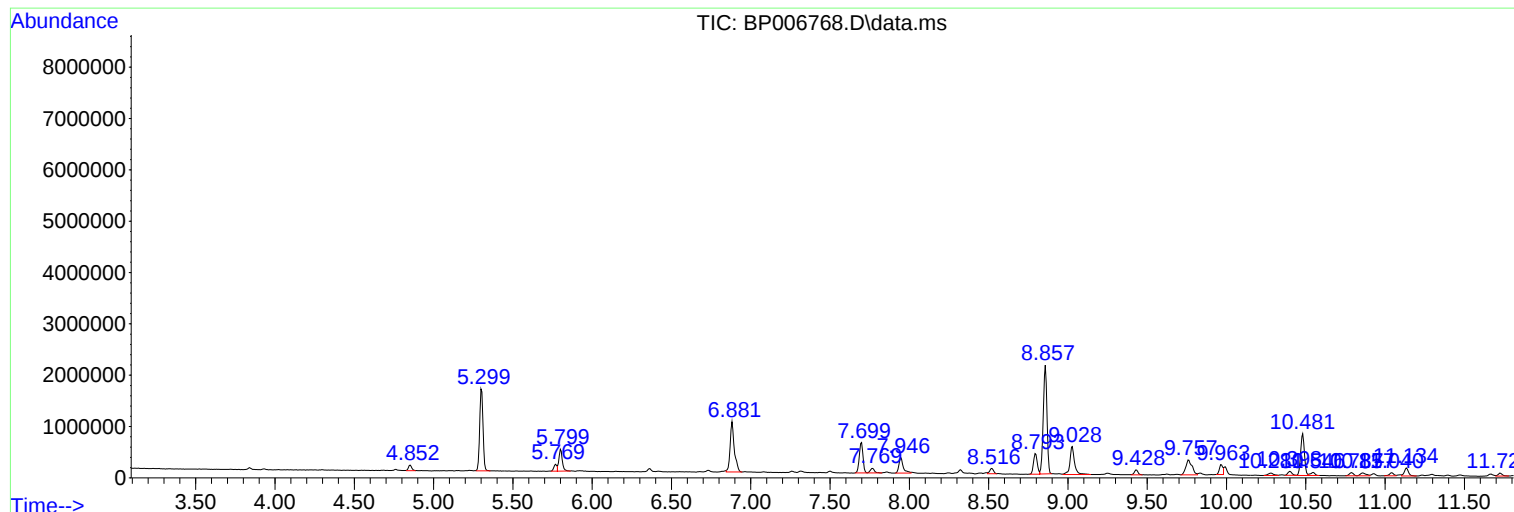

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006768.D
Acq On : 19 Aug 2021 04:32
Operator : CG/JU
Sample : M3435-35
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-EB-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006768.D
Acq On : 19 Aug 2021 04:32
Operator : CG/JU
Sample : M3435-35
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-12-EB-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------