
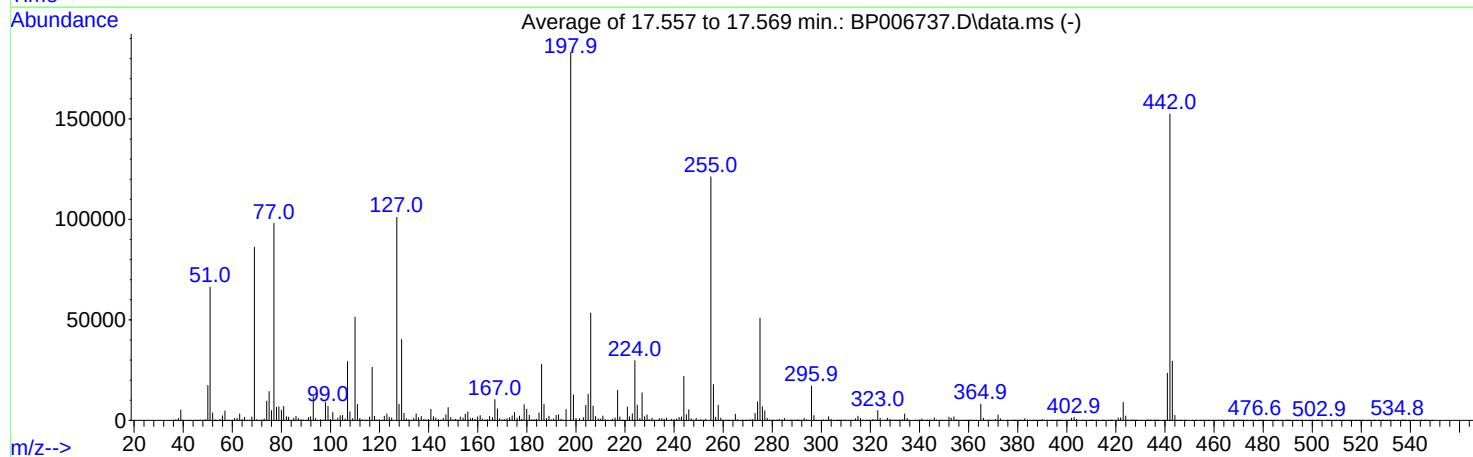


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006737.D
 Acq On : 18 Aug 2021 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 18:17:59 2021

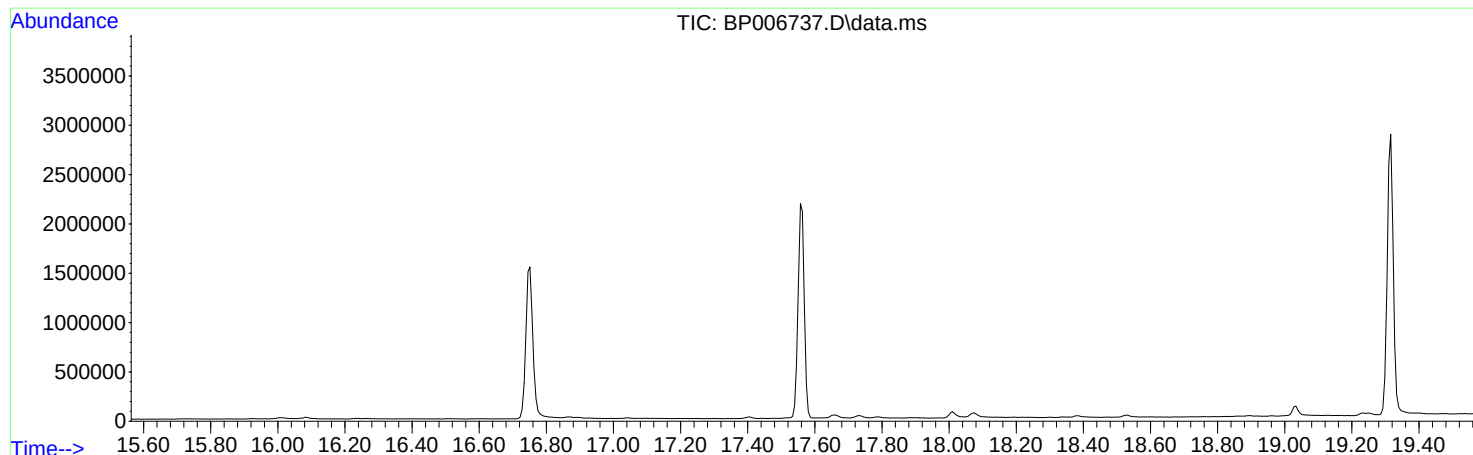




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	66248	PASS
68	69	0.00	2	1.9	1646	PASS
69	198	0.00	100	47.1	86177	PASS
70	69	0.00	2	0.5	435	PASS
127	198	10	80	55.2	101069	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	183039	PASS
199	198	5	9	6.9	12701	PASS
275	198	10	60	27.8	50904	PASS
365	198	1	100	4.4	8055	PASS
441	198	0.01	100	12.8	23461	PASS
442	442	100	100	100.0	152432	PASS
443	442	15	24	19.3	29477	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006737.D
Acq On : 18 Aug 2021 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 18 12:04:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

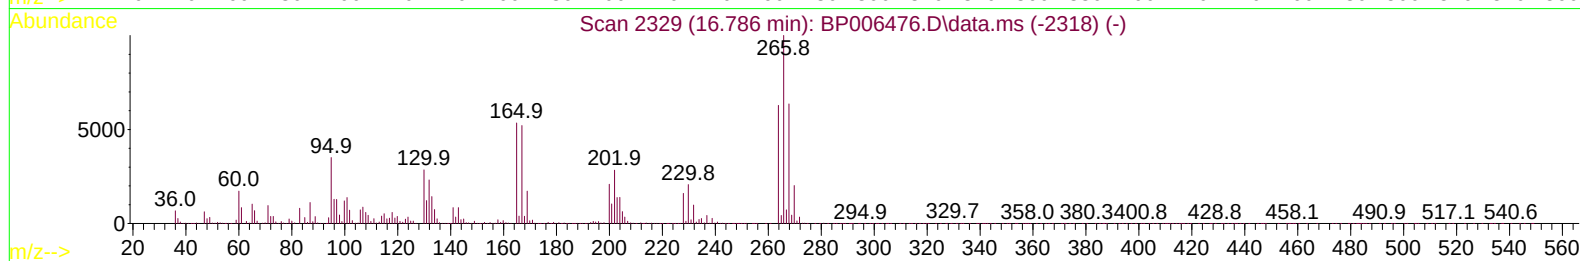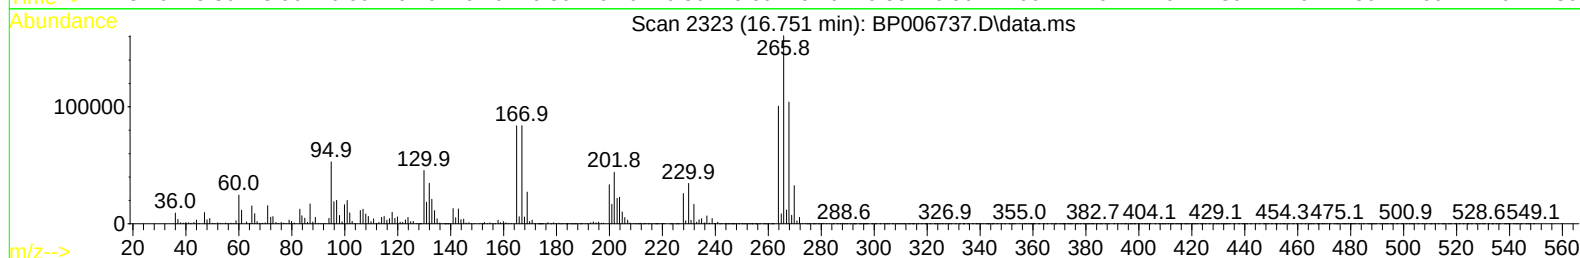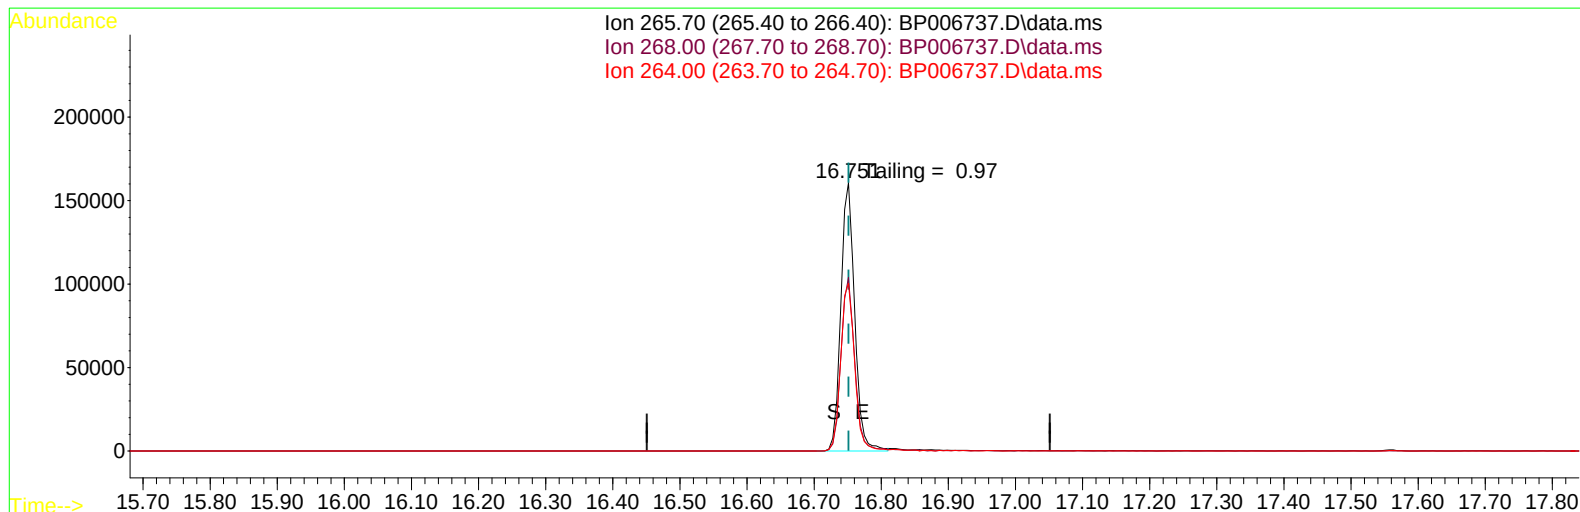

TIC: BP006737.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.000) 1675779.11 ng




response 232188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.72
264.00	62.90	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006737.D
 Acq On : 18 Aug 2021 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 18 12:04:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 18:17:59 2021
 Response via : Initial Calibration

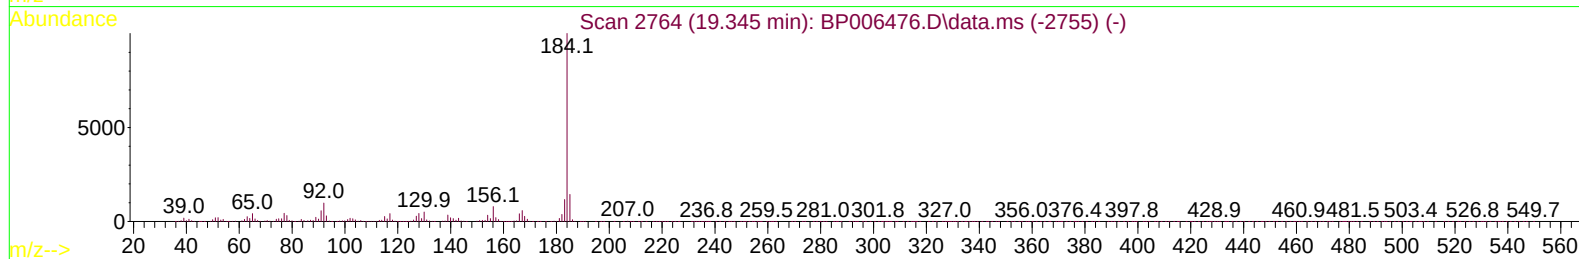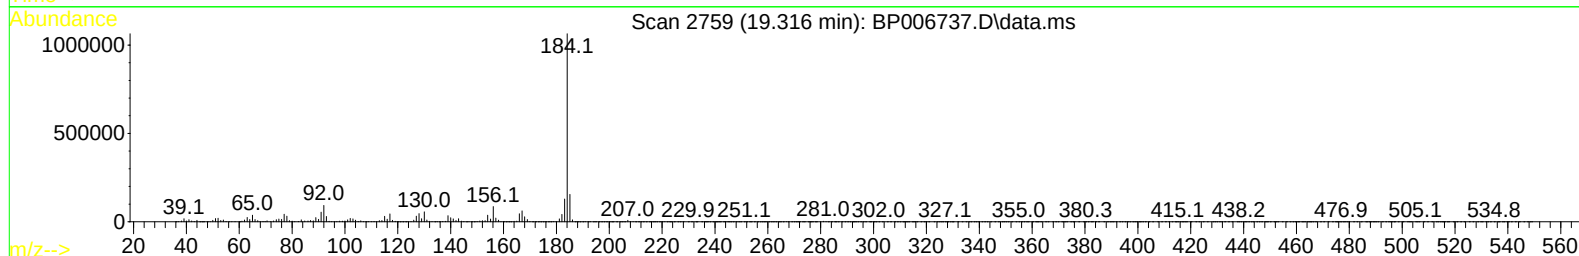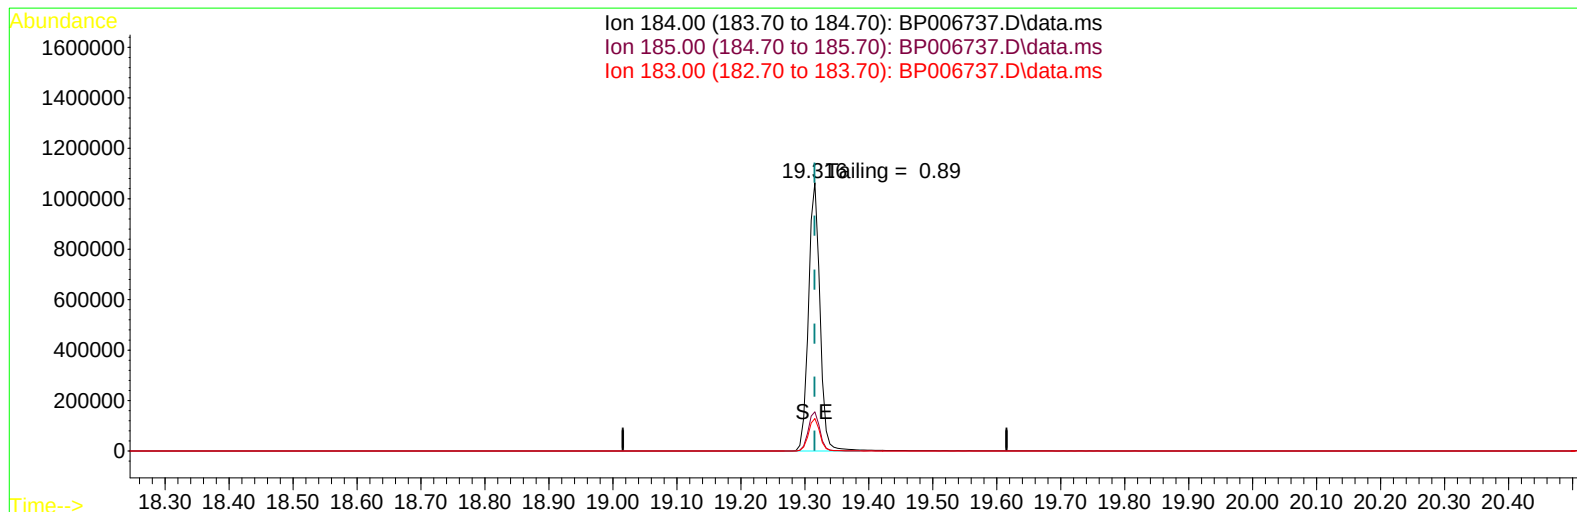

TIC: BP006737.D\data.ms

(77) Benzidine

19.316min (+ 0.000) 228781.44 ng

response 1345345

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.59
183.00	11.90	12.10
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
8/18/2021	BNA_P	<u>BP006737.D</u>
Compound Name	Response	Retention Time
DDT	705290	20.51
DDD	1371	20.09
DDE	1046	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2417	707707	0.34