


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006750.D
 Acq On : 18 Aug 2021 18:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 18:17:59 2021

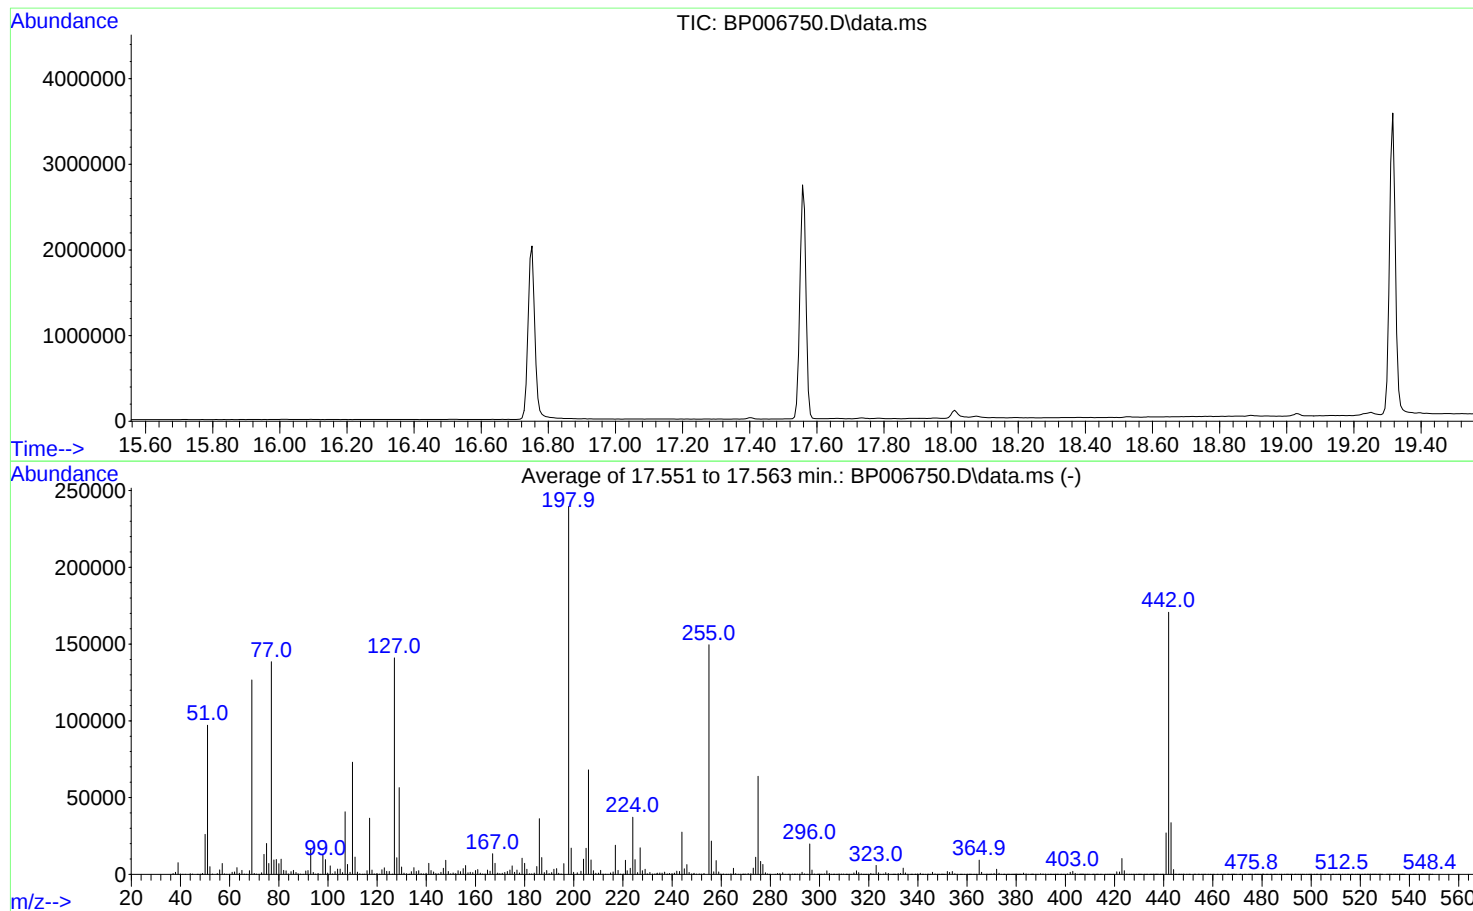




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	97101	PASS
68	69	0.00	2	1.9	2432	PASS
69	198	0.00	100	52.8	126632	PASS
70	69	0.00	2	0.5	653	PASS
127	198	10	80	58.9	141077	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	239626	PASS
199	198	5	9	7.1	17051	PASS
275	198	10	60	26.6	63855	PASS
365	198	1	100	3.9	9324	PASS
441	198	0.01	100	11.3	26989	PASS
442	442	100	100	100.0	170759	PASS
443	442	15	24	19.7	33632	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
 Data File : BP006750.D
 Acq On : 18 Aug 2021 18:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 19 06:17:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 18:17:59 2021
 Response via : Initial Calibration

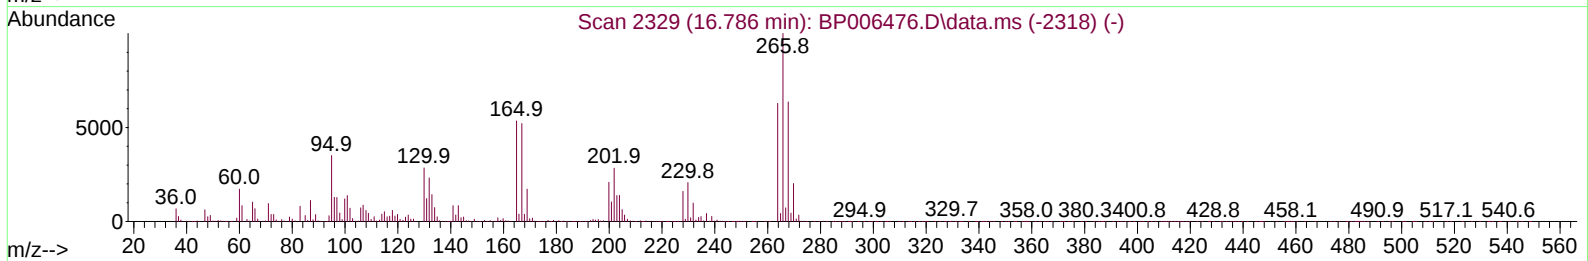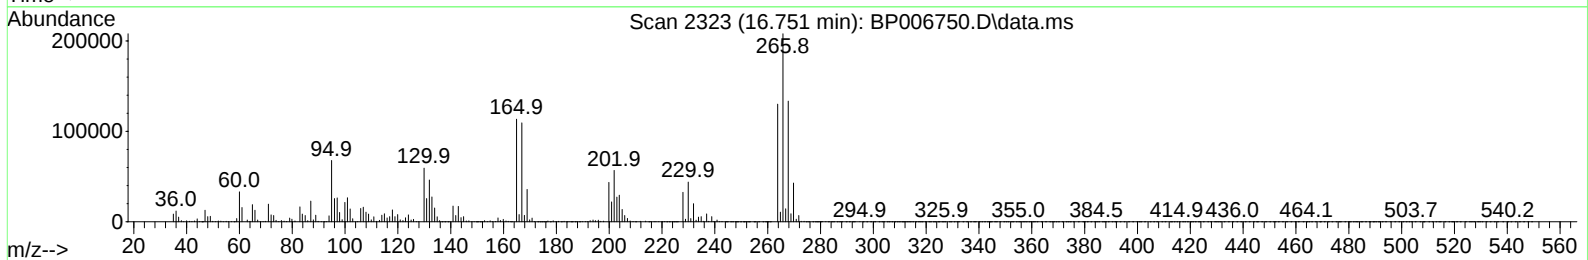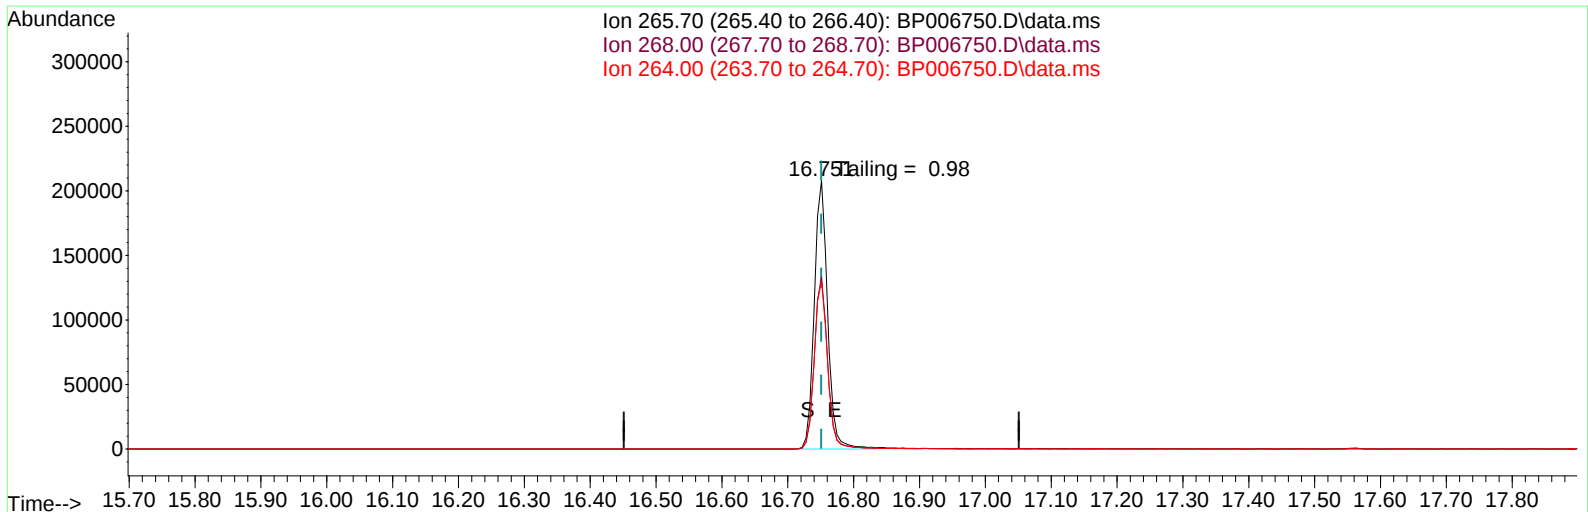

TIC: BP006750.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.000) 229374.78 ng




response 293975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.17
264.00	62.90	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081821\
Data File : BP006750.D
Acq On : 18 Aug 2021 18:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 19 06:17:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:17:59 2021
Response via : Initial Calibration

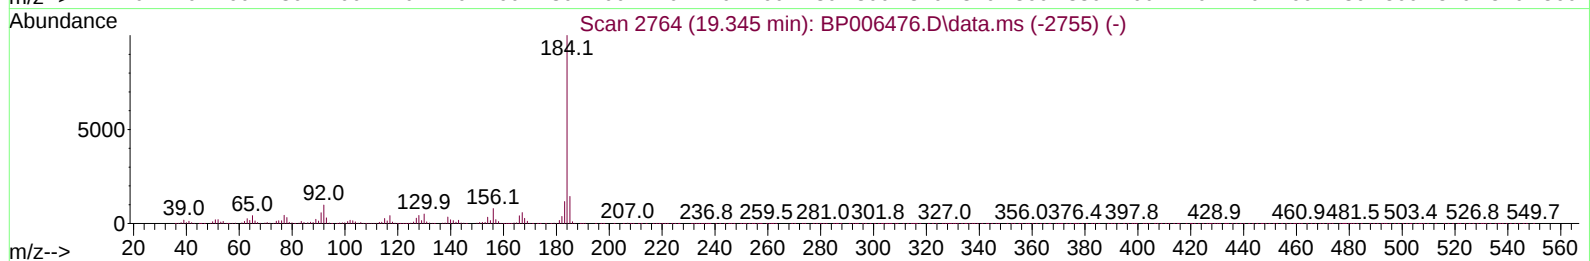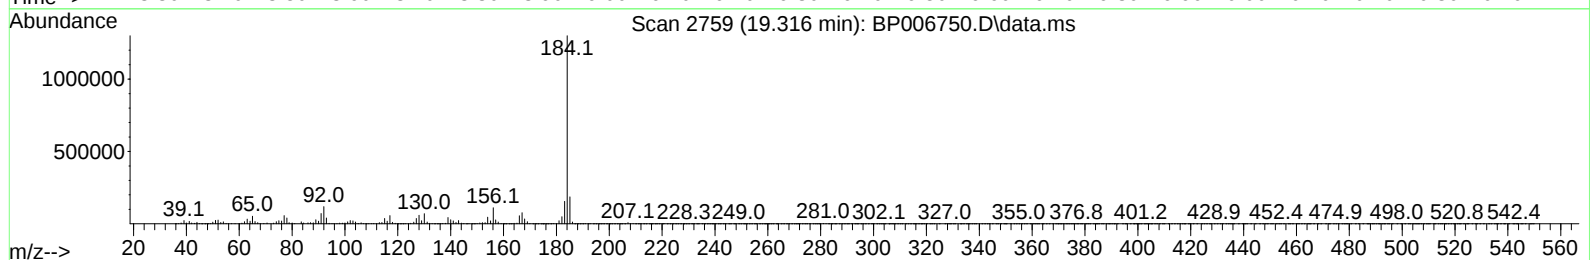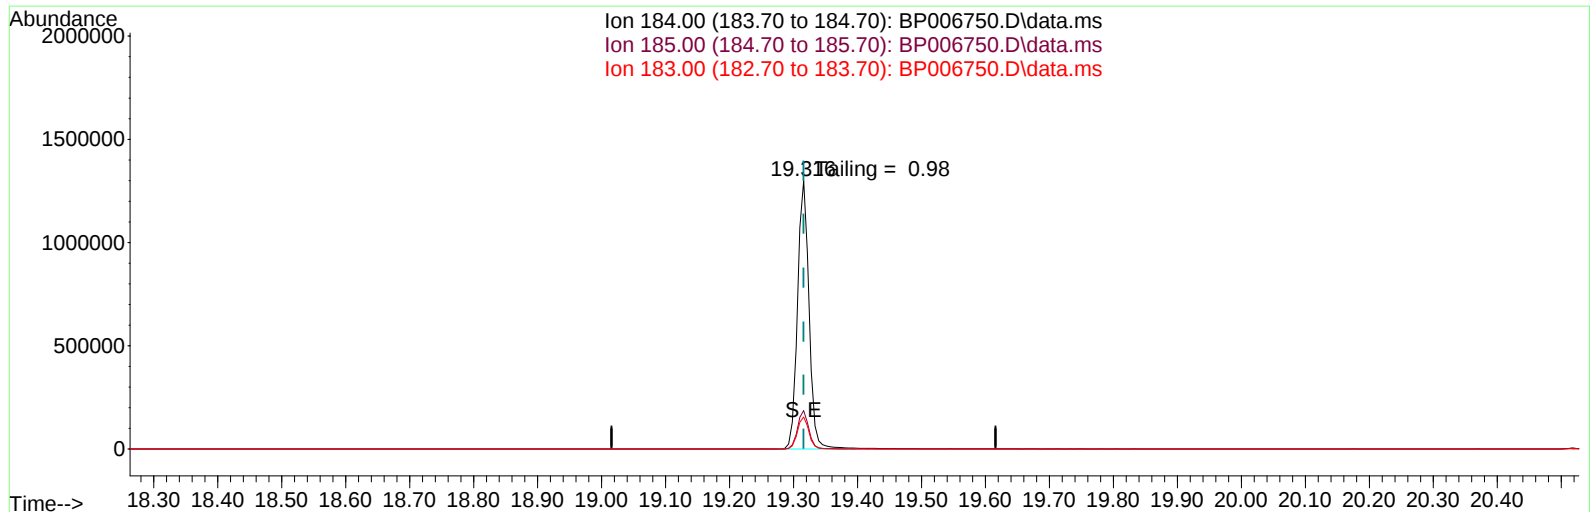

TIC: BP006750.D\data.ms

(77) Benzidine

19.316min (+ 0.000) 564119.53 ng

response 1637473

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.32
183.00	11.90	11.94
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
8/18/2021	BNA_P	BP006750.D
Compound Name	Response	Retention Time
DDT	838570	20.516
DDD	7531	20.086
DDE	1368	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8899	847469	1.05