

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016633.D
 Acq On : 18 Aug 2023 09:00
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020690

Quant Time: Aug 18 22:27:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	288718	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1366411	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.704	164	859377	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.475	188	1916594	20.000	ng/u1	0.00
79) Chrysene-d12	21.574	240	1861857	20.000	ng/u1	0.01
88) Perylene-d12	24.162	264	2095843	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	65228	8.585	ng/uL	0.00
4) Pyridine-d5	3.828	84	473212	20.471	ng/u1	0.00
7) Phenol-d5	7.193	99	552712	20.765	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	361234	20.605	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	418634	21.897	ng/u1	0.00
15) 4-Methylphenol-d8	8.757	113	451949	21.354	ng/u1	0.00
21) Nitrobenzene-d5	9.246	128	212731	22.126	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	221429	24.248	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	406552	22.623	ng/u1	0.00
31) 4-Chloroaniline-d4	11.040	131	653828	21.205	ng/u1	0.00
46) Dimethylphthalate-d6	14.116	166	1340118	21.560	ng/u1	0.00
49) Acenaphthylene-d8	14.404	160	1535062	21.880	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	282846	22.337	ng/u1	0.00
60) Fluorene-d10	15.698	176	1110890	20.964	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	205571	22.546	ng/u1	0.00
73) Anthracene-d10	17.569	188	1765540	21.297	ng/u1	0.00
81) Pyrene-d10	19.804	212	2065907	21.176	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	2120170	21.109	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.428	88	71025	8.502	ng/uL	96
5) Pyridine	3.846	79	491089	20.475	ng/u1	97
6) Benzaldehyde	7.205	77	360145	24.545	ng/u1	97
8) Phenol	7.222	94	580652	20.410	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.481	93	478993	20.843	ng/u1	98
12) 2-Chlorophenol	7.604	128	430177	21.385	ng/u1	96
13) 2-Methylphenol	8.487	108	440454	21.314	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.563	45	662073	20.671	ng/u1	98
16) Acetophenone	8.899	105	736257	21.542	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.869	70	413419	22.554	ng/u1	99
18) 4-Methylphenol	8.822	108	480109	21.139	ng/u1	98
19) Hexachloroethane	9.128	117	179021	21.301	ng/u1	99
22) Nitrobenzene	9.293	77	571400	21.230	ng/u1	97
23) Isophorone	9.804	82	1154880	22.718	ng/u1	99
25) 2-Nitrophenol	9.998	139	247185	23.678	ng/u1	98
26) 2,4-Dimethylphenol	10.034	107	530004	21.536	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.293	93	688868	21.140	ng/u1	99
29) 2,4-Dichlorophenol	10.516	162	410563	22.205	ng/u1	99
30) Naphthalene	10.934	128	1471739	20.615	ng/u1	99
32) 4-Chloroaniline	11.063	127	647144	21.190	ng/u1	100
33) Hexachlorobutadiene	11.169	225	238674	21.414	ng/u1	100
34) Caprolactam	11.869	113	166341	23.125	ng/u1	98
35) 4-Chloro-3-methylphenol	12.157	107	512916	22.695	ng/u1	99
36) 2-Methylnaphthalene	12.534	142	1006364	21.044	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016633.D
 Acq On : 18 Aug 2023 09:00
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020690


Quant Time: Aug 18 22:27:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.751	142	1021710	21.219	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.881	216	482050	20.971	ng/ul	99
40) Hexachlorocyclopentadiene	12.834	237	275183	19.676	ng/ul	98
41) 2,4,6-Trichlorophenol	13.134	196	329447	23.030	ng/ul	99
42) 2,4,5-Trichlorophenol	13.198	196	359258	23.168	ng/ul	99
43) 1,1'-Biphenyl	13.539	154	1317530	20.626	ng/ul	98
44) 2-Chloronaphthalene	13.587	162	1028987	20.704	ng/ul	99
45) 2-Nitroaniline	13.816	65	348017	23.159	ng/ul	91
47) Dimethylphthalate	14.163	163	1340567	21.094	ng/ul	99
48) 2,6-Dinitrotoluene	14.304	165	261790	23.782	ng/ul	96
50) Acenaphthylene	14.434	152	1759328	21.293	ng/ul	99
51) 3-Nitroaniline	14.639	138	285288	23.114	ng/ul	95
52) Acenaphthene	14.769	153	1136936	20.556	ng/ul	99
53) 2,4-Dinitrophenol	14.834	184	125927	20.549	ng/ul	98
55) 4-Nitrophenol	14.922	109	224961	21.853	ng/ul	98
56) Dibenzofuran	15.104	168	1551565	20.561	ng/ul	98
57) 2,4-Dinitrotoluene	15.081	165	389235	23.613	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.316	232	310386	23.890	ng/ul	97
59) Diethylphthalate	15.516	149	1382195	21.271	ng/ul	99
61) Fluorene	15.757	166	1293122	20.899	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.745	204	606852	20.893	ng/ul	98
63) 4-Nitroaniline	15.804	138	285482	24.169	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.833	198	224157	22.172	ng/ul	98
67) N-Nitrosodiphenylamine	15.969	169	1104172	21.254	ng/ul	100
68) 4-Bromophenyl-phenylether	16.651	248	369388	21.586	ng/ul	97
69) Hexachlorobenzene	16.733	284	423161	21.163	ng/ul	99
70) Atrazine	16.922	200	413268	22.111	ng/ul	99
71) Pentachlorophenol	17.092	266	280182	22.759	ng/ul	98
72) Phenanthrene	17.516	178	2079889	20.598	ng/ul	100
74) Anthracene	17.604	178	2129440	20.996	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.492	216	512916	21.058	ng/ul	97
76) Pentachlorobenzene	14.998	250	462446	21.160	ng/ul	98
77) Carbazole	17.886	167	2006744	21.470	ng/ul	99
78) Di-n-butylphthalate	18.398	149	2492376	23.036	ng/ul	100
80) Fluoranthene	19.474	202	2479983	21.299	ng/ul	99
82) Pyrene	19.833	202	2583079	21.009	ng/ul	97
83) Butylbenzylphthalate	20.692	149	1200957	24.247	ng/ul	93
84) 3,3'-Dichlorobenzidine	21.492	252	908891	22.418	ng/ul	100
85) Benzo(a)anthracene	21.557	228	2622355	20.957	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.433	149	1796427	24.991	ng/ul#	99
87) Chrysene	21.610	228	2423785	20.700	ng/ul	99
89) Di-n-octyl phthalate	22.421	149	3142218	24.027	ng/ul	100
90) Benzo(b)fluoranthene	23.351	252	2625049	21.035	ng/ul	99
91) Benzo(k)fluoranthene	23.410	252	2547254	20.575	ng/ul	98
93) Benzo(a)pyrene	24.045	252	2429497	20.638	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.909	276	2572272	18.514	ng/ul	98
95) Dibenzo(a,h)anthracene	26.945	278	2148445	18.582	ng/ul	99
96) Benzo(g,h,i)perylene	27.774	276	2000490	18.091	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 18 22:27:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 8.502 ng/uL
 RT: 3.428 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BP016633.D
 Acq: 18 Aug 2023 09:00




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020690


Tgt Ion: 88 Resp: 71025
 Ion Ratio Lower Upper
 88 100
 43 27.8 23.5 35.3
 58 68.3 57.1 85.7

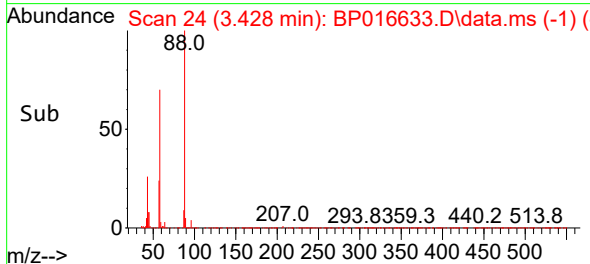

#5
 Pyridine
 Concen: 20.475 ng/uL
 RT: 3.846 min Scan# 95
 Delta R.T. -0.006 min
 Lab File: BP016633.D
 Acq: 18 Aug 2023 09:00

Tgt Ion: 79 Resp: 491089
 Ion Ratio Lower Upper
 79 100
 52 74.5 56.6 84.8
 51 33.6 26.9 40.3


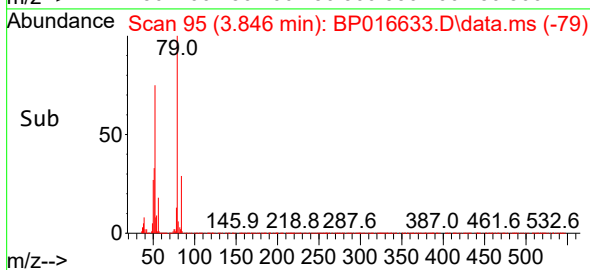

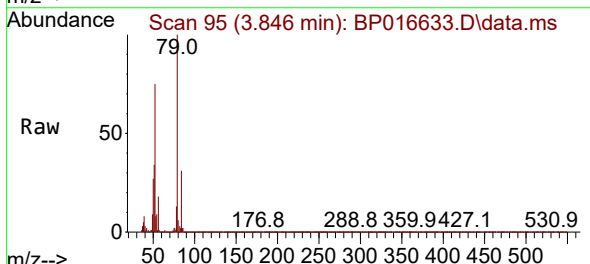




#6
Benzaldehyde
Concen: 24.545 ng/ul
RT: 7.205 min Scan# 666
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion: 77 Resp: 360145
Ion Ratio Lower Upper
77 100
105 93.0 71.8 107.6
106 90.9 70.2 105.2



#8
Phenol
Concen: 20.410 ng/ul
RT: 7.222 min Scan# 669
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion: 94 Resp: 580652
Ion Ratio Lower Upper
94 100
65 27.9 22.3 33.5
66 36.1 28.7 43.1



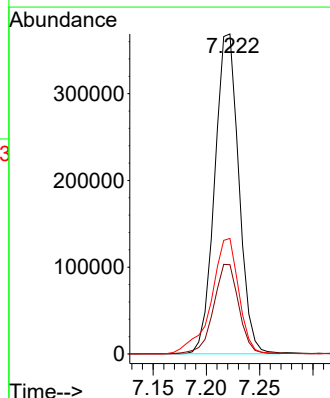





#10
Bis(2-Chloroethyl)ether
Concen: 20.843 ng/ul
RT: 7.481 min Scan# 713
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion: 93 Resp: 478993
Ion Ratio Lower Upper
93 100
63 76.9 60.1 90.1
95 33.1 25.4 38.2

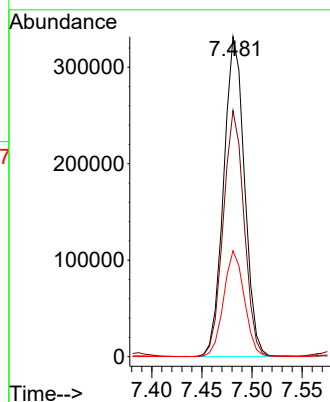

#12
2-Chlorophenol
Concen: 21.385 ng/ul
RT: 7.604 min Scan# 734
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:128 Resp: 430177
Ion Ratio Lower Upper
128 100
64 49.2 41.4 62.0
130 30.5 26.0 39.0





#13

2-Methylphenol

Concen: 21.314 ng/ul

RT: 8.487 min Scan# 884

Delta R.T. -0.000 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :





SSTD020690

Tgt Ion:108 Resp: 440454

Ion Ratio Lower Upper

108 100

107 88.7 70.5 105.7

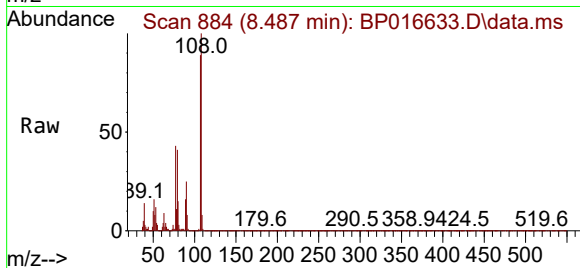

#14

2,2'-oxybis(1-Chloropropane)

Concen: 20.671 ng/ul

RT: 8.563 min Scan# 897

Delta R.T. -0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion: 45 Resp: 662073


Ion Ratio Lower Upper

45 100

77 14.6 12.1 18.1

79 11.2 8.2 12.4




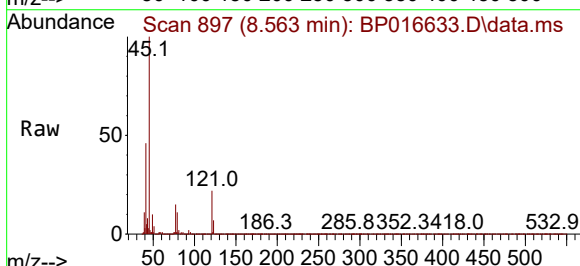




#16
Acetophenone
Concen: 21.542 ng/ul
RT: 8.899 min Scan# 911
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:105 Resp: 736257
Ion Ratio Lower Upper
105 100
77 83.3 64.4 96.6
51 27.2 21.2 31.8



#17
N-Nitroso-di-n-propylamine
Concen: 22.554 ng/ul
RT: 8.869 min Scan# 949
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion: 70 Resp: 413419
Ion Ratio Lower Upper
70 100
42 53.1 43.0 64.4
101 9.4 6.8 10.2
130 18.6 14.2 21.4



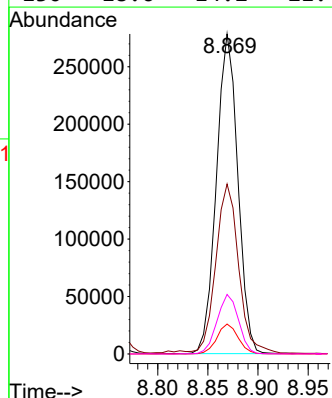





#18
4-Methylphenol
Concen: 21.139 ng/ul
RT: 8.822 min Scan# 941
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:108 Resp: 480109
Ion Ratio Lower Upper
108 100
107 110.7 87.3 130.9



#19
Hexachloroethane
Concen: 21.301 ng/ul
RT: 9.128 min Scan# 993
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:117 Resp: 179021
Ion Ratio Lower Upper
117 100
201 88.7 71.8 107.6
199 55.4 45.2 67.8









#22
Nitrobenzene
Concen: 21.230 ng/ul
RT: 9.293 min Scan# 1021
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion: 77 Resp: 571400
Ion Ratio Lower Upper
77 100
123 43.3 32.5 48.7
65 13.0 10.3 15.5



#23
Isophorone
Concen: 22.718 ng/ul
RT: 9.804 min Scan# 1108
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion: 82 Resp: 1154880
Ion Ratio Lower Upper
82 100
95 6.7 5.3 7.9
138 15.4 12.7 19.1









#25
2-Nitrophenol
Concen: 23.678 ng/ul
RT: 9.998 min Scan# 1141
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:139 Resp: 247185
Ion Ratio Lower Upper
139 100
65 55.6 46.4 69.6
109 31.5 25.3 37.9



#26
2,4-Dimethylphenol
Concen: 21.536 ng/ul
RT: 10.034 min Scan# 1147
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:107 Resp: 530004
Ion Ratio Lower Upper
107 100
121 48.6 39.1 58.7
122 83.6 66.9 100.3









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.140 ng/ul
 RT: 10.293 min Scan# 1191
 Delta R.T. -0.000 min
 Lab File: BP016633.D
 Acq: 18 Aug 2023 09:00




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020690


Tgt Ion: 93 Resp: 688868
 Ion Ratio Lower Upper
 93 100
 95 31.8 25.8 38.8
 123 10.5 8.7 13.1

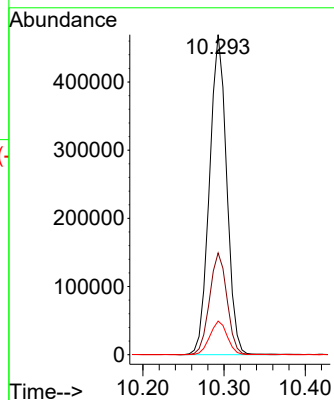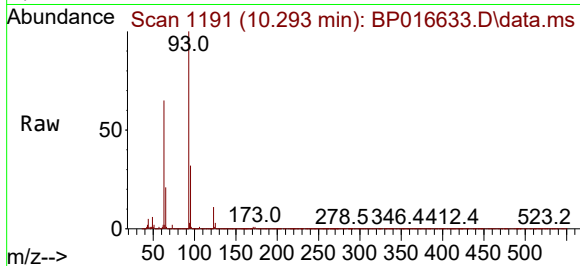

#29
 2,4-Dichlorophenol
 Concen: 22.205 ng/ul
 RT: 10.516 min Scan# 1229
 Delta R.T. -0.000 min
 Lab File: BP016633.D
 Acq: 18 Aug 2023 09:00

Tgt Ion: 162 Resp: 410563
 Ion Ratio Lower Upper
 162 100
 164 66.1 52.9 79.3
 98 39.9 32.7 49.1



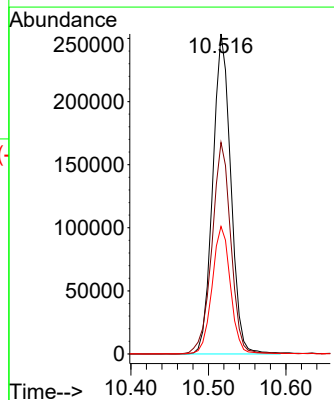
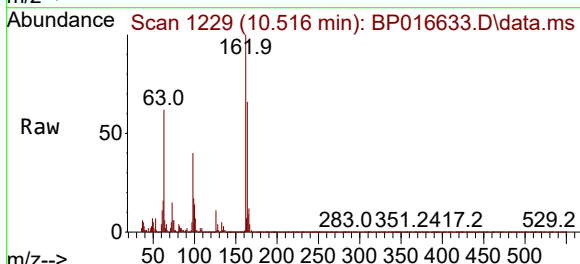




#30
Naphthalene
Concen: 20.615 ng/ul
RT: 10.934 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:128 Resp: 1471739
Ion Ratio Lower Upper
128 100
129 11.2 8.6 13.0
127 13.3 10.3 15.5

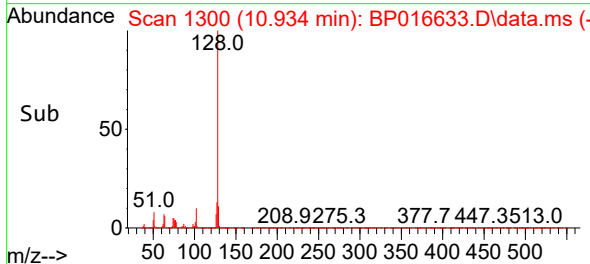

#32
4-Chloroaniline
Concen: 21.190 ng/ul
RT: 11.063 min Scan# 1322
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:127 Resp: 647144
Ion Ratio Lower Upper
127 100
129 31.9 25.6 38.4


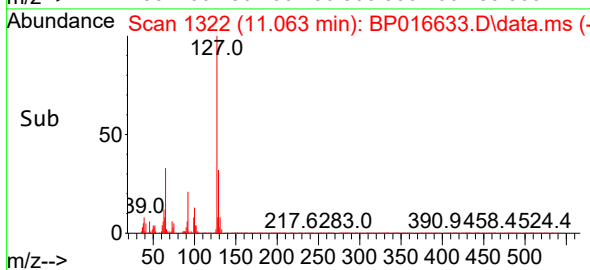

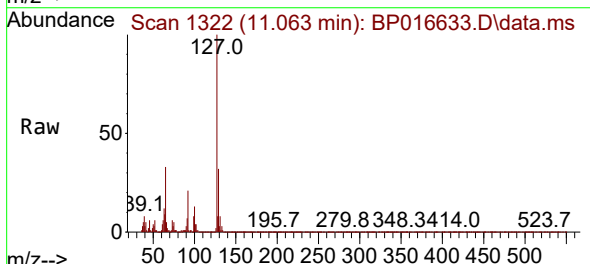




#33
Hexachlorobutadiene
Concen: 21.414 ng/ul
RT: 11.169 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:225 Resp: 238674
Ion Ratio Lower Upper
225 100
223 62.1 50.2 75.2
227 63.6 50.8 76.2



#34
Caprolactam
Concen: 23.125 ng/ul
RT: 11.869 min Scan# 1459
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:113 Resp: 166341
Ion Ratio Lower Upper
113 100
55 169.2 134.8 202.2
56 123.6 101.5 152.3



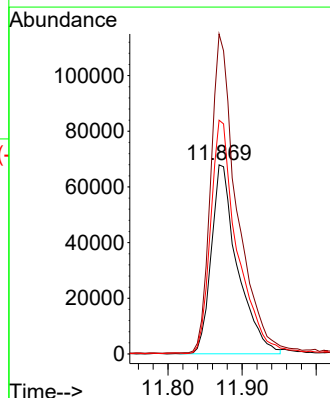





#35
4-Chloro-3-methylphenol
Concen: 22.695 ng/ul
RT: 12.157 min Scan# 1508
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:107 Resp: 512916
Ion Ratio Lower Upper
107 100
144 24.0 19.0 28.6
142 76.1 60.2 90.4



#36
2-Methylnaphthalene
Concen: 21.044 ng/ul
RT: 12.534 min Scan# 1572
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:142 Resp: 1006364
Ion Ratio Lower Upper
142 100
141 88.4 71.4 107.0









#37
1-Methylnaphthalene
Concen: 21.219 ng/ul
RT: 12.751 min Scan# 1609
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:142 Resp: 1021710
Ion Ratio Lower Upper
142 100
141 91.5 74.5 111.7
116 3.8 3.0 4.4

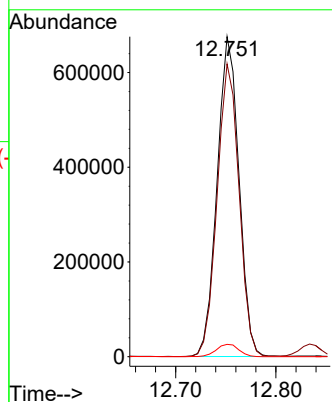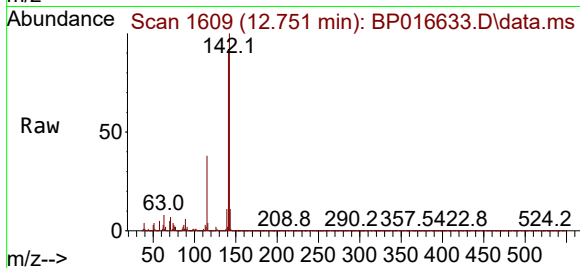

#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.971 ng/ul
RT: 12.881 min Scan# 1631
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:216 Resp: 482050
Ion Ratio Lower Upper
216 100
214 79.1 63.8 95.6
179 22.4 17.9 26.9
108 19.6 16.3 24.5




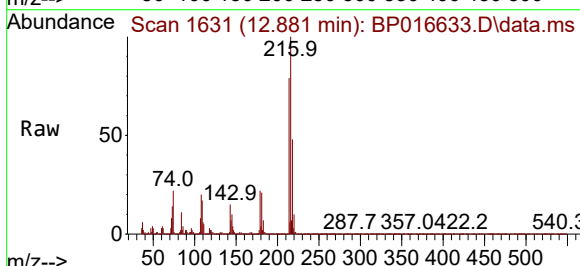




#40
Hexachlorocyclopentadiene
Concen: 19.676 ng/ul
RT: 12.834 min Scan# 1623
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:237 Resp: 275183
Ion Ratio Lower Upper
237 100
235 63.4 49.7 74.5
272 13.3 9.8 14.8

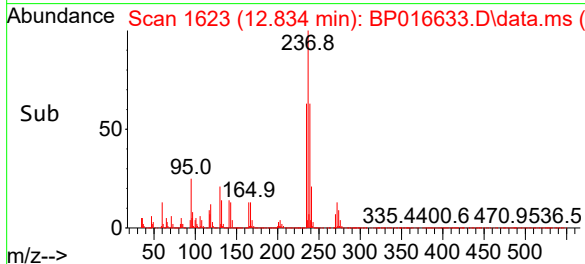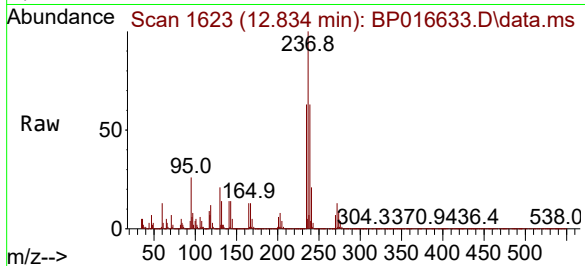

#41
2,4,6-Trichlorophenol
Concen: 23.030 ng/ul
RT: 13.134 min Scan# 1674
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:196 Resp: 329447
Ion Ratio Lower Upper
196 100
198 97.4 77.0 115.4
200 31.2 24.9 37.3


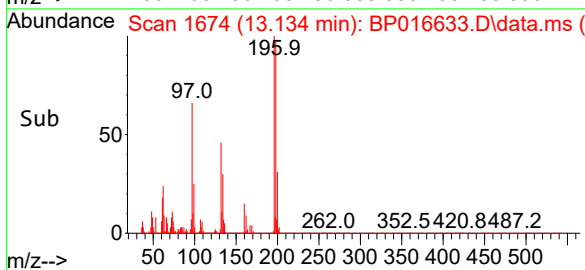

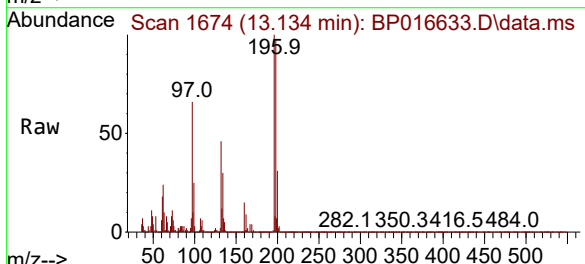




#42
2,4,5-Trichlorophenol
Concen: 23.168 ng/ul
RT: 13.198 min Scan# 1685
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:196 Resp: 359258
Ion Ratio Lower Upper
196 100
198 97.1 76.7 115.1
200 30.4 24.2 36.2

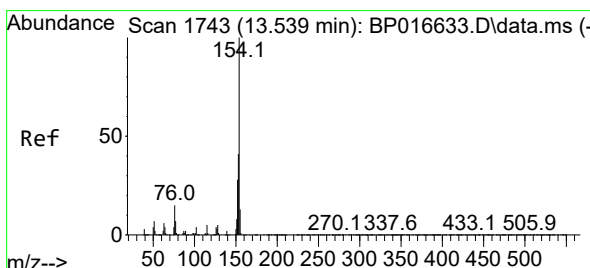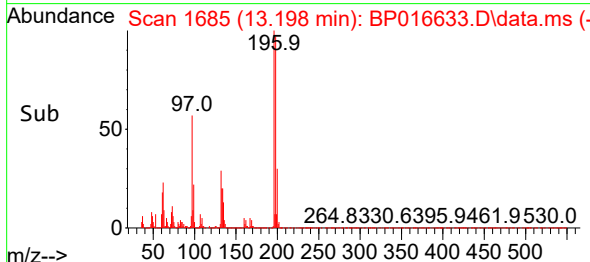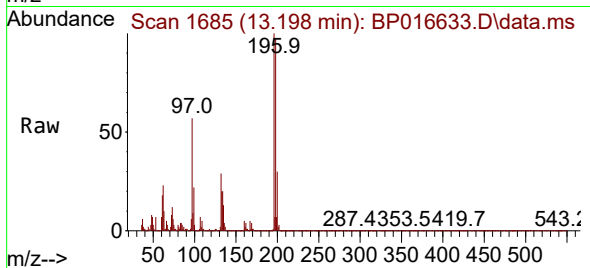

#43
1,1'-Biphenyl
Concen: 20.626 ng/ul
RT: 13.539 min Scan# 1743
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:154 Resp: 1317530
Ion Ratio Lower Upper
154 100
153 40.6 31.4 47.2
76 14.9 13.0 19.4


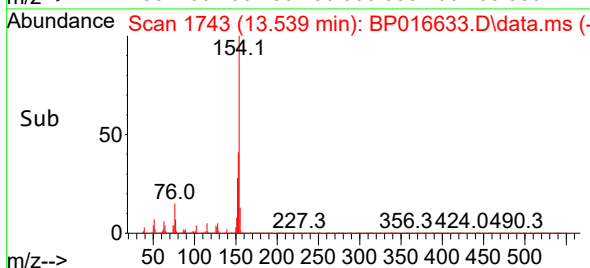

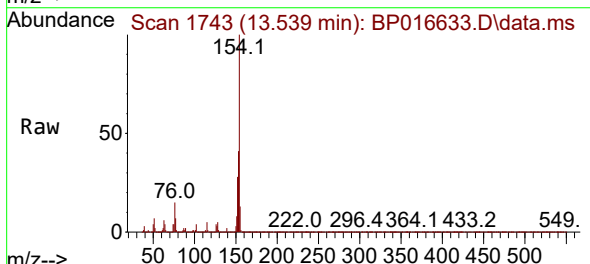




#44
2-Chloronaphthalene
Concen: 20.704 ng/ul
RT: 13.587 min Scan# 1751
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:162 Resp: 1028987
Ion Ratio Lower Upper
162 100
164 32.9 25.8 38.6
127 40.1 32.9 49.3

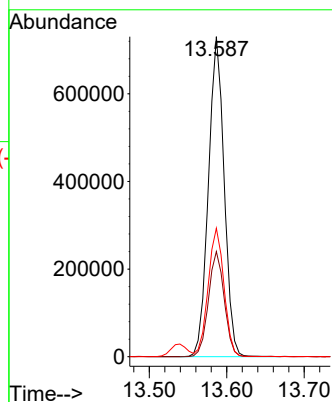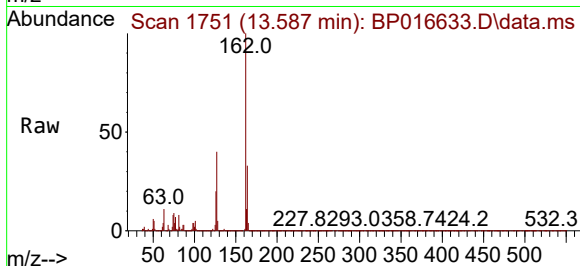

#45
2-Nitroaniline
Concen: 23.159 ng/ul
RT: 13.816 min Scan# 1790
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion: 65 Resp: 348017
Ion Ratio Lower Upper
65 100
92 70.6 54.5 81.7
138 102.2 72.1 108.1


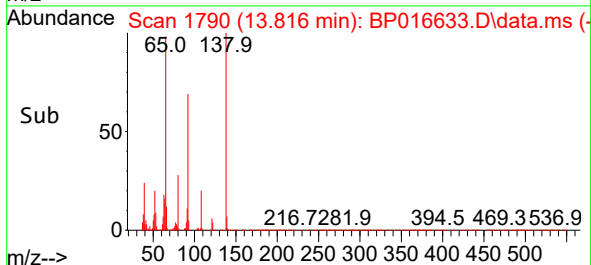

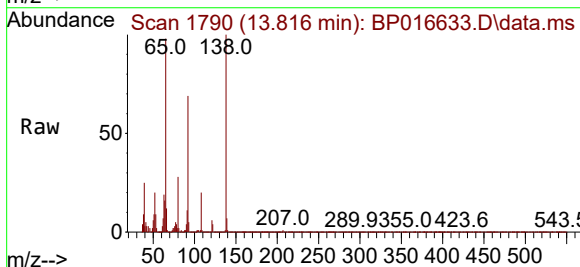




#47
Dimethylphthalate
Concen: 21.094 ng/ul
RT: 14.163 min Scan# 1849
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:163 Resp: 1340567
Ion Ratio Lower Upper
163 100
194 4.0 3.0 4.6
164 10.2 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 23.782 ng/ul
RT: 14.304 min Scan# 1873
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:165 Resp: 261790
Ion Ratio Lower Upper
165 100
89 63.3 53.2 79.8
121 22.2 18.8 28.2



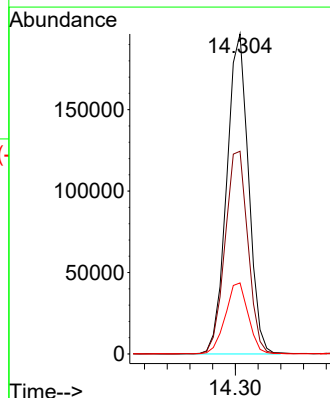





#50
Acenaphthylene
Concen: 21.293 ng/ul
RT: 14.434 min Scan# 1895
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:152 Resp: 1759328
Ion Ratio Lower Upper
152 100
151 20.4 15.7 23.5
153 13.1 10.6 15.8



#51
3-Nitroaniline
Concen: 23.114 ng/ul
RT: 14.639 min Scan# 1930
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:138 Resp: 285288
Ion Ratio Lower Upper
138 100
108 11.8 10.9 16.3
92 125.5 105.0 157.6









#52
Acenaphthene
Concen: 20.556 ng/ul
RT: 14.769 min Scan# 1952
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:153 Resp: 1136936
Ion Ratio Lower Upper
153 100
152 47.8 38.7 58.1
154 89.1 72.0 108.0

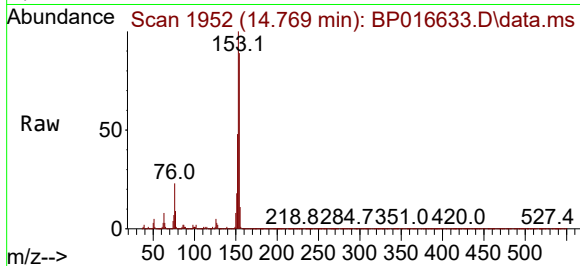

#53
2,4-Dinitrophenol
Concen: 20.549 ng/ul
RT: 14.834 min Scan# 1963
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:184 Resp: 125927
Ion Ratio Lower Upper
184 100
63 81.3 65.0 97.6
154 67.5 56.2 84.2




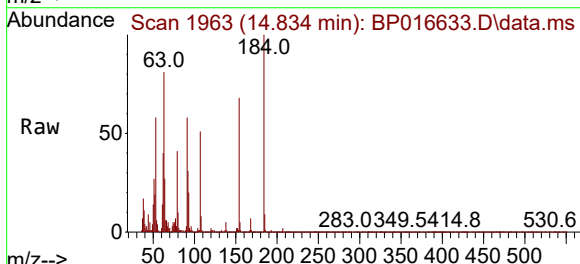




#55
4-Nitrophenol
Concen: 21.853 ng/ul
RT: 14.922 min Scan# 1978
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:109 Resp: 224961
Ion Ratio Lower Upper
109 100
139 131.1 101.1 151.7
65 135.4 108.9 163.3



#56
Dibenzofuran
Concen: 20.561 ng/ul
RT: 15.104 min Scan# 2009
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:168 Resp: 1551565
Ion Ratio Lower Upper
168 100
139 37.9 31.4 47.0









#57
2,4-Dinitrotoluene
Concen: 23.613 ng/ul
RT: 15.081 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:165 Resp: 389235
Ion Ratio Lower Upper
165 100
63 50.8 40.4 60.6
182 2.4 1.9 2.9

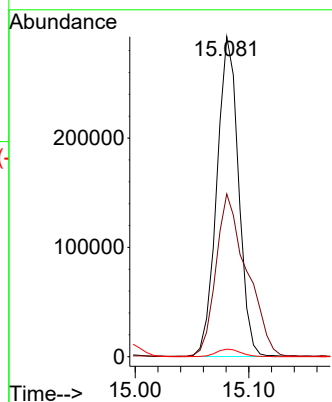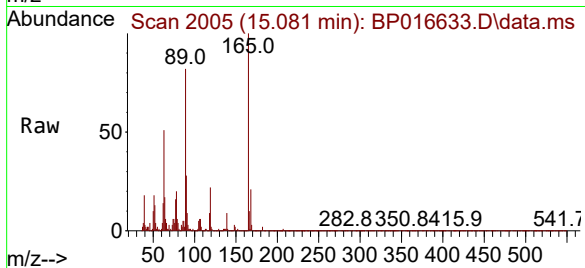

#58
2,3,4,6-Tetrachlorophenol
Concen: 23.890 ng/ul
RT: 15.316 min Scan# 2045
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:232 Resp: 310386
Ion Ratio Lower Upper
232 100
131 50.1 42.9 64.3
130 2.7 2.2 3.4
166 33.6 26.7 40.1




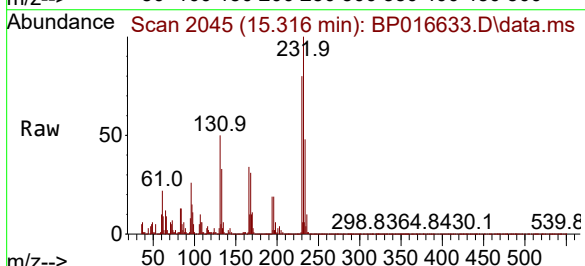




#59
Diethylphthalate
Concen: 21.271 ng/ul
RT: 15.516 min Scan# 2079
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:149 Resp: 1382195
Ion Ratio Lower Upper
149 100
177 21.0 16.5 24.7
150 12.3 10.0 15.0

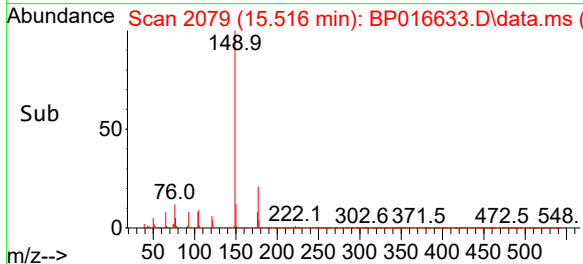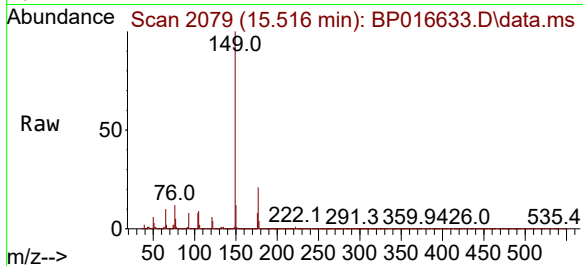

#61
Fluorene
Concen: 20.899 ng/ul
RT: 15.757 min Scan# 2120
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:166 Resp: 1293122
Ion Ratio Lower Upper
166 100
165 97.0 78.3 117.5
167 13.3 10.8 16.2


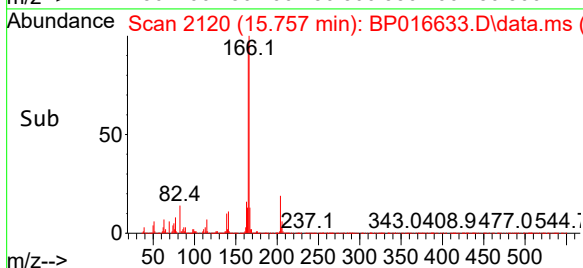
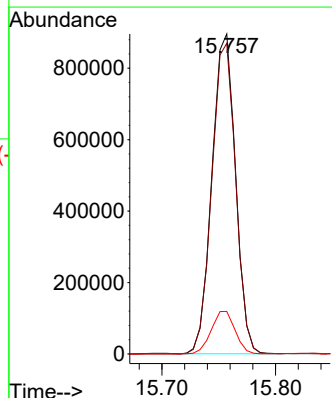
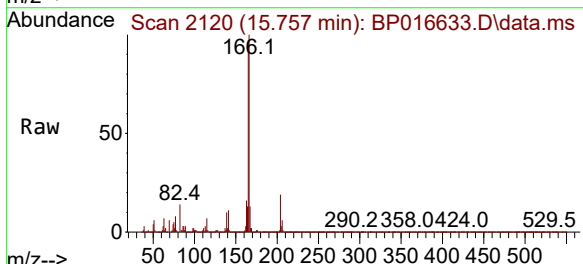




#62
4-Chlorophenyl-phenylether
Concen: 20.893 ng/ul
RT: 15.745 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:204 Resp: 606852
Ion Ratio Lower Upper
204 100
206 33.0 25.5 38.3
141 63.5 52.2 78.2

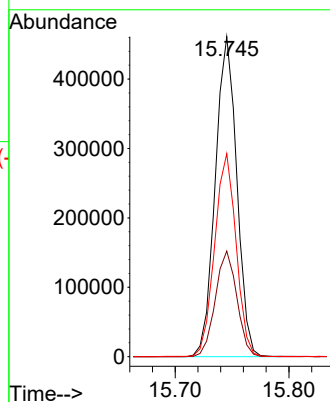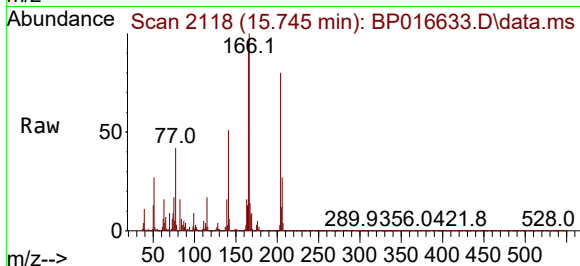

#63
4-Nitroaniline
Concen: 24.169 ng/ul
RT: 15.804 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:138 Resp: 285482
Ion Ratio Lower Upper
138 100
92 57.5 46.7 70.1
108 91.5 73.7 110.5



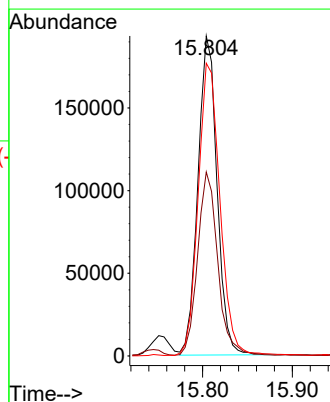
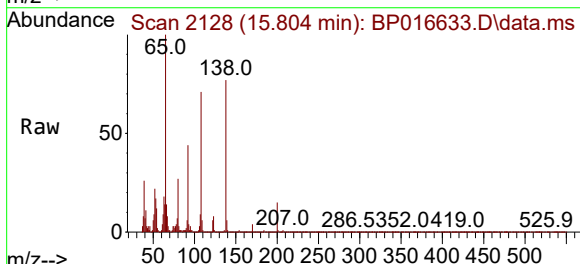




#66
 4,6-Dinitro-2-methylphenol
 Concen: 22.172 ng/ul
 RT: 15.833 min Scan# 2133
 Delta R.T. 0.006 min
 Lab File: BP016633.D
 Acq: 18 Aug 2023 09:00




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020690


Tgt Ion:198 Resp: 224157
 Ion Ratio Lower Upper
 198 100
 182 4.5 3.9 5.9
 77 30.7 25.8 38.6

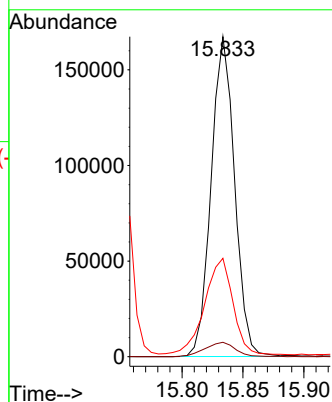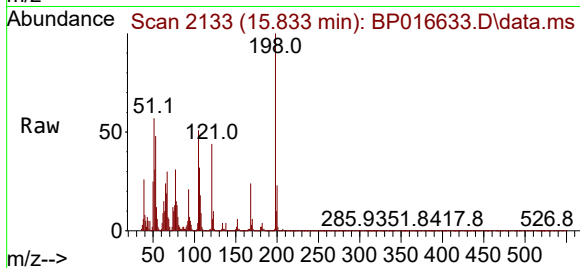

#67
 N-Nitrosodiphenylamine
 Concen: 21.254 ng/ul
 RT: 15.969 min Scan# 2156
 Delta R.T. 0.006 min
 Lab File: BP016633.D
 Acq: 18 Aug 2023 09:00

Tgt Ion:169 Resp: 1104172
 Ion Ratio Lower Upper
 169 100
 168 67.3 53.9 80.9
 167 36.2 29.0 43.6



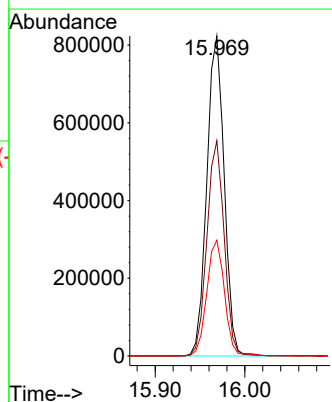
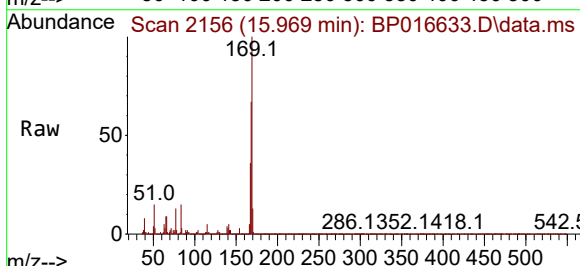




#68
4-Bromophenyl-phenylether
Concen: 21.586 ng/ul
RT: 16.651 min Scan# 2272
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:248 Resp: 369388
Ion Ratio Lower Upper
248 100
250 97.3 76.9 115.3
141 80.3 67.6 101.4

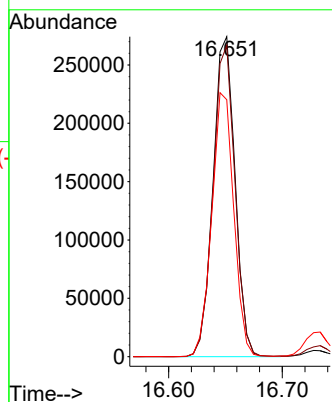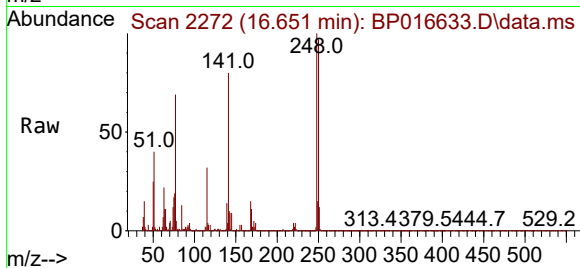

#69
Hexachlorobenzene
Concen: 21.163 ng/ul
RT: 16.733 min Scan# 2286
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:284 Resp: 423161
Ion Ratio Lower Upper
284 100
142 38.9 31.9 47.9
249 31.6 24.7 37.1

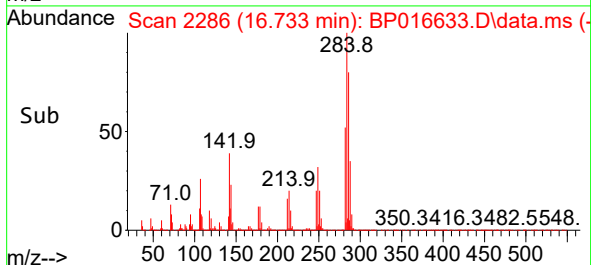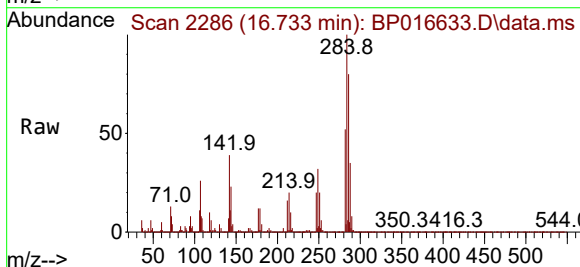



#70

Atrazine

Concen: 22.111 ng/ul

RT: 16.922 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:200 Resp: 413268

Ion Ratio Lower Upper

200 100

173 27.1 22.2 33.2

215 47.2 38.4 57.6

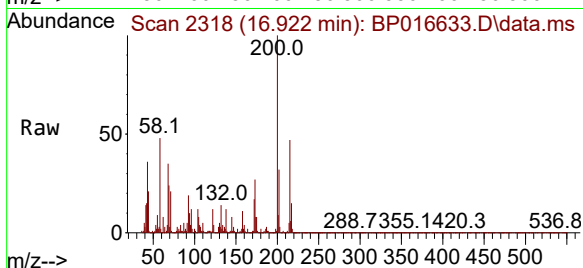

#71

Pentachlorophenol

Concen: 22.759 ng/ul

RT: 17.092 min Scan# 2347

Delta R.T. -0.000 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:266 Resp: 280182


Ion Ratio Lower Upper

266 100

264 62.6 50.7 76.1

268 63.5 53.0 79.6

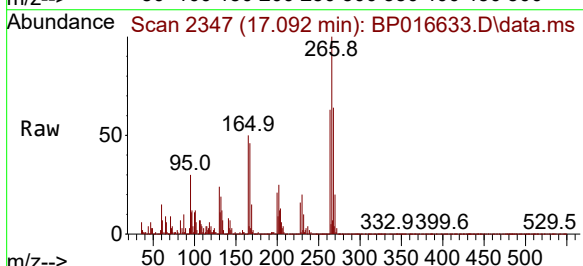



#72

Phenanthrene

Concen: 20.598 ng/ul

RT: 17.516 min Scan# 2419

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:178 Resp: 2079889

Ion Ratio Lower Upper

178 100

179 15.4 12.4 18.6

176 19.2 15.5 23.3



#74

Anthracene

Concen: 20.996 ng/ul

RT: 17.604 min Scan# 2434

Delta R.T. -0.000 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:178 Resp: 2129440


Ion Ratio Lower Upper

178 100

179 15.5 12.5 18.7

176 18.4 14.9 22.3


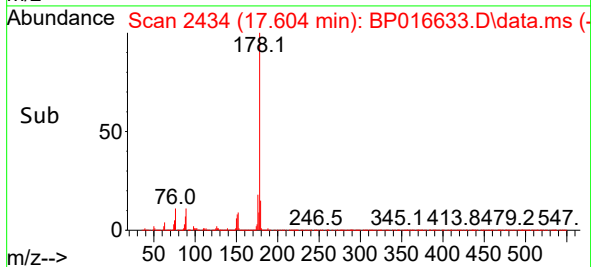

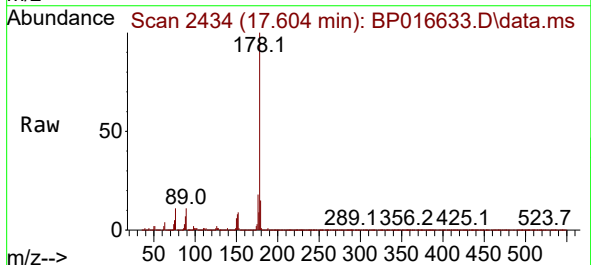




#75
1,2,3,4-Tetrachlorobenzene
Concen: 21.058 ng/uL
RT: 13.492 min Scan# 1735
Delta R.T. -0.000 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00




Instrument :
BNA_P
ClientSampleId :
SSTD020690


Tgt Ion:216 Resp: 512916
Ion Ratio Lower Upper
216 100
214 77.8 65.4 98.2
218 48.8 39.3 58.9



#76
Pentachlorobenzene
Concen: 21.160 ng/uL
RT: 14.998 min Scan# 1991
Delta R.T. 0.006 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:250 Resp: 462446
Ion Ratio Lower Upper
250 100
248 61.7 50.2 75.2
252 62.0 51.0 76.4





#77

Carbazole

Concen: 21.470 ng/ul

RT: 17.886 min Scan# 2482

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:167 Resp: 2006744

Ion Ratio Lower Upper

167 100

166 21.6 16.8 25.2

139 13.3 10.6 16.0



#78

Di-n-butylphthalate

Concen: 23.036 ng/ul

RT: 18.398 min Scan# 2569

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:149 Resp: 2492376


Ion Ratio Lower Upper

149 100

150 9.2 7.3 10.9

104 5.7 4.6 6.8

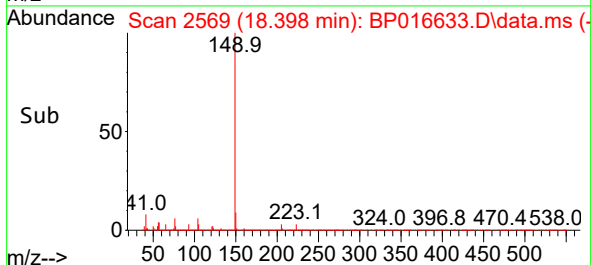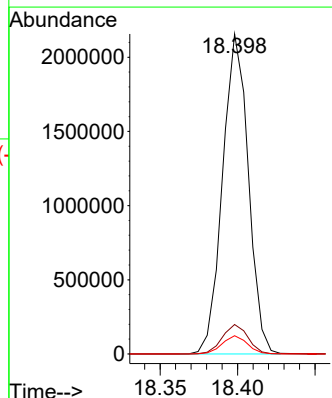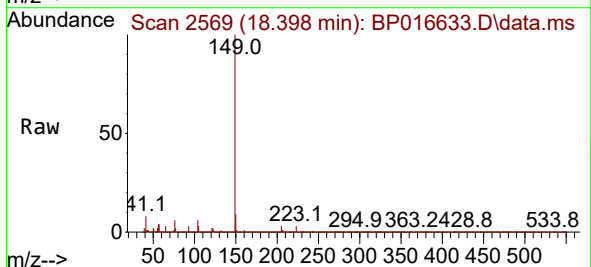



#80

Fluoranthene

Concen: 21.299 ng/ul

RT: 19.474 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:202 Resp: 2479983

Ion Ratio Lower Upper

202 100

101 13.9 10.6 16.0

100 10.4 8.1 12.1



#82

Pyrene

Concen: 21.009 ng/ul

RT: 19.833 min Scan# 2813

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:202 Resp: 2583079


Ion Ratio Lower Upper

202 100

101 15.1 13.4 20.2

100 12.9 11.0 16.4

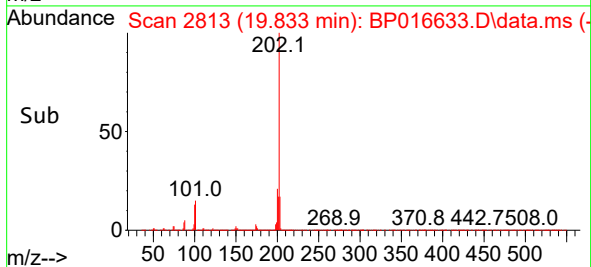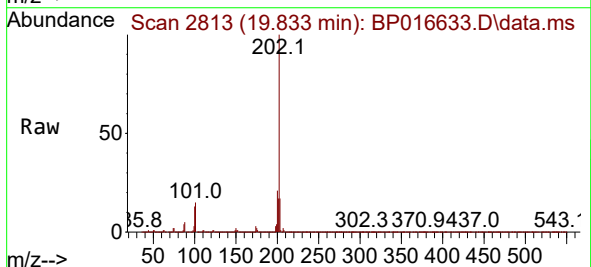



#83

Butylbenzylphthalate

Concen: 24.247 ng/ul

RT: 20.692 min Scan# 2959

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:149 Resp: 1200957

Ion Ratio Lower Upper

149 100

91 77.6 67.8 101.6

206 19.9 14.4 21.6

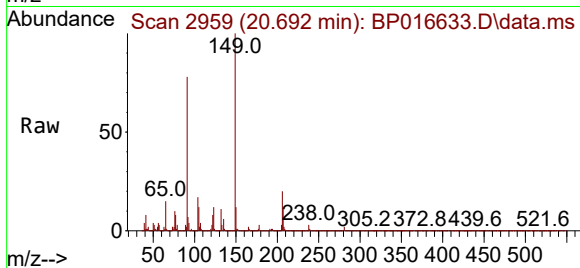

#84

3,3'-Dichlorobenzidine

Concen: 22.418 ng/ul

RT: 21.492 min Scan# 3095

Delta R.T. 0.012 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:252 Resp: 908891


Ion Ratio Lower Upper

252 100

254 64.2 51.3 76.9

126 12.4 10.2 15.4

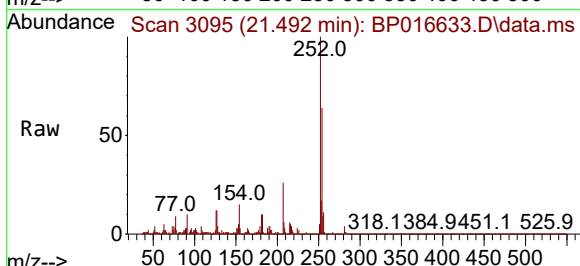



#85

Benzo(a)anthracene

Concen: 20.957 ng/ul

RT: 21.557 min Scan# 3106

Delta R.T. 0.012 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:228 Resp: 2622355

Ion Ratio Lower Upper

228 100

229 19.7 15.8 23.6

226 27.6 21.8 32.6

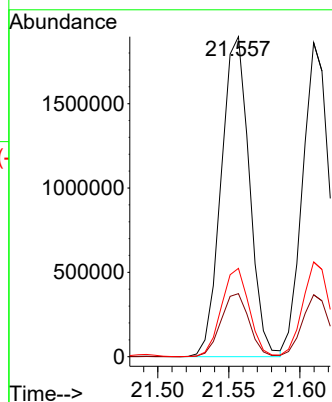

#86

Bis(2-ethylhexyl)phthalate

Concen: 24.991 ng/ul

RT: 21.433 min Scan# 3085

Delta R.T. 0.012 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:149 Resp: 1796427


Ion Ratio Lower Upper

149 100

167 26.8 20.9 31.3

279 4.0 2.6 4.0#





#87

Chrysene

Concen: 20.700 ng/ul

RT: 21.610 min Scan# 3115

Delta R.T. 0.006 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:228 Resp: 2423785

Ion Ratio Lower Upper

228 100

226 30.2 24.6 36.8

229 19.7 16.4 24.6

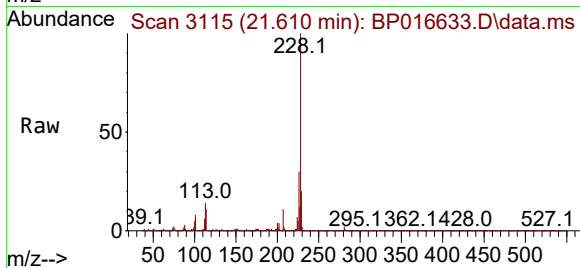

#89

Di-n-octyl phthalate

Concen: 24.027 ng/ul




RT: 22.421 min Scan# 3253


Delta R.T. 0.012 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Tgt Ion:149 Resp: 3142218

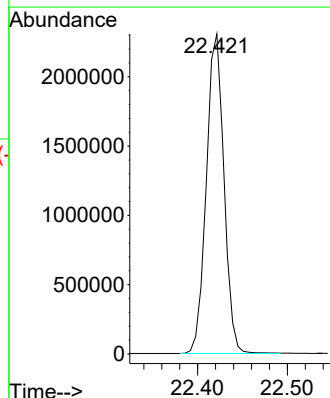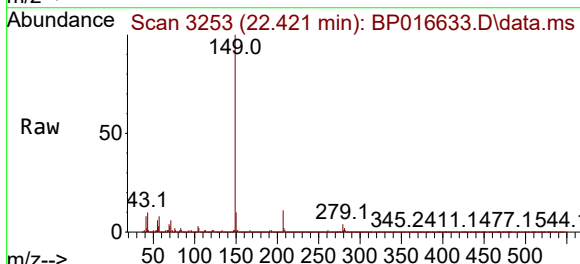



#90

Benzo(b)fluoranthene

Concen: 21.035 ng/ul

RT: 23.351 min Scan# 3411

Delta R.T. 0.012 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:252 Resp: 2625049

Ion Ratio Lower Upper

252 100

253 22.0 17.4 26.2

125 12.0 10.0 15.0

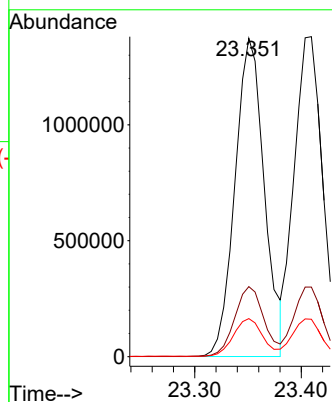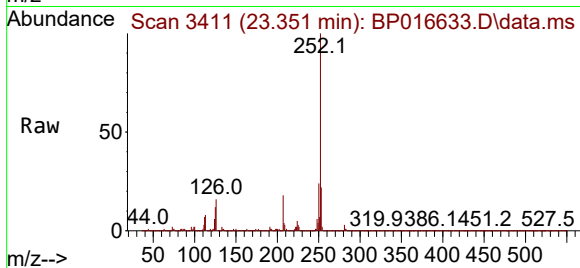

#91

Benzo(k)fluoranthene

Concen: 20.575 ng/ul

RT: 23.410 min Scan# 3421

Delta R.T. 0.017 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:252 Resp: 2547254


Ion Ratio Lower Upper

252 100

253 21.8 18.0 27.0

125 11.7 9.8 14.8

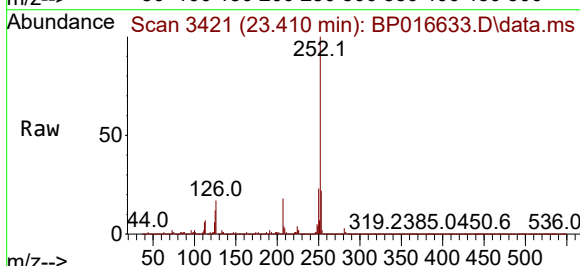



#93

Benzo(a)pyrene

Concen: 20.638 ng/ul

RT: 24.045 min Scan# 3529

Delta R.T. 0.017 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00

Instrument :

BNA_P

ClientSampleId :

SSTD020690





Tgt Ion:252 Resp: 2429497

Ion Ratio Lower Upper

252 100

253 21.8 17.7 26.5

125 13.1 10.6 15.8

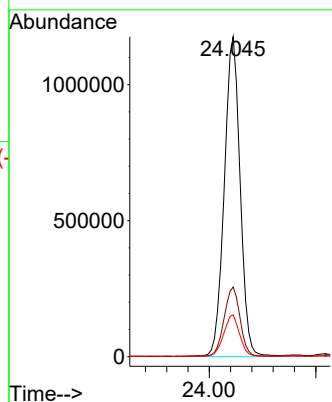

#94

Indeno(1,2,3-cd)pyrene

Concen: 18.514 ng/ul

RT: 26.909 min Scan# 4016

Delta R.T. 0.023 min

Lab File: BP016633.D

Acq: 18 Aug 2023 09:00




Tgt Ion:276 Resp: 2572272


Ion Ratio Lower Upper

276 100

138 25.4 21.7 32.5

277 24.1 19.5 29.3









#95
Dibenzo(a,h)anthracene
Concen: 18.582 ng/ul
RT: 26.945 min Scan# 4022
Delta R.T. 0.029 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Instrument :
BNA_P
ClientSampleId :
SSTD020690

Tgt Ion:278 Resp: 2148445
Ion Ratio Lower Upper
278 100
139 18.2 15.5 23.3
279 23.9 19.1 28.7

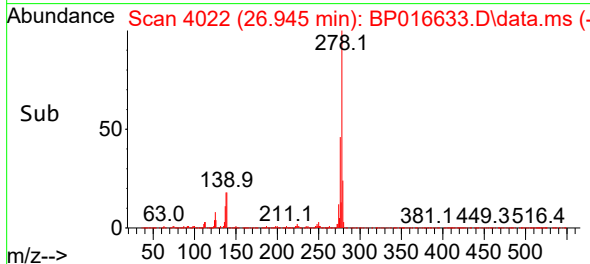

#96
Benzo(g,h,i)perylene
Concen: 18.091 ng/ul
RT: 27.774 min Scan# 4163
Delta R.T. 0.029 min
Lab File: BP016633.D
Acq: 18 Aug 2023 09:00

Tgt Ion:276 Resp: 2000490
Ion Ratio Lower Upper
276 100
138 24.7 21.5 32.3
277 23.6 19.3 28.9

