

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081823\  
 Data File : BP016650.D  
 Acq On : 18 Aug 2023 20:22  
 Operator : MA/JU  
 Sample : 03968-28  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A48P7

Quant Time: Aug 18 22:34:10 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP081423.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Aug 17 01:38:34 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.052  | 152  | 316578   | 20.000 | ng/ul | 0.00     |
| 20) Naphthalene-d8            | 10.881 | 136  | 1446700  | 20.000 | ng/ul | 0.00     |
| 38) Acenaphthene-d10          | 14.704 | 164  | 924508   | 20.000 | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 17.469 | 188  | 2020169  | 20.000 | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.563 | 240  | 1683276  | 20.000 | ng/ul | 0.00     |
| 88) Perylene-d12              | 24.151 | 264  | 1490441  | 20.000 | ng/ul | 0.00     |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.393  | 96   | 56550    | 6.788  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.828  | 84   | 663705   | 26.184 | ng/ul | 0.00     |
| 7) Phenol-d5                  | 7.193  | 99   | 879133   | 30.122 | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.387  | 67   | 551380   | 28.683 | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.569  | 132  | 626026   | 29.863 | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8         | 8.752  | 113  | 721323   | 31.082 | ng/ul | 0.00     |
| 21) Nitrobenzene-d5           | 9.246  | 128  | 333347   | 32.747 | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.963  | 143  | 356544   | 36.878 | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.487 | 165  | 649247   | 34.123 | ng/ul | 0.00     |
| 31) 4-Chloroaniline-d4        | 11.034 | 131  | 1026673  | 31.449 | ng/ul | 0.00     |
| 46) Dimethylphthalate-d6      | 14.110 | 166  | 2474821  | 37.010 | ng/ul | 0.00     |
| 49) Acenaphthylene-d8         | 14.404 | 160  | 2733654  | 36.219 | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.904 | 143  | 408460   | 29.985 | ng/ul | 0.00     |
| 60) Fluorene-d10              | 15.698 | 176  | 2110645  | 37.025 | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.816 | 200  | 249060   | 25.915 | ng/ul | 0.00     |
| 73) Anthracene-d10            | 17.569 | 188  | 3345740  | 38.288 | ng/ul | 0.00     |
| 81) Pyrene-d10                | 19.798 | 212  | 3797829  | 43.059 | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.980 | 264  | 2797689  | 39.168 | ng/ul | 0.00     |
| Target Compounds              |        |      |          |        |       |          |
| 86) Bis(2-ethylhexyl)phtha... | 21.422 | 149  | 86841    | 1.336  | ng/ul | 99       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081823\  
Data File : BP016650.D  
Acq On : 18 Aug 2023 20:22  
Operator : MA/JU  
Sample : 03968-28  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
A48P7

Quant Time: Aug 18 22:34:10 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP081423.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Aug 17 01:38:34 2023  
Response via : Initial Calibration

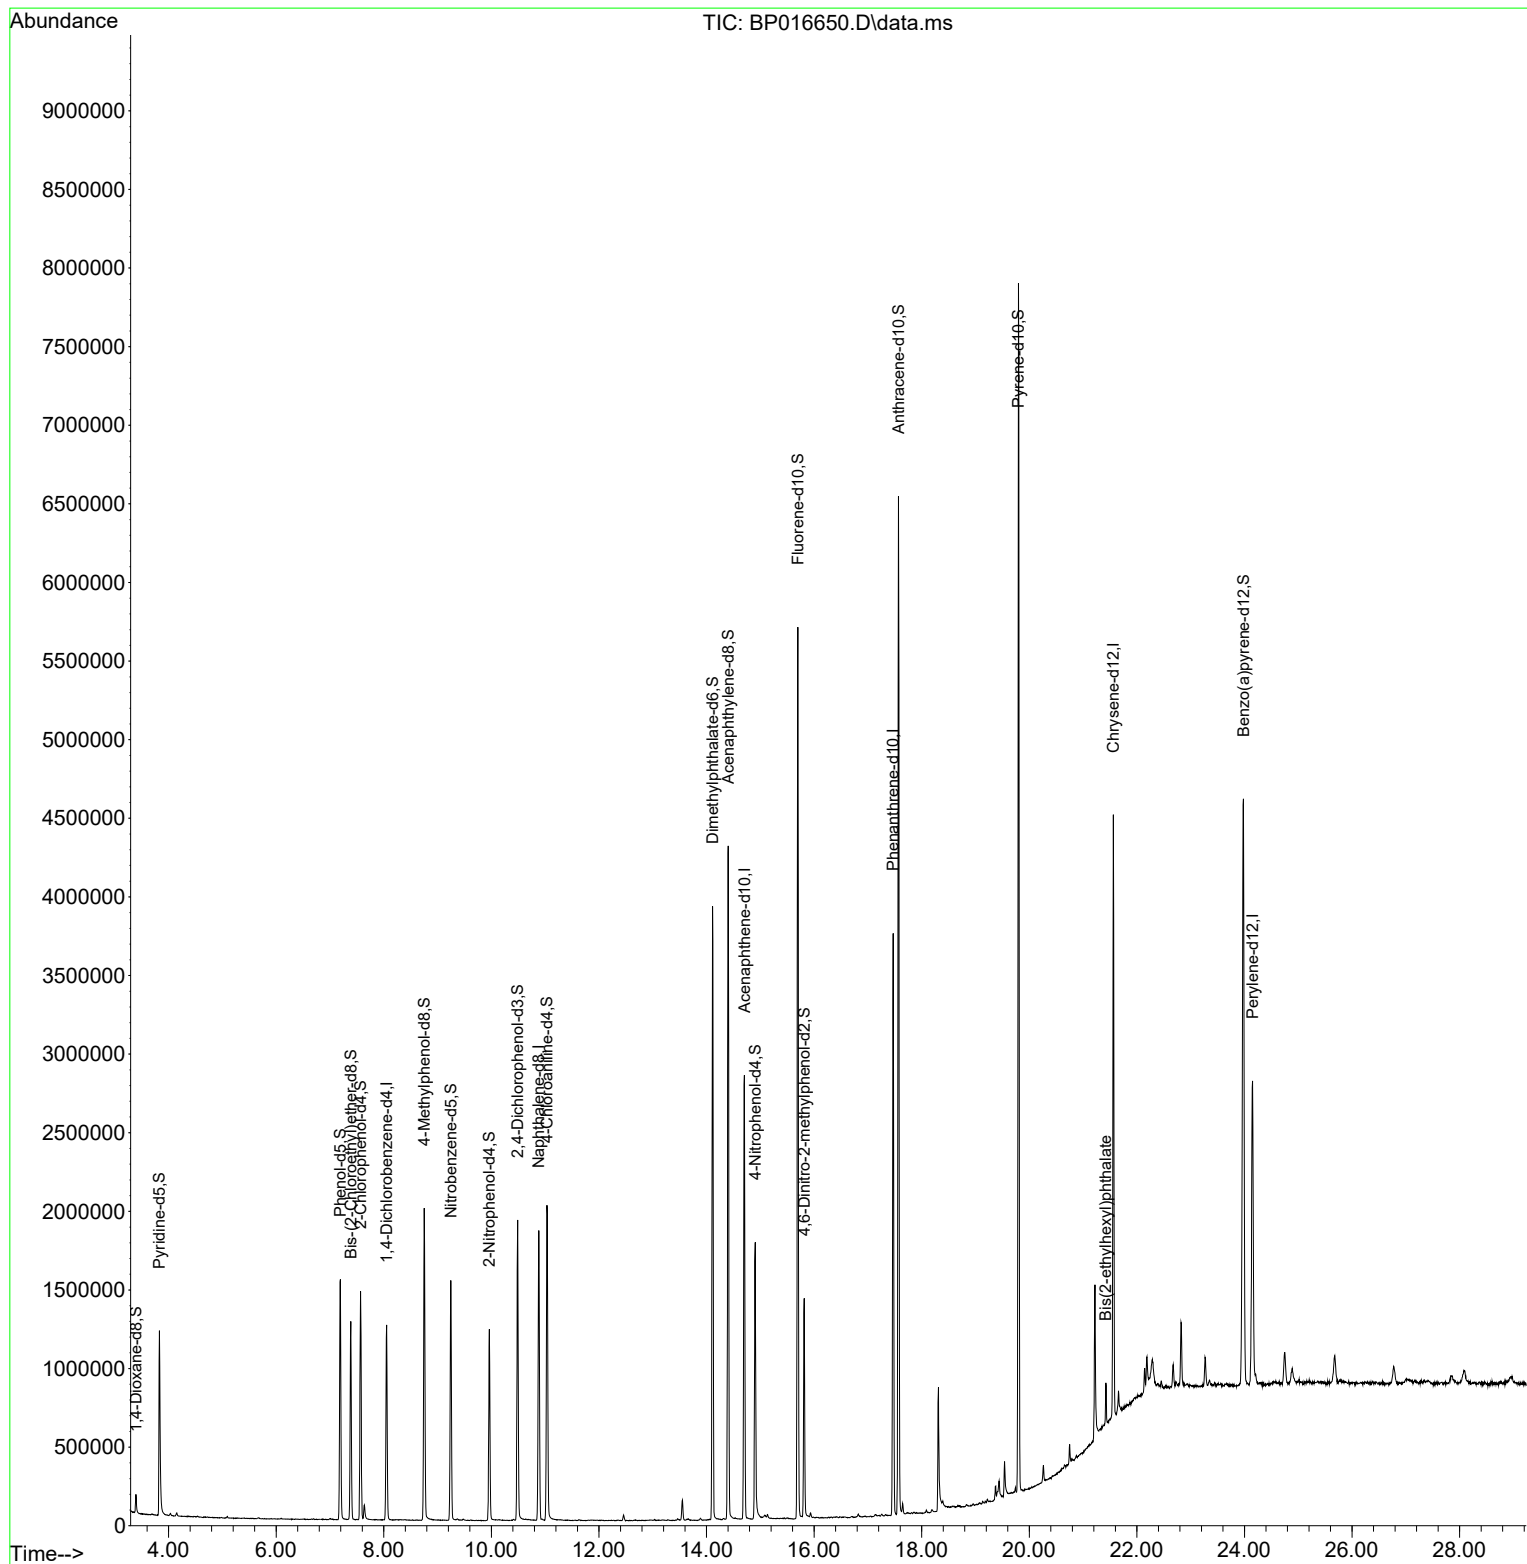

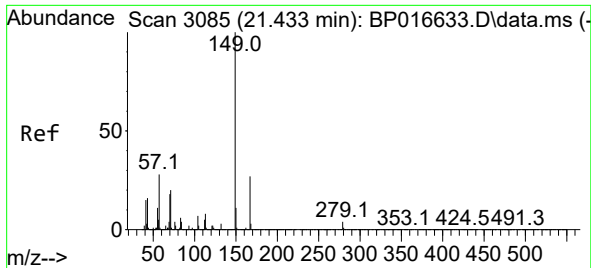

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 1.336 ng/ul  
 RT: 21.422 min Scan# 3083  
 Delta R.T. 0.000 min  
 Lab File: BP016650.D  
 Acq: 18 Aug 2023 20:22

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A48P7

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 149   | Resp: | 86841 |
| Ion Ratio | Lower | Upper |       |
| 149       | 100   |       |       |
| 167       | 25.7  | 20.9  | 31.3  |
| 279       | 3.4   | 2.6   | 4.0   |

