

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016636.D
 Acq On : 18 Aug 2023 11:16
 Operator : MA/JU
 Sample : 03970-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48H5

Quant Time: Aug 18 22:44:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	226450	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	1030154	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164	666836	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1499975	20.000	ng/ul	0.00
79) Chrysene-d12	21.568	240	1473551	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1677855	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	28656	4.809	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.187	99	425756	20.394	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	291376	21.190	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	308263	20.558	ng/ul	0.00
15) 4-Methylphenol-d8	8.751	113	299166	18.022	ng/ul	0.00
21) Nitrobenzene-d5	9.246	128	161832	22.326	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	164876	23.949	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	286436	21.142	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	402417	17.311	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	1170514	24.269	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	1253524	23.026	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	167711	17.069	ng/ul	0.00
60) Fluorene-d10	15.698	176	993429	24.160	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	121659	17.049	ng/ul	0.00
73) Anthracene-d10	17.569	188	1612095	24.847	ng/ul	0.00
81) Pyrene-d10	19.804	212	1956702	25.342	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	2033284	25.287	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.899	105	64176	2.394	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016636.D
Acq On : 18 Aug 2023 11:16
Operator : MA/JU
Sample : 03970-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48H5

Quant Time: Aug 18 22:44:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

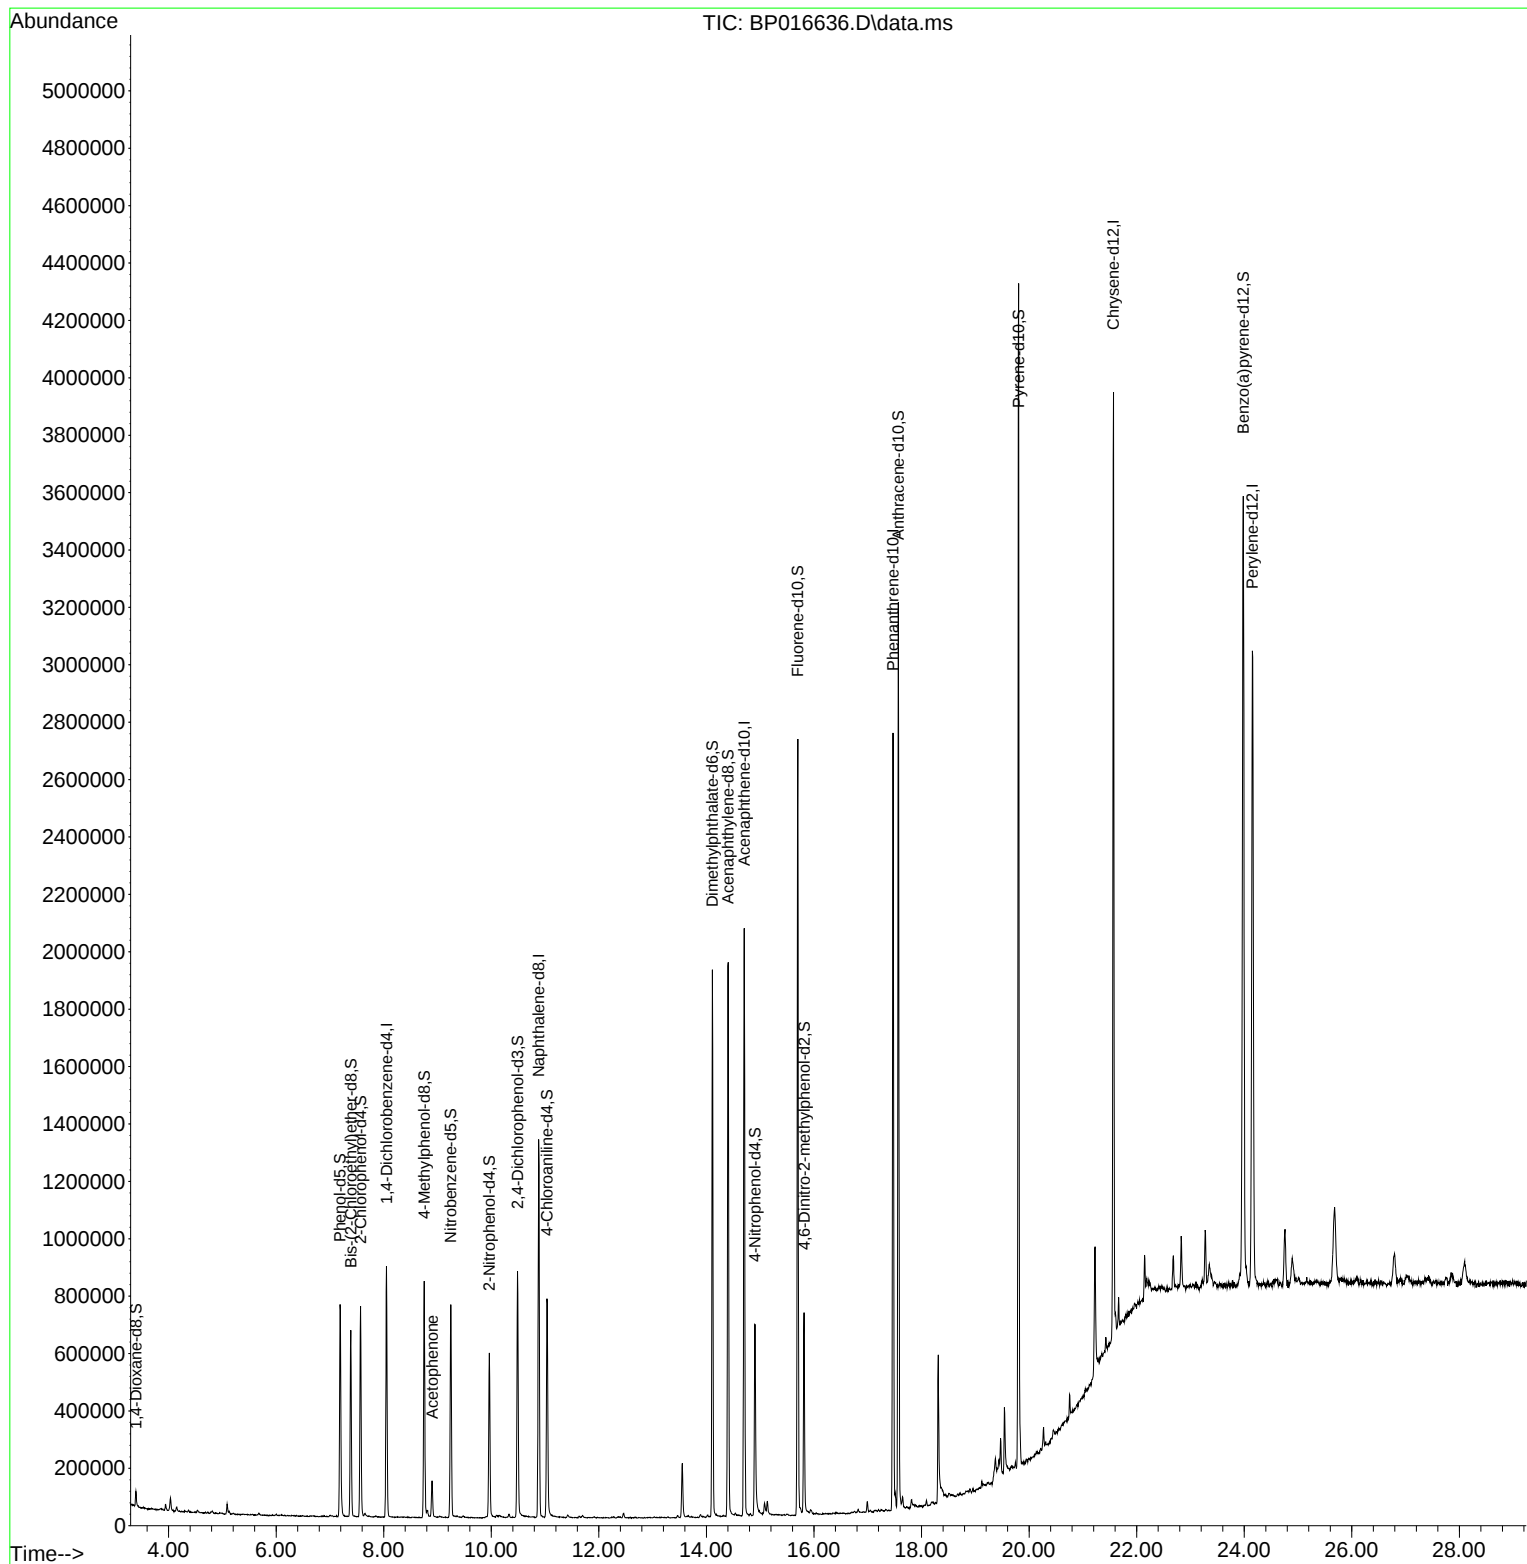

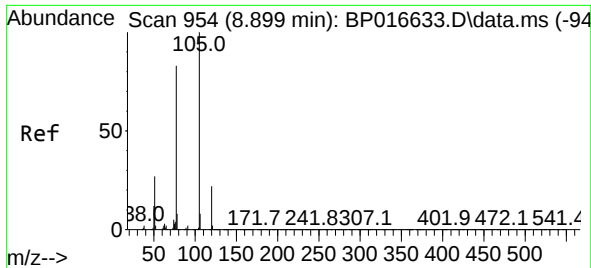

#16
 Acetophenone
 Concen: 2.394 ng/ul
 RT: 8.899 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP016636.D
 Acq: 18 Aug 2023 11:16

Instrument :
 BNA_P
 ClientSampleId :
 A48H5

Tgt Ion:	105	Resp:	64176
Ion	Ratio	Lower	Upper
105	100		
77	81.7	64.4	96.6
51	24.9	21.2	31.8

