

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016640.D
 Acq On : 18 Aug 2023 13:32
 Operator : MA/JU
 Sample : 03968-23
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48N8

Quant Time: Aug 18 23:12:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	266727	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1217633	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.704	164	779480	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.469	188	1736768	20.000	ng/u1	0.00
79) Chrysene-d12	21.568	240	1603113	20.000	ng/u1	0.00
88) Perylene-d12	24.157	264	1738109	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	37141	5.291	ng/uL	0.00
4) Pyridine-d5	3.828	84	339493	15.897	ng/u1	0.00
7) Phenol-d5	7.187	99	572182	23.269	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	364240	22.489	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	406068	22.991	ng/u1	0.00
15) 4-Methylphenol-d8	8.752	113	445720	22.796	ng/u1	0.00
21) Nitrobenzene-d5	9.246	128	208601	24.348	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	215073	26.430	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	390352	24.376	ng/u1	0.00
31) 4-Chloroaniline-d4	11.040	131	409208	14.893	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	1426118	25.295	ng/u1	0.00
49) Acenaphthylene-d8	14.404	160	1558984	24.499	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	257526	22.422	ng/u1	0.00
60) Fluorene-d10	15.698	176	1211407	25.204	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	154457	18.694	ng/u1	0.00
73) Anthracene-d10	17.569	188	1937439	25.790	ng/u1	0.00
81) Pyrene-d10	19.804	212	2390637	28.460	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.980	264	2254973	27.072	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.899	105	57029	1.806	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016640.D
Acq On : 18 Aug 2023 13:32
Operator : MA/JU
Sample : 03968-23
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48N8

Quant Time: Aug 18 23:12:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

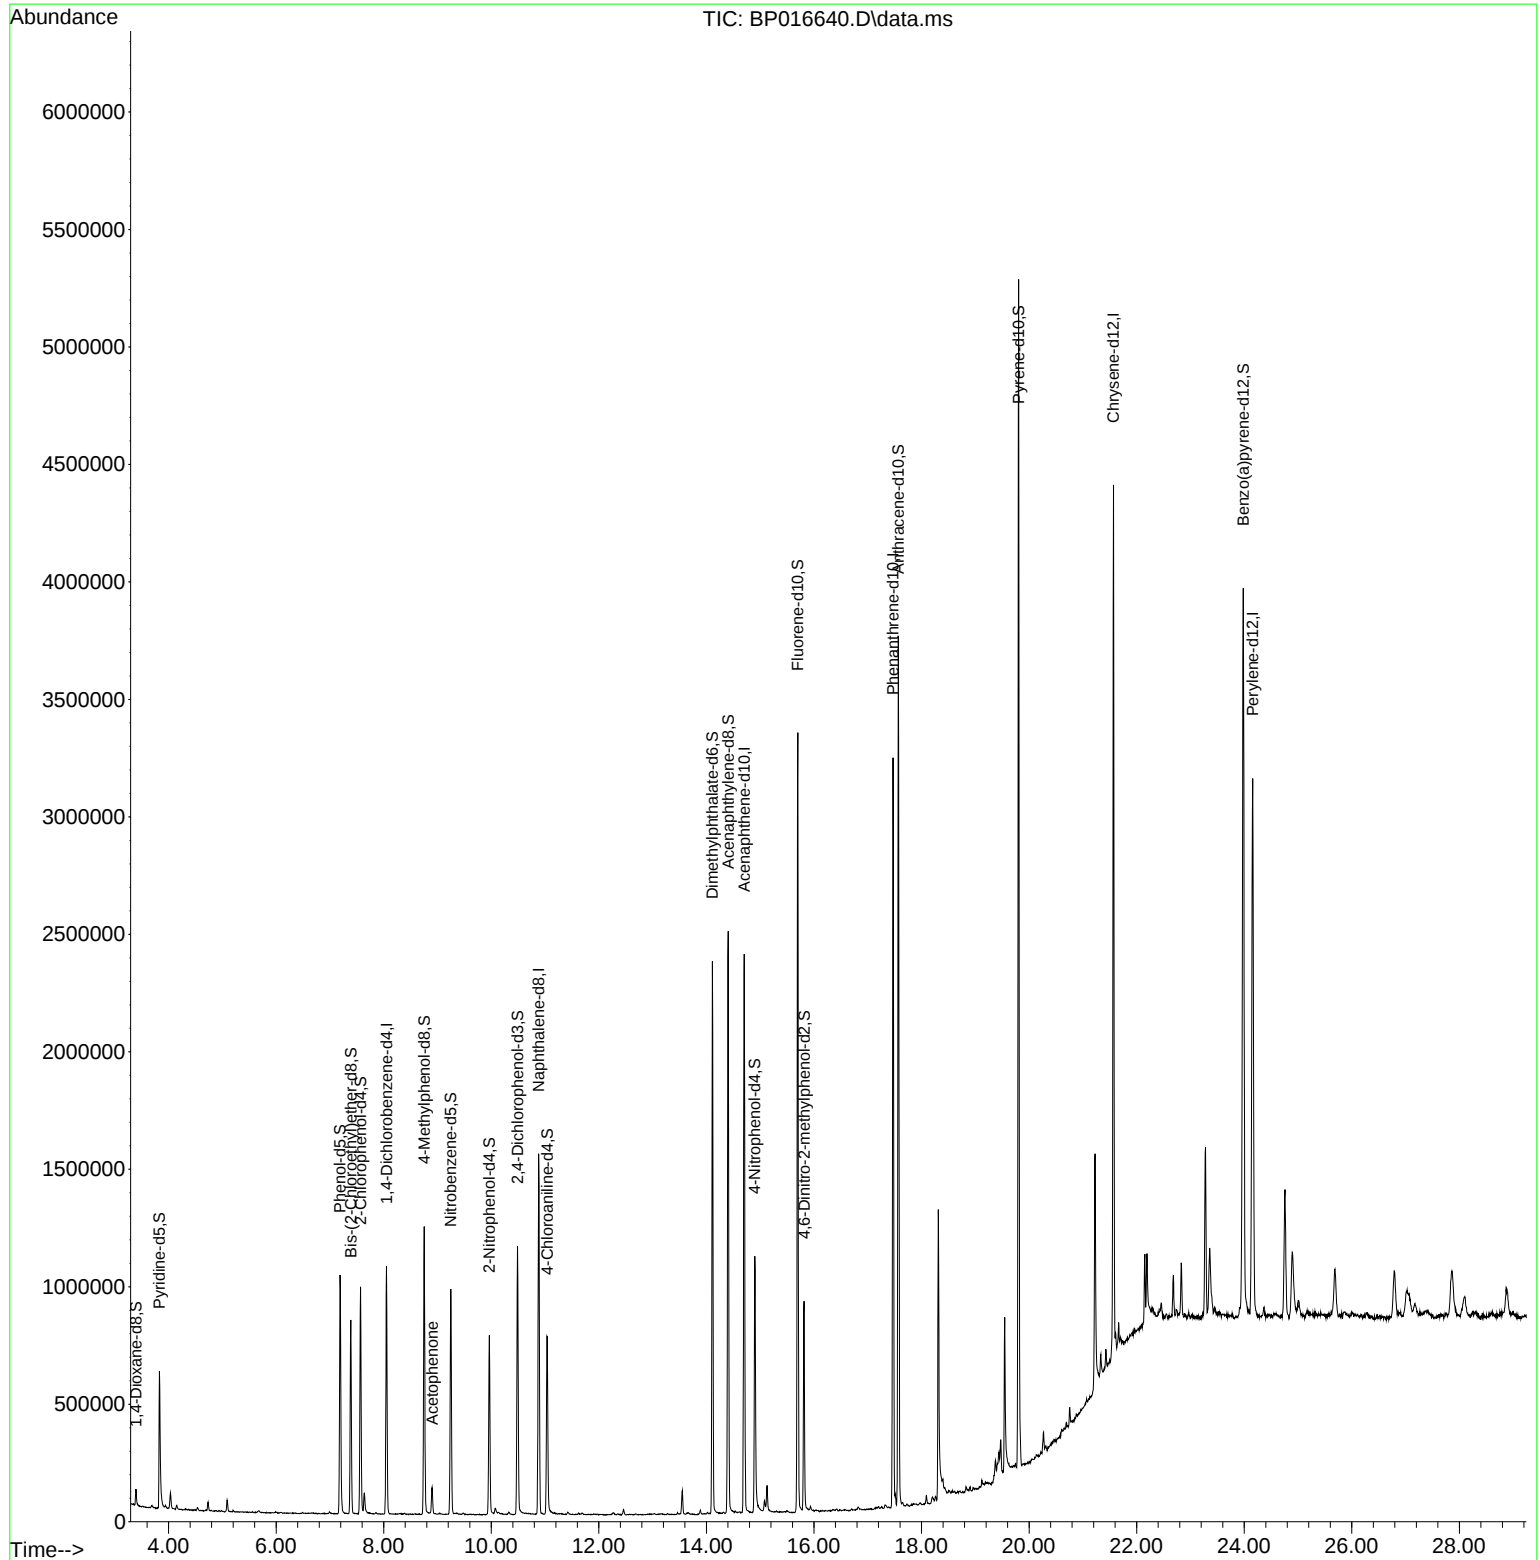

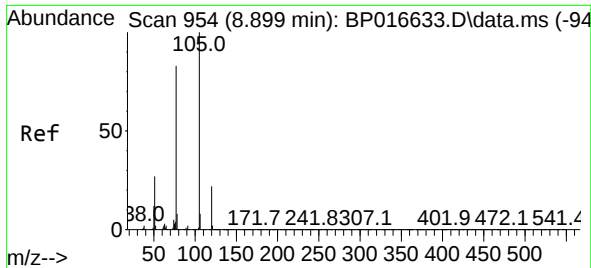

#16
 Acetophenone
 Concen: 1.806 ng/ul
 RT: 8.899 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP016640.D
 Acq: 18 Aug 2023 13:32

Instrument :
 BNA_P
 ClientSampleId :
 A48N8

Tgt Ion:	105	Resp:	57029
Ion	Ratio	Lower	Upper
105	100		
77	83.6	64.4	96.6
51	30.2	21.2	31.8

