

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016643.D
 Acq On : 18 Aug 2023 16:23
 Operator : MA/JU
 Sample : 03968-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48H4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :mohammad ahmed 08/21/2023

Quant Time: Aug 18 23:18:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	317180	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1464514	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.704	164	910477	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.469	188	2043259	20.000	ng/u1	0.00
79) Chrysene-d12	21.569	240	1993187	20.000	ng/u1	0.00
88) Perylene-d12	24.157	264	2035856	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	50438	6.043	ng/uL	0.00
4) Pyridine-d5	3.840	84	19136m	0.754	ng/u1	0.01
7) Phenol-d5	7.187	99	739811	25.300	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	494949	25.699	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	567672	27.028	ng/u1	0.00
15) 4-Methylphenol-d8	8.752	113	456598	19.638	ng/u1	0.00
21) Nitrobenzene-d5	9.246	128	293065	28.440	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	309834	31.657	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	585327	30.389	ng/u1	0.00
31) 4-Chloroaniline-d4	11.040	131	500104	15.133	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	1947616	29.575	ng/u1	0.00
49) Acenaphthylene-d8	14.404	160	2224824	29.932	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	337988	25.194	ng/u1	0.00
60) Fluorene-d10	15.698	176	1700074	30.282	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	248847	25.600	ng/u1	0.00
73) Anthracene-d10	17.569	188	2654674	30.037	ng/u1	0.00
81) Pyrene-d10	19.804	212	3323651	31.824	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	3093562	31.707	ng/u1	0.01
Target Compounds					Qvalue	
16) Acetophenone	8.899	105	190442	5.072	ng/u1	99
61) Fluorene	15.751	166	69782	1.064	ng/u1	99
72) Phenanthrene	17.510	178	1074345	9.980	ng/u1	99
74) Anthracene	17.604	178	234929	2.173	ng/u1	99
77) Carbazole	17.881	167	102880	1.032	ng/u1	99
80) Fluoranthene	19.469	202	1651621	13.250	ng/u1	99
82) Pyrene	19.833	202	1445862	10.985	ng/u1	97
85) Benzo(a)anthracene	21.551	228	738254	5.511	ng/u1	99
86) Bis(2-ethylhexyl)phtha...	21.427	149	77466	1.007	ng/u1	99
87) Chrysene	21.604	228	755362	6.026	ng/u1	98
90) Benzo(b)fluoranthene	23.345	252	1018383	8.401	ng/u1#	94
91) Benzo(k)fluoranthene	23.398	252	290337m	2.414	ng/u1	
93) Benzo(a)pyrene	24.039	252	622720	5.446	ng/u1	99
94) Indeno(1,2,3-cd)pyrene	26.892	276	382079	2.831	ng/u1	96
96) Benzo(g,h,i)perylene	27.757	276	361149	3.362	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016643.D
Acq On : 18 Aug 2023 16:23
Operator : MA/JU
Sample : 03968-01
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A48H4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023


Quant Time: Aug 18 23:18:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

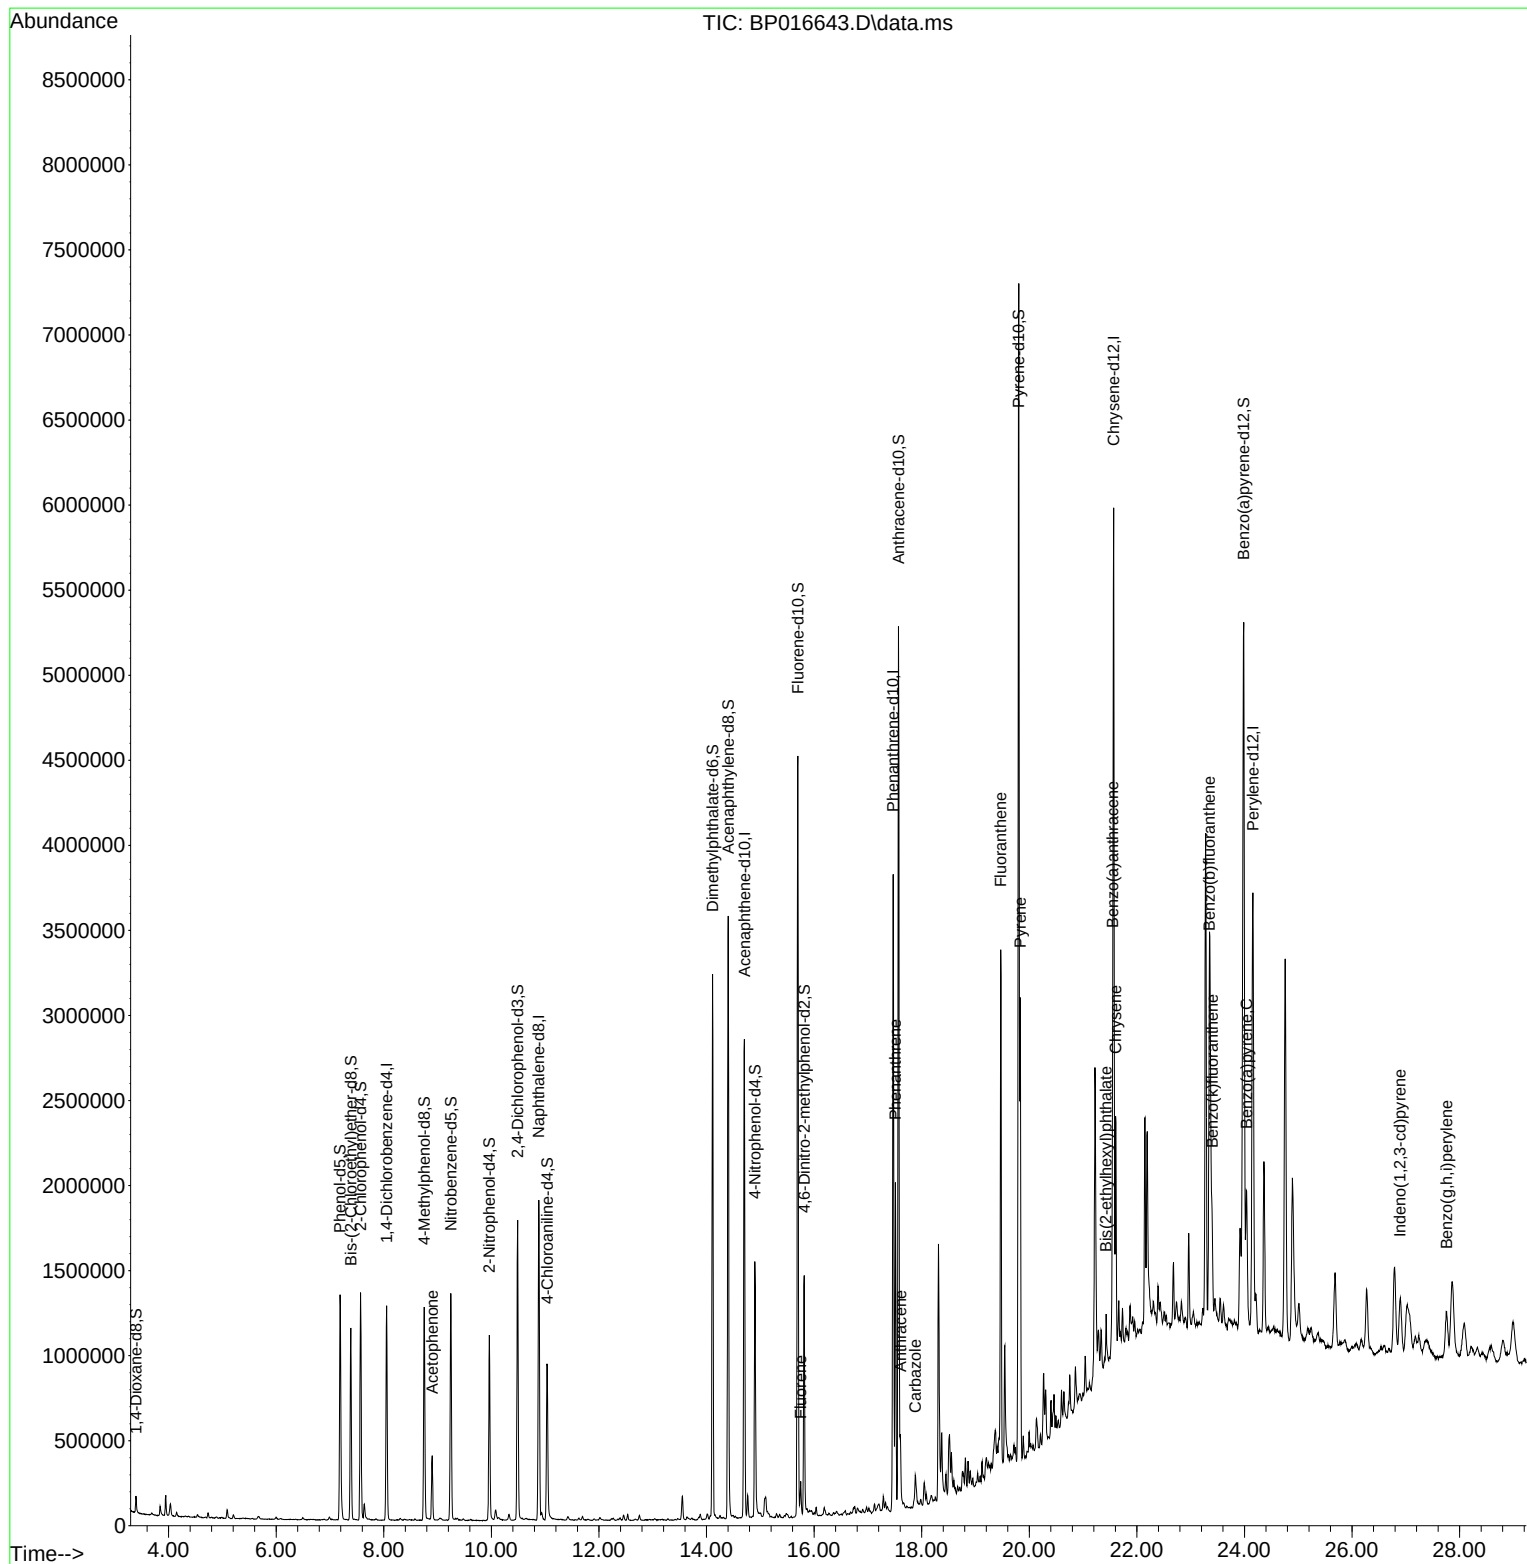

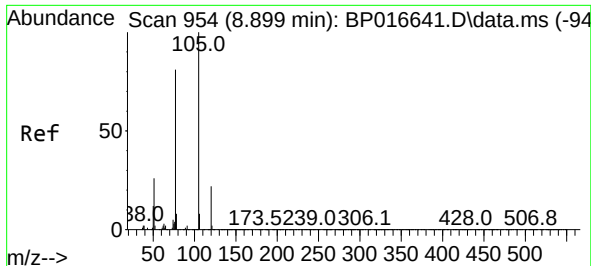

#16
Acetophenone
Concen: 5.072 ng/ul
RT: 8.899 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP016643.D
Acq: 18 Aug 2023 16:23




Instrument :
BNA_P
ClientSampleId :
A48H4

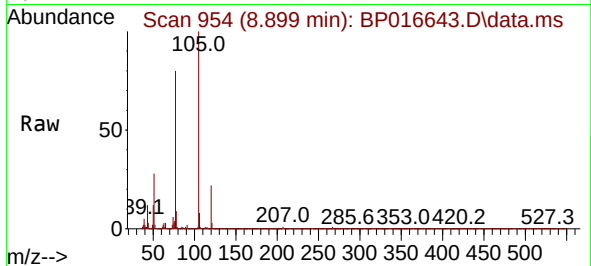

Tgt Ion:105 Resp: 19044
Ion Ratio Lower Upper
105 100
77 79.8 64.4 96.6
51 27.6 21.2 31.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

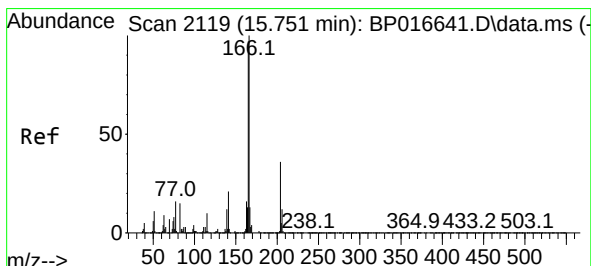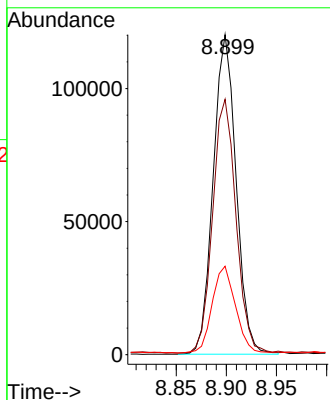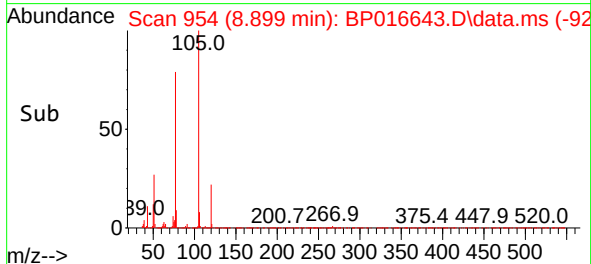

#61
Fluorene
Concen: 1.064 ng/ul
RT: 15.751 min Scan# 2119
Delta R.T. -0.000 min
Lab File: BP016643.D
Acq: 18 Aug 2023 16:23

Tgt Ion:166 Resp: 69782
Ion Ratio Lower Upper
166 100
165 99.2 78.3 117.5
167 13.1 10.8 16.2

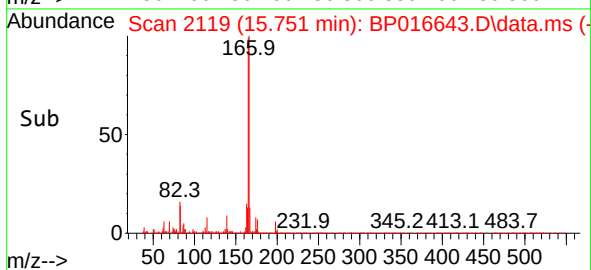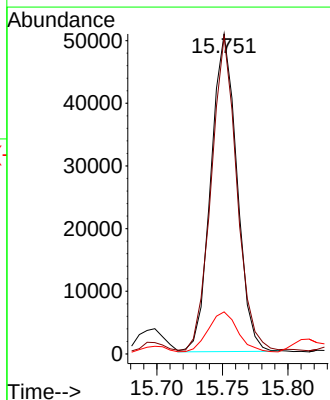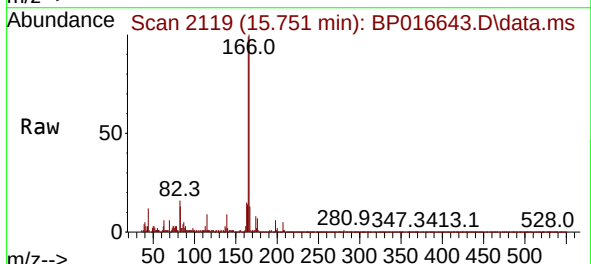

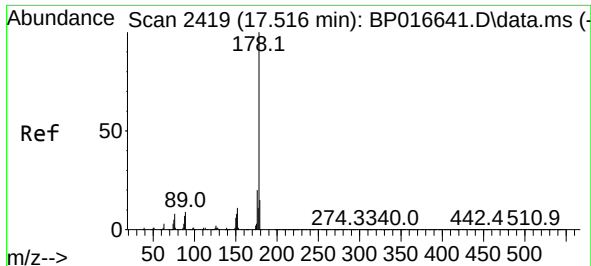





#72
Phenanthrene
Concen: 9.980 ng/ul
RT: 17.510 min Scan# 2419
Delta R.T. -0.000 min
Lab File: BP016643.D
Acq: 18 Aug 2023 16:23

Instrument :
BNA_P
ClientSampleId :
A48H4

Tgt Ion:178 Resp: 107434
Ion Ratio Lower Upper
178 100
179 15.8 12.4 18.6
176 19.1 15.5 23.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2023
Supervised By :mohammad ahmed 08/21/2023

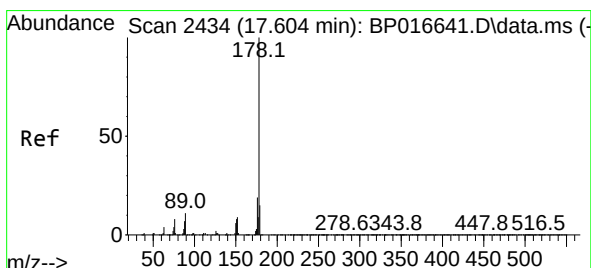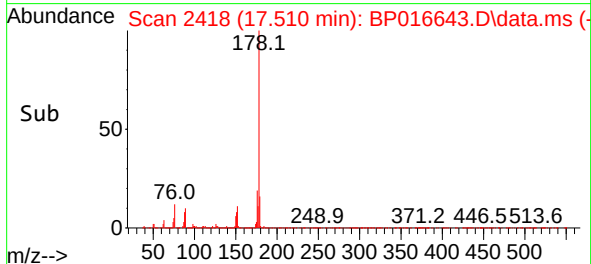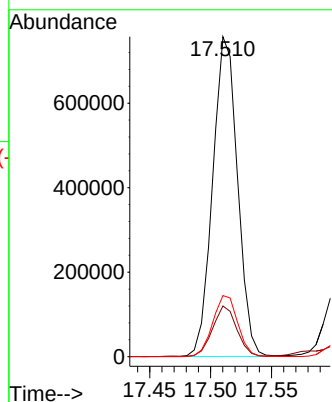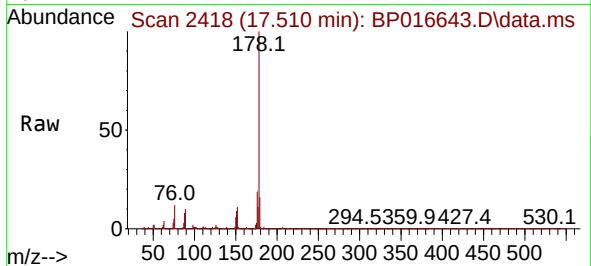

#74
Anthracene
Concen: 2.173 ng/ul
RT: 17.604 min Scan# 2434
Delta R.T. -0.000 min
Lab File: BP016643.D
Acq: 18 Aug 2023 16:23

Tgt Ion:178 Resp: 234929
Ion Ratio Lower Upper
178 100
179 16.0 12.5 18.7
176 18.3 14.9 22.3

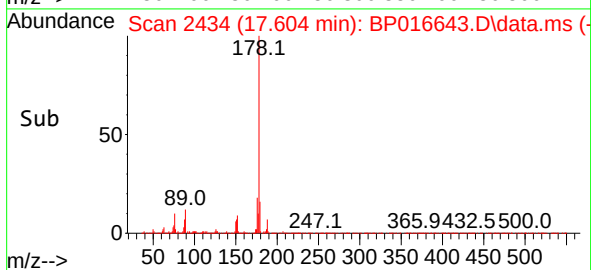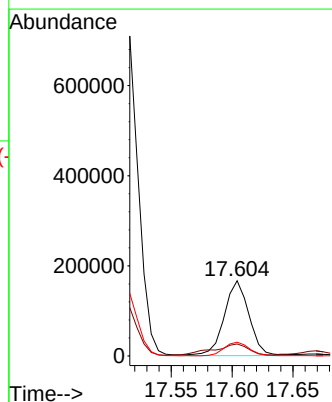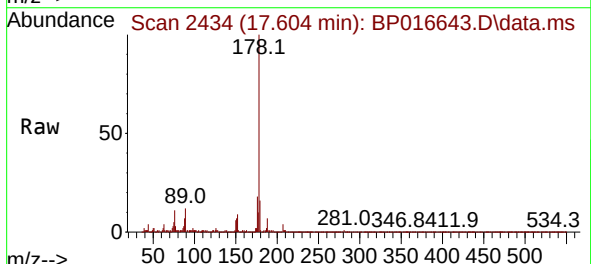

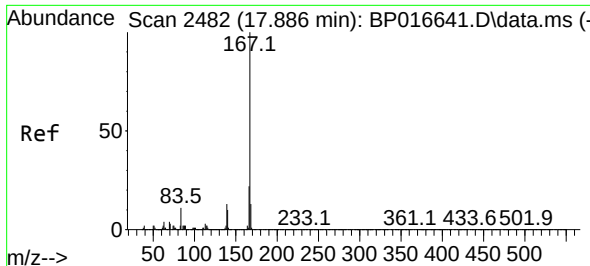





#77
 Carbazole
 Concen: 1.032 ng/ul
 RT: 17.881 min Scan# 2482
 Delta R.T. -0.000 min
 Lab File: BP016643.D
 Acq: 18 Aug 2023 16:23

Instrument :
 BNA_P
 ClientSampleId :
 A48H4

Tgt Ion:167 Resp: 102880
 Ion Ratio Lower Upper
 167 100
 166 20.7 16.8 25.2
 139 13.9 10.6 16.0




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :mohammad ahmed 08/21/2023

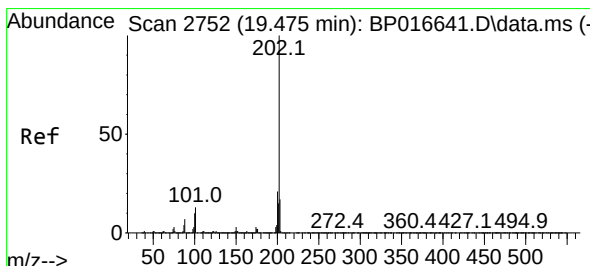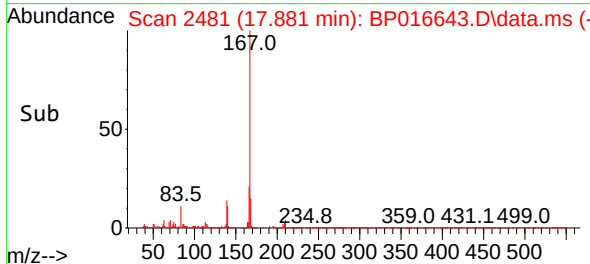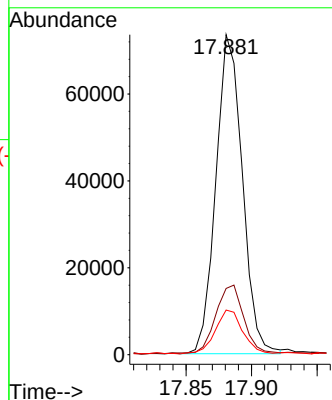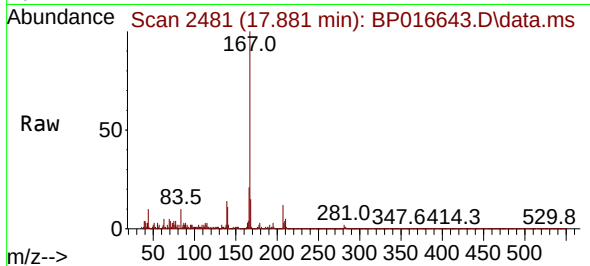

#80
 Fluoranthene
 Concen: 13.250 ng/ul
 RT: 19.469 min Scan# 2751
 Delta R.T. -0.000 min
 Lab File: BP016643.D
 Acq: 18 Aug 2023 16:23


Tgt Ion:202 Resp: 1651621
 Ion Ratio Lower Upper
 202 100
 101 13.9 10.6 16.0
 100 10.7 8.1 12.1

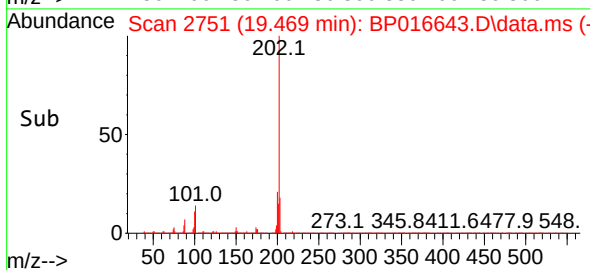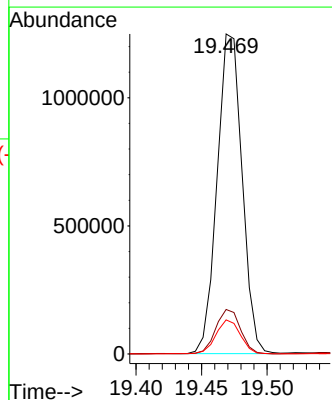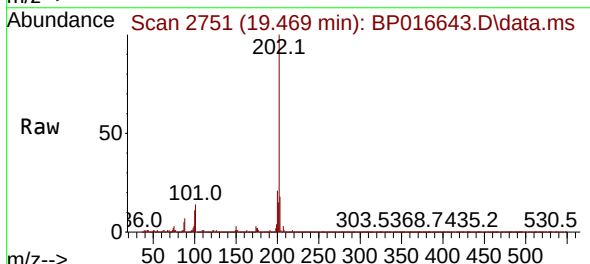

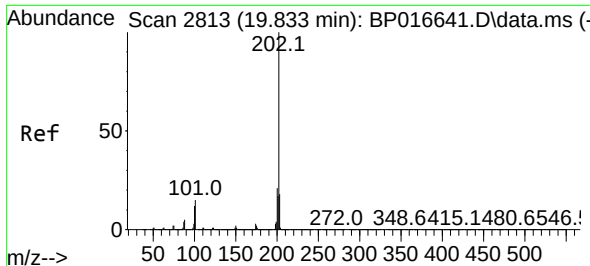

#82
 Pyrene
 Concen: 10.985 ng/ul
 RT: 19.833 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP016643.D
 Acq: 18 Aug 2023 16:23




Instrument :
 BNA_P
 ClientSampleId :
 A48H4

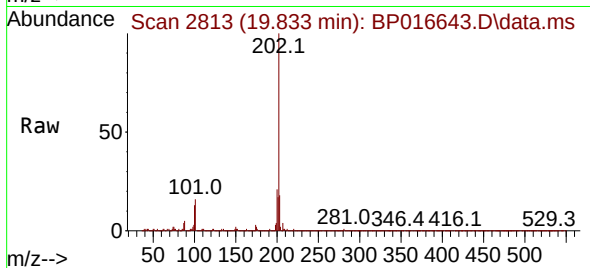

Tgt Ion:202 Resp: 144586
 Ion Ratio Lower Upper
 202 100
 101 15.5 13.4 20.2
 100 12.5 11.0 16.4




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :mohammad ahmed 08/21/2023

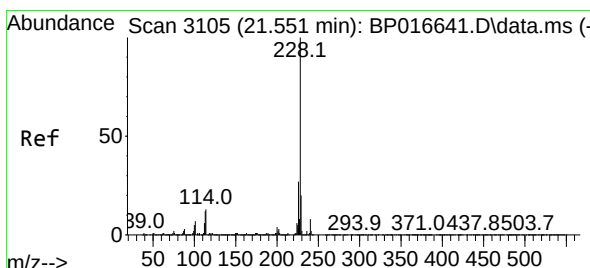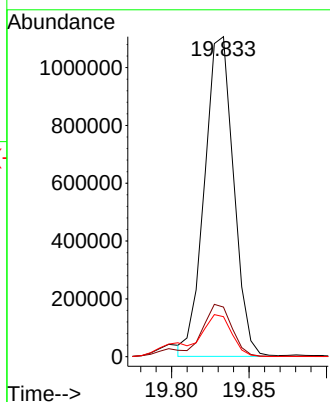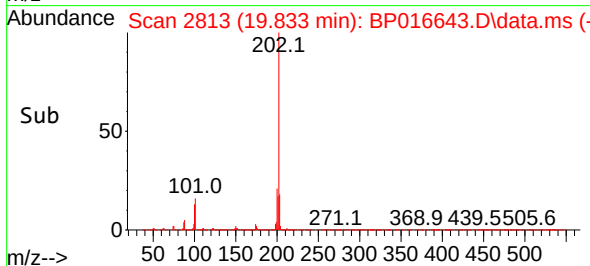

#85
 Benzo(a)anthracene
 Concen: 5.511 ng/ul
 RT: 21.551 min Scan# 3105
 Delta R.T. 0.006 min
 Lab File: BP016643.D
 Acq: 18 Aug 2023 16:23


Tgt Ion:228 Resp: 738254
 Ion Ratio Lower Upper
 228 100
 229 20.7 15.8 23.6
 226 27.5 21.8 32.6

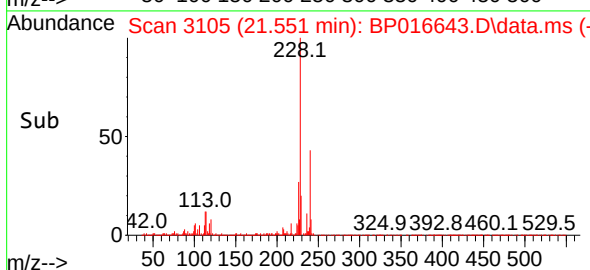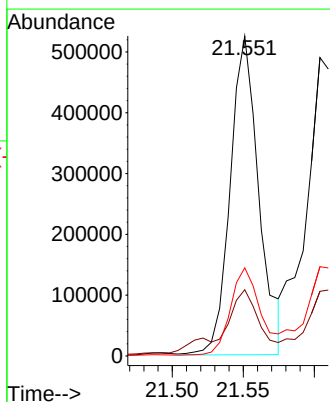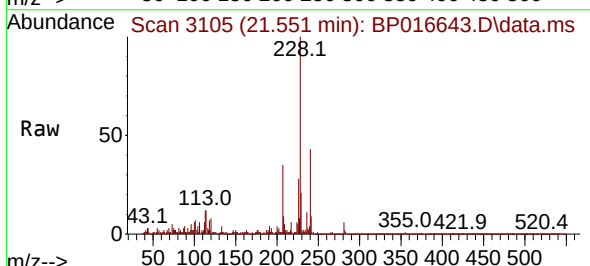

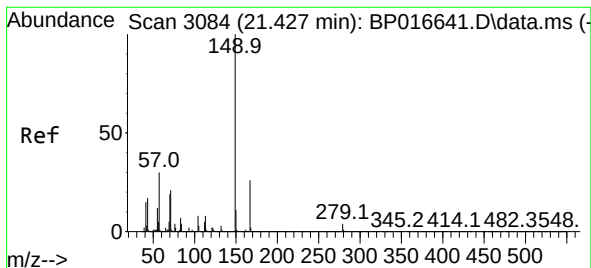

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.007 ng/ul
 RT: 21.427 min Scan# 3084
 Delta R.T. 0.006 min
 Lab File: BP016643.D
 Acq: 18 Aug 2023 16:23




Instrument :
 BNA_P
 ClientSampleId :
 A48H4

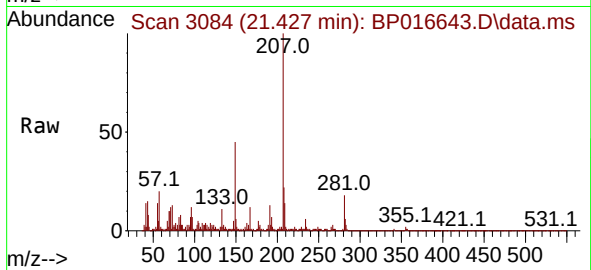

Tgt Ion:149 Resp: 77460
 Ion Ratio Lower Upper
 149 100
 167 26.5 20.9 31.3
 279 3.3 2.6 4.0




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :mohammad ahmed 08/21/2023

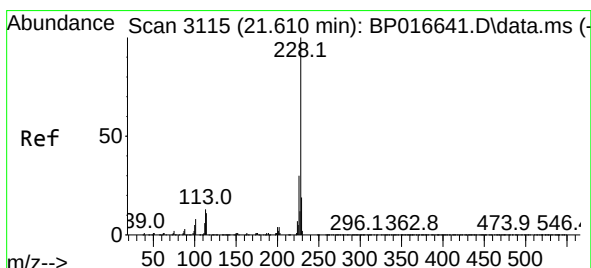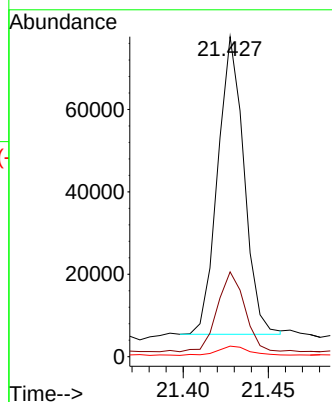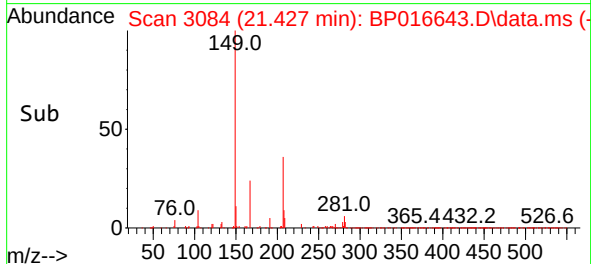

#87
 Chrysene
 Concen: 6.026 ng/ul
 RT: 21.604 min Scan# 3114
 Delta R.T. -0.000 min
 Lab File: BP016643.D
 Acq: 18 Aug 2023 16:23

Tgt Ion:228 Resp: 755362
 Ion Ratio Lower Upper
 228 100
 226 29.9 24.6 36.8
 229 21.7 16.4 24.6

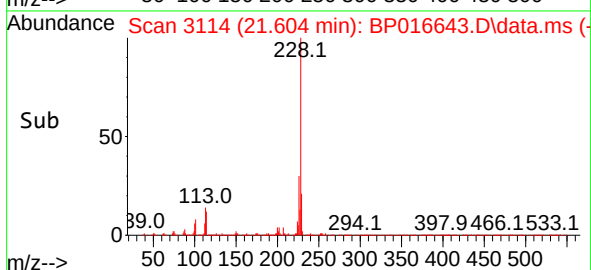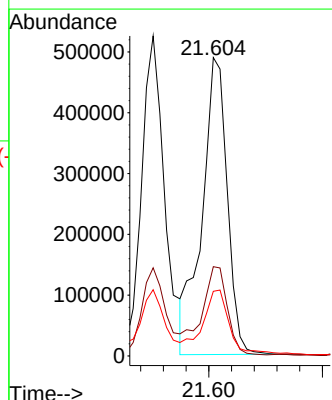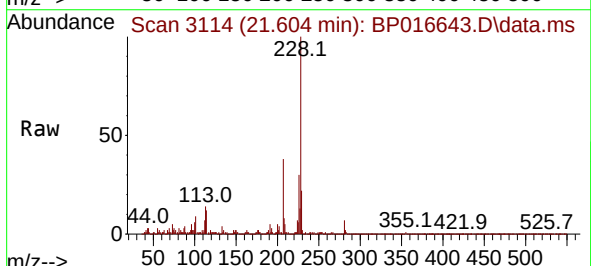

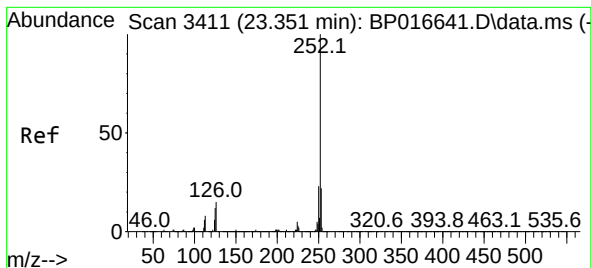

#90

Benzo(b)fluoranthene

Concen: 8.401 ng/ul

RT: 23.345 min Scan# 3411

Delta R.T. 0.006 min

Lab File: BP016643.D

Acq: 18 Aug 2023 16:23

Instrument :

BNA_P

ClientSampleId :

A48H4

Tgt Ion:252 Resp: 101838

Ion Ratio Lower Upper

252 100

253 23.4 17.4 26.2





125 16.5 10.0 15.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/21/2023

Supervised By :mohammad ahmed 08/21/2023

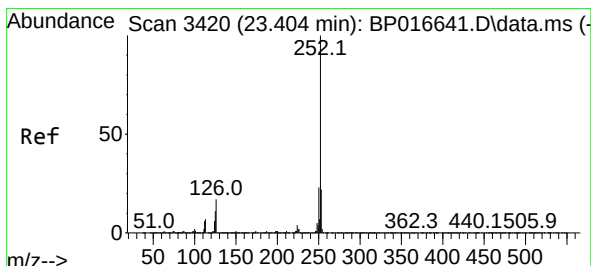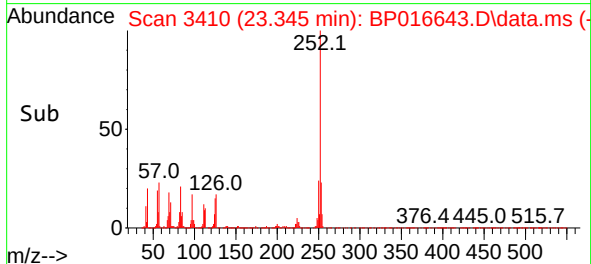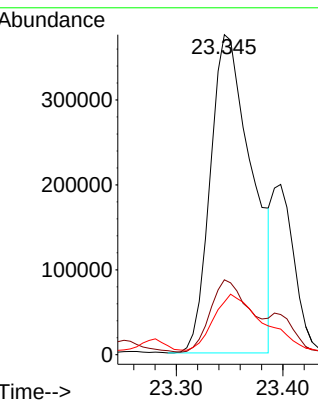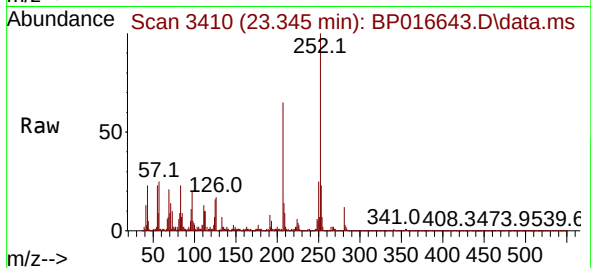

#91

Benzo(k)fluoranthene

Concen: 2.414 ng/ul m

RT: 23.398 min Scan# 3419

Delta R.T. 0.006 min

Lab File: BP016643.D

Acq: 18 Aug 2023 16:23




Tgt Ion:252 Resp: 290337


Ion Ratio Lower Upper

252 100

253 23.6 18.0 27.0

125 15.0 9.8 14.8

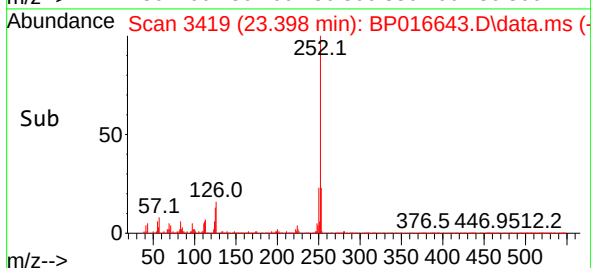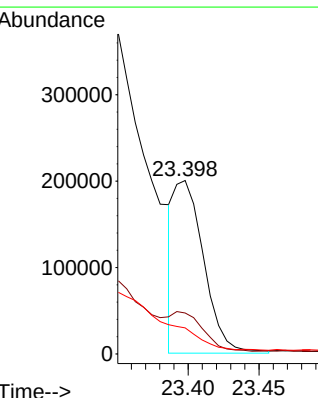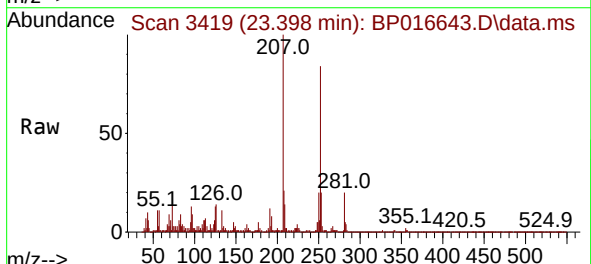

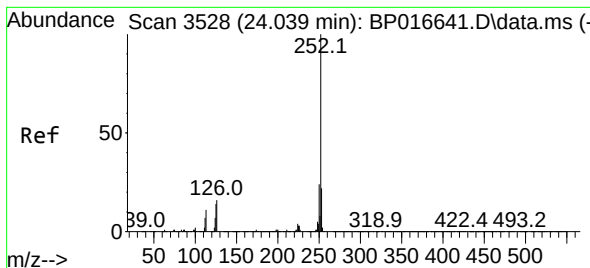

#93

Benzo(a)pyrene

Concen: 5.446 ng/ul

RT: 24.039 min Scan# 3528

Delta R.T. 0.012 min

Lab File: BP016643.D

Acq: 18 Aug 2023 16:23

Instrument :

BNA_P

ClientSampleId :

A48H4





Tgt Ion:	252	Resp:	622720
Ion Ratio	Lower	Upper	
252	100		
253	22.7	17.7	26.5
125	13.9	10.6	15.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/21/2023

Supervised By :mohammad ahmed 08/21/2023

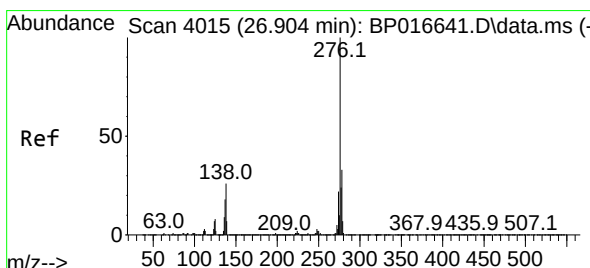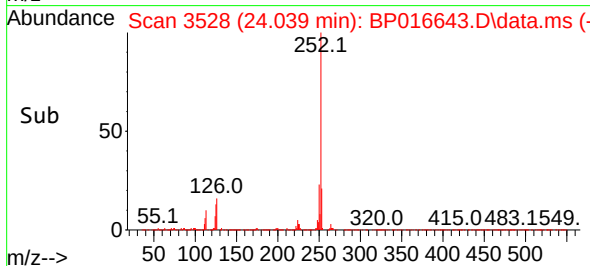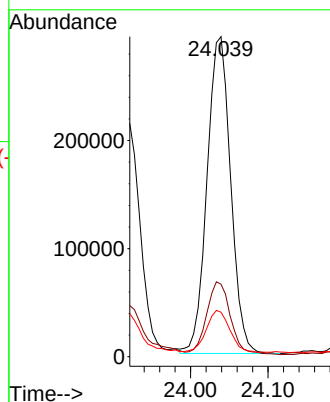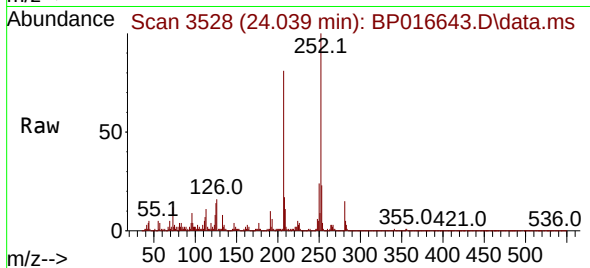

#94

Indeno(1,2,3-cd)pyrene

Concen: 2.831 ng/ul




RT: 26.892 min Scan# 4013


Delta R.T. 0.006 min

Lab File: BP016643.D

Acq: 18 Aug 2023 16:23


Tgt Ion:	276	Resp:	382079
Ion Ratio	Lower	Upper	
276	100		
138	24.6	21.7	32.5
277	25.4	19.5	29.3

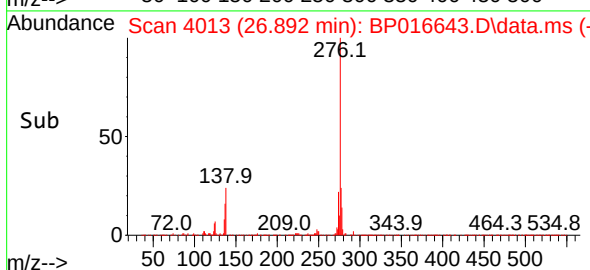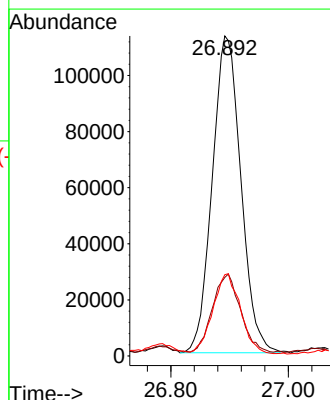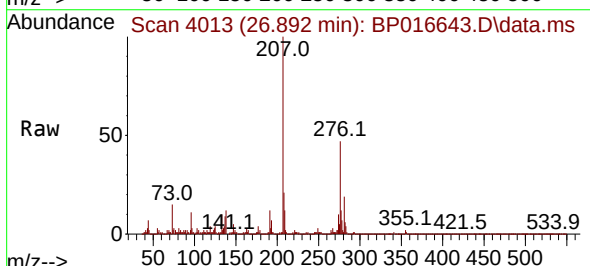

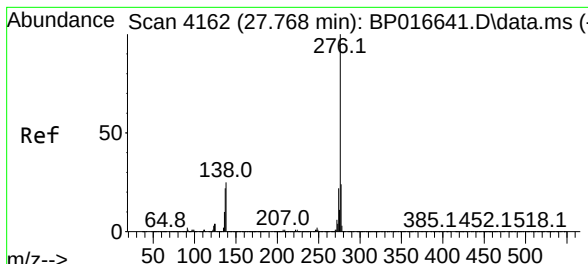

#96
 Benzo(g,h,i)perylene
 Concen: 3.362 ng/ul
 RT: 27.757 min Scan# 4160
 Delta R.T. 0.012 min
 Lab File: BP016643.D
 Acq: 18 Aug 2023 16:23

Instrument :
 BNA_P
 ClientSampleId :
 A48H4

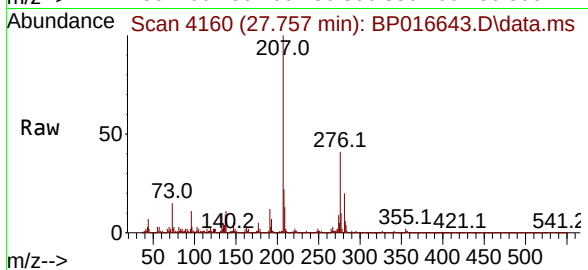

Tgt Ion:	276	Resp:	361149
Ion Ratio	Lower	Upper	
276	100		
138	26.6	21.5	32.3
277	25.1	19.3	28.9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :mohammad ahmed 08/21/2023

