

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016650.D
 Acq On : 18 Aug 2023 20:22
 Operator : MA/JU
 Sample : 03968-28
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A48P7

Quant Time: Aug 18 23:35:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	316578	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	1446700	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164	924508	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	2020169	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	1683276	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1490441	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	56550	6.788	ng/uL	0.00
4) Pyridine-d5	3.828	84	663705	26.184	ng/ul	0.00
7) Phenol-d5	7.193	99	879133	30.122	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	551380	28.683	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	626026	29.863	ng/ul	0.00
15) 4-Methylphenol-d8	8.752	113	721323	31.082	ng/ul	0.00
21) Nitrobenzene-d5	9.246	128	333347	32.747	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	356544	36.878	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	649247	34.123	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	1026673	31.449	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	2474821	37.010	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	2733654	36.219	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	408460	29.985	ng/ul	0.00
60) Fluorene-d10	15.698	176	2110645	37.025	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	249060	25.915	ng/ul	0.00
73) Anthracene-d10	17.569	188	3345740	38.288	ng/ul	0.00
81) Pyrene-d10	19.798	212	3797829	43.059	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	2797689	39.168	ng/ul	0.00


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.422	149	86841	1.336 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016650.D
Acq On : 18 Aug 2023 20:22
Operator : MA/JU
Sample : 03968-28
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A48P7

Quant Time: Aug 18 23:35:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

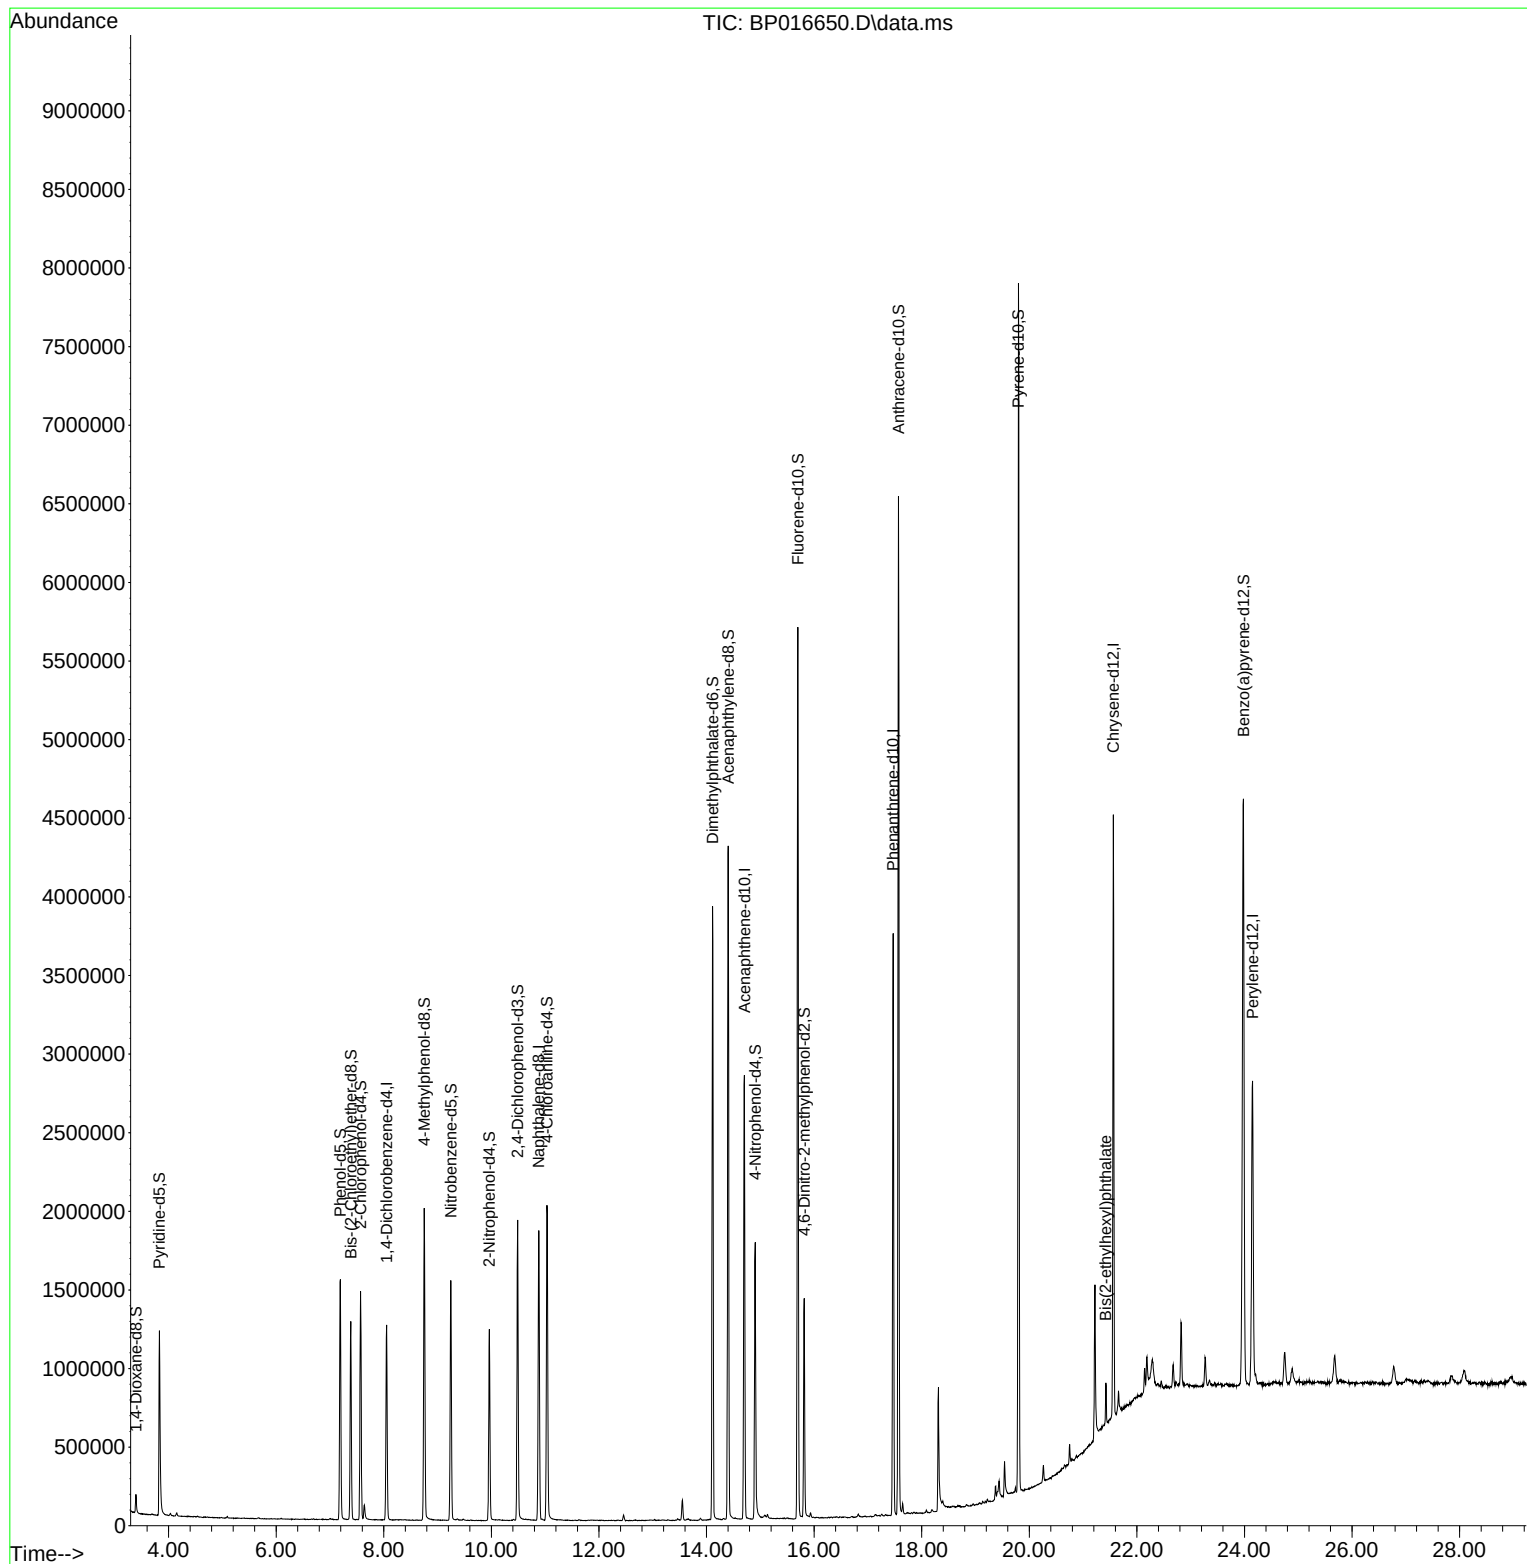

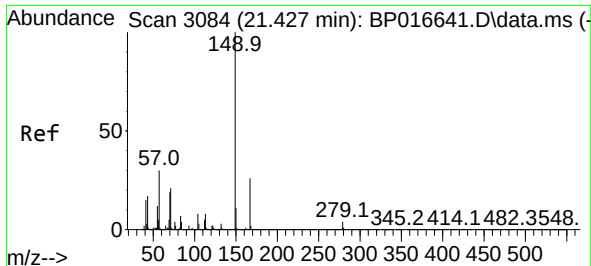

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.336 ng/ul
 RT: 21.422 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BP016650.D
 Acq: 18 Aug 2023 20:22

Instrument :
 BNA_P
 ClientSampleId :
 A48P7

Tgt Ion:149 Resp: 86841
 Ion Ratio Lower Upper
 149 100
 167 25.7 20.9 31.3
 279 3.4 2.6 4.0

