

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016660.D
 Acq On : 19 Aug 2023 03:11
 Operator : MA/JU
 Sample : 04049-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH8T5

Quant Time: Aug 19 04:00:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	278801	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1245767	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.698	164	764586	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.469	188	1687345	20.000	ng/u1	0.00
79) Chrysene-d12	21.563	240	1481674	20.000	ng/u1	0.00
88) Perylene-d12	24.145	264	1362707	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	36407	4.962	ng/uL	0.00
4) Pyridine-d5	3.828	84	413739	18.534	ng/u1	0.00
7) Phenol-d5	7.187	99	304207	11.835	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	760156	44.902	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	694522	37.620	ng/u1	0.00
15) 4-Methylphenol-d8	8.752	113	517102	25.301	ng/u1	0.00
21) Nitrobenzene-d5	9.246	128	450954	51.446	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	458094	55.024	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	752335	45.919	ng/u1	0.00
31) 4-Chloroaniline-d4	11.034	131	1118344	39.783	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	2766203	50.020	ng/u1	0.00
49) Acenaphthylene-d8	14.398	160	3075768	49.276	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	110374	9.797	ng/u1	0.00
60) Fluorene-d10	15.692	176	2378883	50.458	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	371313	46.257	ng/u1	0.00
73) Anthracene-d10	17.569	188	3995189	54.739	ng/u1	0.00
81) Pyrene-d10	19.798	212	4581496	59.012	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.980	264	3682578	56.389	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.428	88	32993	4.090	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016660.D
Acq On : 19 Aug 2023 03:11
Operator : MA/JU
Sample : 04049-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH8T5

Quant Time: Aug 19 04:00:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

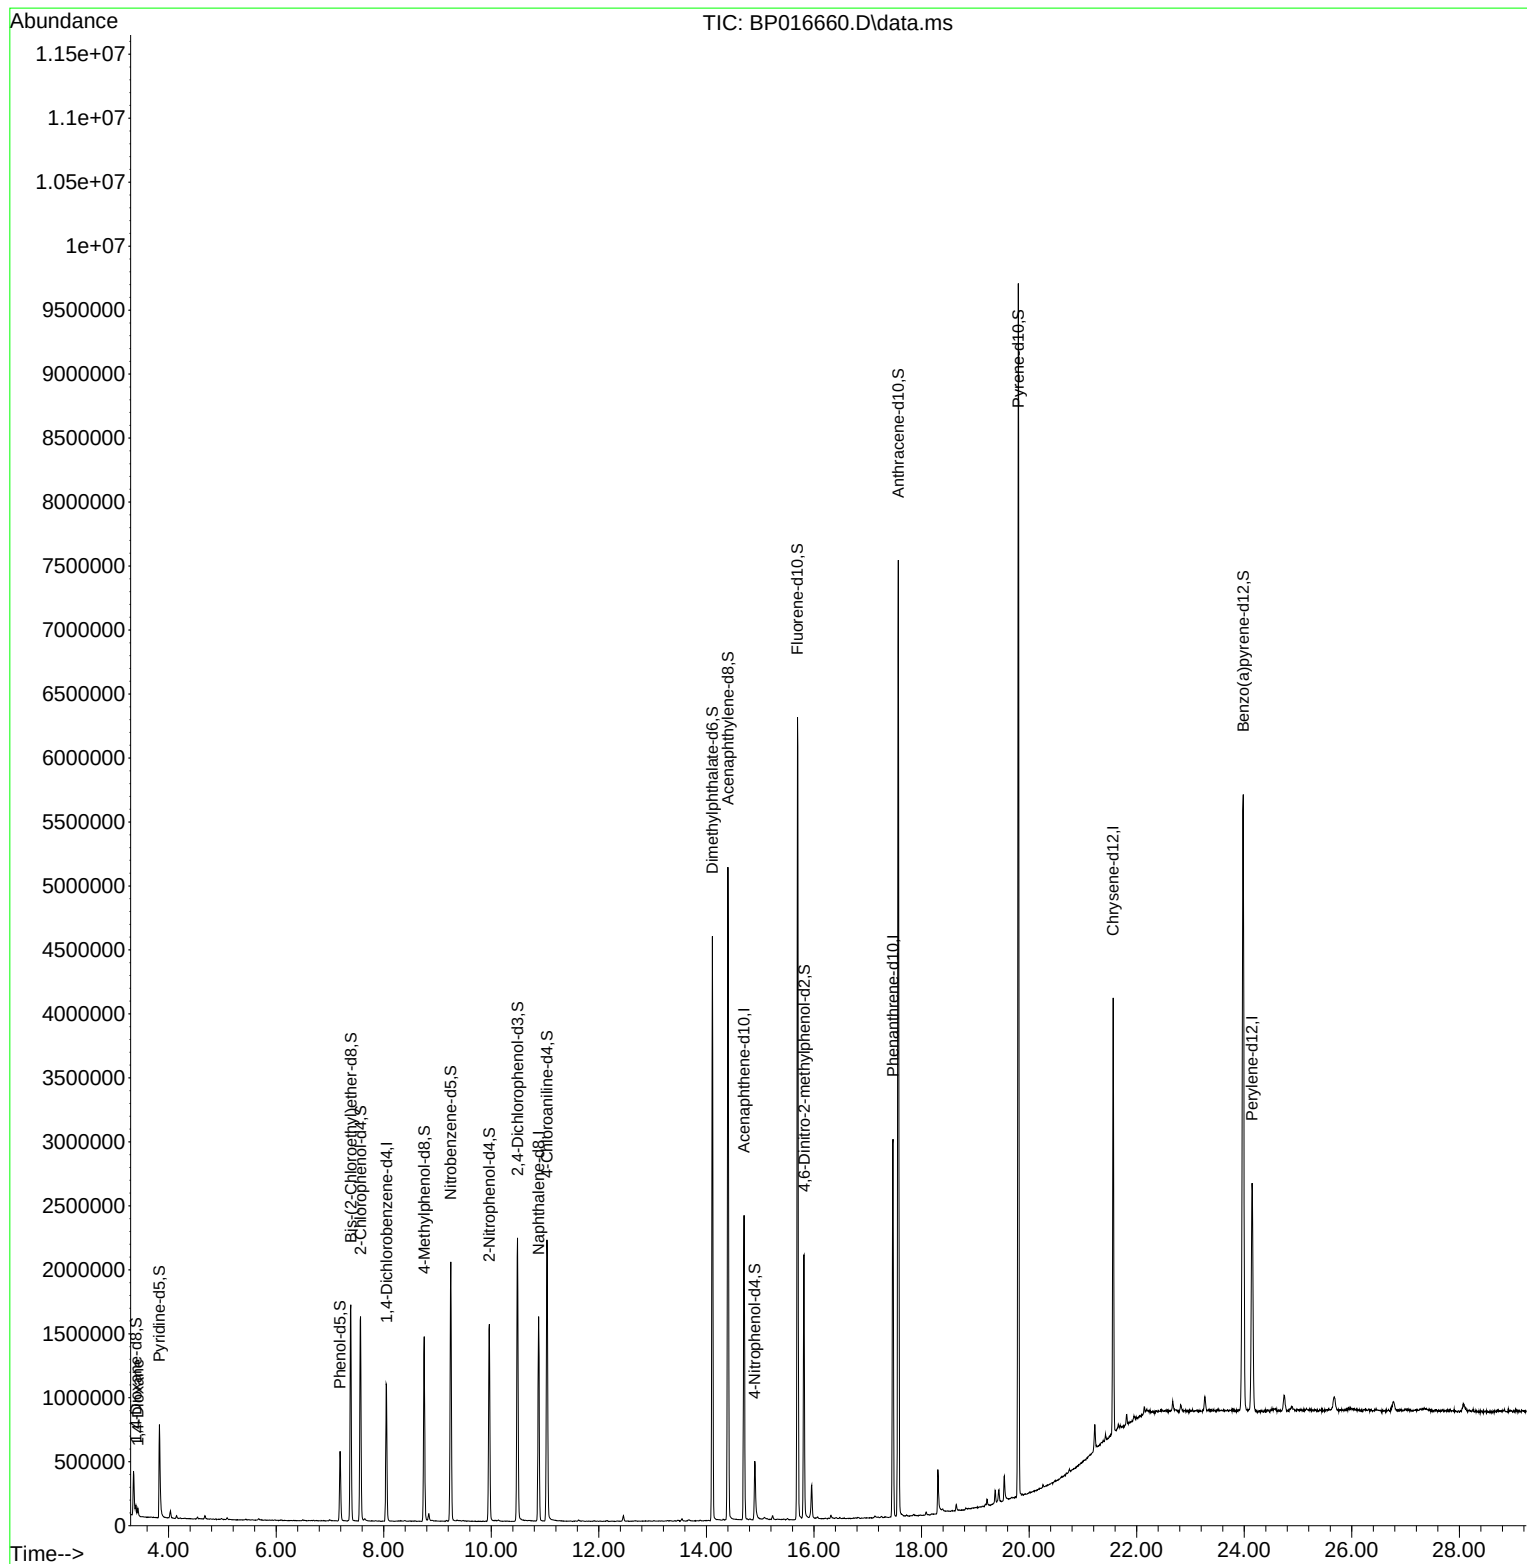

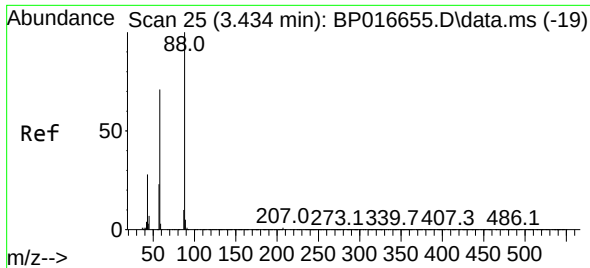

#2
 1,4-Dioxane
 Concen: 4.090 ng/uL
 RT: 3.428 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BP016660.D
 Acq: 19 Aug 2023 03:11

Instrument :
 BNA_P
 ClientSampleId :
 BH8T5

Tgt Ion: 88	Resp: 32993
Ion Ratio	Lower Upper
88	100
43	32.4 23.5 35.3
58	73.2 57.1 85.7

