

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016661.D
 Acq On : 19 Aug 2023 03:45
 Operator : MA/JU
 Sample : 04049-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH944

Quant Time: Aug 19 04:16:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 01:38:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	324320	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1447103	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.699	164	887032	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.469	188	1939124	20.000	ng/u1	0.00
79) Chrysene-d12	21.563	240	1644171	20.000	ng/u1	0.00
88) Perylene-d12	24.145	264	1477389	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	26924	3.155	ng/uL	0.00
4) Pyridine-d5	3.829	84	317341	12.221	ng/u1	0.00
7) Phenol-d5	7.187	99	221284	7.401	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	650853	33.049	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	565781	26.345	ng/u1	0.00
15) 4-Methylphenol-d8	8.752	113	405696	17.064	ng/u1	0.00
21) Nitrobenzene-d5	9.246	128	381937	37.510	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	380974	39.394	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	636011	33.418	ng/u1	0.00
31) 4-Chloroaniline-d4	11.034	131	775181	23.739	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	2437177	37.987	ng/u1	0.00
49) Acenaphthylene-d8	14.399	160	2673210	36.915	ng/u1	0.00
54) 4-Nitrophenol-d4	14.899	143	73631	5.634	ng/u1	0.00
60) Fluorene-d10	15.693	176	2083016	38.084	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	309237	33.521	ng/u1	0.00
73) Anthracene-d10	17.569	188	3571854	42.584	ng/u1	0.00
81) Pyrene-d10	19.798	212	4056137	47.082	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	3088038	43.615	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.429	88	42524	4.531	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016661.D
Acq On : 19 Aug 2023 03:45
Operator : MA/JU
Sample : 04049-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH944

Quant Time: Aug 19 04:16:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 01:38:34 2023
Response via : Initial Calibration

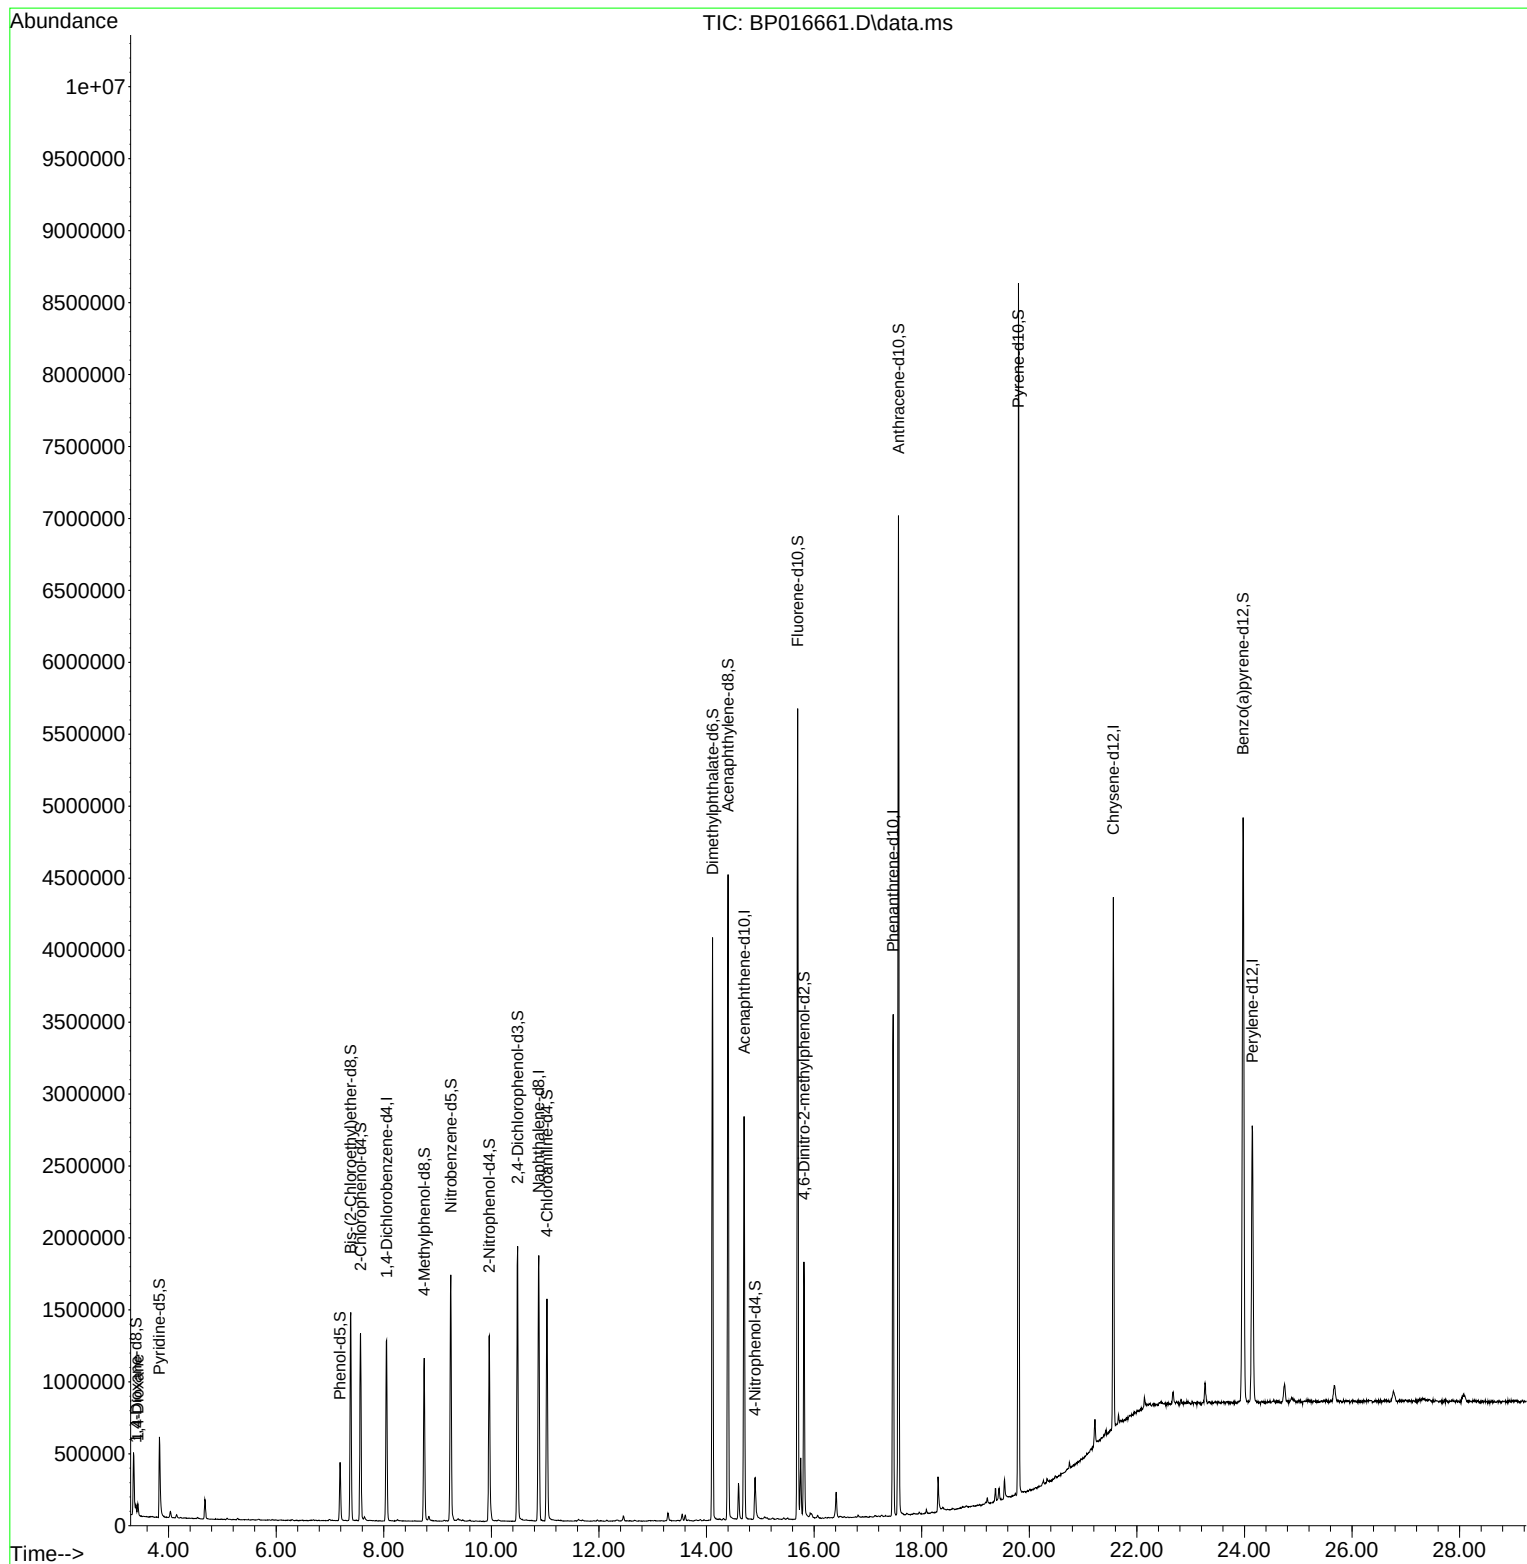

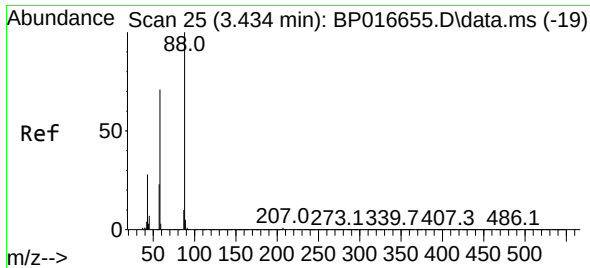

#2
 1,4-Dioxane
 Concen: 4.531 ng/uL
 RT: 3.429 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BP016661.D
 Acq: 19 Aug 2023 03:45

Instrument :
 BNA_P
 ClientSampleId :
 BH944

Tgt Ion: 88 Resp: 42524
 Ion Ratio Lower Upper
 88 100
 43 31.6 23.5 35.3
 58 76.1 57.1 85.7

