

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
 Data File : BP016634.D
 Acq On : 18 Aug 2023 09:34
 Operator : MA/JU
 Sample : PB154871BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK871

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	14	18	26	rVB	121514	166128	1.83%	0.174%
2	3.828	88	92	109	rBV	1297987	2012670	22.22%	2.112%
3	4.146	142	146	155	rVB	73839	115054	1.27%	0.121%
4	7.193	656	664	679	rBV	1463124	2354817	26.00%	2.471%
5	7.387	690	697	706	rBV	1273903	1918351	21.18%	2.013%
6	7.569	720	728	737	rBV	1451016	2269760	25.06%	2.382%
7	8.052	802	810	818	rBV	1316593	2045917	22.59%	2.147%
8	8.752	921	929	946	rBV	1795179	2912365	32.15%	3.056%
9	9.246	1006	1013	1025	rBV	1408358	2326578	25.69%	2.442%
10	9.963	1121	1135	1146	rBV	1169728	1918629	21.18%	2.013%
11	10.487	1216	1224	1237	rBV	1674405	2789439	30.80%	2.927%
12	10.881	1280	1291	1299	rBV	1887866	3126044	34.51%	3.281%
13	11.040	1308	1318	1331	rBV	1795974	3134250	34.60%	3.289%
14	12.457	1552	1559	1566	rBV	28985	53641	0.59%	0.056%
15	13.551	1740	1745	1751	rBV3	32270	54002	0.60%	0.057%
16	14.110	1834	1840	1855	rBV	3407189	4740590	52.34%	4.975%
17	14.404	1883	1890	1907	rBV	3733222	5484199	60.55%	5.755%
18	14.704	1934	1941	1949	rBV	2950013	4327010	47.77%	4.541%
19	14.904	1967	1975	1990	rBV	1612020	2600417	28.71%	2.729%
20	15.081	2002	2005	2012	rBV7	16965	32011	0.35%	0.034%
21	15.698	2103	2110	2119	rBV	4834192	6814110	75.23%	7.151%
22	15.816	2124	2130	2146	rVV	1563448	2166542	23.92%	2.274%
23	15.934	2146	2150	2161	rVB2	26670	49307	0.54%	0.052%
24	16.487	2239	2244	2248	rBV7	6837	11922	0.13%	0.013%
25	17.134	2351	2354	2358	rBV6	7035	10392	0.11%	0.011%
26	17.257	2371	2375	2380	rBV3	9250	15555	0.17%	0.016%
27	17.469	2405	2411	2422	rBV	3775940	5385329	59.46%	5.651%
28	17.569	2422	2428	2440	rVV2	5227236	7684414	84.84%	8.064%
29	18.310	2550	2554	2564	rBV3	134685	272388	3.01%	0.286%
30	19.375	2732	2735	2740	rVB	65324	85760	0.95%	0.090%
31	19.445	2743	2747	2752	rVB	64632	88207	0.97%	0.093%
32	19.545	2761	2764	2770	rBV4	70052	112441	1.24%	0.118%
33	19.804	2802	2808	2819	rBV	6860714	9057812	100.00%	9.505%
34	21.569	3103	3108	3117	rBV	4281206	5586164	61.67%	5.862%
35	23.986	3511	3519	3529	rVB2	3836763	8332101	91.99%	8.744%
36	24.157	3541	3548	3560	rVB	2352794	5236582	57.81%	5.495%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016634.D
Acq On : 18 Aug 2023 09:34
Operator : MA/JU
Sample : PB154871BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 95290898

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016634.D
Acq On : 18 Aug 2023 09:34
Operator : MA/JU
Sample : PB154871BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

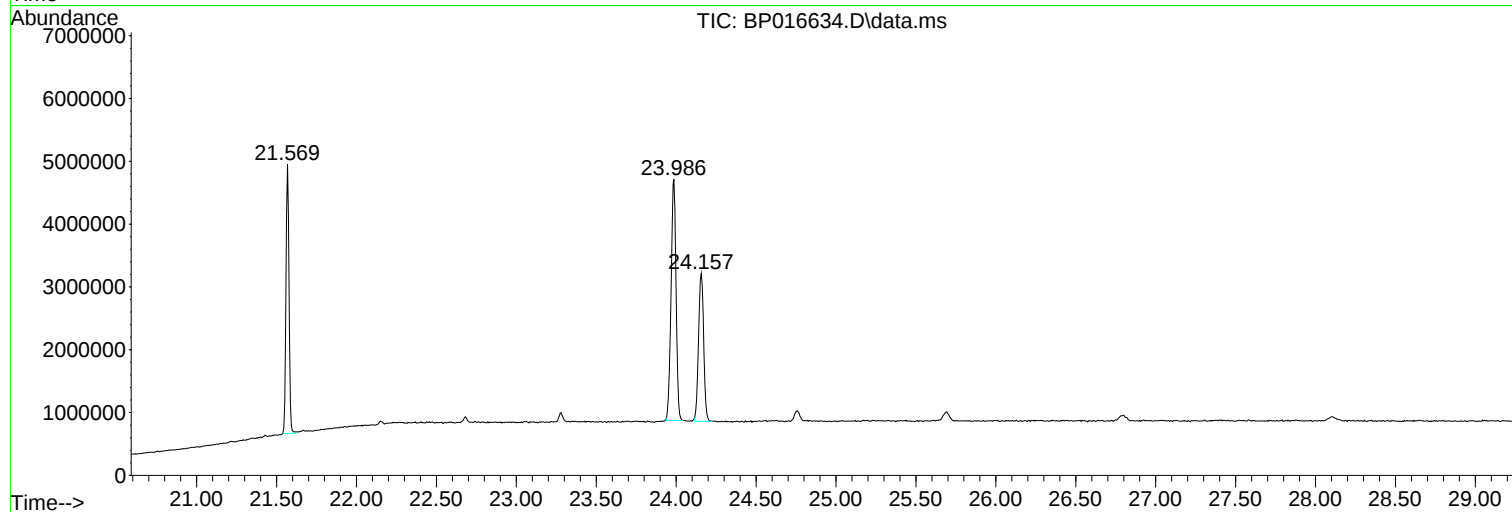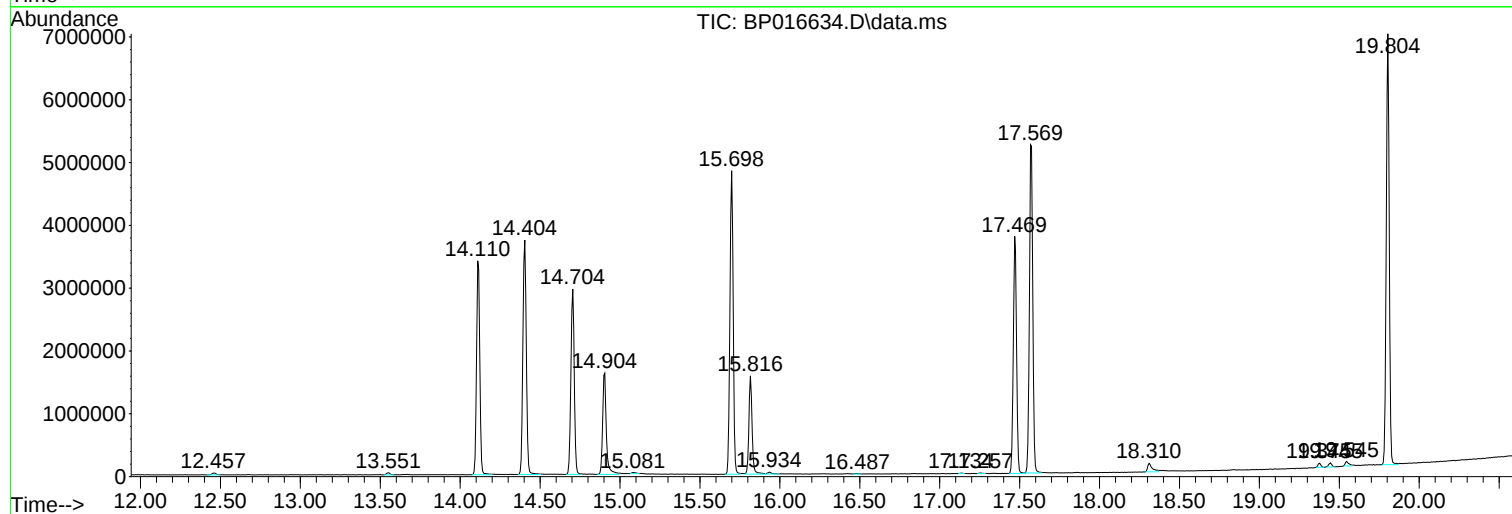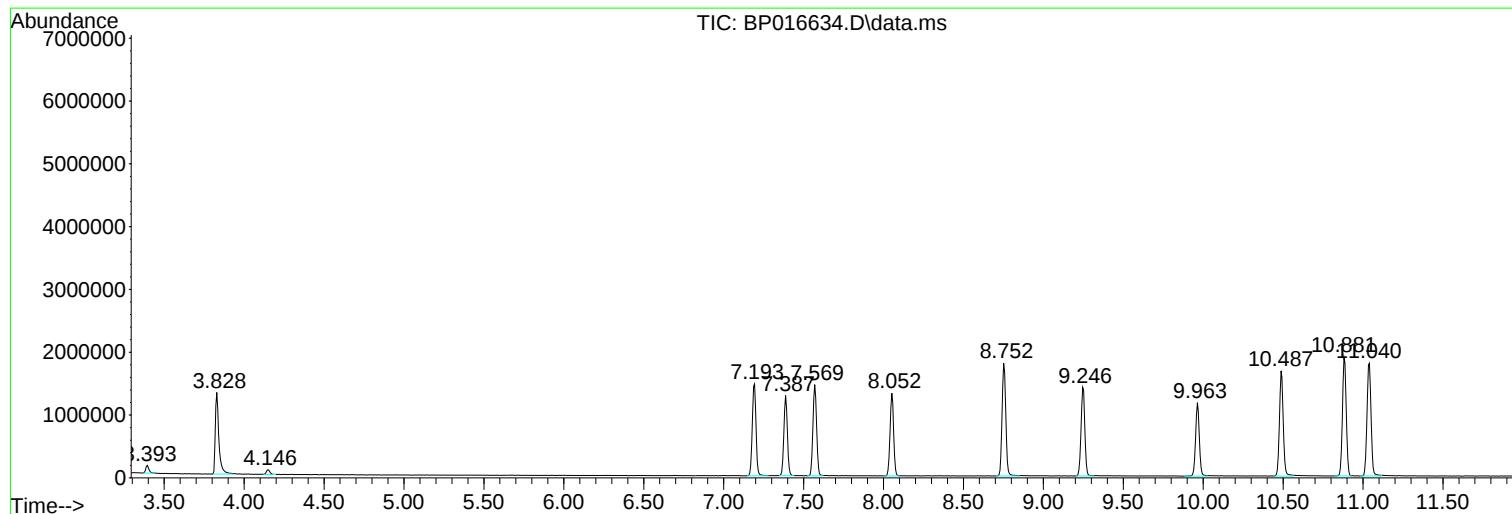

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016634.D
Acq On : 18 Aug 2023 09:34
Operator : MA/JU
Sample : PB154871BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081823\
Data File : BP016634.D
Acq On : 18 Aug 2023 09:34
Operator : MA/JU
Sample : PB154871BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
